

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031119\
 Data File : PL045675.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2019 16:20
 Operator : AJ\SJ
 Sample : K1817-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-027-SW015-030719

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:09:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	85743833	27373838	12.464	12.782
28)	SA Decachlor...	8.046	9.039	78435057	22716197	9.374	9.942
Target Compounds							
10)	B gamma-Chl...	5.279f	6.087	125.4E6	10300732	12.817	3.839 #
11)	B alpha-Chl...	5.313	6.163	17984162	33475366	1.855	12.409 #
12)	B 4,4'-DDE	5.482	6.317	6098698	2125283	0.695	0.910 #
15)	B Endosulfa...	6.140	0.000	8042682	0	0.928	N.D. #
17)	MA 4,4'-DDT	6.228	7.106	9345490	2474054	1.246	1.254
25)	Chlordane-3	5.279f	6.087	125.4E6	10300732	109.363	26.437 #
26)	Chlordane-4	5.313	6.163	17984162	33475366	16.965	71.555 #
27)	Chlordane-5	6.140	6.965	8042682	1924029	23.289	21.181



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031119\
Data File : PL045675.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2019 16:20
Operator : AJ\SJ
Sample : K1817-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EXT-027-SW015-030719

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:09:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

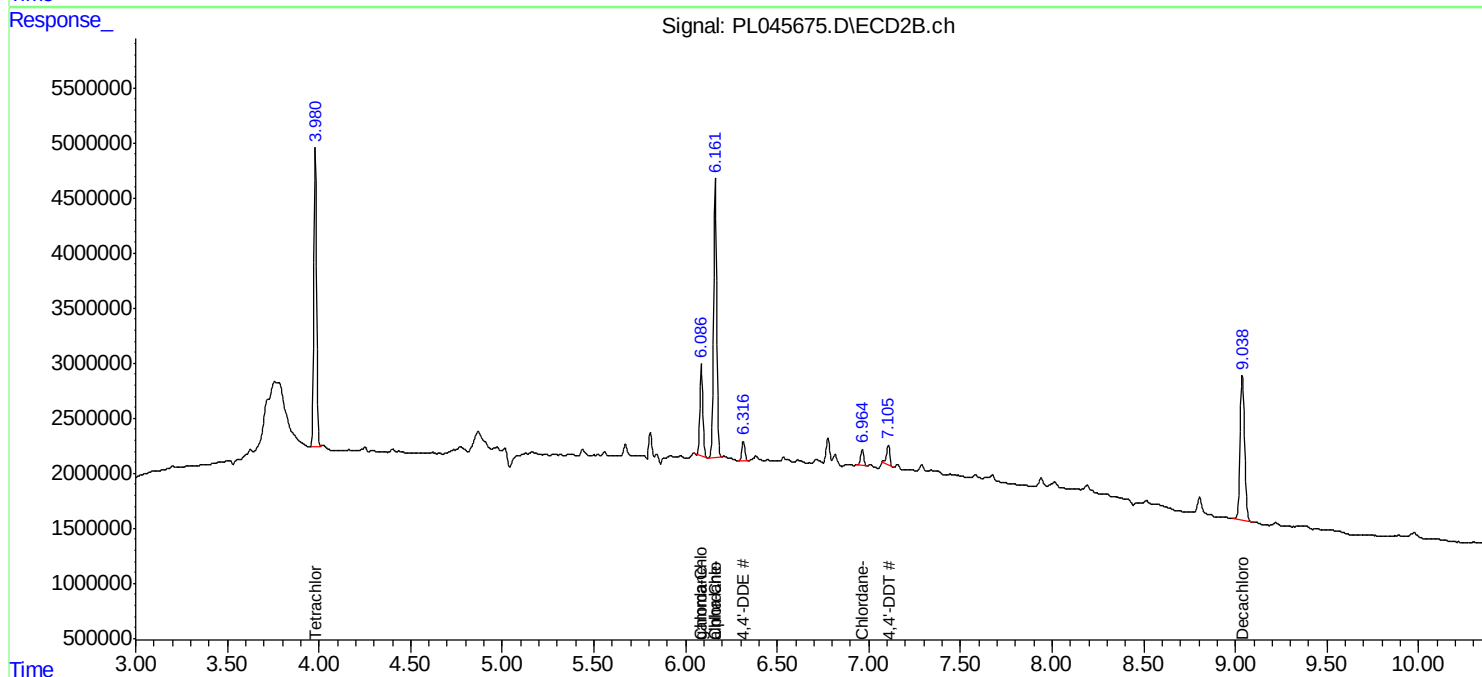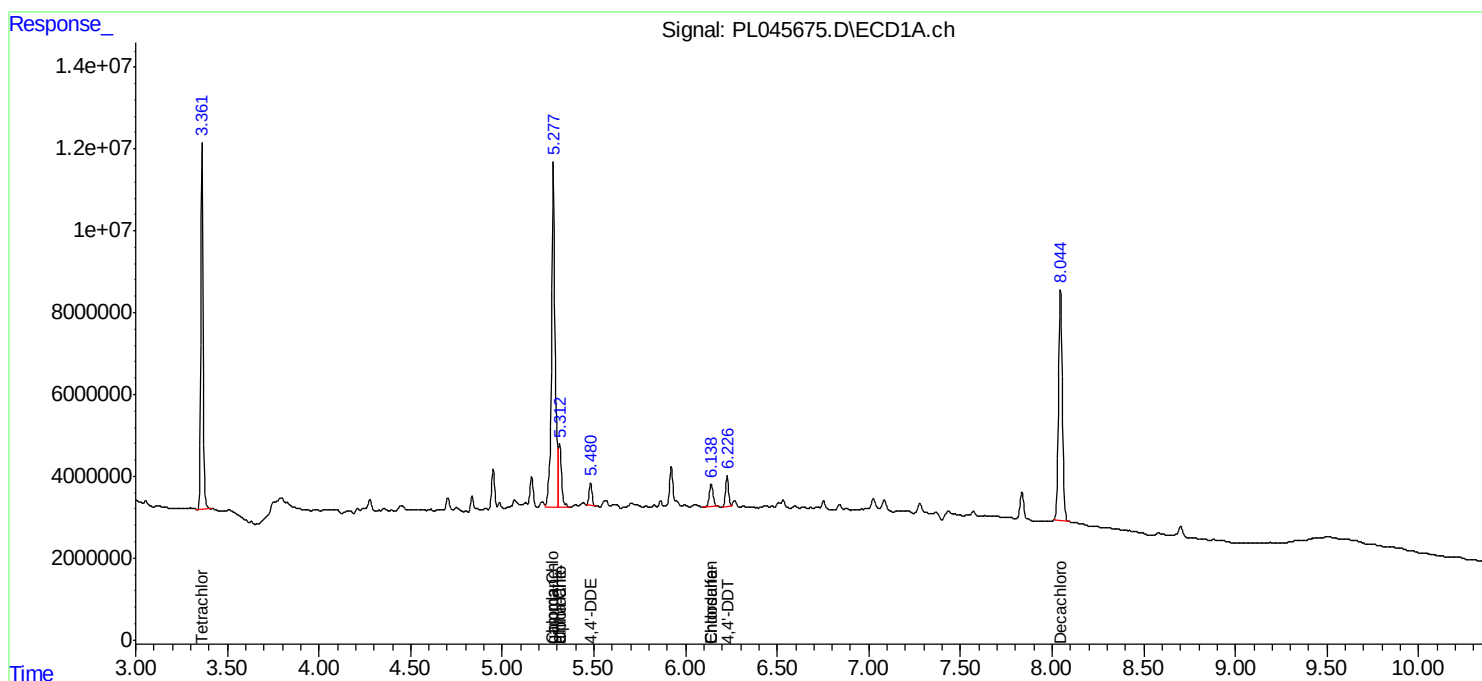


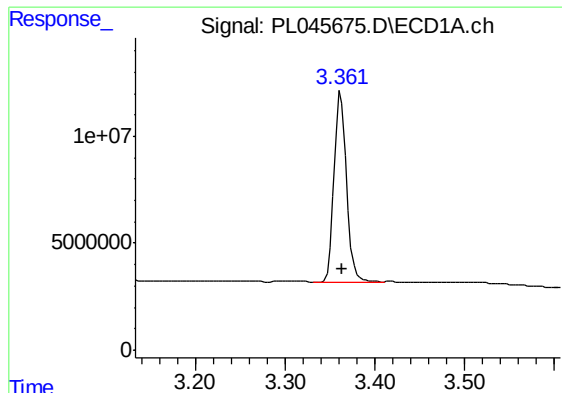

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 85743833
Conc: 12.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-027-SW015-030719

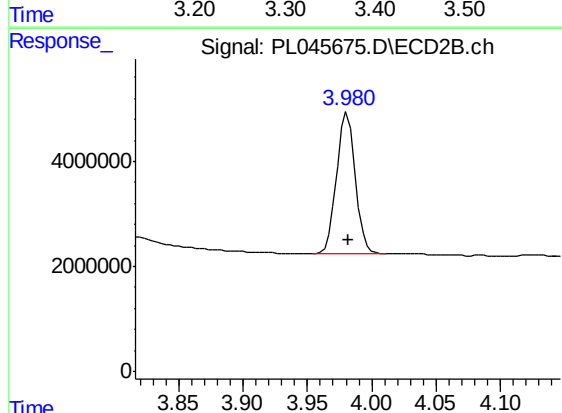


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 27373838
Conc: 12.78 ng/ml

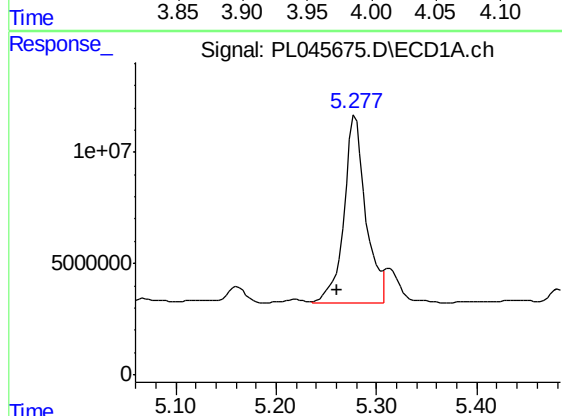


#10 gamma-Chlordane

R.T.: 5.279 min
Delta R.T.: 0.018 min
Response: 125441349
Conc: 12.82 ng/ml

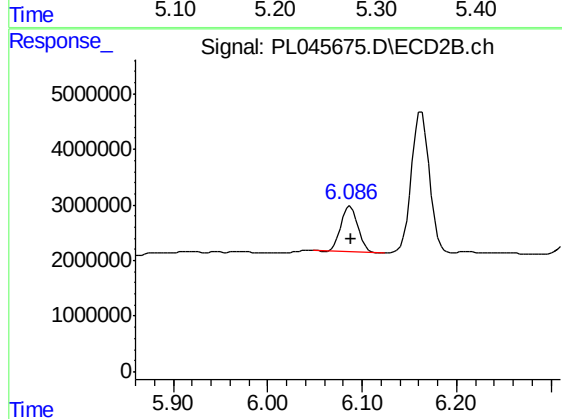

#10 gamma-Chlordane


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 10300732
Conc: 3.84 ng/ml

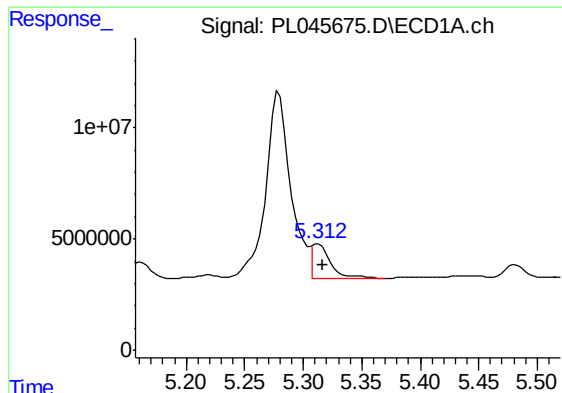

#11 alpha-Chlordane


R.T.: 5.313 min
Delta R.T.: -0.003 min
Response: 17984162
Conc: 1.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-027-SW015-030719

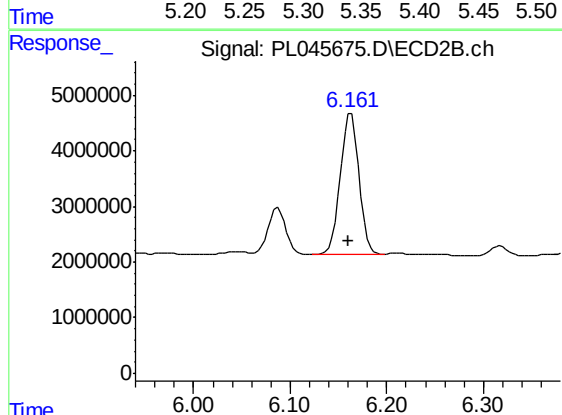


#11 alpha-Chlordane

R.T.: 6.163 min
Delta R.T.: 0.003 min
Response: 33475366
Conc: 12.41 ng/ml

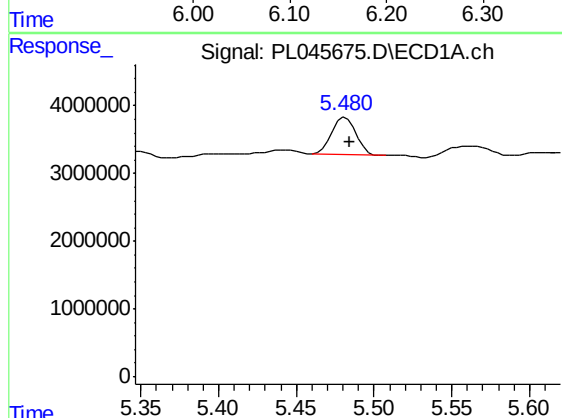


#12 4,4'-DDE

R.T.: 5.482 min
Delta R.T.: -0.002 min
Response: 6098698
Conc: 0.69 ng/ml

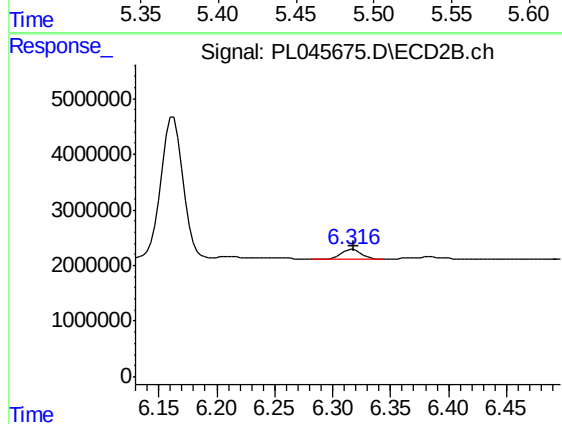

#12 4,4'-DDE


R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 2125283
Conc: 0.91 ng/ml

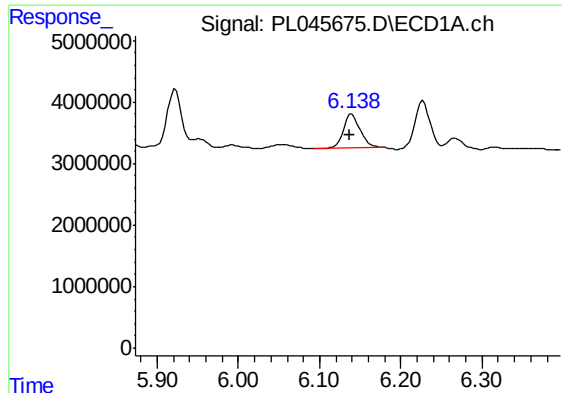

#15 Endosulfan II


R.T.: 6.140 min
Delta R.T.: 0.003 min
Response: 8042682
Conc: 0.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-027-SW015-030719

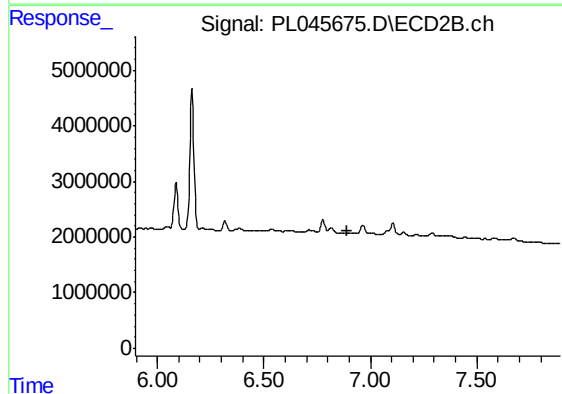


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.894 min
Response: 0
Conc: N.D.

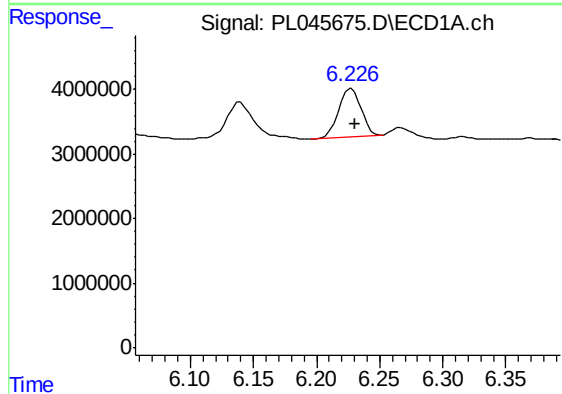


#17 4,4'-DDT

R.T.: 6.228 min
Delta R.T.: -0.003 min
Response: 9345490
Conc: 1.25 ng/ml

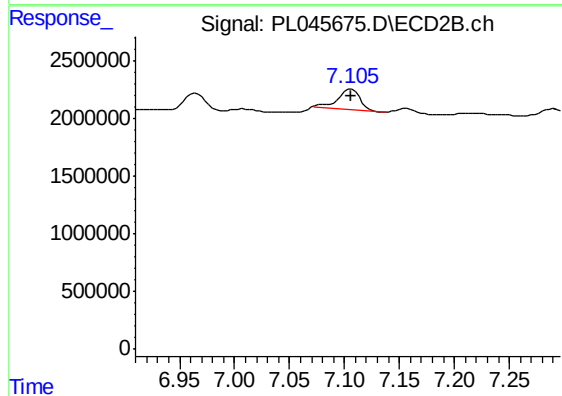

#17 4,4'-DDT


R.T.: 7.106 min
Delta R.T.: 0.000 min
Response: 2474054
Conc: 1.25 ng/ml

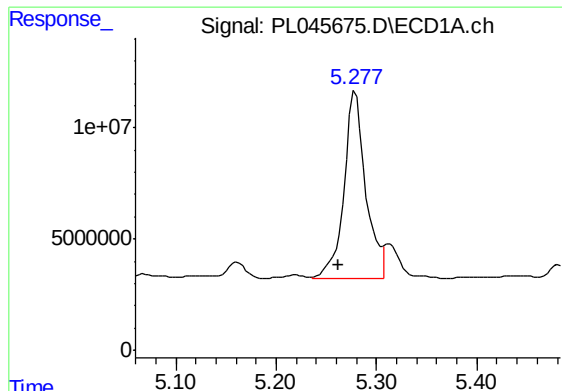

#25 Chlordane-3


R.T.: 5.279 min
Delta R.T.: 0.017 min
Response: 125441349
Conc: 109.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-027-SW015-030719

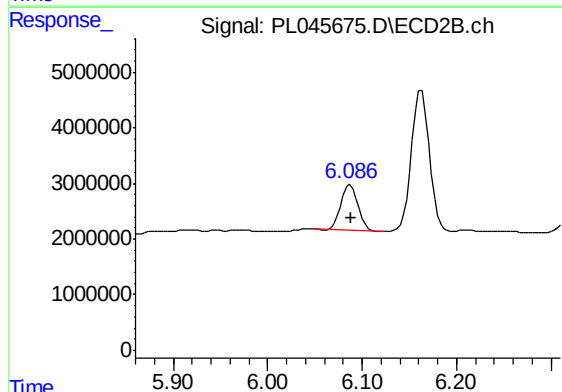


#25 Chlordane-3

R.T.: 6.087 min
Delta R.T.: -0.001 min
Response: 10300732
Conc: 26.44 ng/ml

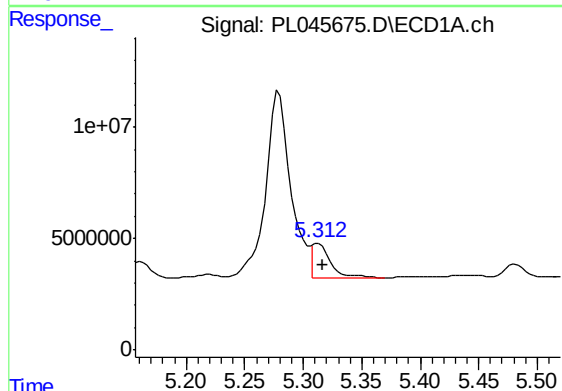


#26 Chlordane-4

R.T.: 5.313 min
Delta R.T.: -0.003 min
Response: 17984162
Conc: 16.97 ng/ml

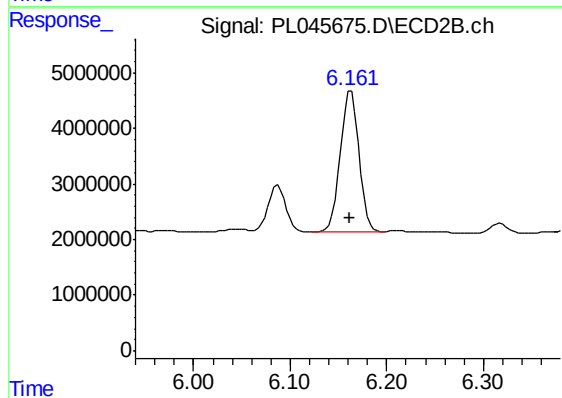

#26 Chlordane-4


R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 33475366
Conc: 71.56 ng/ml

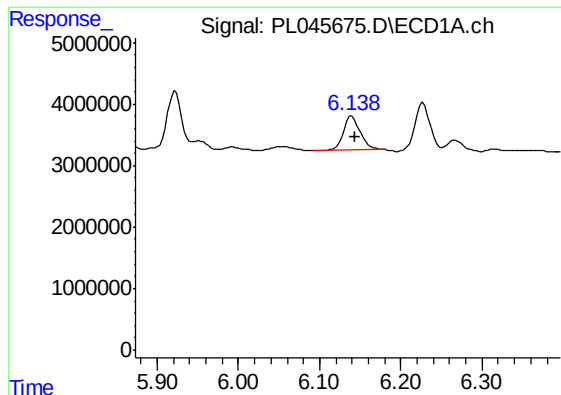

#27 Chlordane-5


R.T.: 6.140 min
Delta R.T.: -0.003 min
Response: 8042682
Conc: 23.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-027-SW015-030719

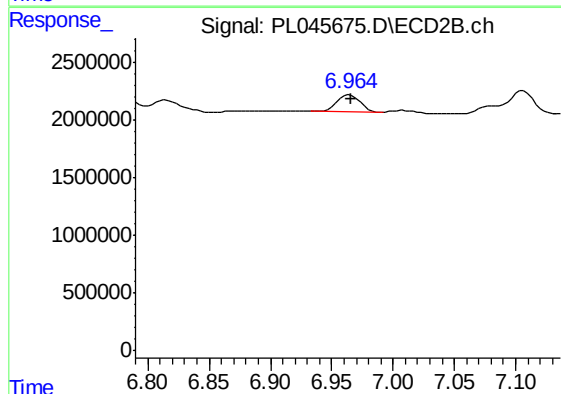


#27 Chlordane-5

R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 1924029
Conc: 21.18 ng/ml

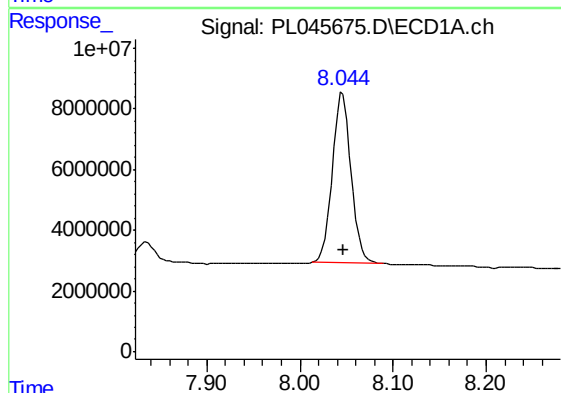

#28 Decachlorobiphenyl

R.T.: 8.046 min
Delta R.T.: -0.001 min
Response: 78435057
Conc: 9.37 ng/ml

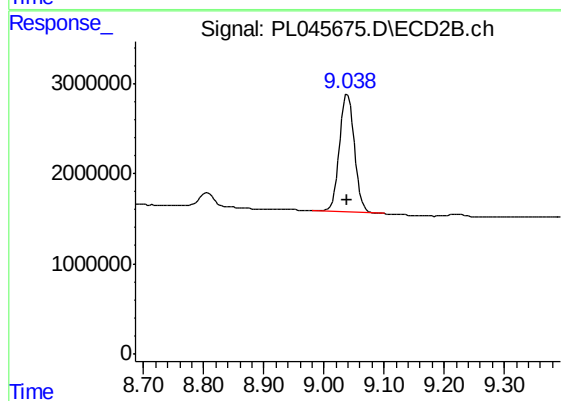

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 22716197
Conc: 9.94 ng/ml