

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031119\
 Data File : PL045688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2019 19:24
 Operator : AJ\SJ
 Sample : K1817-17
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-028-SW012-1-030619

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:12:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	115.7E6	34324933	16.815	16.028
28)	SA Decachlor...	8.045	9.039	80062870	23178299	9.568	10.144
Target Compounds							
23)	Chlordane-1	4.237f	0.000	13274170	0	39.396	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031119\
Data File : PL045688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2019 19:24
Operator : AJ\SJ
Sample : K1817-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-028-SW012-1-030619

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:12:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

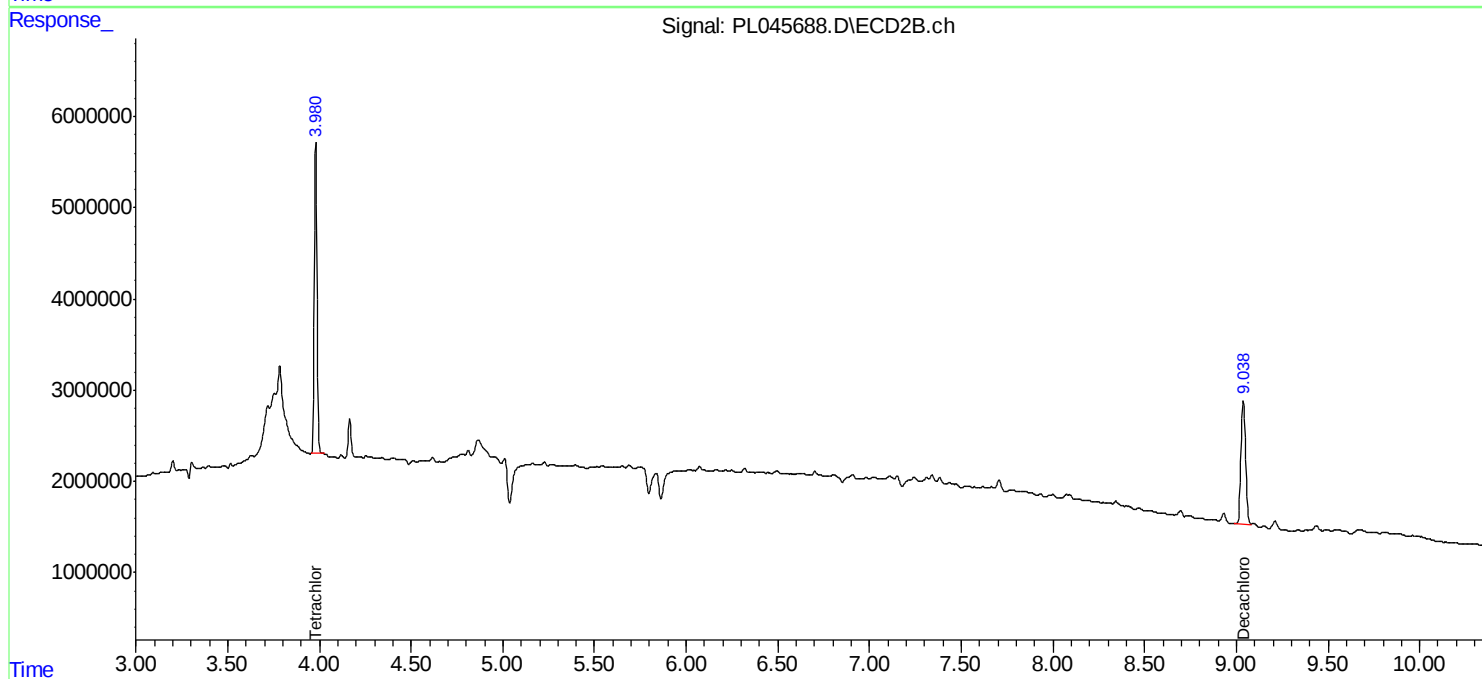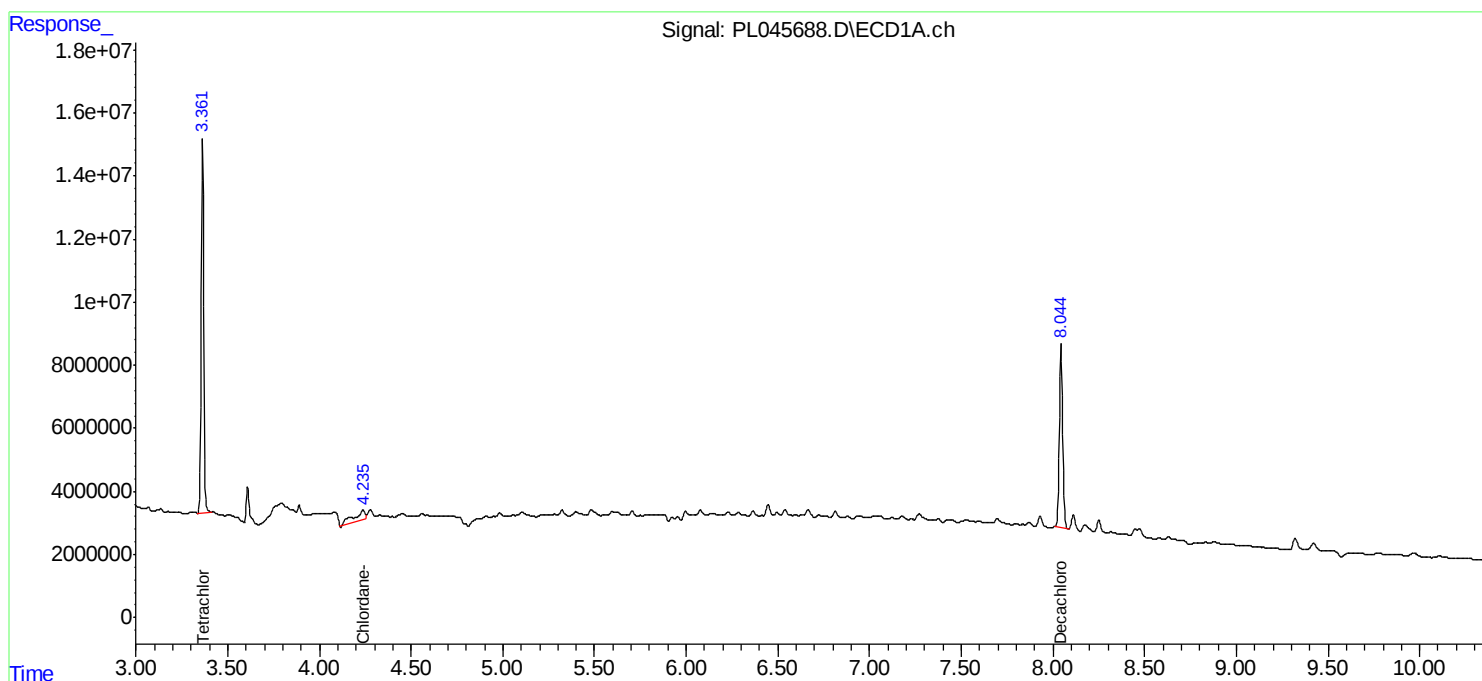


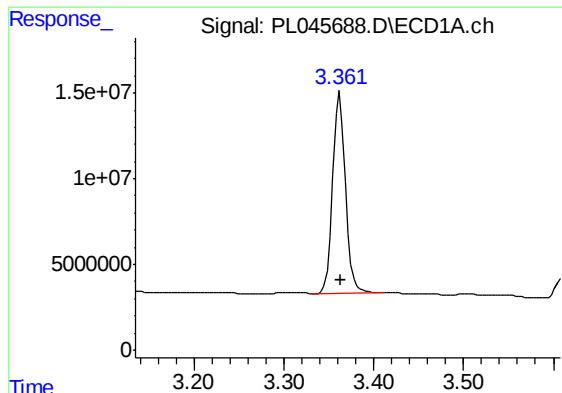

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 115677078
Conc: 16.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-028-SW012-1-030619

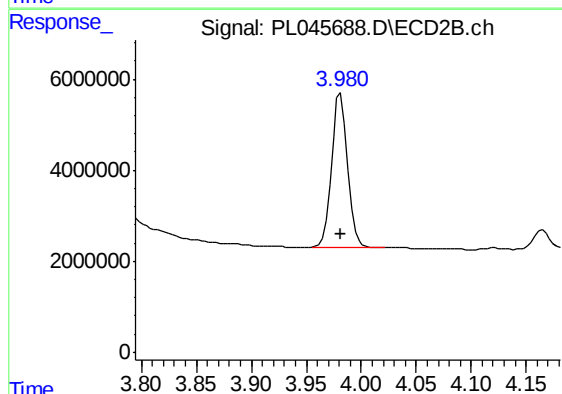


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 34324933
Conc: 16.03 ng/ml

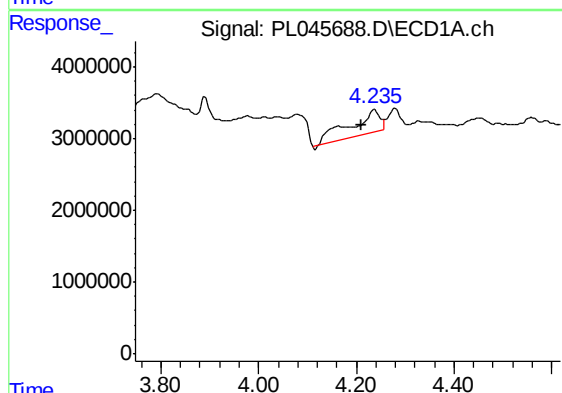


#23 Chlordane-1

R.T.: 4.237 min
Delta R.T.: 0.026 min
Response: 13274170
Conc: 39.40 ng/ml

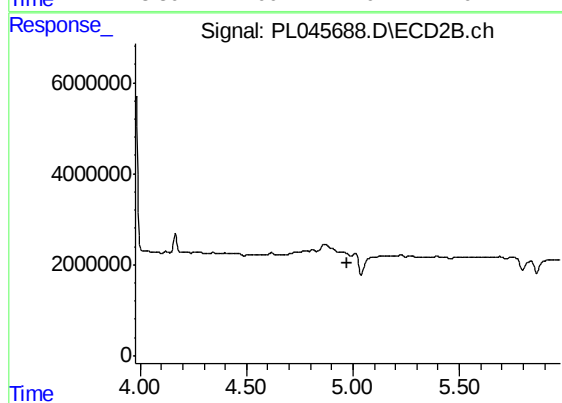

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

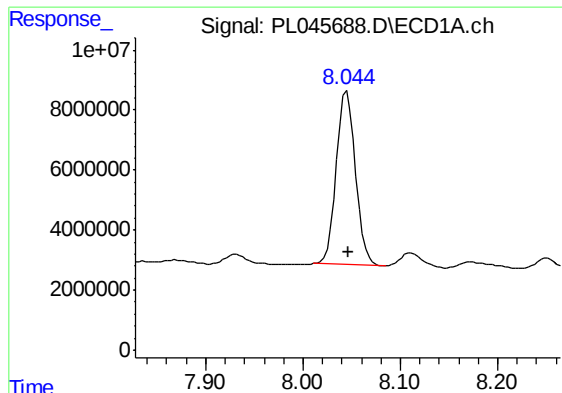

#28 Decachlorobiphenyl

R.T.: 8.045 min
Delta R.T.: -0.002 min
Response: 80062870
Conc: 9.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-028-SW012-1-030619

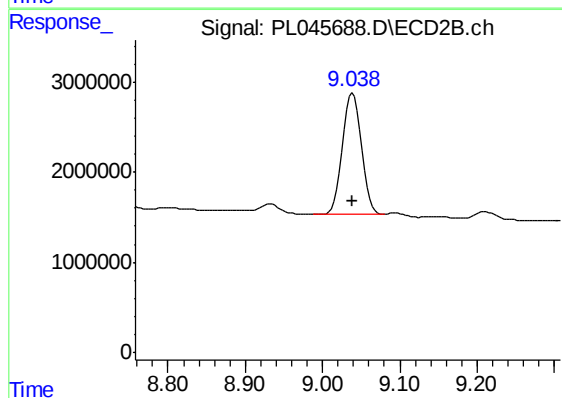

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 23178299
Conc: 10.14 ng/ml