

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031119\
 Data File : PL045691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2019 20:06
 Operator : AJ\SJ
 Sample : K1817-20
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-028-B007-1-030619

Manual Integrations
 APPROVED

Sohil
 3/12/2019 9:31:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:13:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	166.4E6	47666305	24.182	22.258
28)	SA Decachlor...	8.045	9.039	150.8E6	45187328	18.023	19.776
Target Compounds							
17)	MA 4,4'-DDT	6.226	7.107	3398292	934090	0.453m	0.473m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031119\
Data File : PL045691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2019 20:06
Operator : AJ\SJ
Sample : K1817-20
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PST-028-B007-1-030619


Manual Integrations
APPROVED

Sohil
3/12/2019 9:31:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:13:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

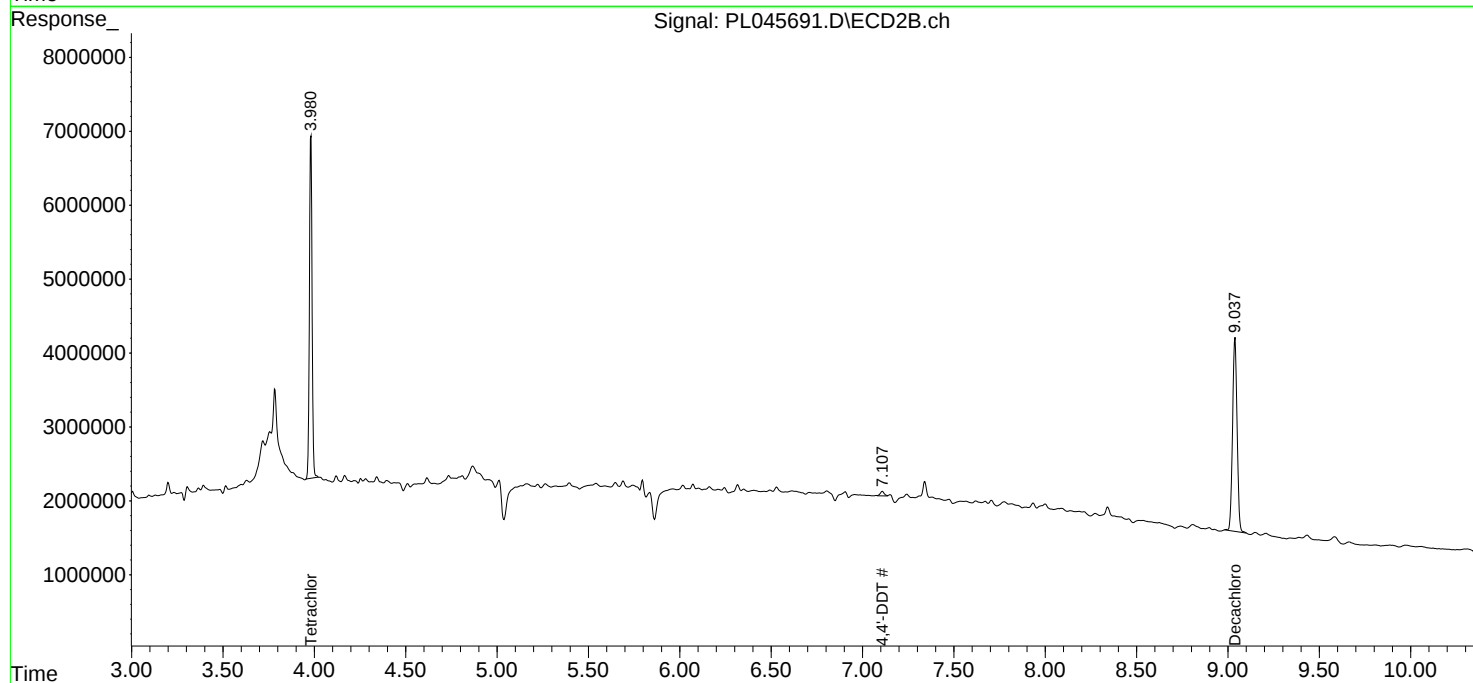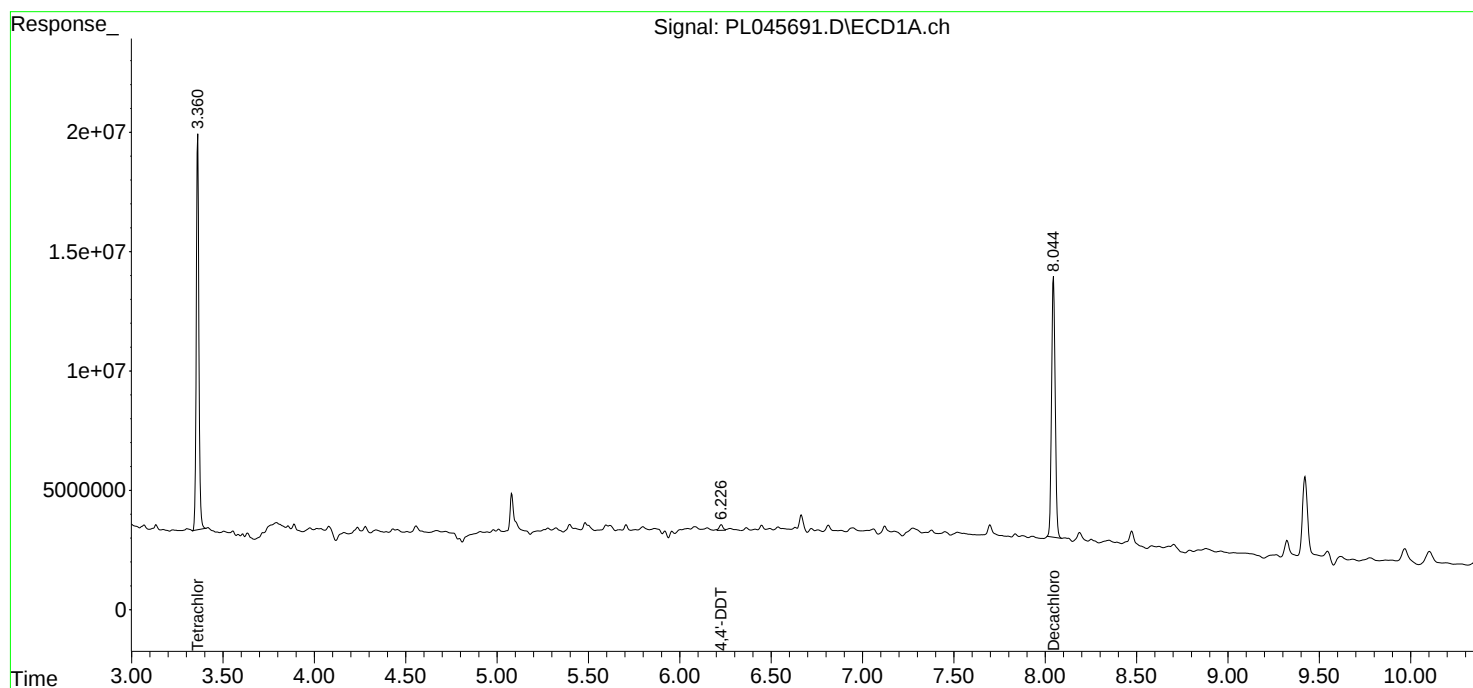

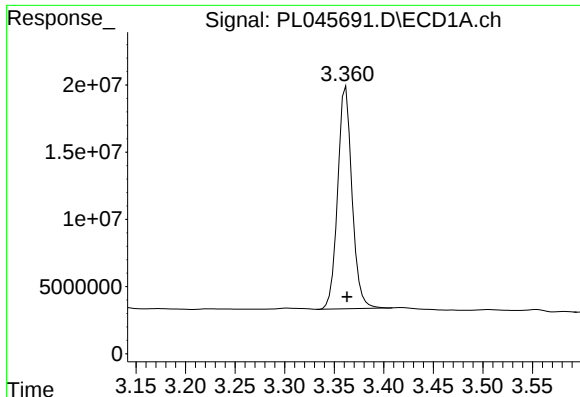


#1 Tetrachloro-m-xylene

R.T.: 3.362 min
Delta R.T.: -0.001 min
Response: 166358074
Conc: 24.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-028-B007-1-030619


Manual Integrations
APPROVED

Sohil
3/12/2019 9:31:06 AM

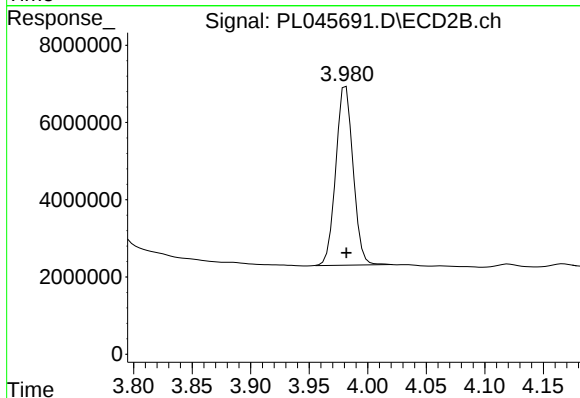


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 47666305
Conc: 22.26 ng/ml

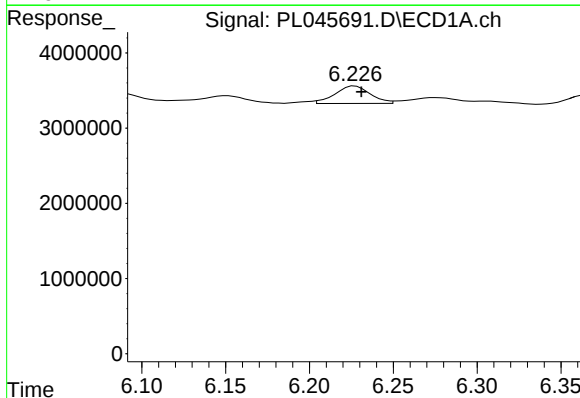


#17 4,4'-DDT

R.T.: 6.226 min
Delta R.T.: -0.005 min
Response: 3398292
Conc: 0.45 ng/ml m

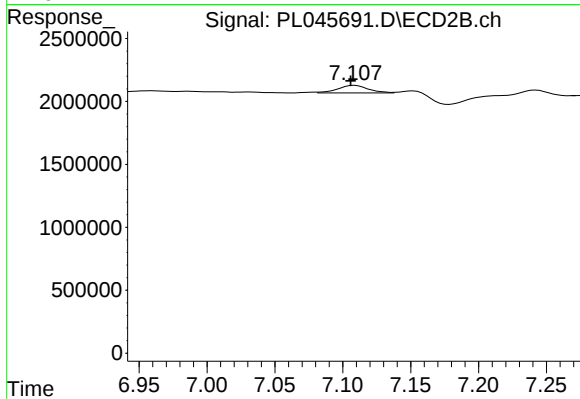

#17 4,4'-DDT

R.T.: 7.107 min
Delta R.T.: 0.002 min
Response: 934090
Conc: 0.47 ng/ml m

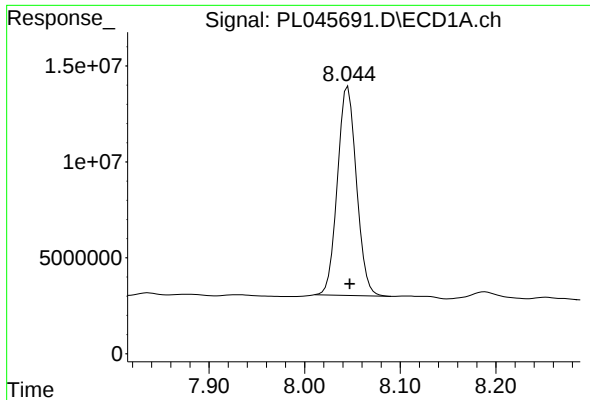


#28 Decachlorobiphenyl

R.T.: 8.045 min
Delta R.T.: -0.002 min
Response: 150802918
Conc: 18.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-028-B007-1-030619

Manual Integrations
APPROVED

Sohil
3/12/2019 9:31:06 AM

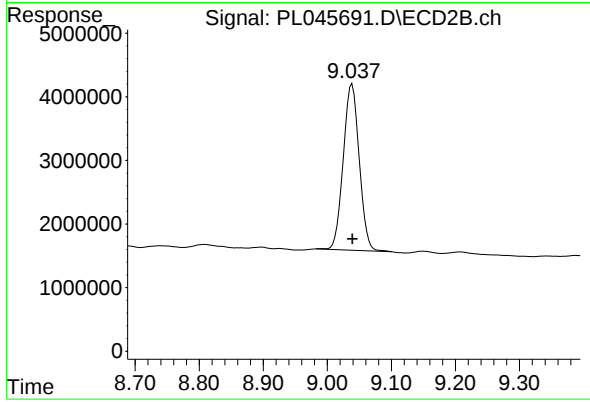

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 45187328
Conc: 19.78 ng/ml