

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031120\
 Data File : PL057221.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2020 18:47
 Operator : AJ\MA
 Sample : L1852-23
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 06:41:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 11 17:44:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	146.5E6	36437219	17.189	17.078
28)	SA Decachlor...	8.208	8.982	160.9E6	39072381	16.652	18.389
Target Compounds							
14)	MA Endrin	6.010	6.638	15947960	4840535	1.466m	1.877m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031120\
Data File : PL057221.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2020 18:47
Operator : AJ\MA
Sample : L1852-23
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-4-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 06:41:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 11 17:44:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

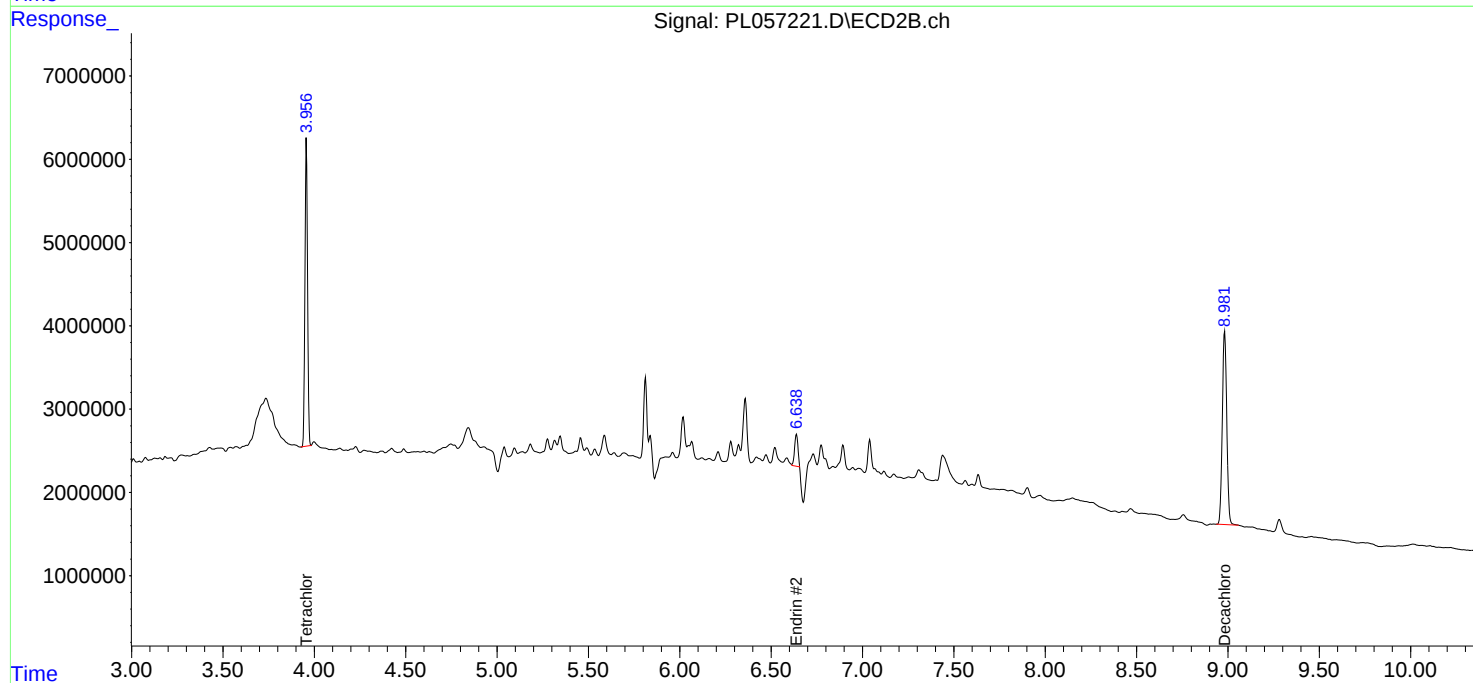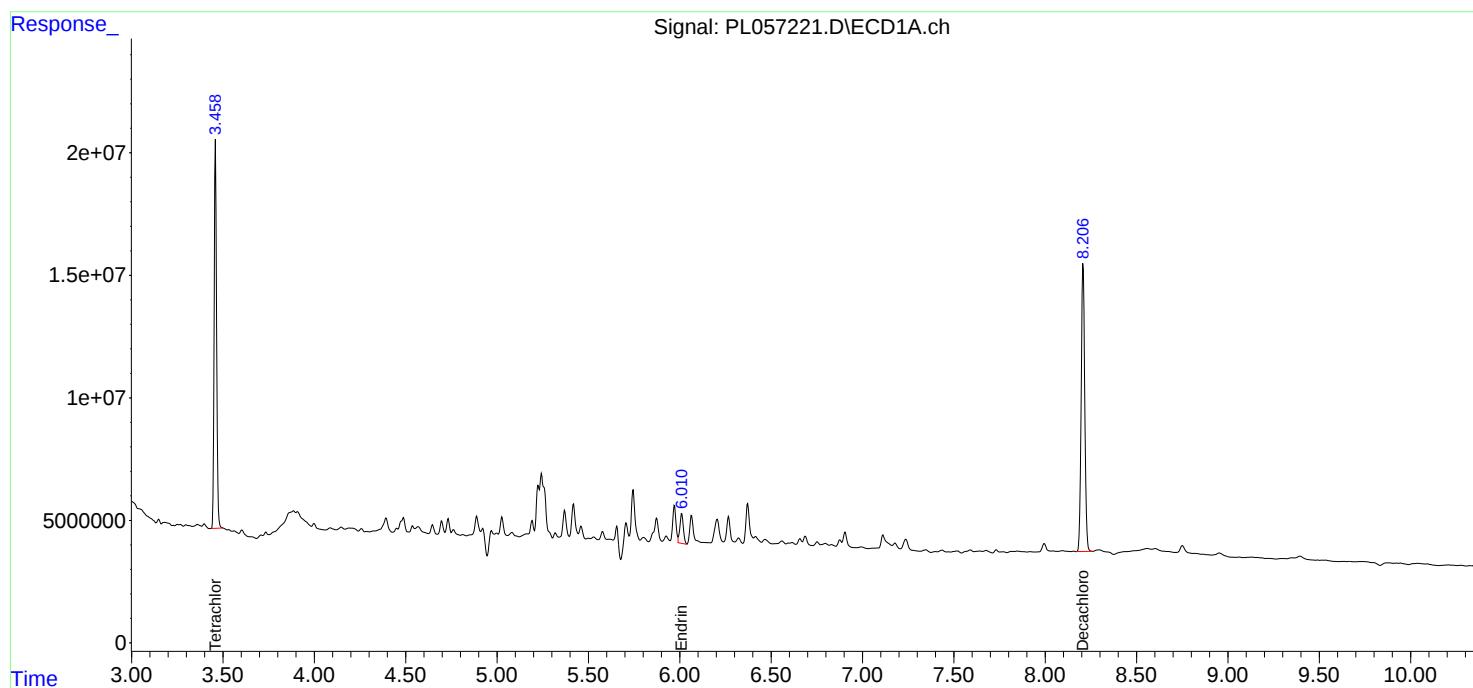


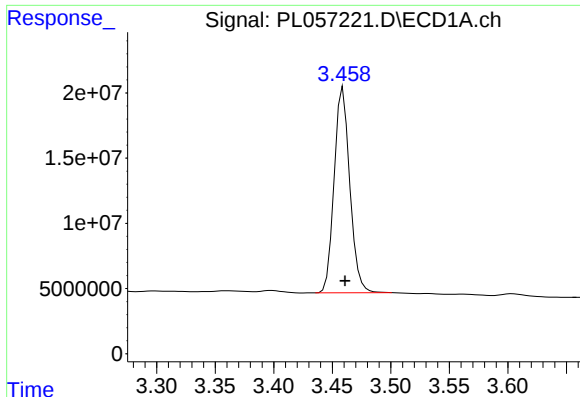

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 146492836
Conc: 17.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-S

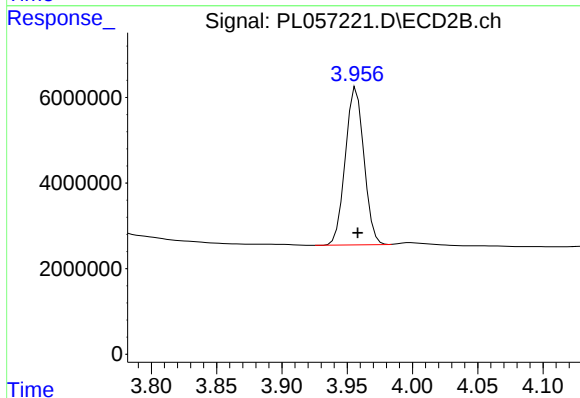


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.001 min
Response: 36437219
Conc: 17.08 ng/ml

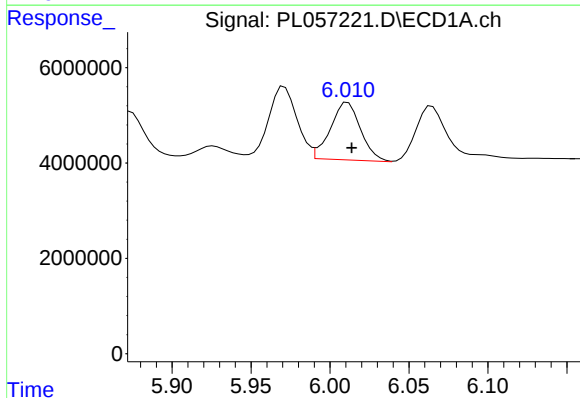


#14 Endrin

R.T.: 6.010 min
Delta R.T.: -0.004 min
Response: 15947960
Conc: 1.47 ng/ml m

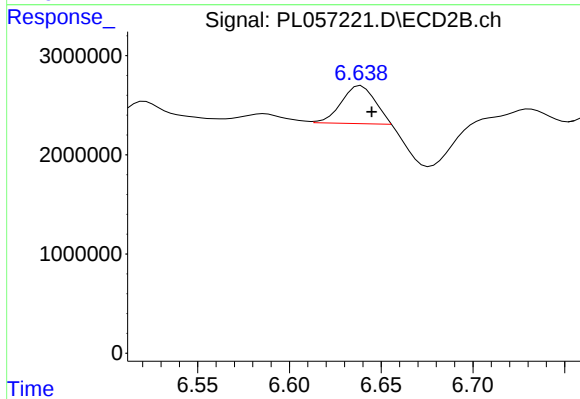

#14 Endrin

R.T.: 6.638 min
Delta R.T.: -0.007 min
Response: 4840535
Conc: 1.88 ng/ml m

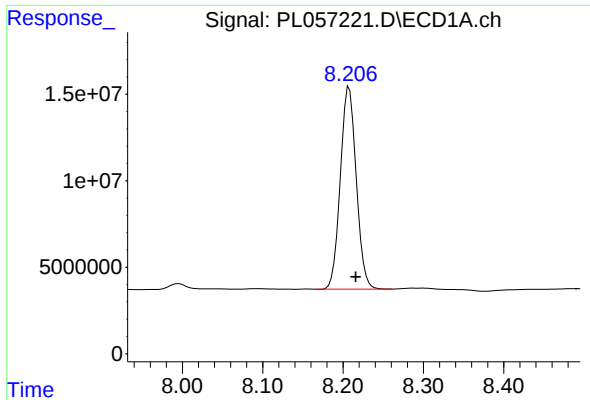

#28 Decachlorobiphenyl


R.T.: 8.208 min

Delta R.T.: -0.008 min

Response: 160943180

Conc: 16.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-S

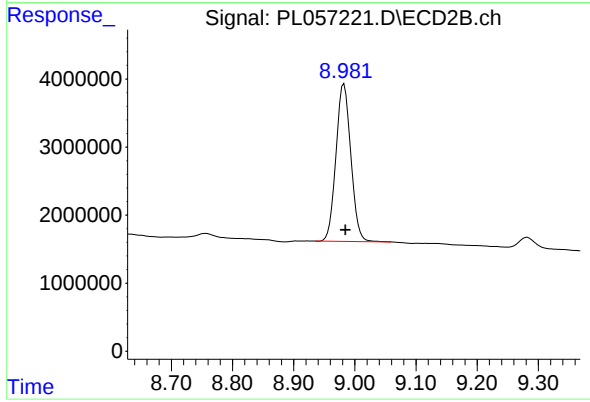

#28 Decachlorobiphenyl

R.T.: 8.982 min

Delta R.T.: -0.002 min

Response: 39072381

Conc: 18.39 ng/ml