

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031121\
 Data File : PL065222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2021 04:43
 Operator : AR\AJ
 Sample : M1344-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT2-2021-04

Manual Integrations
 APPROVED

Ankita
 3/11/2021 3:49:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 05:54:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031021CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 11 02:46:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.096	71560234	61992013	24.432	24.315
27)	SA Decachlor...	8.137	9.249	122.4E6	106.0E6	43.783	46.512
Target Compounds							
22)	Toxaphene-1	5.653	6.523	2774648	1450111	123.932	112.839
23)	Toxaphene-2	6.249	6.819	6495984	1280461	112.417	97.137
24)	Toxaphene-3	6.494	7.304	5749727	4082033	95.581	101.505
25)	Toxaphene-4	6.847	7.392	3306398	3537639	76.081	95.670m#
26)	Toxaphene-5	6.976	7.814	6648369	2907906	104.393	96.091

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031121\
Data File : PL065222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2021 04:43
Operator : AR\AJ
Sample : M1344-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 05:54:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031021CLP.M
Quant Title : GC Extractables
QLast Update : Thu Mar 11 02:46:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

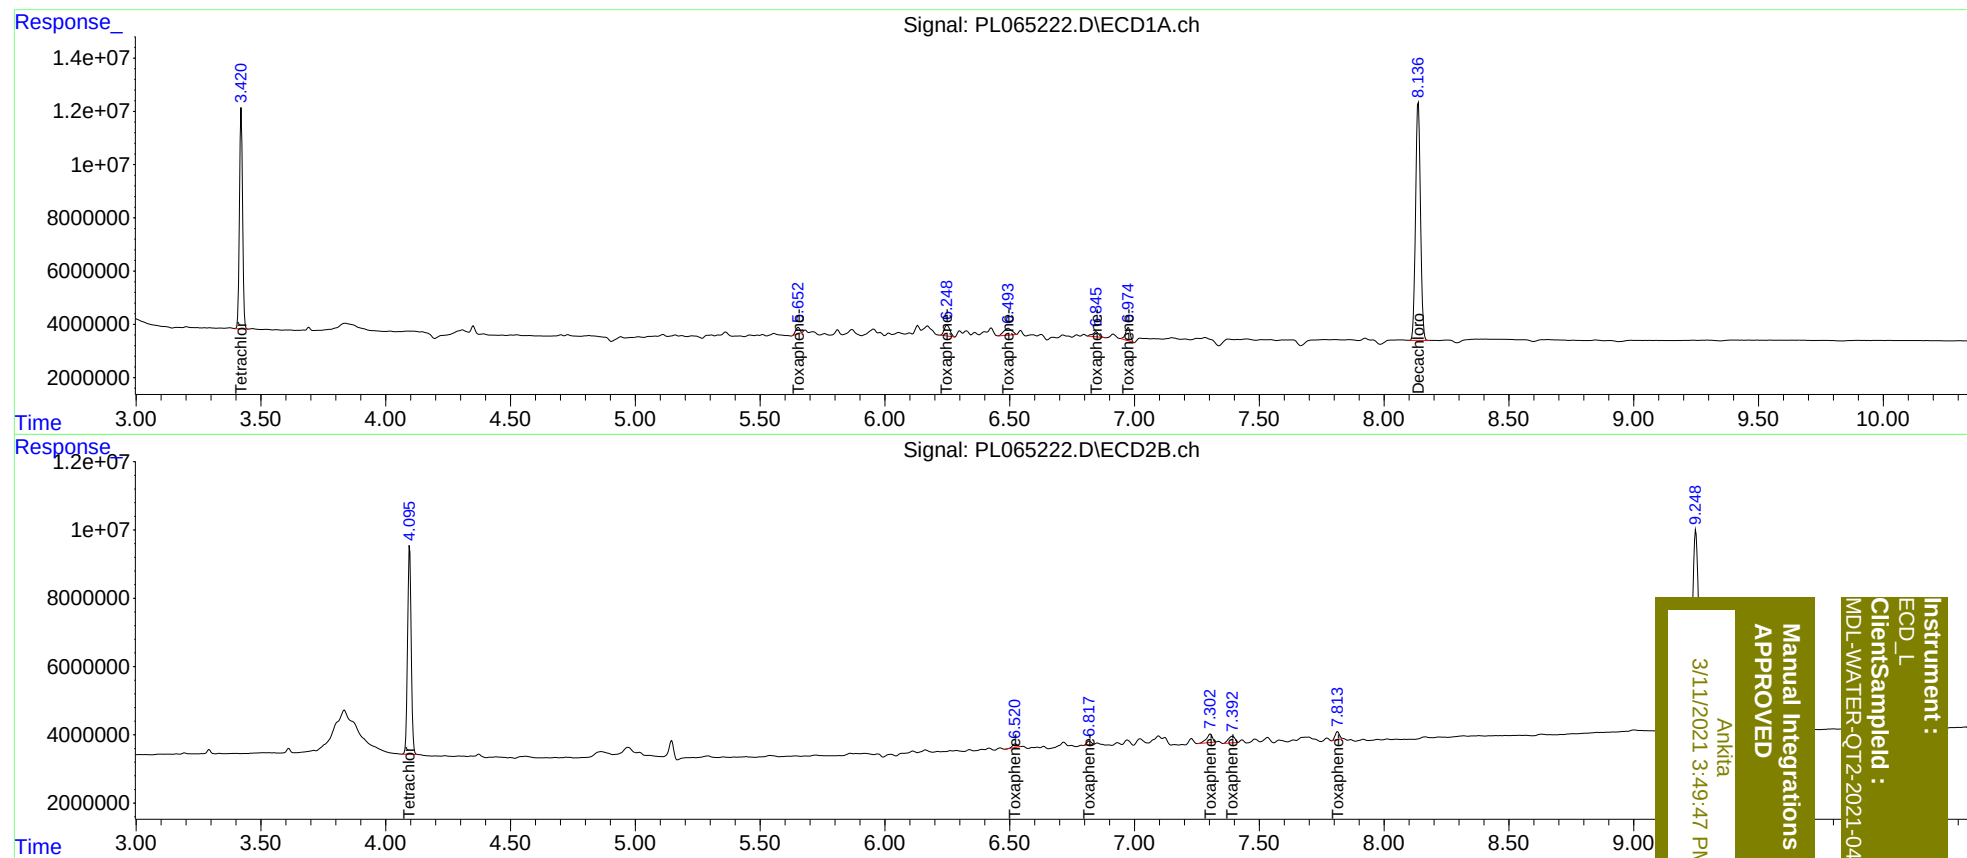

Manual Integrations
APPROVED

3/11/2021 3:49:47 PM
Ankita

Instrument :
ECD_L
Client Sampled :
MDL-WATER-QT2-2021-04