

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031122\
 Data File : PL073281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 21:45
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 05:26:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 12 05:25:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.643	5.491	39358181	168.8E6	99.107	99.794
28)	SA Decachlor...	10.421	11.330	47133004	171.1E6	96.572	97.542
Target Compounds							
23)	Chlordane-1	5.975	6.863	11438391	64913032	981.259	987.203
24)	Chlordane-2	6.665	7.446	15035970	68478891	963.803	977.324
25)	Chlordane-3	7.367	8.195	40677393	281.1E6	1001.596	1010.476
26)	Chlordane-4	7.436	8.281	44105994	338.2E6	1002.495	1003.258
27)	Chlordane-5	8.386	9.150	15845163	55307480	996.298	993.792



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031122\
Data File : PL073281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 21:45
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 05:26:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Sat Mar 12 05:25:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

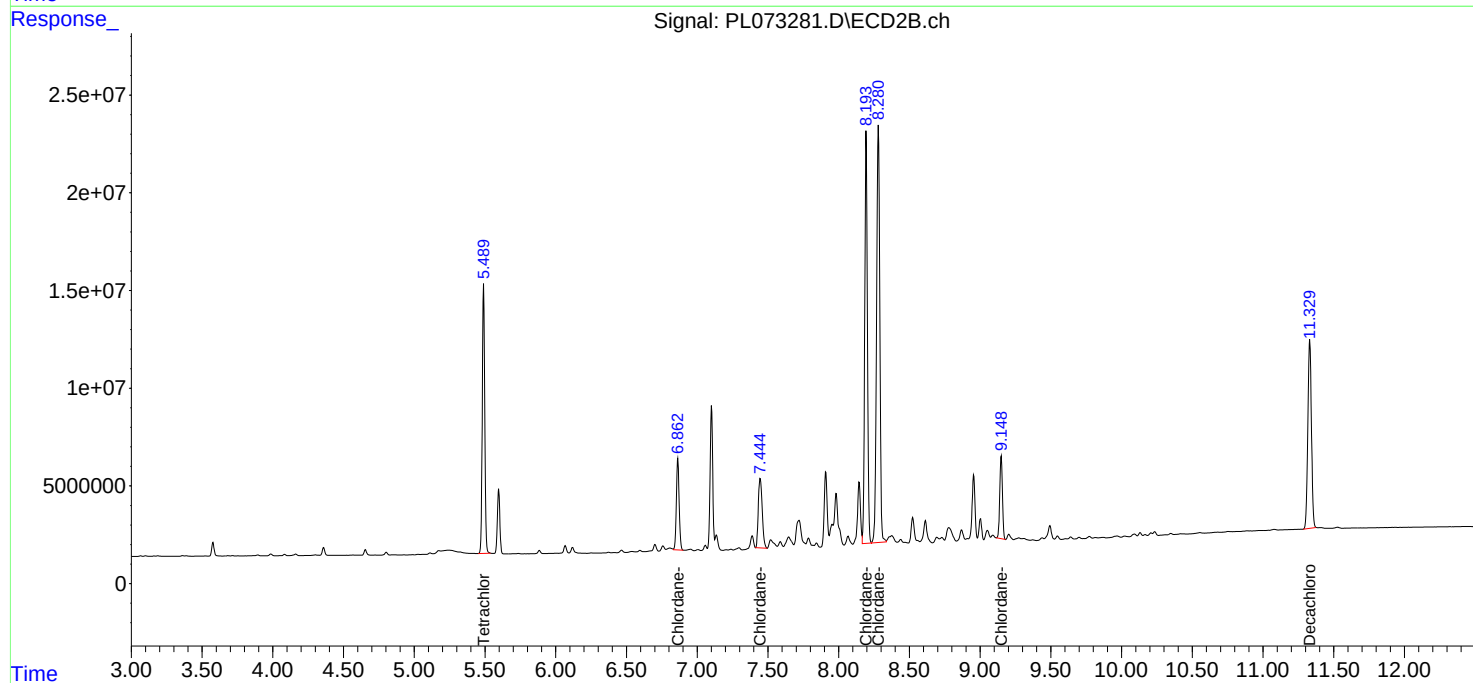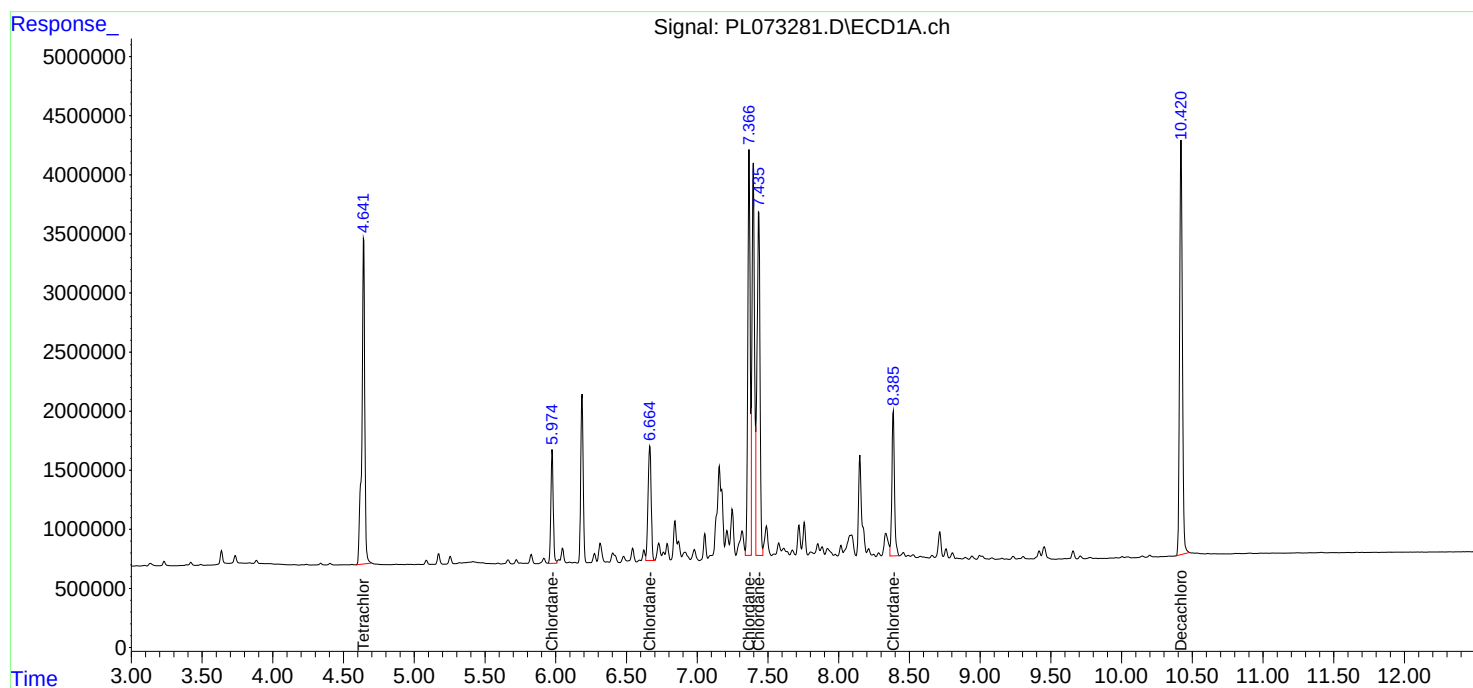


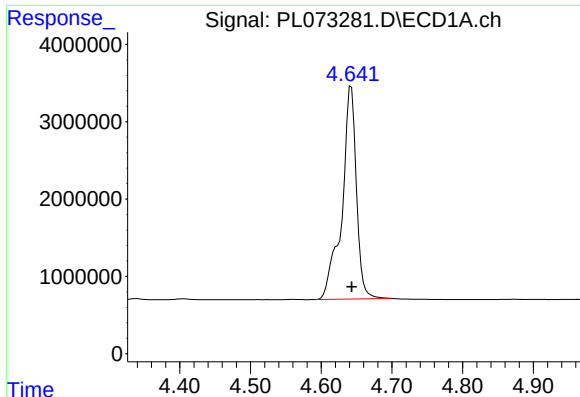

#1 Tetrachloro-m-xylene


R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 39358181
Conc: 99.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

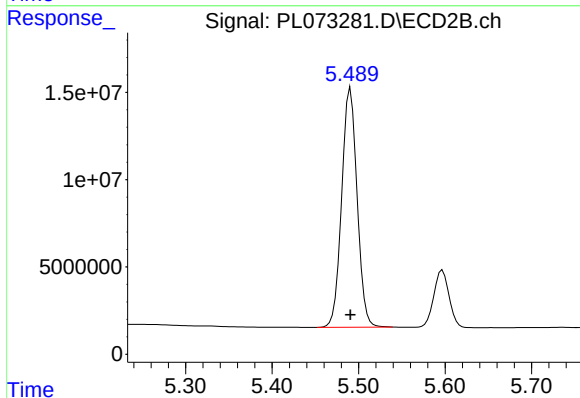


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 168764212
Conc: 99.79 ng/ml

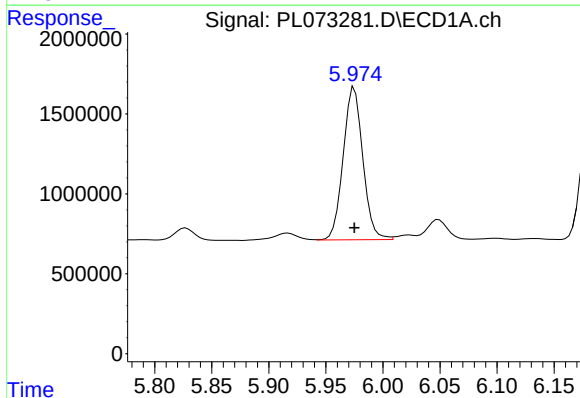


#23 Chlordane-1

R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 11438391
Conc: 981.26 ng/ml

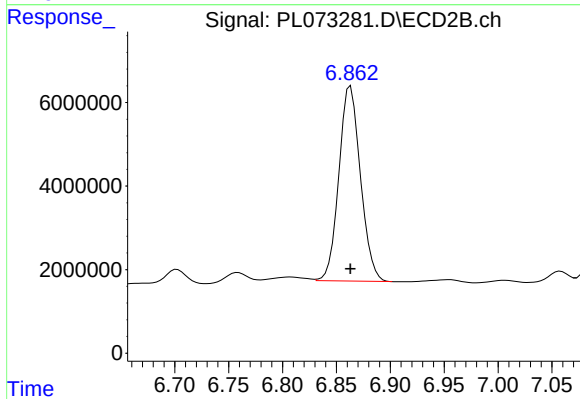

#23 Chlordane-1


R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 64913032
Conc: 987.20 ng/ml

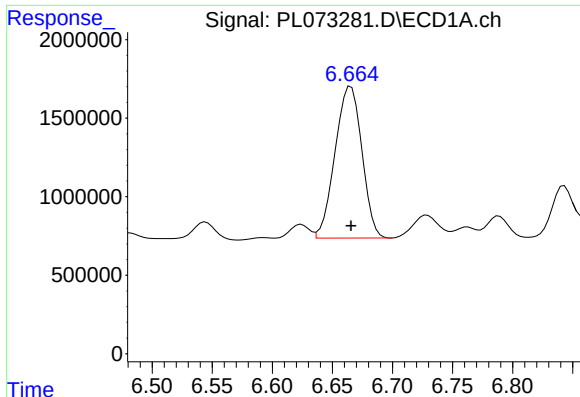

#24 Chlordane-2


R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 15035970
Conc: 963.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

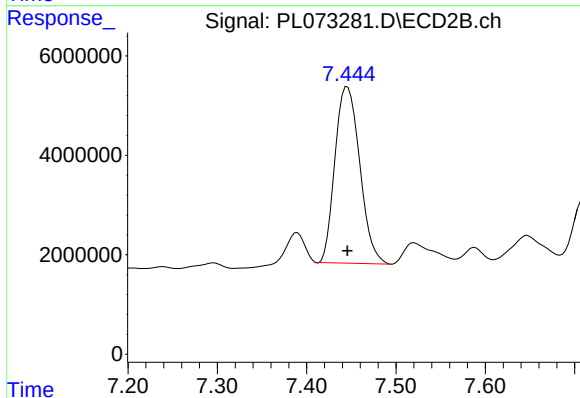


#24 Chlordane-2

R.T.: 7.446 min
Delta R.T.: 0.000 min
Response: 68478891
Conc: 977.32 ng/ml

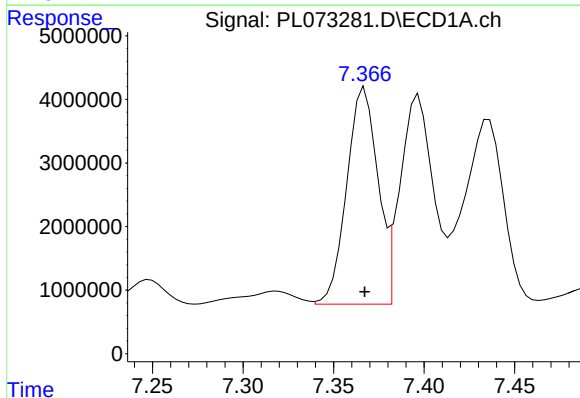


#25 Chlordane-3

R.T.: 7.367 min
Delta R.T.: 0.000 min
Response: 40677393
Conc: 1001.60 ng/ml

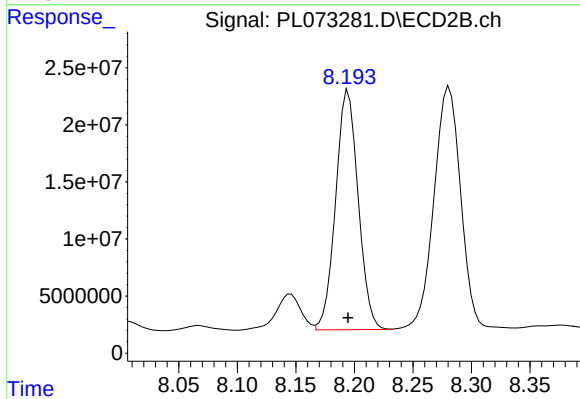

#25 Chlordane-3


R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 281062282
Conc: 1010.48 ng/ml

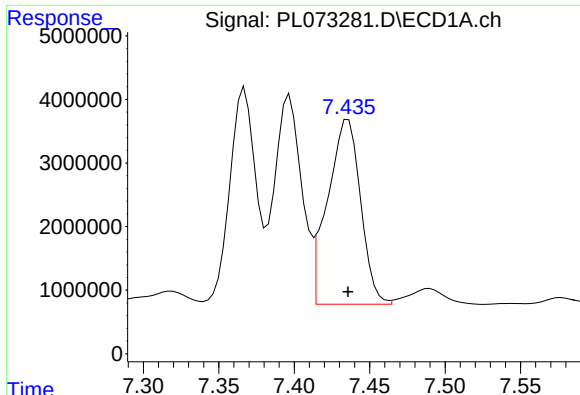

#26 Chlordane-4


R.T.: 7.436 min
Delta R.T.: 0.000 min
Response: 44105994
Conc: 1002.50 ng/m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

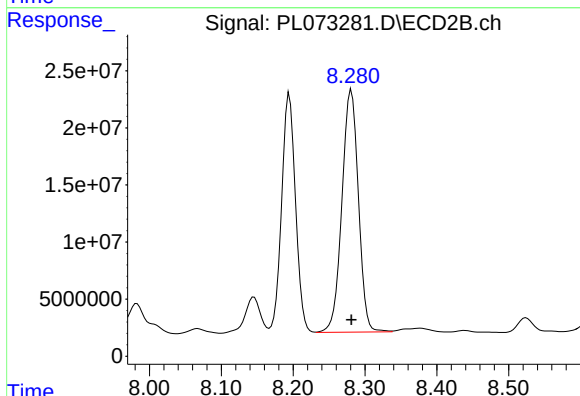


#26 Chlordane-4

R.T.: 8.281 min
Delta R.T.: 0.000 min
Response: 338202374
Conc: 1003.26 ng/ml

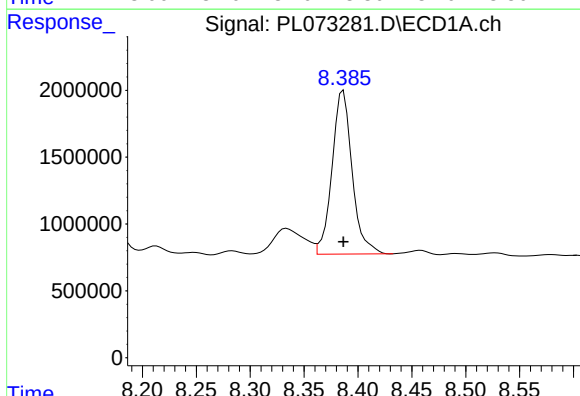


#27 Chlordane-5

R.T.: 8.386 min
Delta R.T.: 0.000 min
Response: 15845163
Conc: 996.30 ng/ml

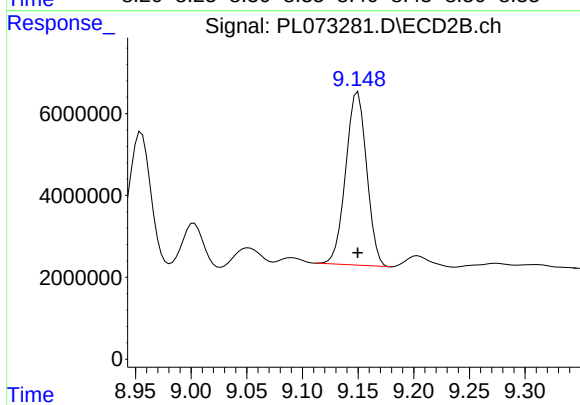

#27 Chlordane-5


R.T.: 9.150 min
Delta R.T.: 0.000 min
Response: 55307480
Conc: 993.79 ng/ml

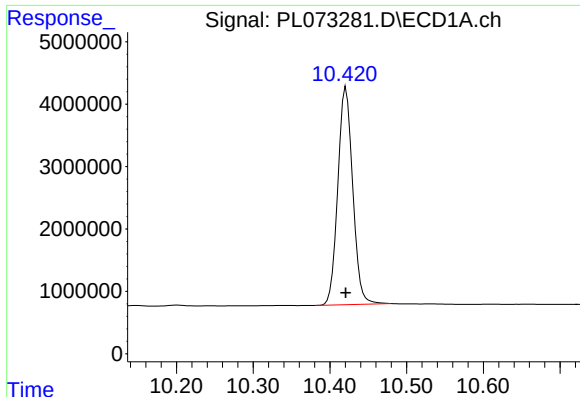

#28 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: 0.000 min
Response: 47133004
Conc: 96.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

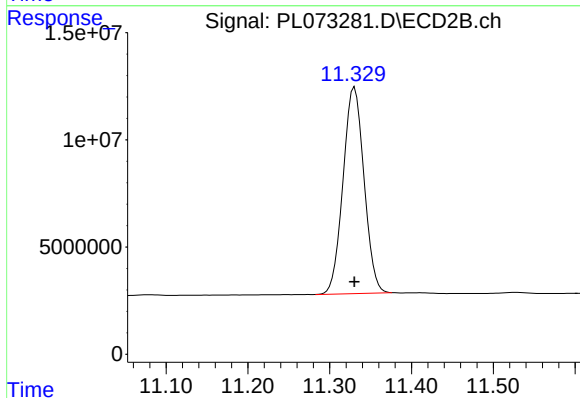

#28 Decachlorobiphenyl

R.T.: 11.330 min
Delta R.T.: 0.000 min
Response: 171093348
Conc: 97.54 ng/ml