

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031122\
 Data File : PL073282.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 22:01
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 05:28:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 12 05:27:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.491	29910714	127.6E6	75.211	75.285
28)	SA Decachlor...	10.421	11.331	36508593	131.7E6	74.869	75.057
Target Compounds							
23)	Chlordane-1	5.976	6.864	8684007	49404626	746.639	750.899
24)	Chlordane-2	6.666	7.446	11580647	52398096	744.861	748.545
25)	Chlordane-3	7.368	8.196	30583985	210.2E6	752.042	753.759
26)	Chlordane-4	7.436	8.281	32967308	254.5E6	749.548	753.301
27)	Chlordane-5	8.387	9.149	11998603	41646815	752.952	748.886



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031122\
Data File : PL073282.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 22:01
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 05:28:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Sat Mar 12 05:27:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

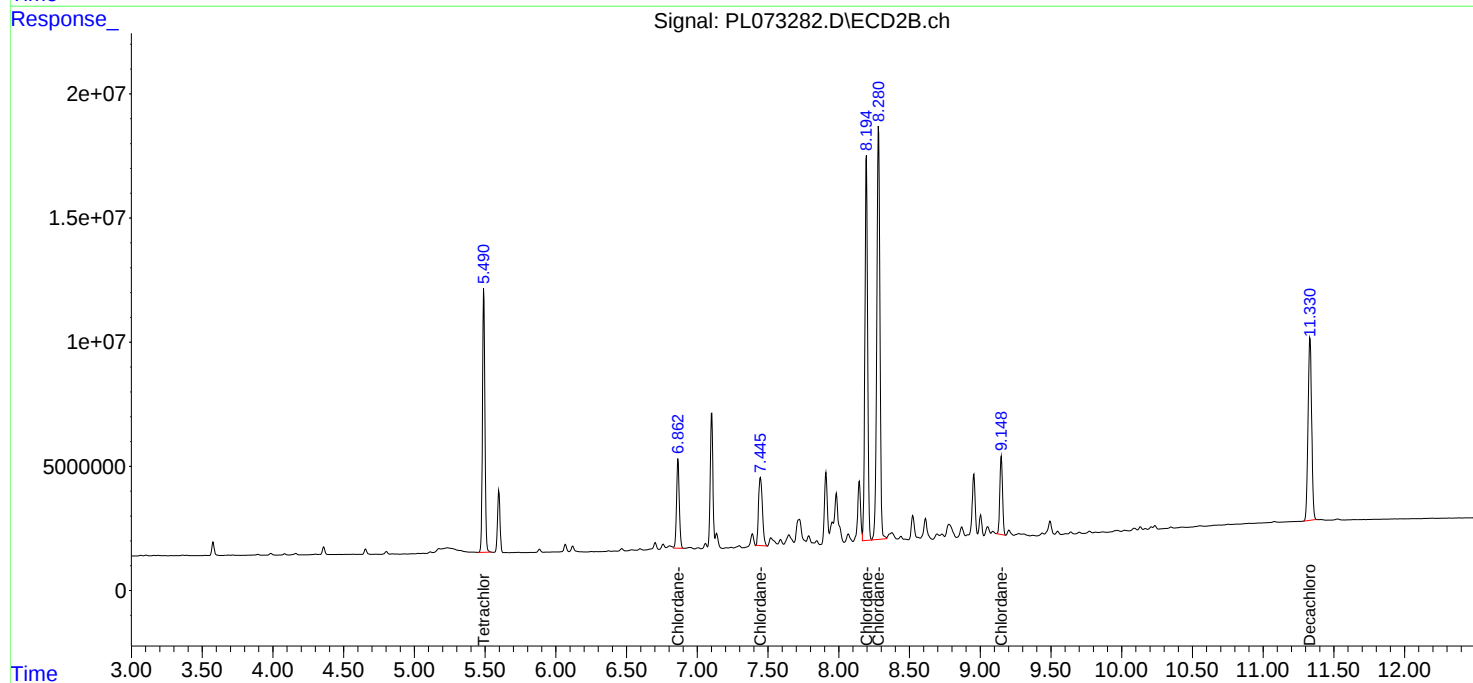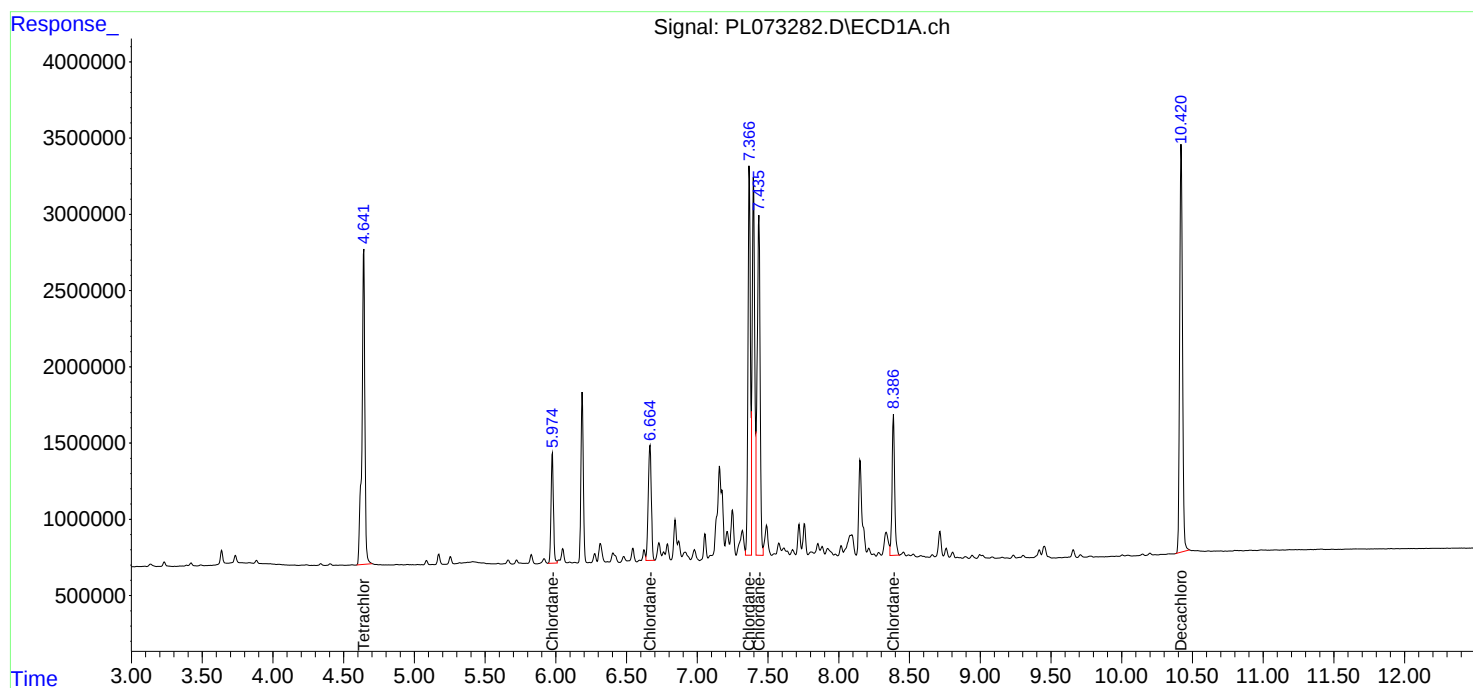


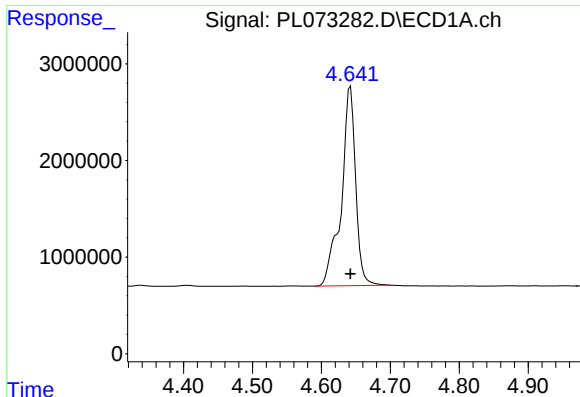

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 29910714
Conc: 75.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

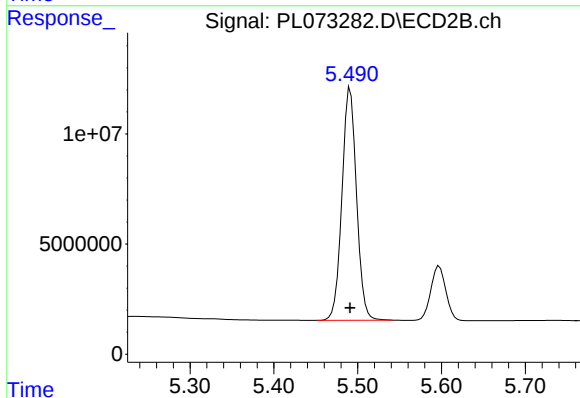


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 127557783
Conc: 75.28 ng/ml

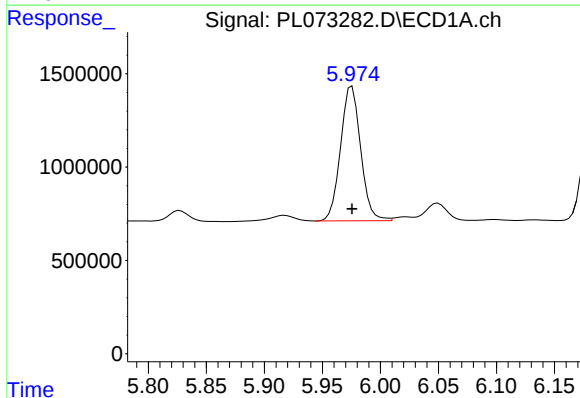


#23 Chlordane-1

R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 8684007
Conc: 746.64 ng/ml

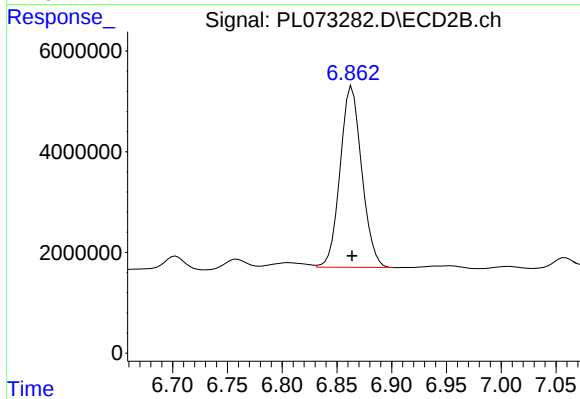

#23 Chlordane-1


R.T.: 6.864 min
Delta R.T.: 0.000 min
Response: 49404626
Conc: 750.90 ng/ml

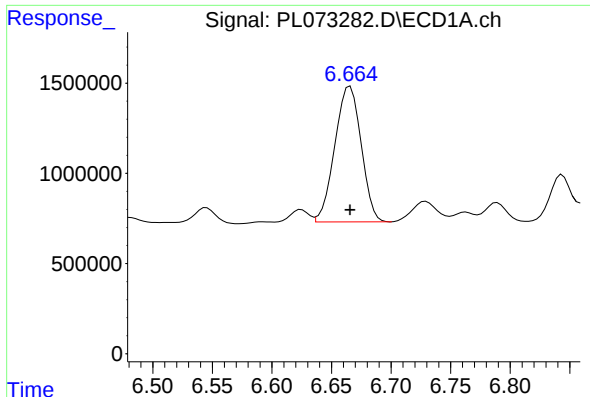

#24 Chlordane-2


R.T.: 6.666 min
Delta R.T.: 0.000 min
Response: 11580647
Conc: 744.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

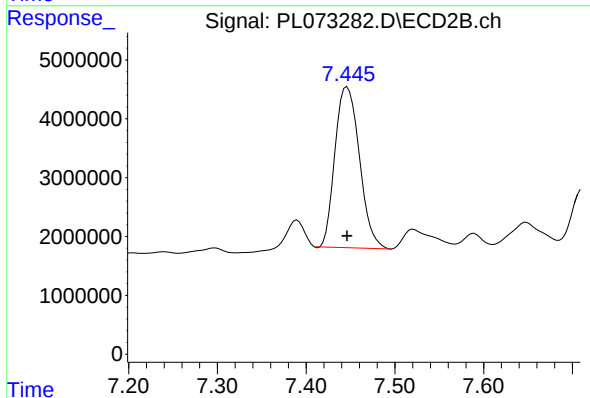


#24 Chlordane-2

R.T.: 7.446 min
Delta R.T.: 0.000 min
Response: 52398096
Conc: 748.55 ng/ml

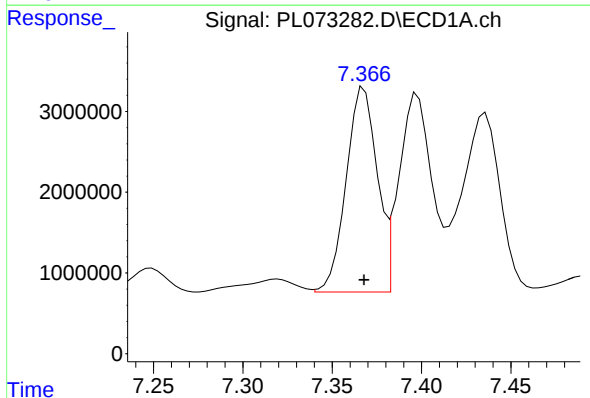


#25 Chlordane-3

R.T.: 7.368 min
Delta R.T.: 0.000 min
Response: 30583985
Conc: 752.04 ng/ml

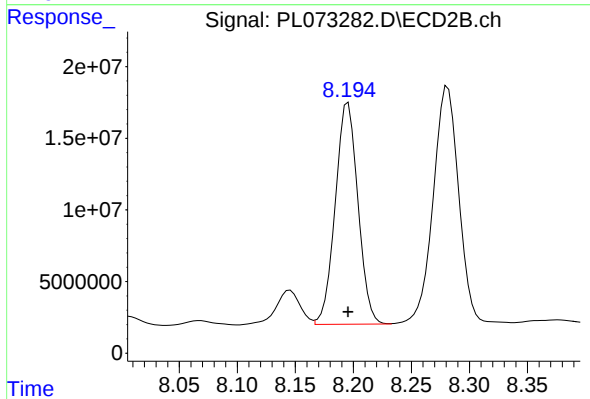

#25 Chlordane-3


R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 210183586
Conc: 753.76 ng/ml

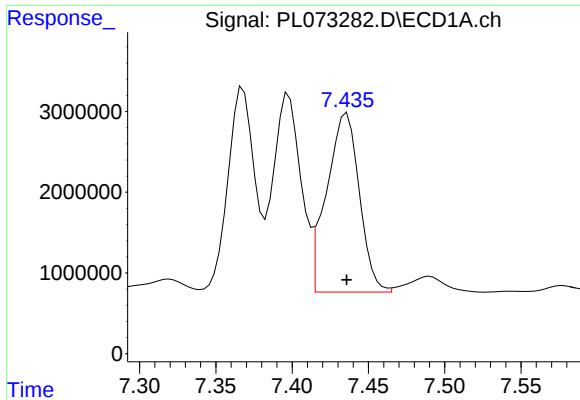

#26 Chlordane-4


R.T.: 7.436 min
Delta R.T.: 0.000 min
Response: 32967308
Conc: 749.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

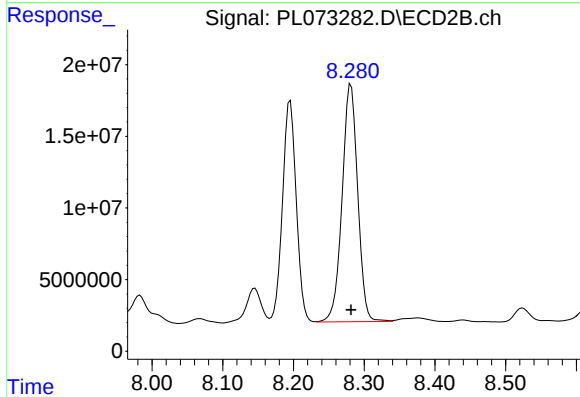


#26 Chlordane-4

R.T.: 8.281 min
Delta R.T.: 0.000 min
Response: 254501123
Conc: 753.30 ng/ml

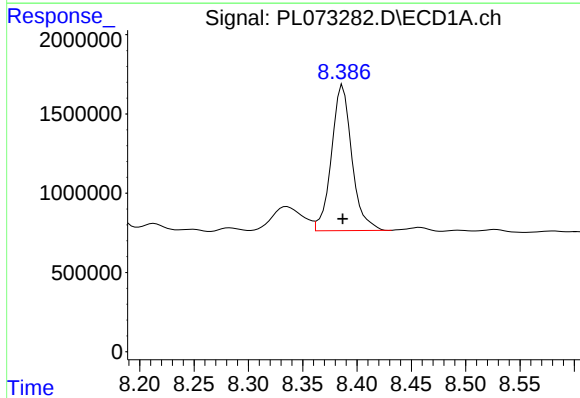


#27 Chlordane-5

R.T.: 8.387 min
Delta R.T.: 0.000 min
Response: 11998603
Conc: 752.95 ng/ml

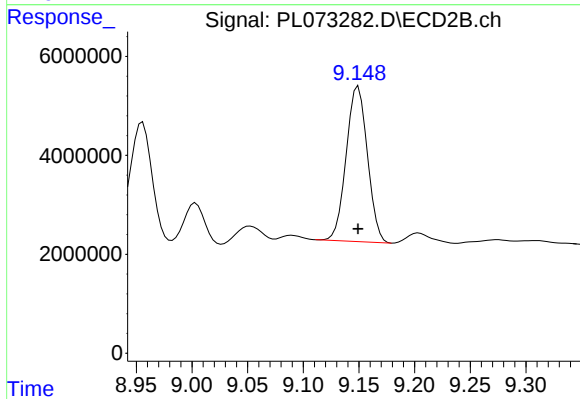

#27 Chlordane-5


R.T.: 9.149 min
Delta R.T.: 0.000 min
Response: 41646815
Conc: 748.89 ng/ml

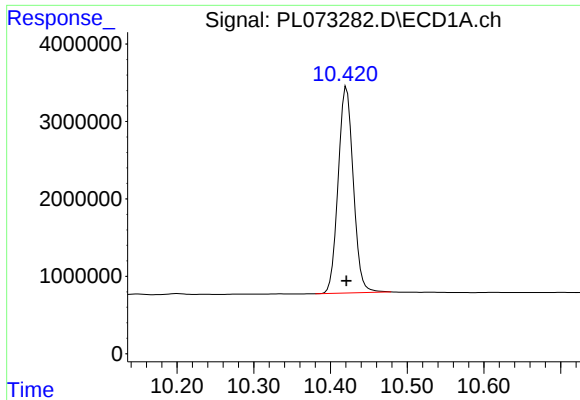

#28 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: 0.000 min
Response: 36508593
Conc: 74.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

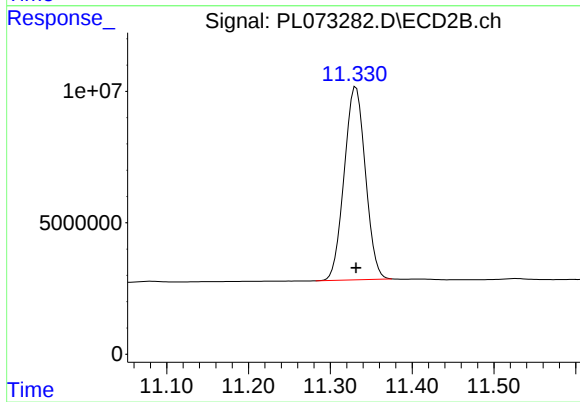

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: 0.000 min
Response: 131702852
Conc: 75.06 ng/ml