

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031122\
 Data File : PL073283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 22:17
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 05:19:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 12 05:18:28 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.491	20033645	84730206	50.000	50.000
28)	SA Decachlor...	10.421	11.331	25239478	89857894	50.000	50.000
Target Compounds							
23)	Chlordane-1	5.976	6.863	5937656	33297978	500.000	500.000
24)	Chlordane-2	6.665	7.446	8082681	35828317	500.000	500.000
25)	Chlordane-3	7.368	8.195	20273882	137.6E6	500.000	500.000
26)	Chlordane-4	7.437	8.281	21943212	168.0E6	500.000	500.000
27)	Chlordane-5	8.387	9.149	7981463	27999238	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031122\
Data File : PL073283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 22:17
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 05:19:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Sat Mar 12 05:18:28 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

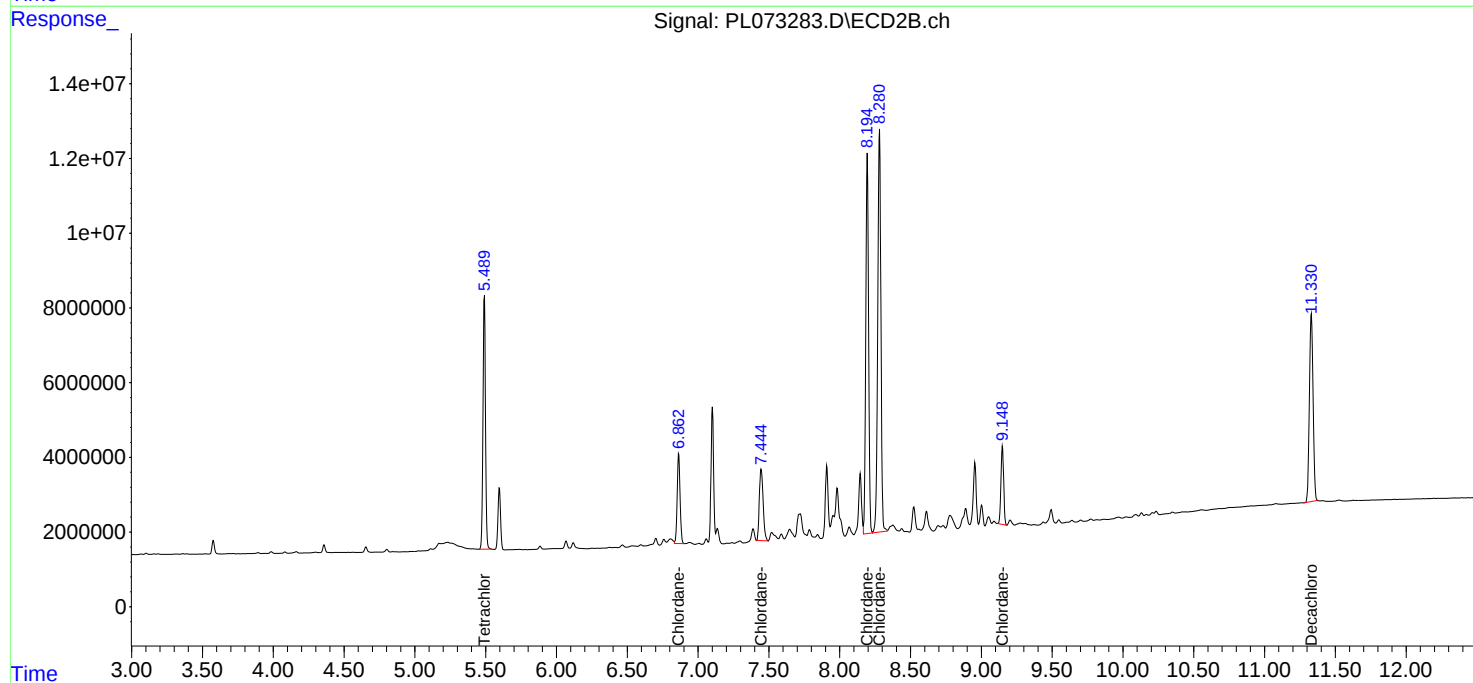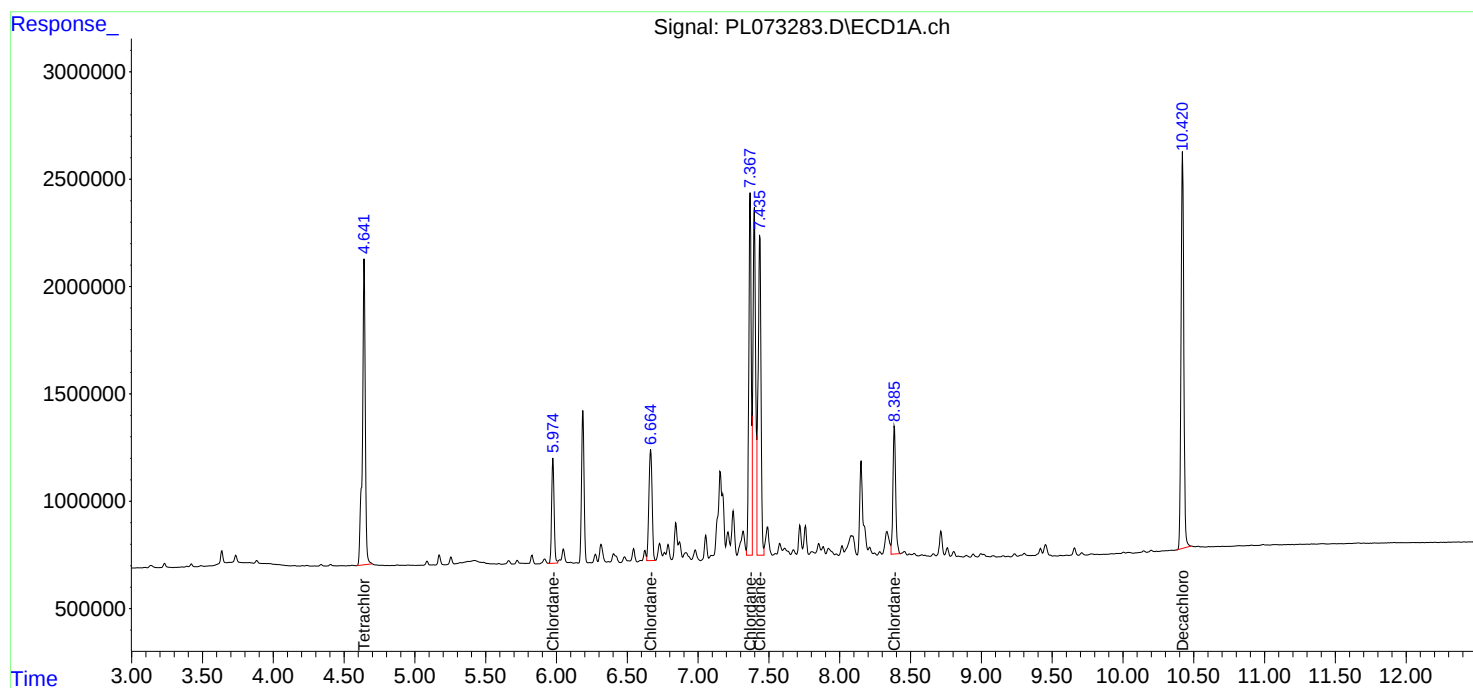


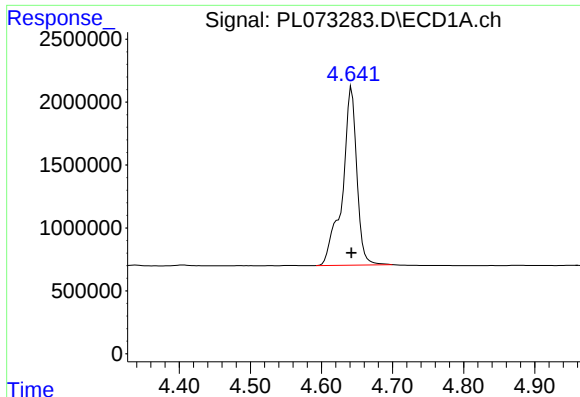

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 20033645
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

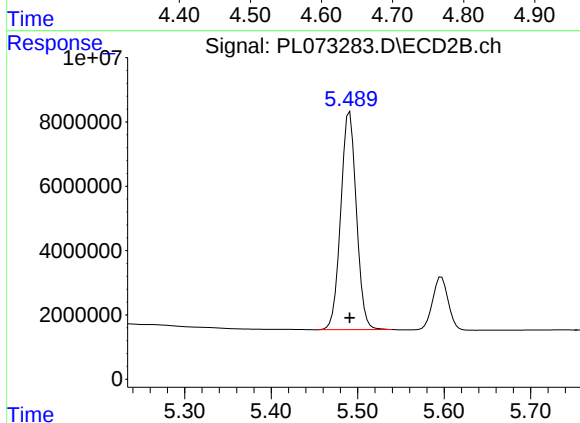


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 84730206
Conc: 50.00 ng/ml

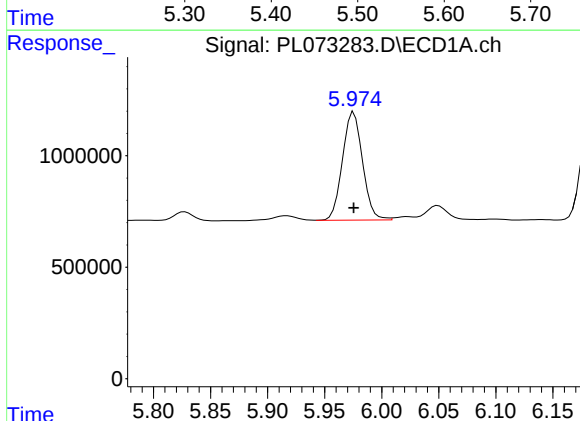


#23 Chlordane-1

R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 5937656
Conc: 500.00 ng/ml

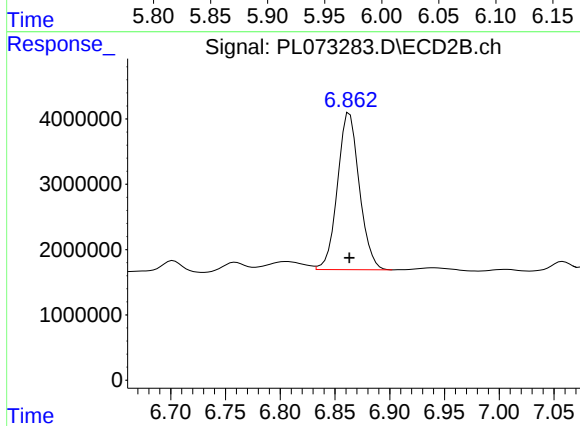

#23 Chlordane-1


R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 33297978
Conc: 500.00 ng/ml

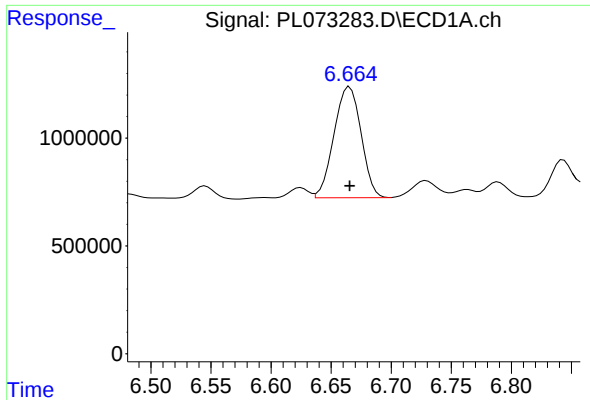

#24 Chlordane-2


R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 8082681
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

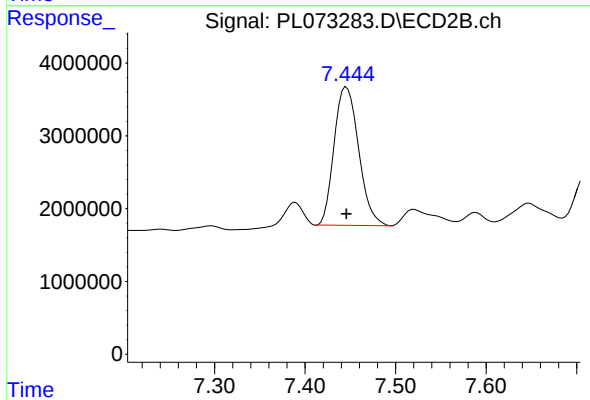


#24 Chlordane-2

R.T.: 7.446 min
Delta R.T.: 0.000 min
Response: 35828317
Conc: 500.00 ng/ml

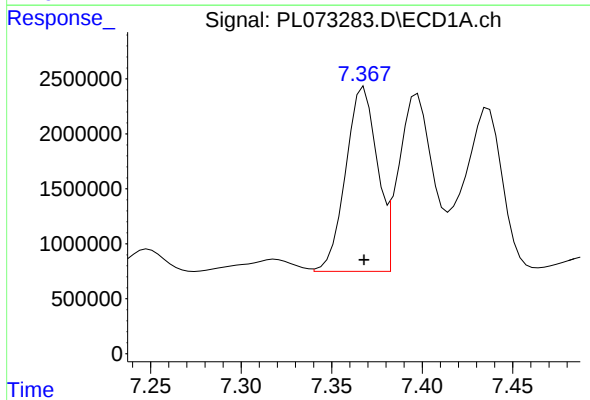


#25 Chlordane-3

R.T.: 7.368 min
Delta R.T.: 0.000 min
Response: 20273882
Conc: 500.00 ng/ml

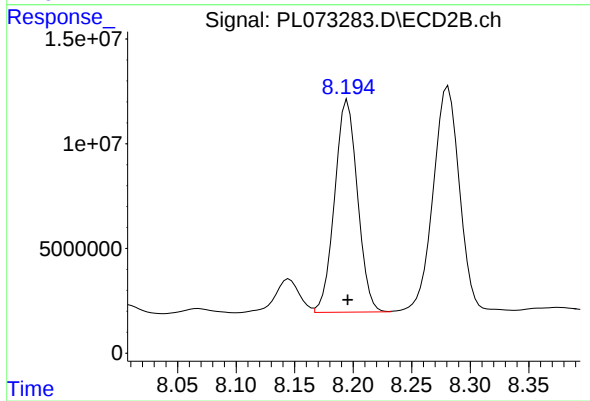

#25 Chlordane-3


R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 137617332
Conc: 500.00 ng/ml

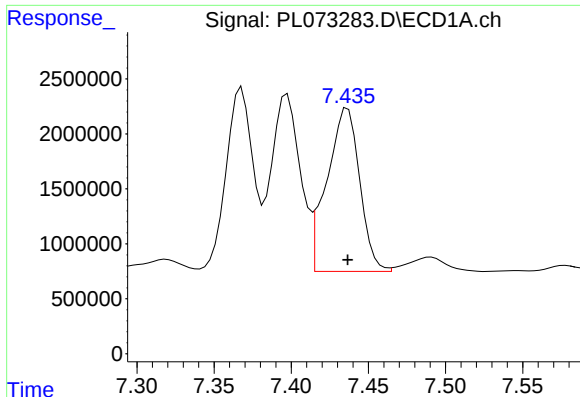

#26 Chlordane-4


R.T.: 7.437 min
Delta R.T.: 0.000 min
Response: 21943212
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

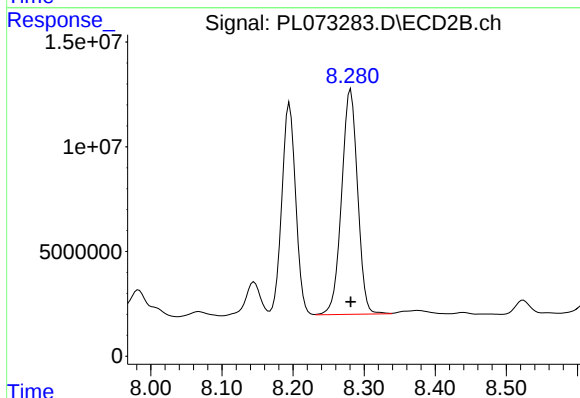


#26 Chlordane-4

R.T.: 8.281 min
Delta R.T.: 0.000 min
Response: 168002847
Conc: 500.00 ng/ml

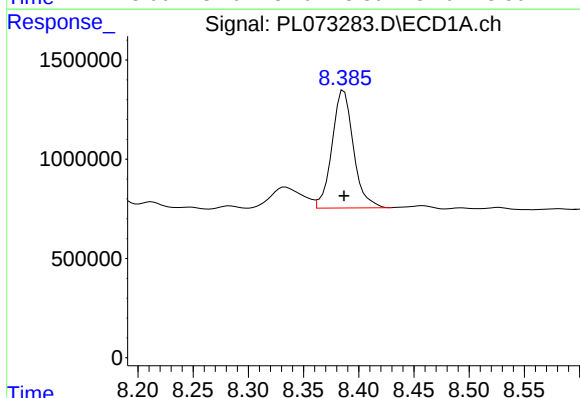


#27 Chlordane-5

R.T.: 8.387 min
Delta R.T.: 0.000 min
Response: 7981463
Conc: 500.00 ng/ml

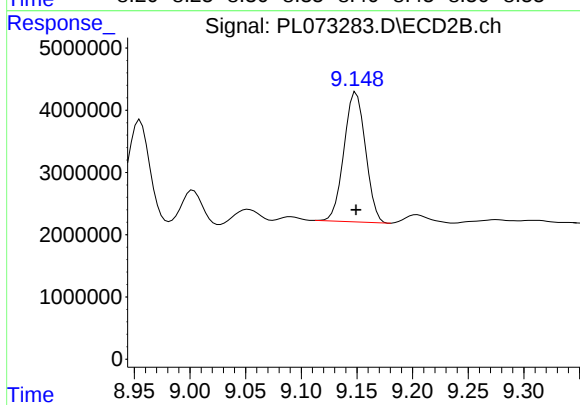

#27 Chlordane-5


R.T.: 9.149 min
Delta R.T.: 0.000 min
Response: 27999238
Conc: 500.00 ng/ml

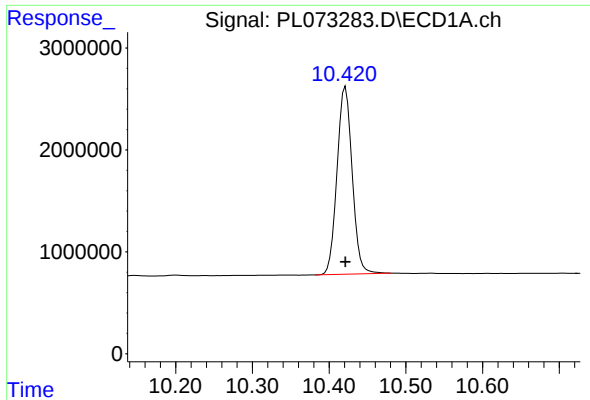

#28 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: 0.000 min
Response: 25239478
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

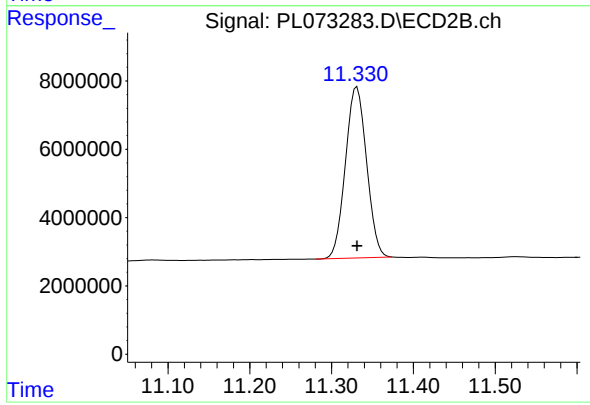

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: 0.000 min
Response: 89857894
Conc: 50.00 ng/ml