

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031124\
 Data File : PL088486.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2024 11:26
 Operator : AR\AJ
 Sample : P1601-02
 Misc : PEST MDL 1PPB WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT1-2024-02

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/12/2024
 Supervised By :Ankita Jodhani 03/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 00:32:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030824CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 08 16:13:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.851	68214091	31885819	22.912	20.788m
27)	SA Decachlor...	9.307	8.083	69543568	40718620	28.198	28.068
Target Compounds							
2)	A alpha-BHC	4.099	3.366	4448683	1897033	1.021	0.868
3)	MA gamma-BHC...	4.438	3.703	4365946	1921259	1.049	0.924
4)	MA Heptachlor	5.038	4.051	5344646	1967485	1.256	0.962
5)	MB Aldrin	5.386	4.337	4534147	1775005	1.238	0.963
6)	B beta-BHC	4.634	4.003	2117725	981232	1.124m	1.017m
7)	B delta-BHC	4.886	4.240	6012883	1617828	1.441	0.795 #
8)	B Heptachlo...	5.816	4.847	4782335	1869955	1.287m	1.055
9)	A Endosulfan I	6.209	5.224	4286715	1769895	1.276	1.052
10)	B trans-Chl...	6.075	5.103	4598060	1983074	1.343m	1.137
11)	B cis-Chlor...	6.158	5.168	4687393	2012476	1.342	1.122
12)	B 4,4'-DDE	6.332	5.360	3795960	1555838	1.207	0.946
13)	MA Dieldrin	6.488	5.493	4366813	1819980	1.224	0.969
14)	MA Endrin	6.720	5.772	3390066	1734711	1.146	1.056
15)	B Endosulfa...	6.940	6.070	3842362	1919410	1.307m	1.217
16)	A 4,4'-DDD	6.855	5.923	3427472	1358551	1.274	0.962
17)	MA 4,4'-DDT	7.174	6.177	3678782	1491824	1.279	0.948m#
18)	B Endrin al...	7.073	6.252	3104208	1487971	1.416	1.276
19)	B Endosulfa...	7.309	6.478	3918593	1740527	1.374	1.146
20)	A Methoxychlor	7.655	6.762	2003427	961004	1.285	1.114
21)	B Endrin ke...	7.801	6.991	3955852	1881457	1.322	1.087

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031124\
Data File : PL088486.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2024 11:26
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL 1PPB WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 00:32:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030824CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 08 16:13:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

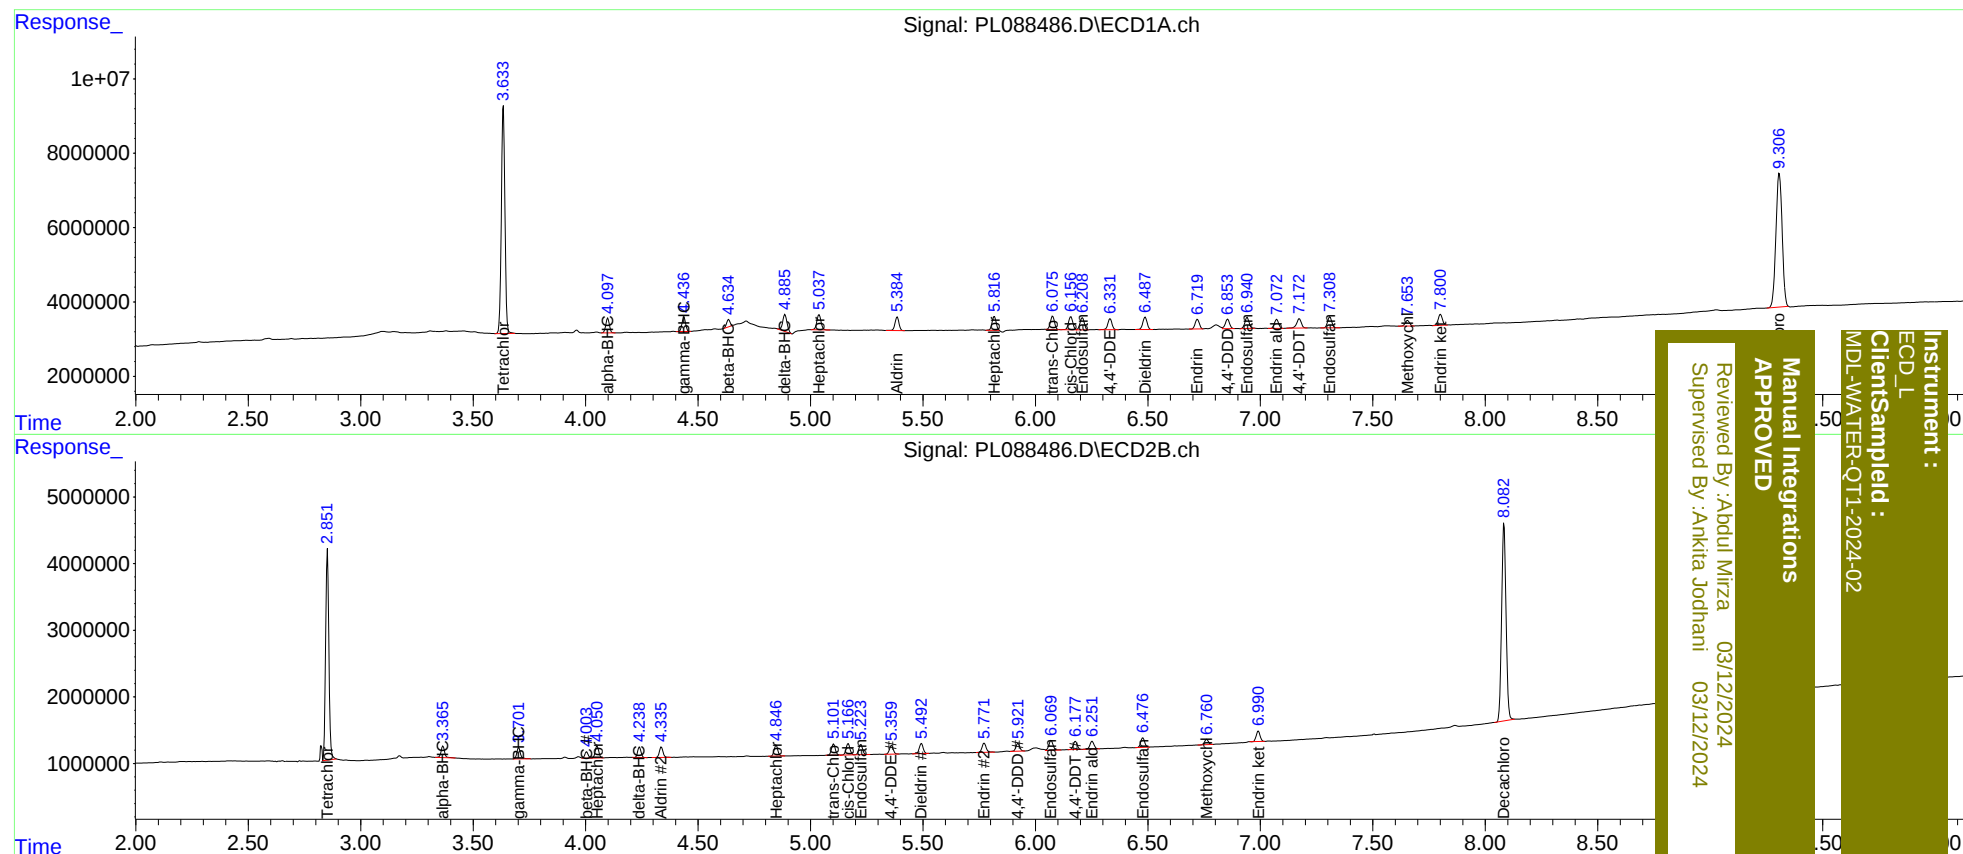

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 03/12/2024
Supervised By: Ankita Jodhani 03/12/2024

Instrument :
ECD_L
Client Sample :
MDL-WATER-QT1-2024-02