

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
 Data File : PL094575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 11:57
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 17:04:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:00:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.771	205.0E6	333.3E6	75.176	75.424
28)	SA Decachlor...	9.055	7.907	148.9E6	301.9E6	74.521	74.646
Target Compounds							
23)	Chlordane-1	4.699	3.768	102.6E6	112.8E6	764.701	751.354
24)	Chlordane-2	5.229	4.345	111.7E6	131.5E6	771.727	751.300
25)	Chlordane-3	5.941	4.974	354.1E6	403.2E6	754.903	751.126
26)	Chlordane-4	6.022	5.037	422.3E6	394.4E6	758.859	750.819
27)	Chlordane-5	6.872	5.933	77516688	149.2E6	744.598	758.619



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
Data File : PL094575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 11:57
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 17:04:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:00:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

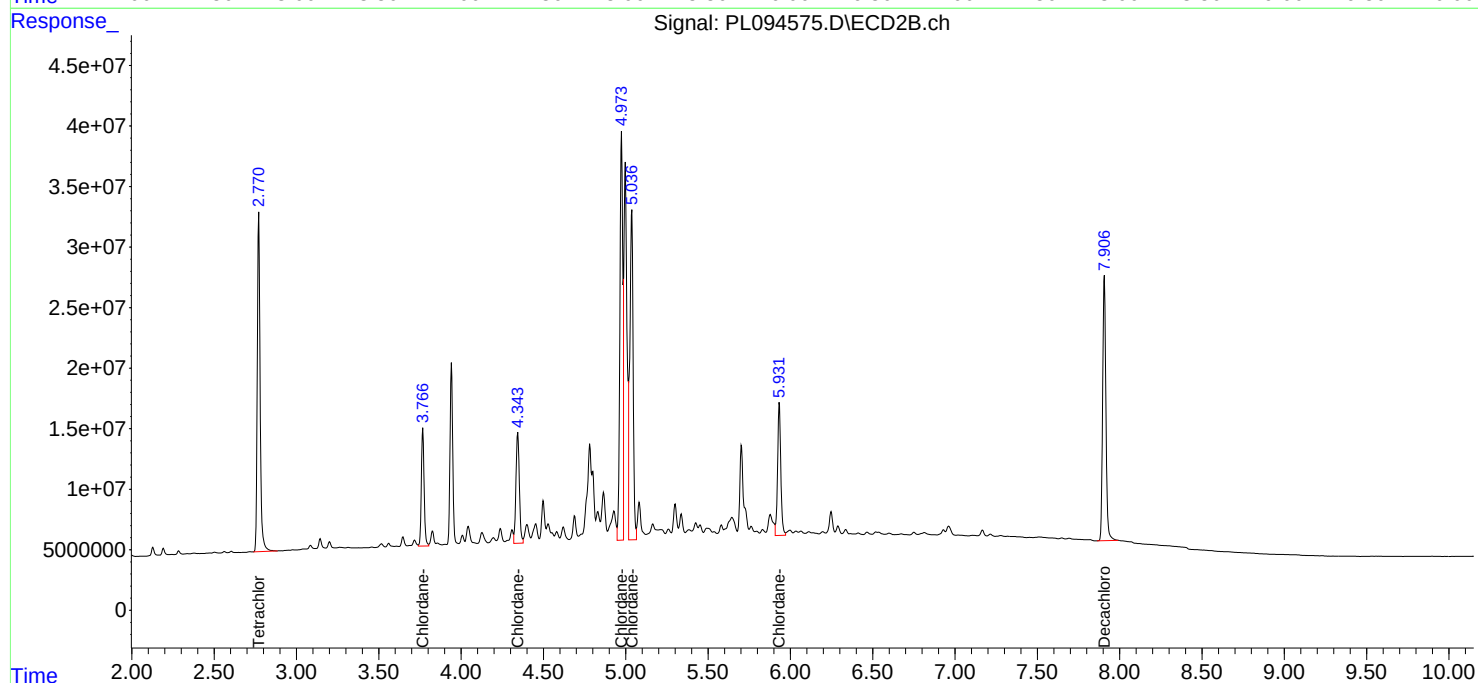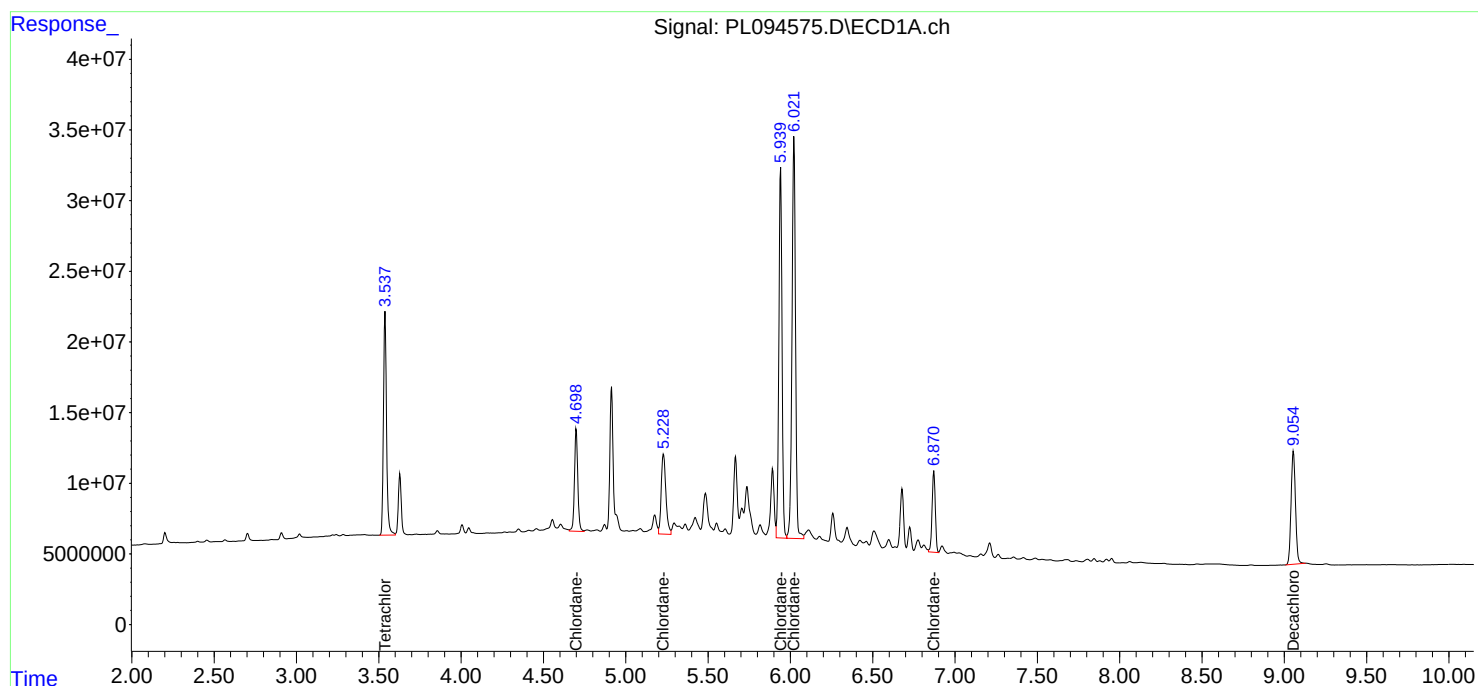


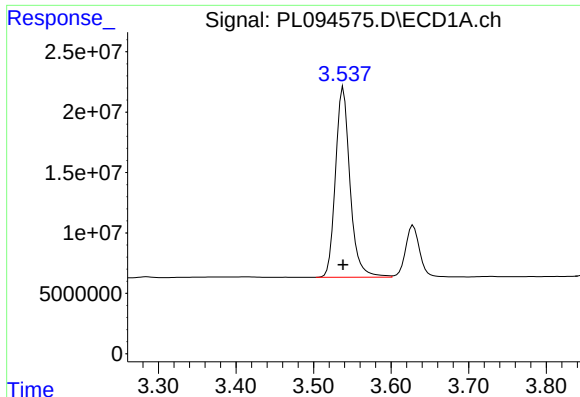

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 205004651
Conc: 75.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

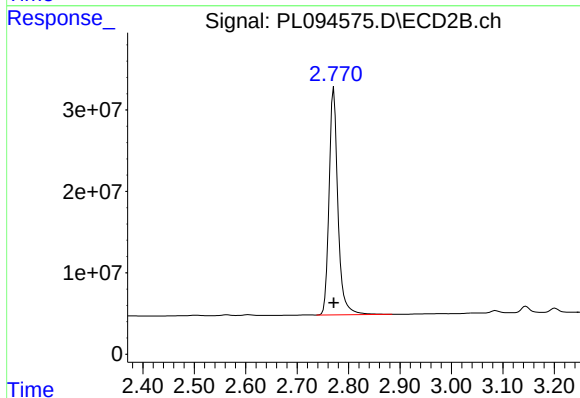


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 333288065
Conc: 75.42 ng/ml

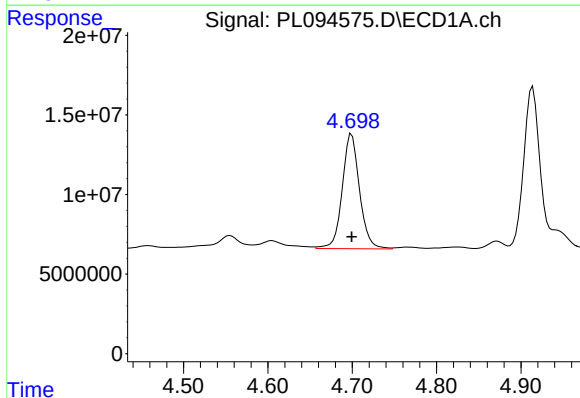


#23 Chlordane-1

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 102561416
Conc: 764.70 ng/ml

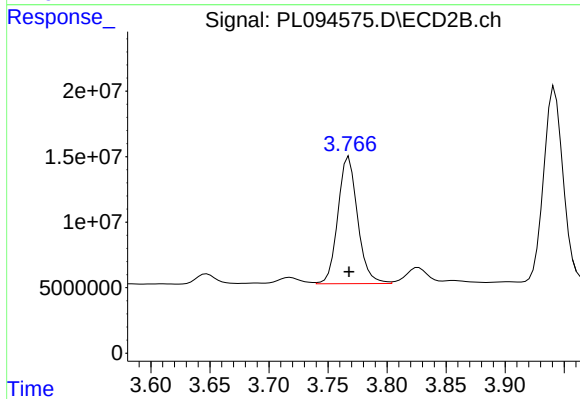

#23 Chlordane-1


R.T.: 3.768 min
Delta R.T.: 0.000 min
Response: 112810208
Conc: 751.35 ng/ml

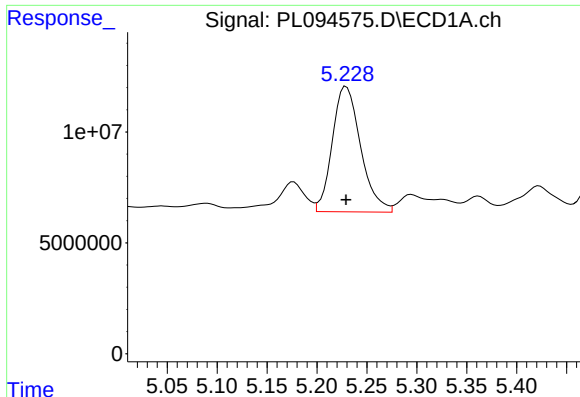

#24 Chlordane-2


R.T.: 5.229 min
Delta R.T.: 0.000 min
Response: 111739384
Conc: 771.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

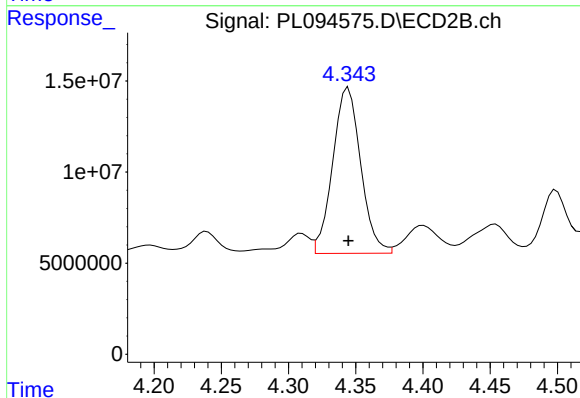


#24 Chlordane-2

R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 131484043
Conc: 751.30 ng/ml

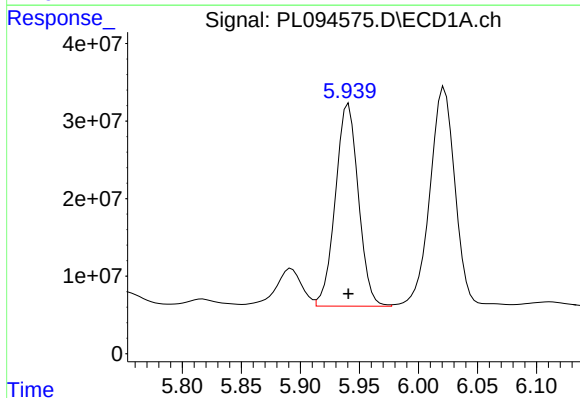


#25 Chlordane-3

R.T.: 5.941 min
Delta R.T.: 0.000 min
Response: 354083667
Conc: 754.90 ng/ml

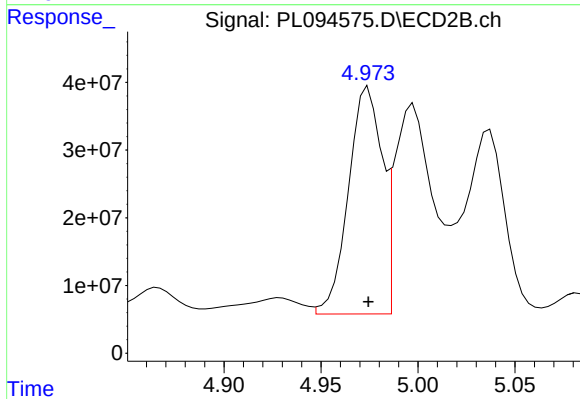

#25 Chlordane-3


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 403173208
Conc: 751.13 ng/ml

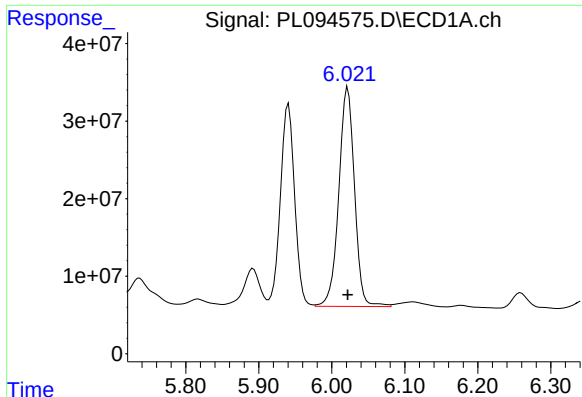

#26 Chlordane-4


R.T.: 6.022 min
Delta R.T.: 0.000 min
Response: 422322513
Conc: 758.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

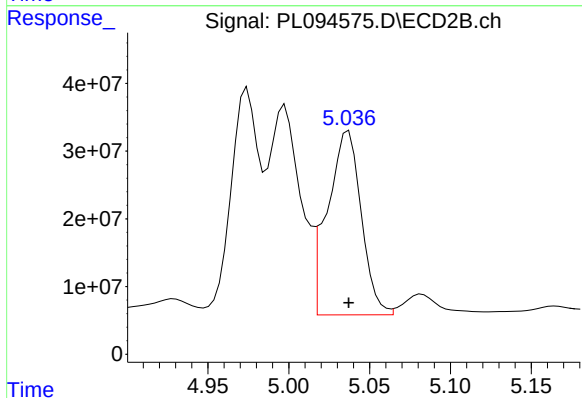


#26 Chlordane-4

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 394429349
Conc: 750.82 ng/ml

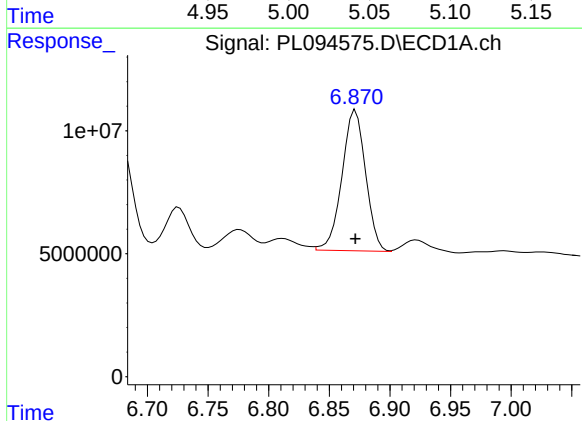


#27 Chlordane-5

R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 77516688
Conc: 744.60 ng/ml

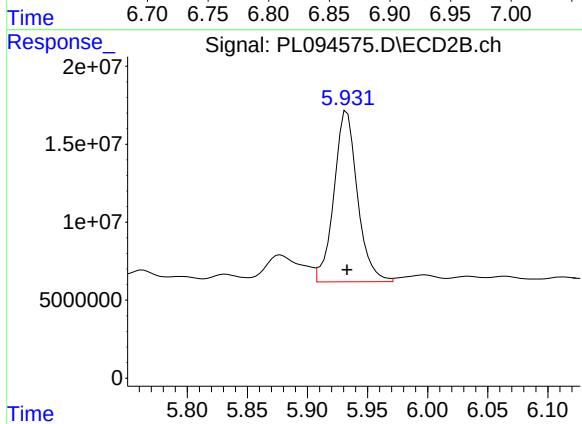

#27 Chlordane-5


R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 149237095
Conc: 758.62 ng/ml

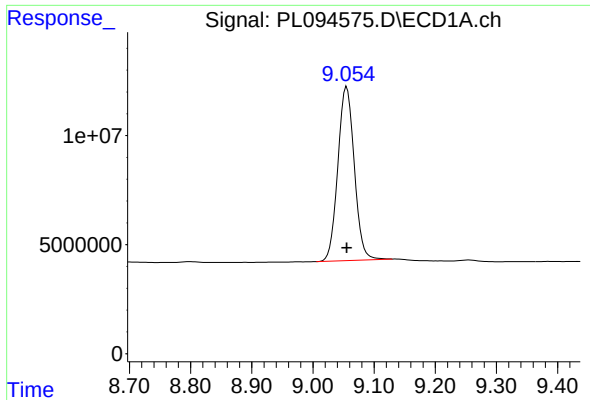

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 148931983
Conc: 74.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

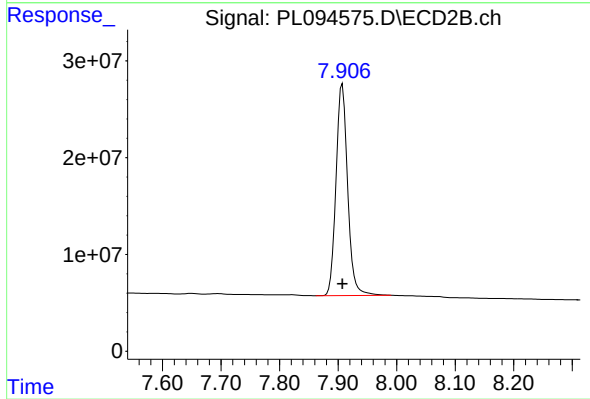

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 301937082
Conc: 74.65 ng/ml