

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
 Data File : PL094576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 12:10
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 17:01:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:00:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.771	137.6E6	217.7E6	50.000	50.000
28)	SA Decachlor...	9.056	7.907	102.8E6	202.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.700	3.768	67315229	74220750	500.000	500.000
24)	Chlordane-2	5.229	4.345	72325929	87338022	500.000	500.000
25)	Chlordane-3	5.940	4.974	232.4E6	261.3E6	500.000	500.000
26)	Chlordane-4	6.022	5.037	273.9E6	257.7E6	500.000	500.000
27)	Chlordane-5	6.871	5.933	52243777	93588494	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
Data File : PL094576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 12:10
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 17:01:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:00:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

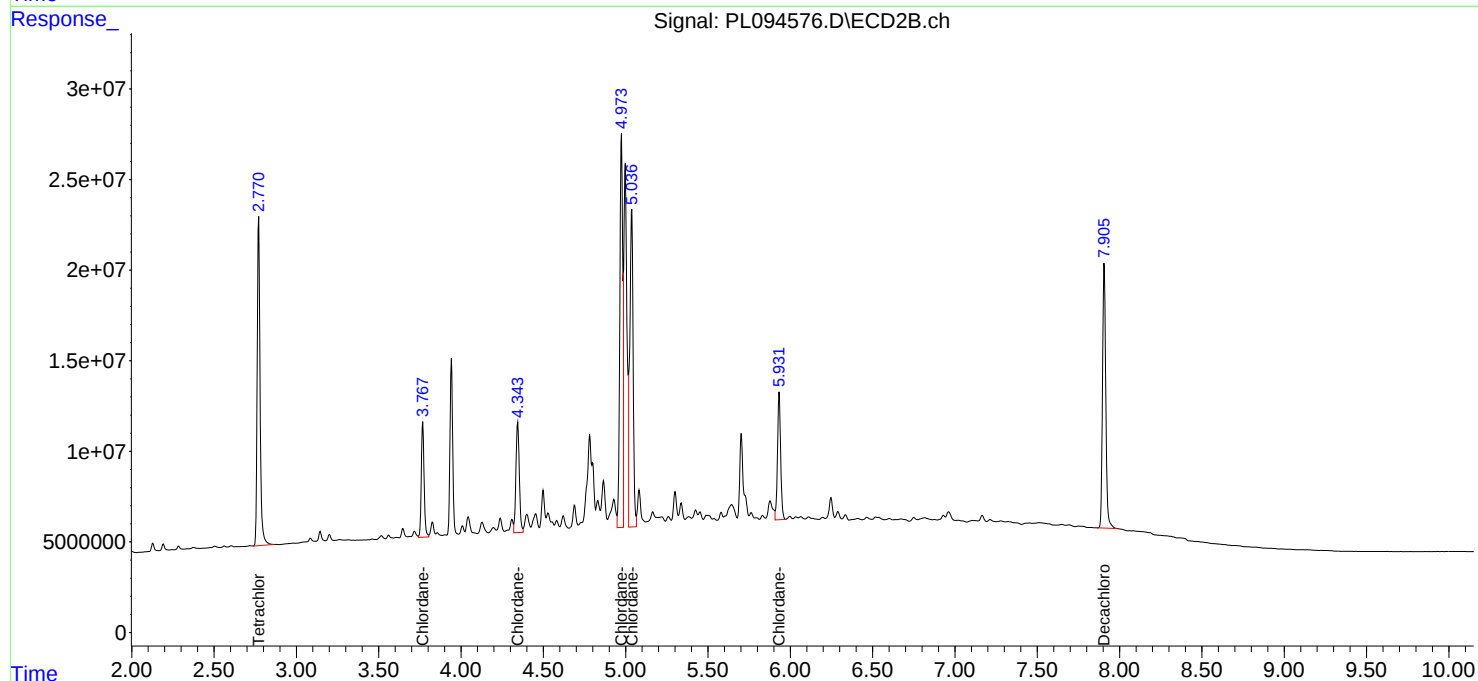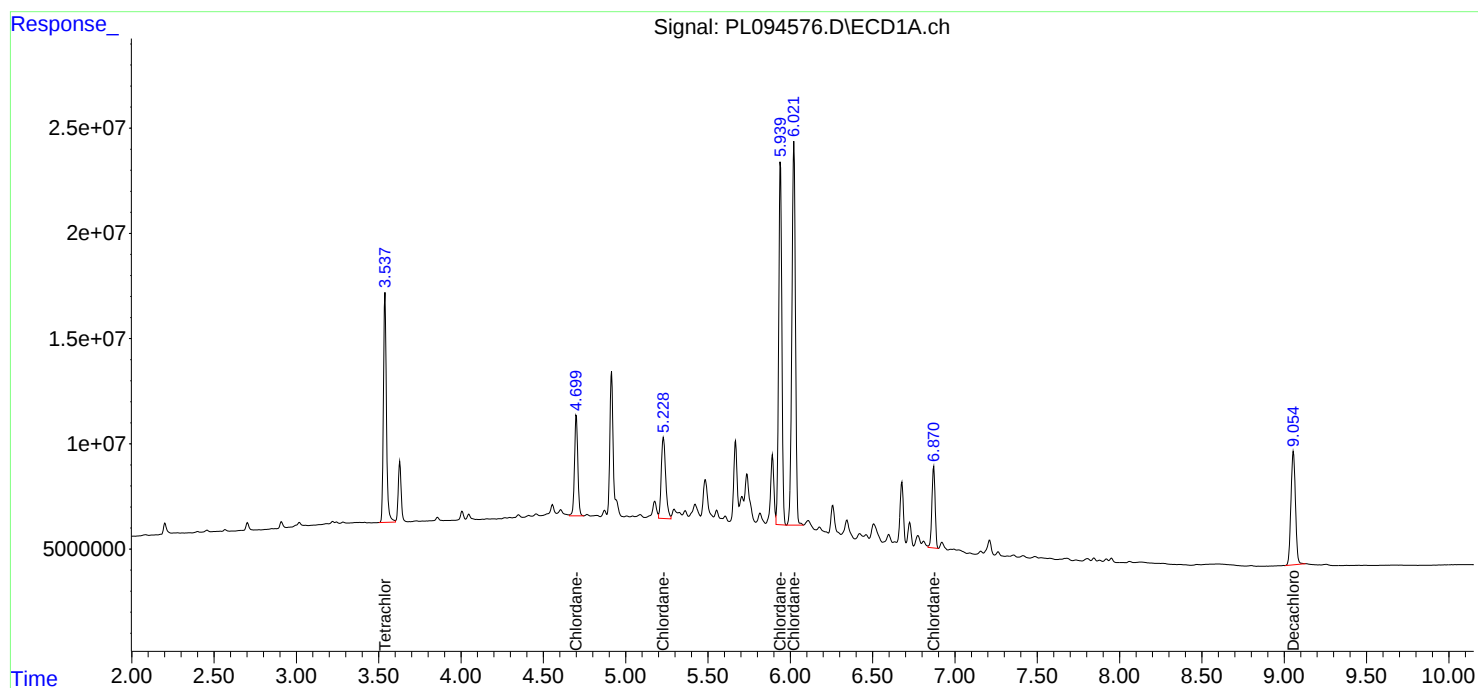


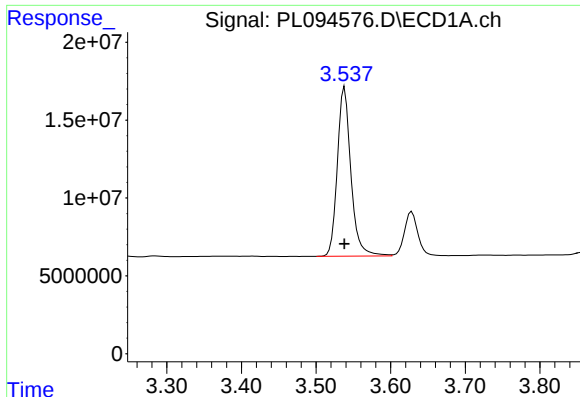

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 137550046
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

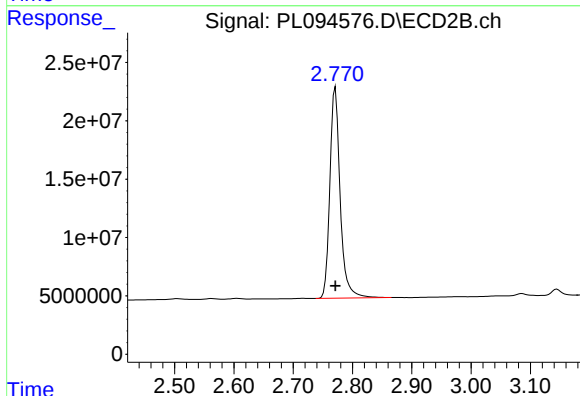


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 217748564
Conc: 50.00 ng/ml

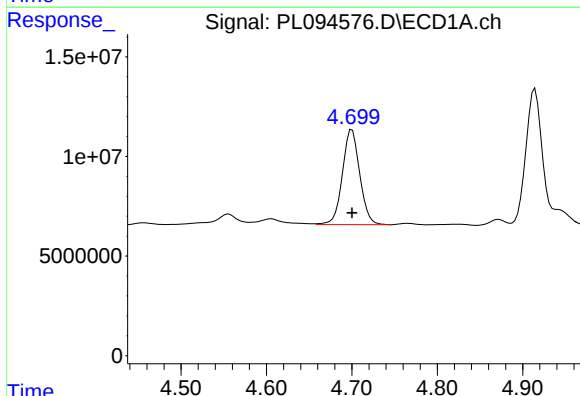


#23 Chlordane-1

R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 67315229
Conc: 500.00 ng/ml

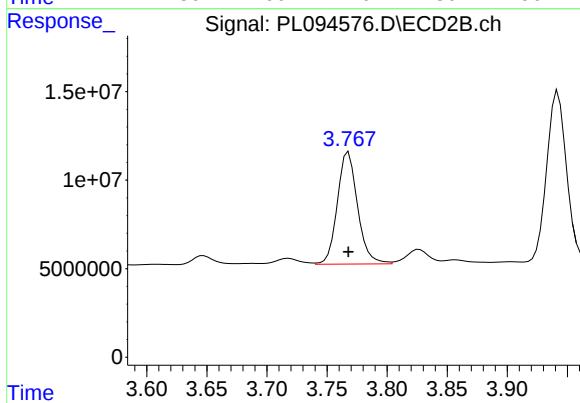

#23 Chlordane-1


R.T.: 3.768 min
Delta R.T.: 0.000 min
Response: 74220750
Conc: 500.00 ng/ml

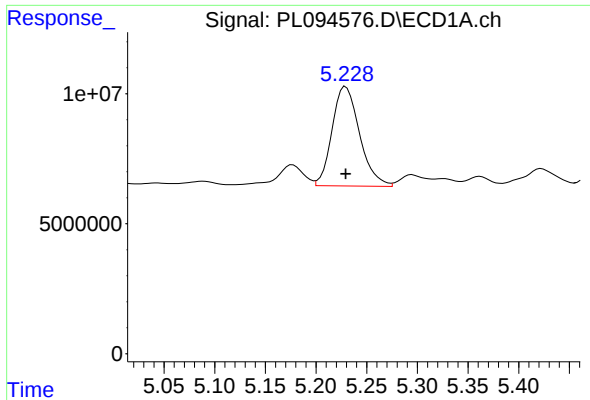

#24 Chlordane-2


R.T.: 5.229 min
Delta R.T.: 0.000 min
Response: 72325929
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

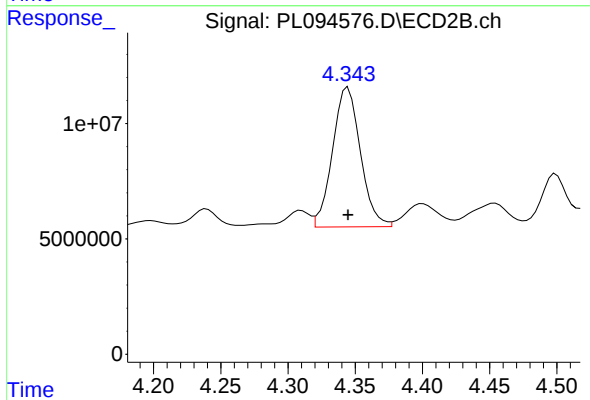


#24 Chlordane-2

R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 87338022
Conc: 500.00 ng/ml

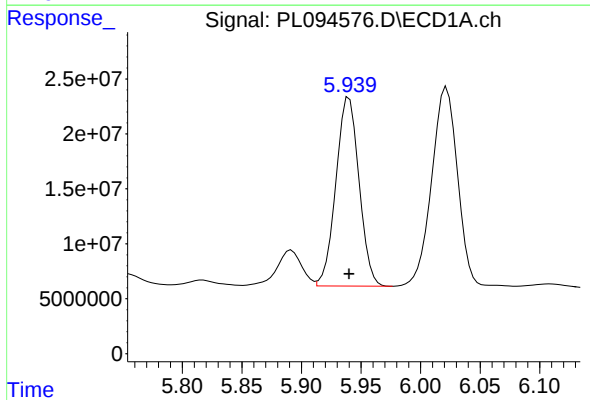


#25 Chlordane-3

R.T.: 5.940 min
Delta R.T.: 0.000 min
Response: 232431687
Conc: 500.00 ng/ml

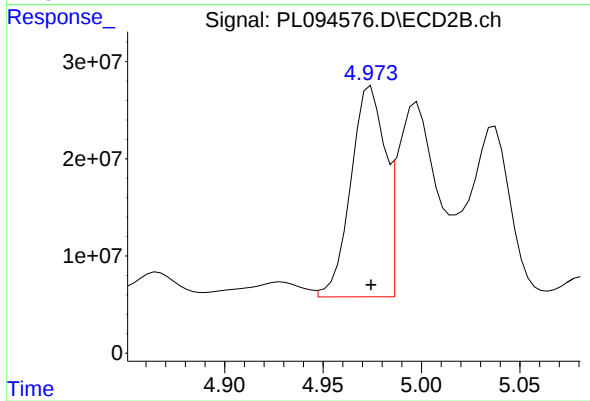

#25 Chlordane-3


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 261258464
Conc: 500.00 ng/ml

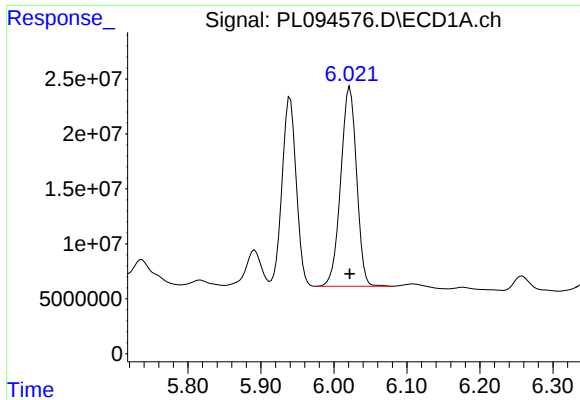

#26 Chlordane-4


R.T.: 6.022 min
Delta R.T.: 0.000 min
Response: 273855108
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

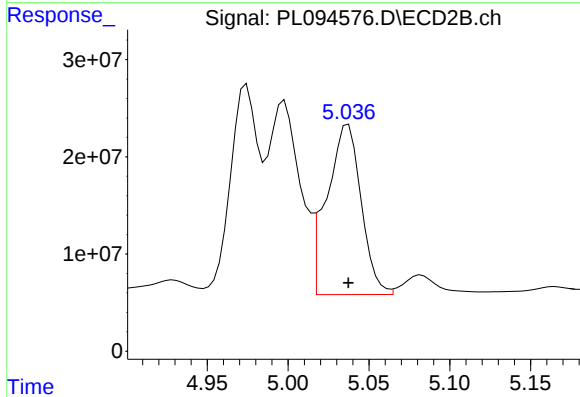


#26 Chlordane-4

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 257709114
Conc: 500.00 ng/ml

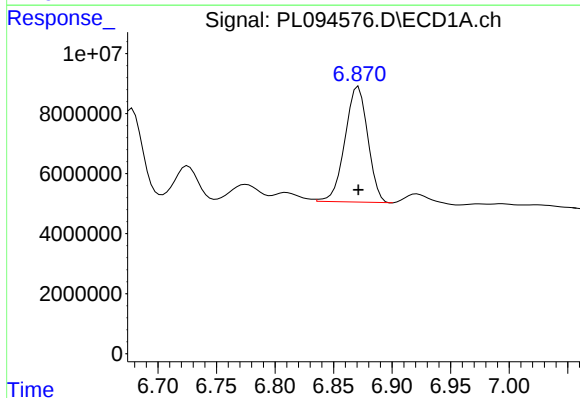


#27 Chlordane-5

R.T.: 6.871 min
Delta R.T.: 0.000 min
Response: 52243777
Conc: 500.00 ng/ml

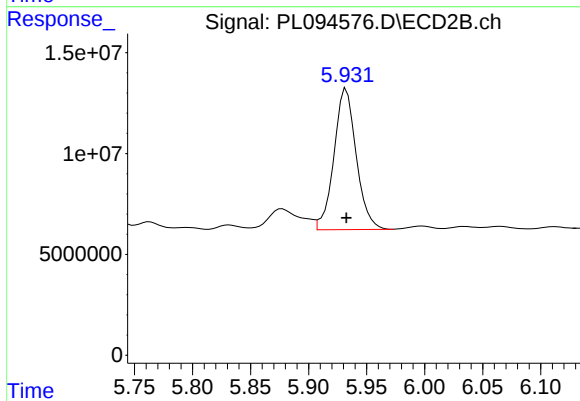

#27 Chlordane-5


R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 93588494
Conc: 500.00 ng/ml

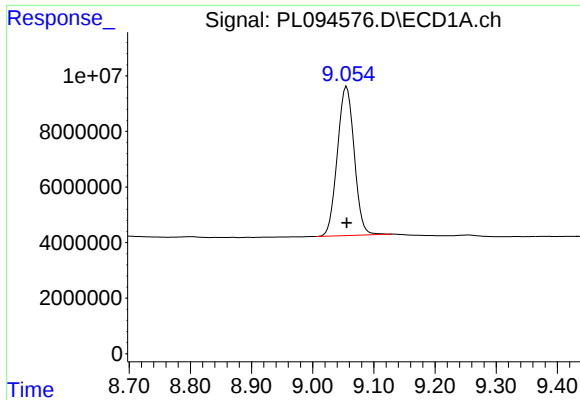

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.000 min
Response: 102794843
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

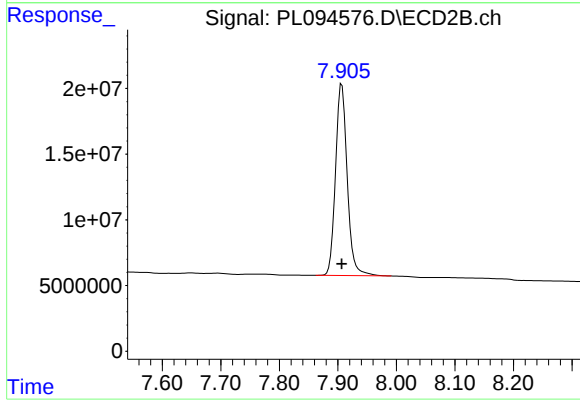

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 202542800
Conc: 50.00 ng/ml