

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
 Data File : PL094577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 12:24
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 17:06:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:00:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.771	72841277	110.4E6	26.262	24.985
28)	SA Decachlor...	9.055	7.907	54683389	106.2E6	26.730	25.929
Target Compounds							
23)	Chlordane-1	4.699	3.768	35256965	36027449	259.535	242.390
24)	Chlordane-2	5.229	4.344	36638637	43804471	252.276	250.224
25)	Chlordane-3	5.940	4.974	123.0E6	129.1E6	259.078	242.822
26)	Chlordane-4	6.021	5.036	145.3E6	126.9E6	258.257	243.554
27)	Chlordane-5	6.870	5.933	27856106	46547567	262.954	239.826



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
Data File : PL094577.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 12:24
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 17:06:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:00:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

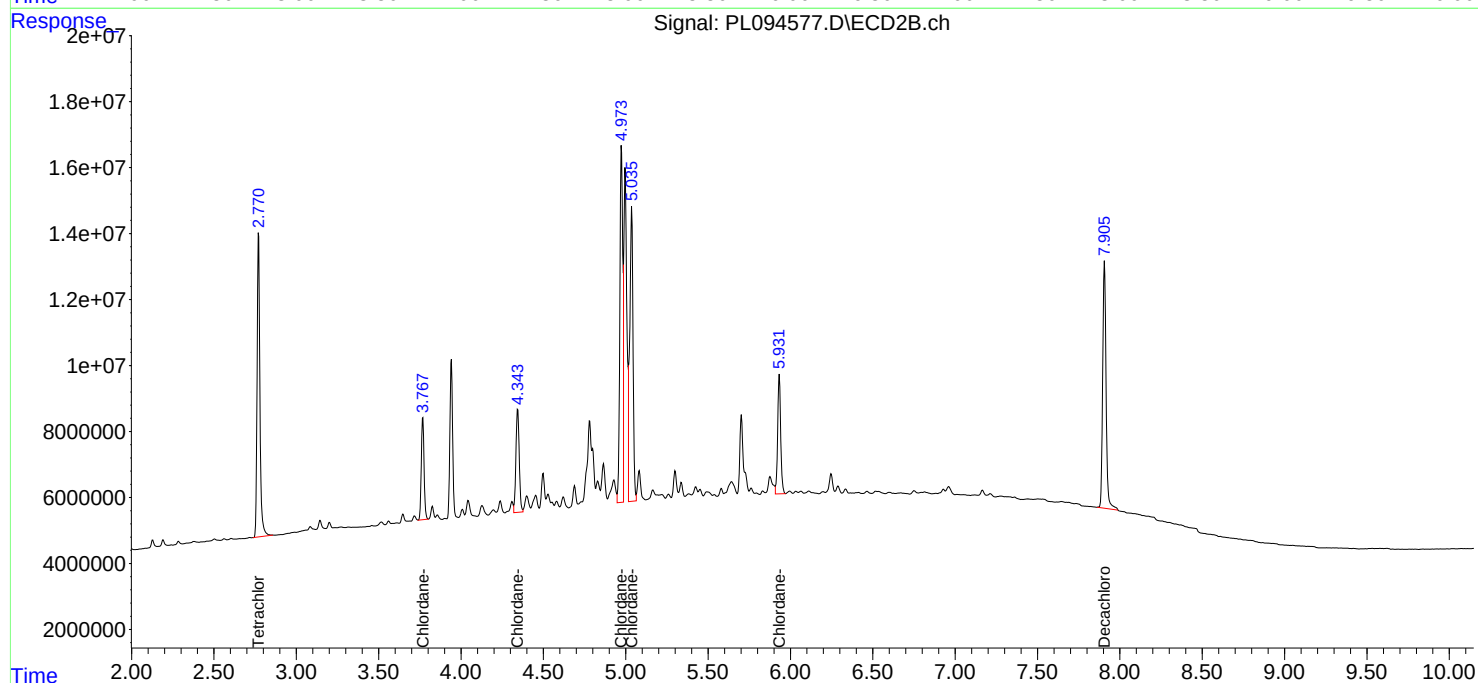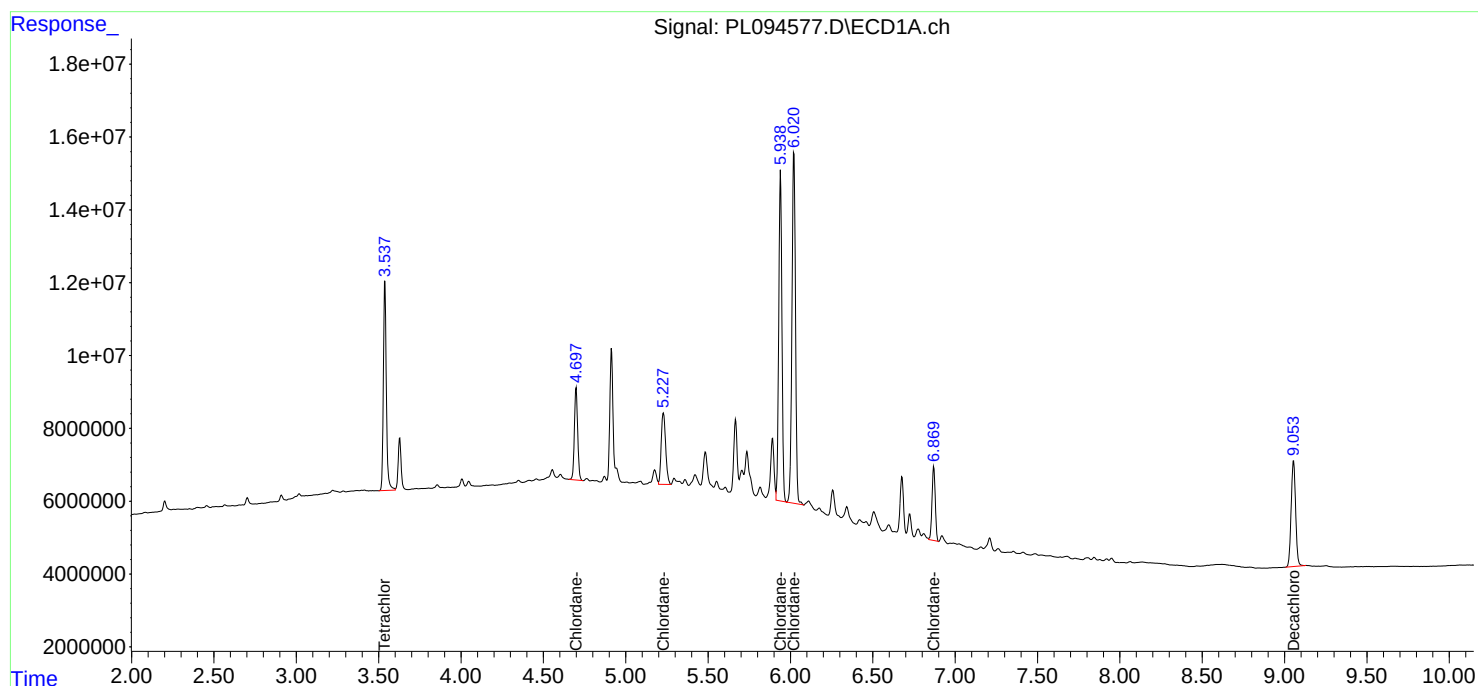


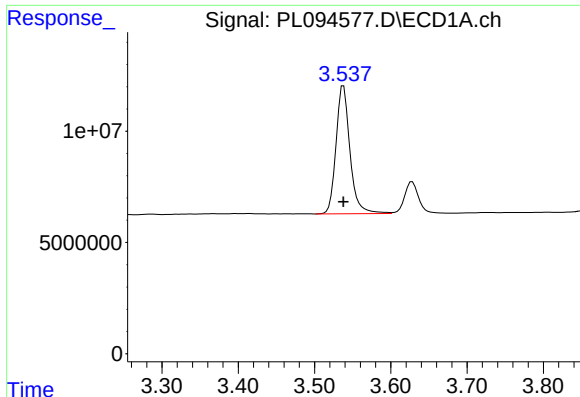

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 72841277
Conc: 26.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

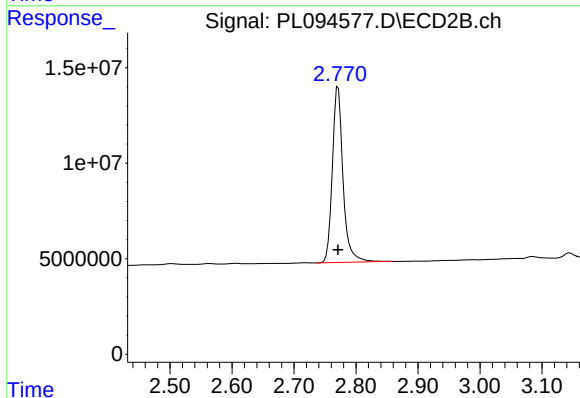


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 110384260
Conc: 24.99 ng/ml

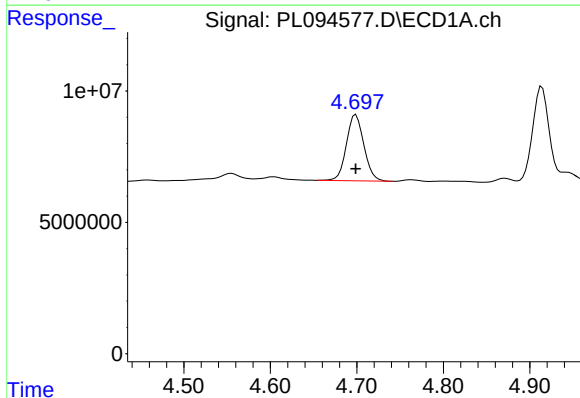


#23 Chlordane-1

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 35256965
Conc: 259.54 ng/ml

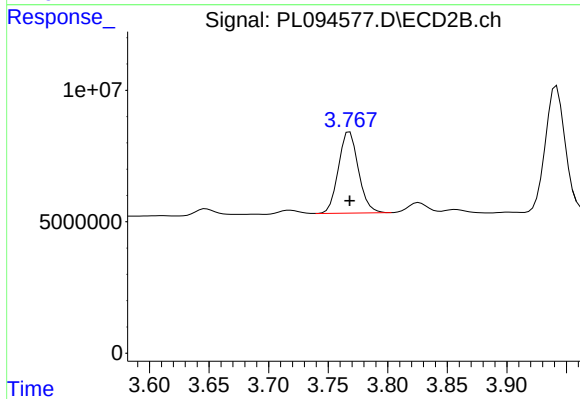

#23 Chlordane-1


R.T.: 3.768 min
Delta R.T.: 0.000 min
Response: 36027449
Conc: 242.39 ng/ml

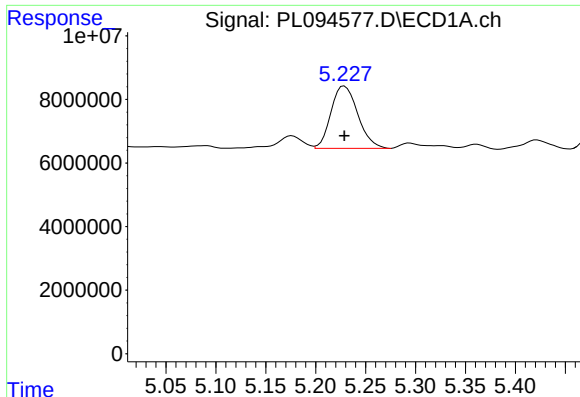

#24 Chlordane-2


R.T.: 5.229 min
Delta R.T.: 0.000 min
Response: 36638637
Conc: 252.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

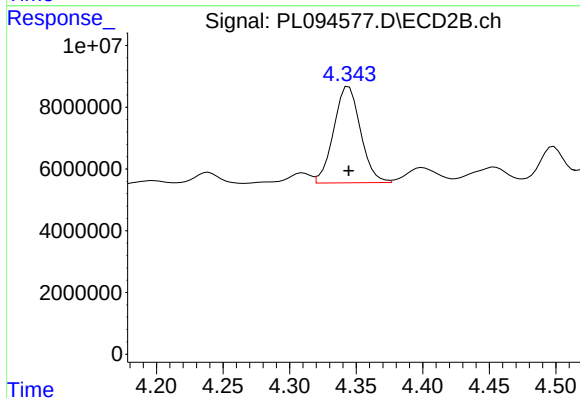


#24 Chlordane-2

R.T.: 4.344 min
Delta R.T.: 0.000 min
Response: 43804471
Conc: 250.22 ng/ml

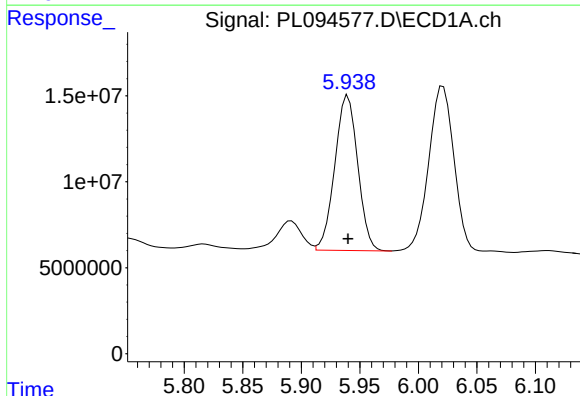


#25 Chlordane-3

R.T.: 5.940 min
Delta R.T.: 0.000 min
Response: 123008037
Conc: 259.08 ng/ml

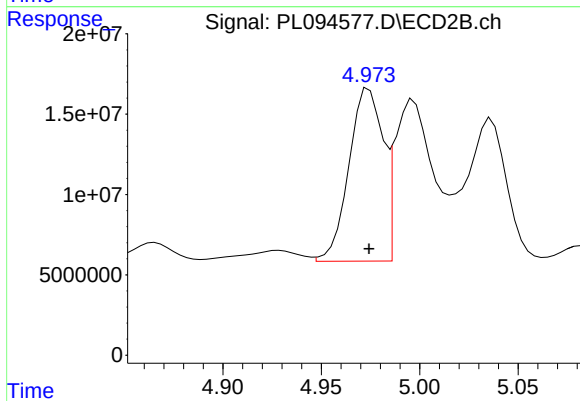

#25 Chlordane-3


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 129101145
Conc: 242.82 ng/ml

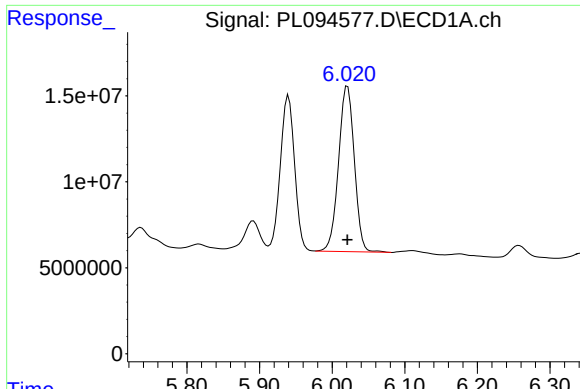

#26 Chlordane-4


R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 145326065
Conc: 258.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

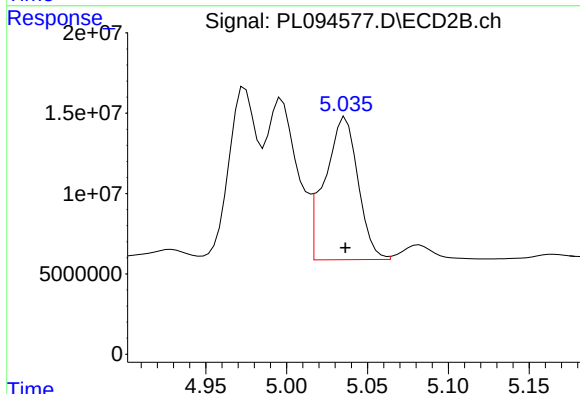


#26 Chlordane-4

R.T.: 5.036 min
Delta R.T.: 0.000 min
Response: 126856744
Conc: 243.55 ng/ml

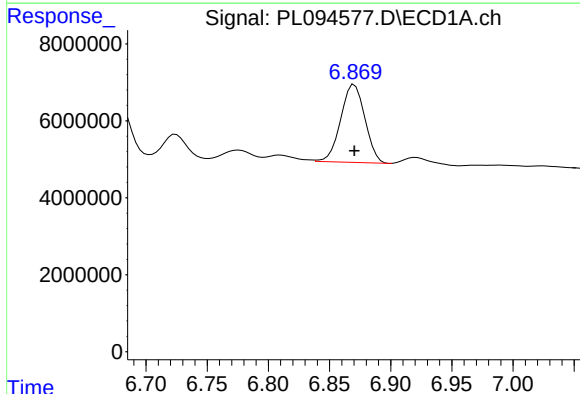


#27 Chlordane-5

R.T.: 6.870 min
Delta R.T.: 0.000 min
Response: 27856106
Conc: 262.95 ng/ml

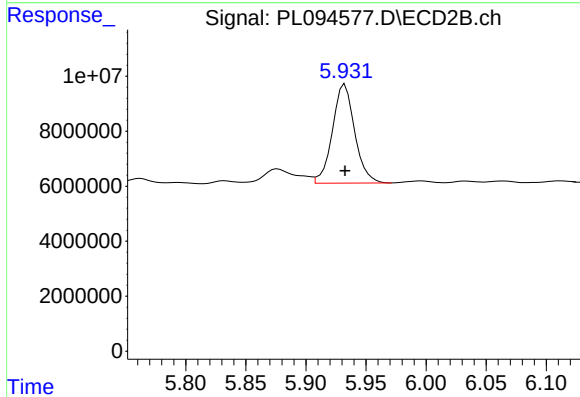

#27 Chlordane-5


R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 46547567
Conc: 239.83 ng/ml

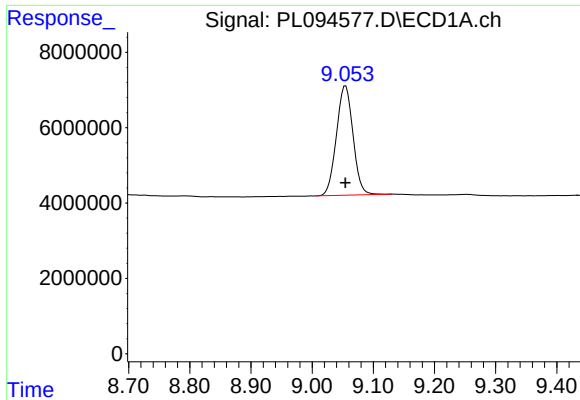

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 54683389
Conc: 26.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

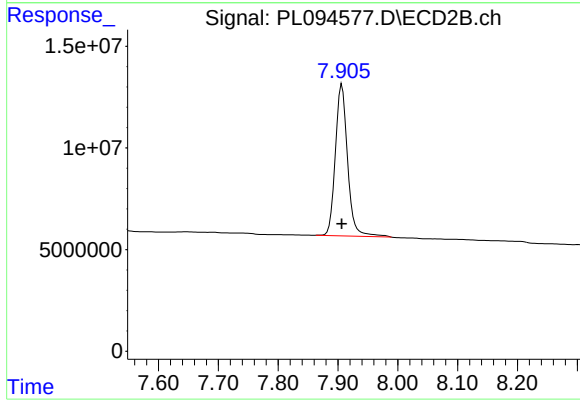

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 106195263
Conc: 25.93 ng/ml