

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
 Data File : PL094602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 21:14
 Operator : AR\AJ
 Sample : PB167086BS
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB167086BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 03:05:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.537	2.770	50139455	76589558	17.713	21.458
28) SA Decachlor...	9.052	7.905	43834752	86144891	20.800	21.326
Target Compounds						
23) Chlordane-1	4.698	3.766	28932608	30099230	206.486	199.291
24) Chlordane-2	5.228	4.342	30794412	37120362	203.525	210.209
25) Chlordane-3	5.938	4.973	107.0E6	110.3E6	214.000	207.415
26) Chlordane-4	6.019	5.035	127.4E6	110.5E6	216.337	212.358
27) Chlordane-5	6.867	5.929	25141143	39522880	228.928m	206.024m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
Data File : PL094602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 21:14
Operator : AR\AJ
Sample : PB167086BS
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB167086BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 03:05:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

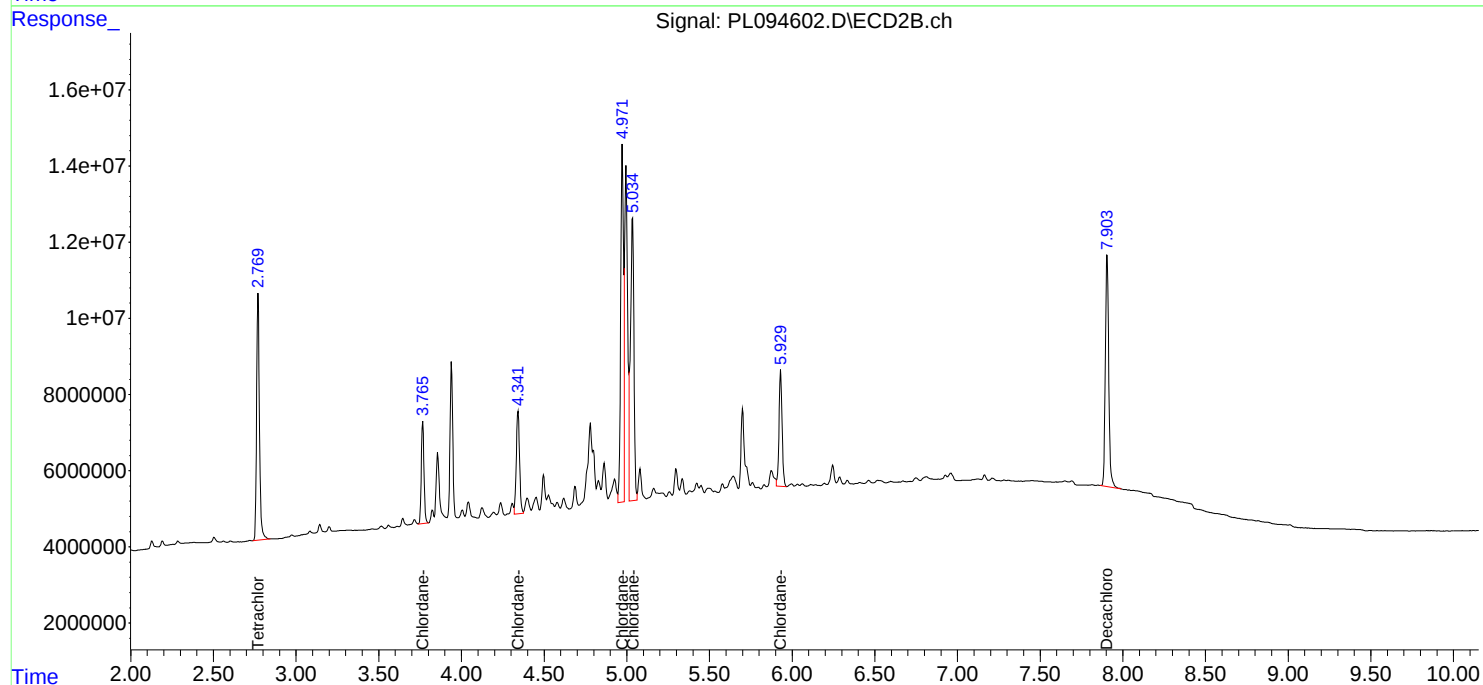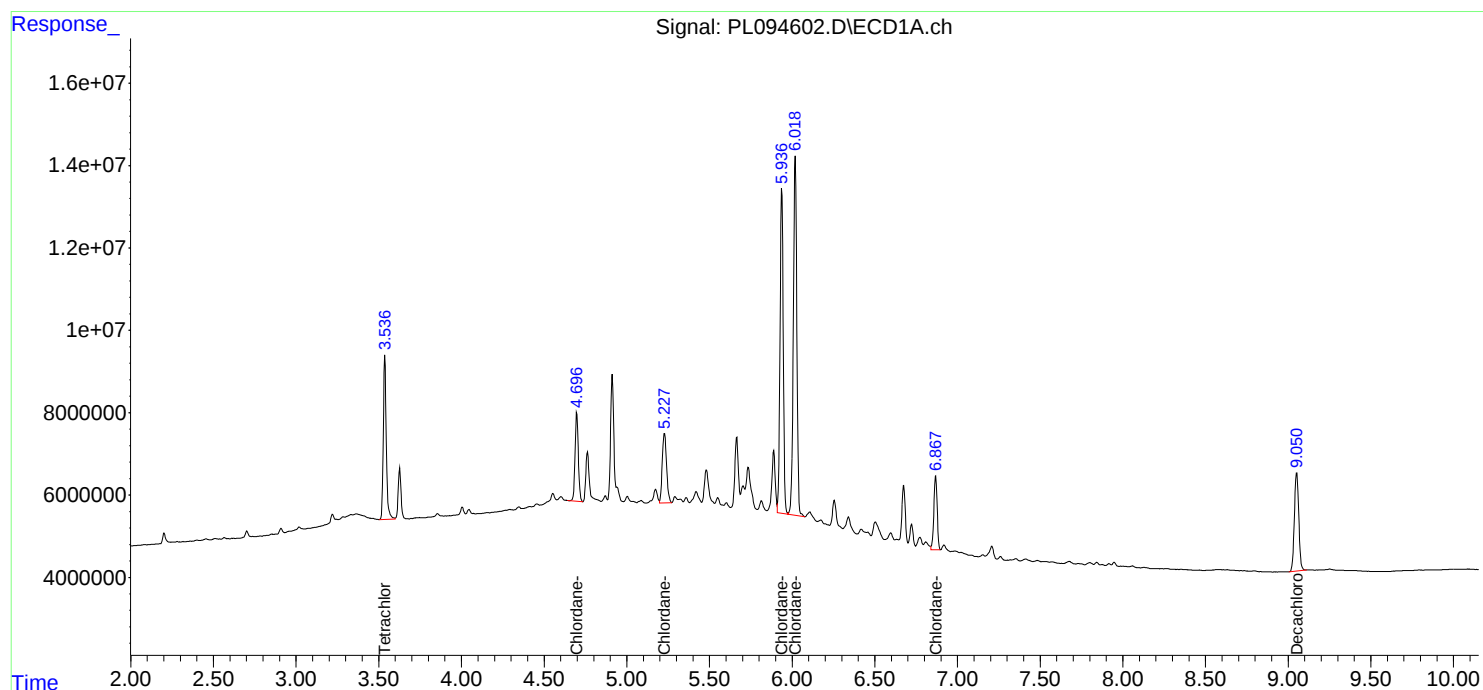


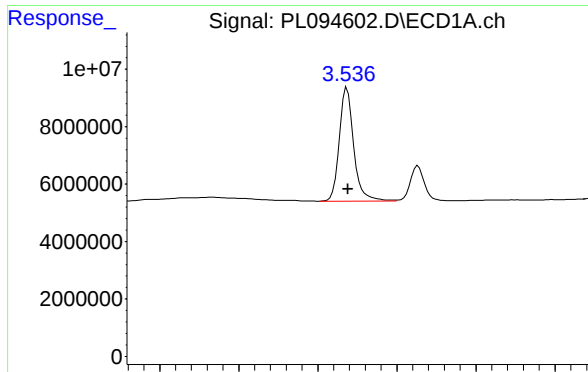

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: -0.001 min
Response: 50139455
Conc: 17.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167086BS

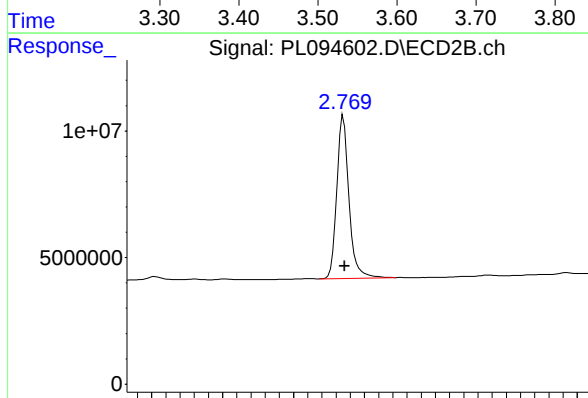


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.002 min
Response: 76589558
Conc: 21.46 ng/ml

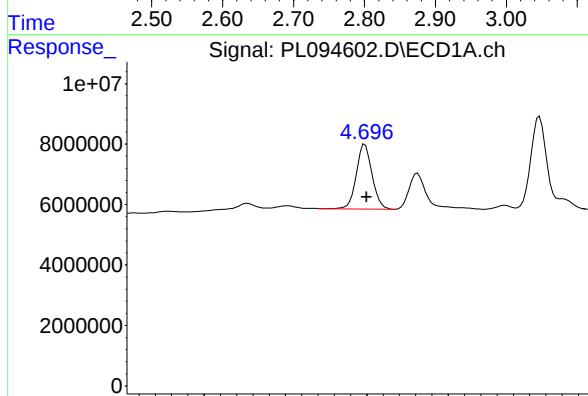


#23 Chlordane-1

R.T.: 4.698 min
Delta R.T.: -0.002 min
Response: 28932608
Conc: 206.49 ng/ml

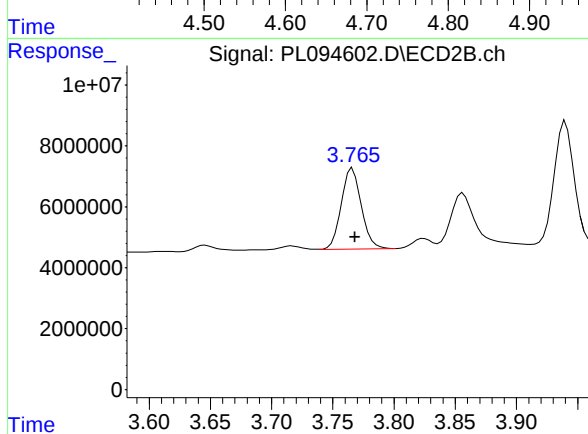

#23 Chlordane-1


R.T.: 3.766 min
Delta R.T.: -0.002 min
Response: 30099230
Conc: 199.29 ng/ml

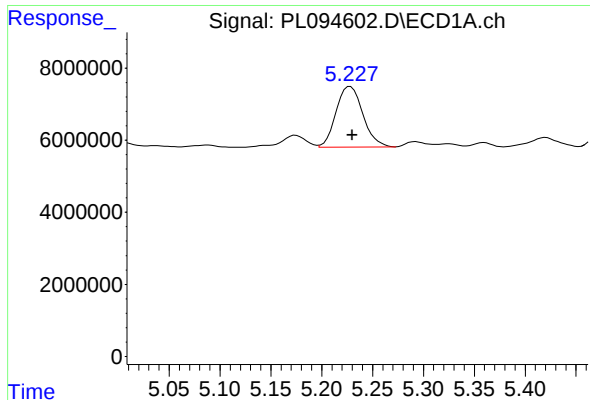

#24 Chlordane-2


R.T.: 5.228 min
Delta R.T.: -0.002 min
Response: 30794412
Conc: 203.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167086BS

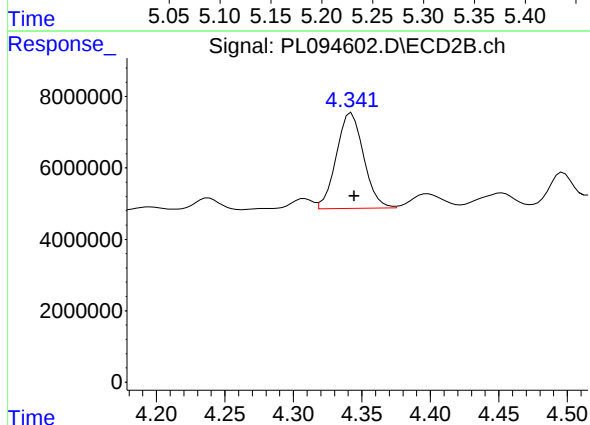


#24 Chlordane-2

R.T.: 4.342 min
Delta R.T.: -0.002 min
Response: 37120362
Conc: 210.21 ng/ml

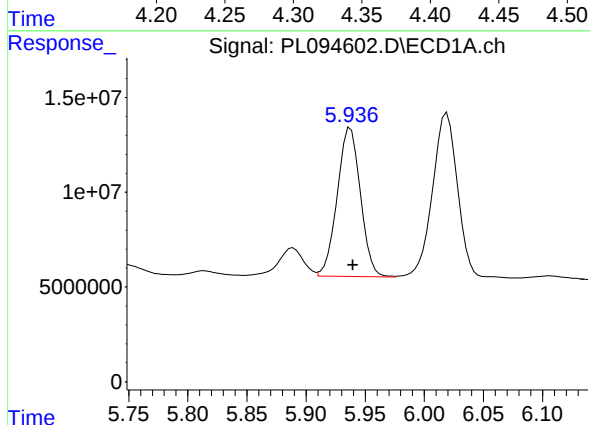


#25 Chlordane-3

R.T.: 5.938 min
Delta R.T.: -0.002 min
Response: 106961798
Conc: 214.00 ng/ml

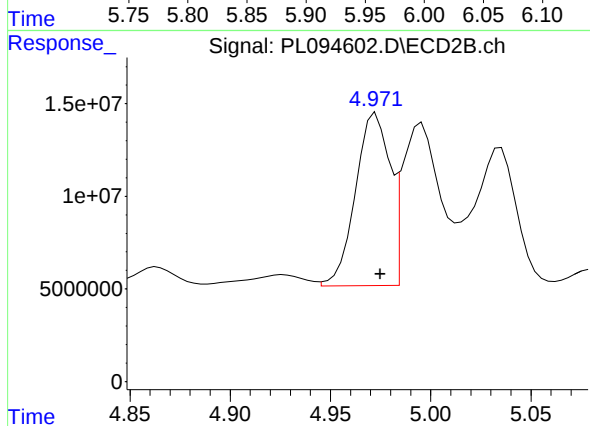

#25 Chlordane-3


R.T.: 4.973 min
Delta R.T.: -0.002 min
Response: 110344136
Conc: 207.41 ng/ml

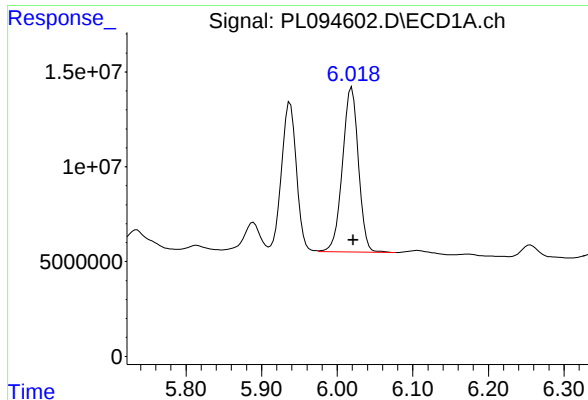

#26 Chlordane-4


R.T.: 6.019 min
Delta R.T.: -0.002 min
Response: 127442685
Conc: 216.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167086BS

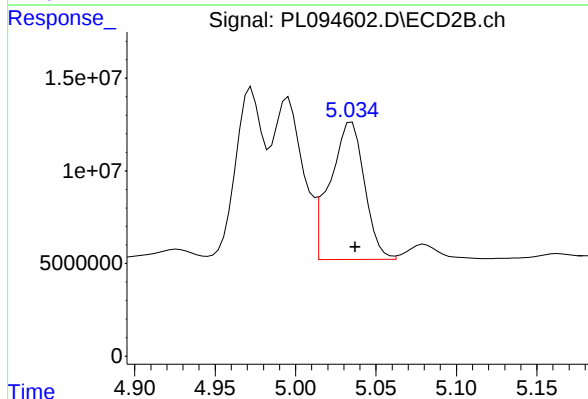


#26 Chlordane-4

R.T.: 5.035 min
Delta R.T.: -0.002 min
Response: 110545025
Conc: 212.36 ng/ml

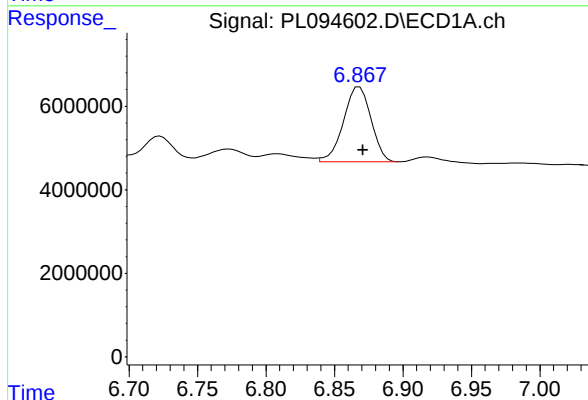


#27 Chlordane-5

R.T.: 6.867 min
Delta R.T.: -0.004 min
Response: 25141143
Conc: 228.93 ng/ml m

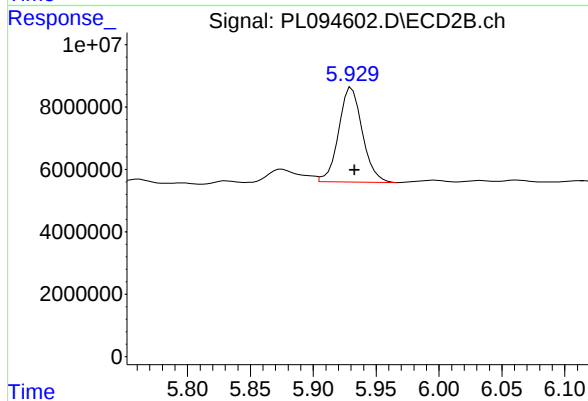

#27 Chlordane-5


R.T.: 5.929 min
Delta R.T.: -0.004 min
Response: 39522880
Conc: 206.02 ng/ml m

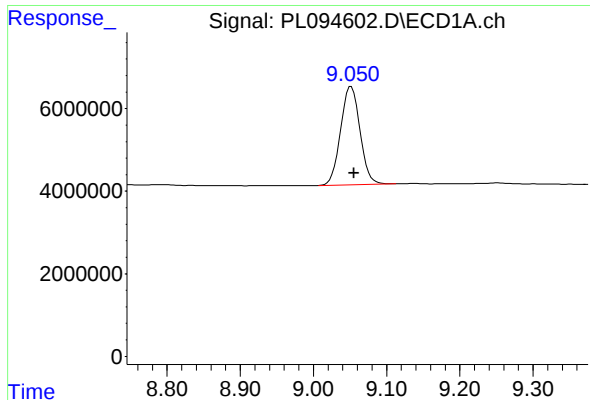

#28 Decachlorobiphenyl

R.T.: 9.052 min
Delta R.T.: -0.004 min
Response: 43834752
Conc: 20.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB167086BS

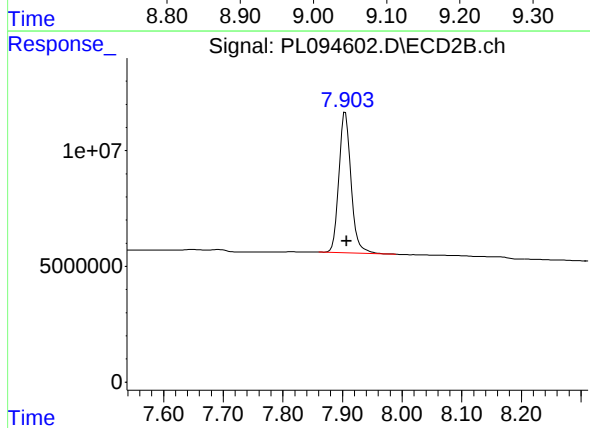

#28 Decachlorobiphenyl

R.T.: 7.905 min
Delta R.T.: -0.002 min
Response: 86144891
Conc: 21.33 ng/ml