

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031219\
 Data File : PL045715.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2019 08:51
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 01:12:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	4.329f	5.162	1938397	2128383	0.184	0.715 #
6) B	beta-BHC	4.329	0.000	1938397	0	0.452	N.D. #
8) B	Heptachlo...	0.000	5.846	0	8822779	N.D.	3.673 #
10) B	gamma-Chl...	5.282f	0.000	11332373	0	1.158	N.D. #
24)	Chlordane-2	0.000	5.427f	0	5360057	N.D.	44.360 #
25)	Chlordane-3	5.282f	0.000	11332373	0	9.880	N.D. #
27)	Chlordane-5	0.000	6.965	0	1050294	N.D.	11.562 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031219\
Data File : PL045715.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2019 08:51
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 01:12:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

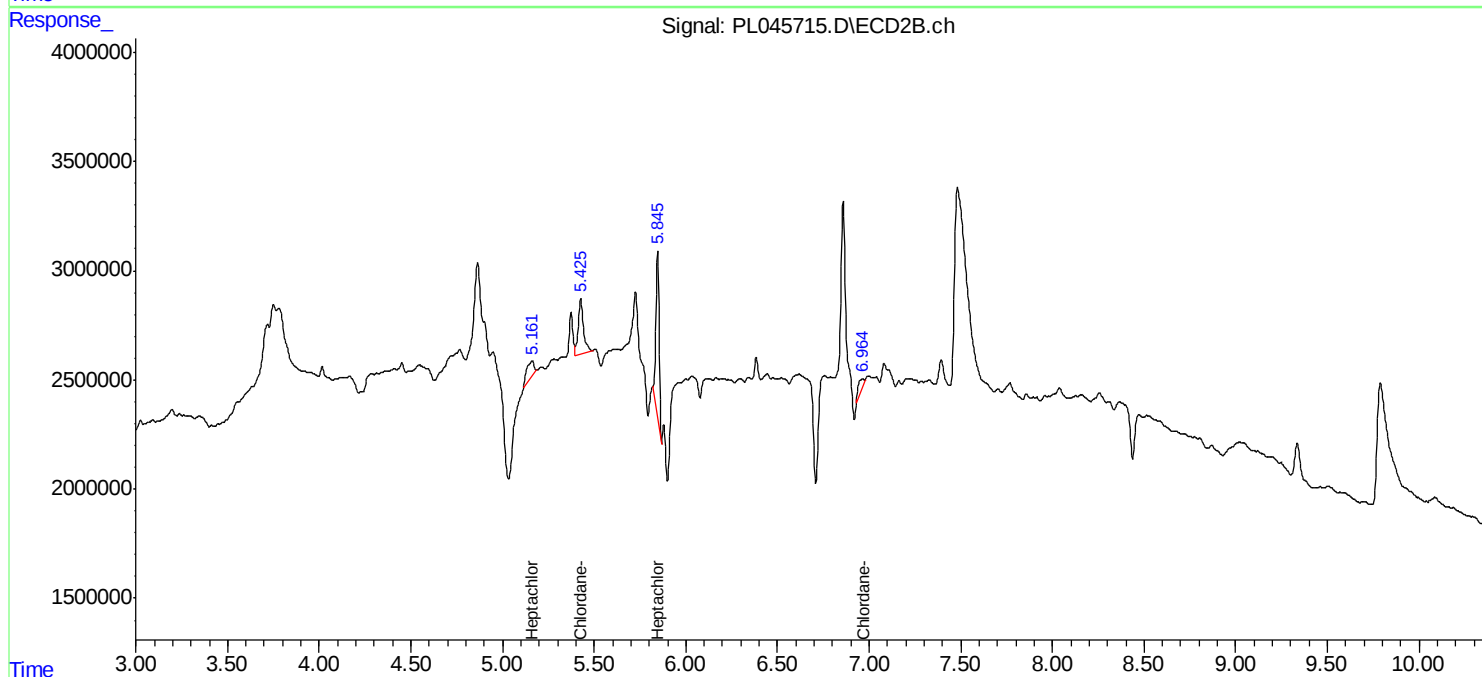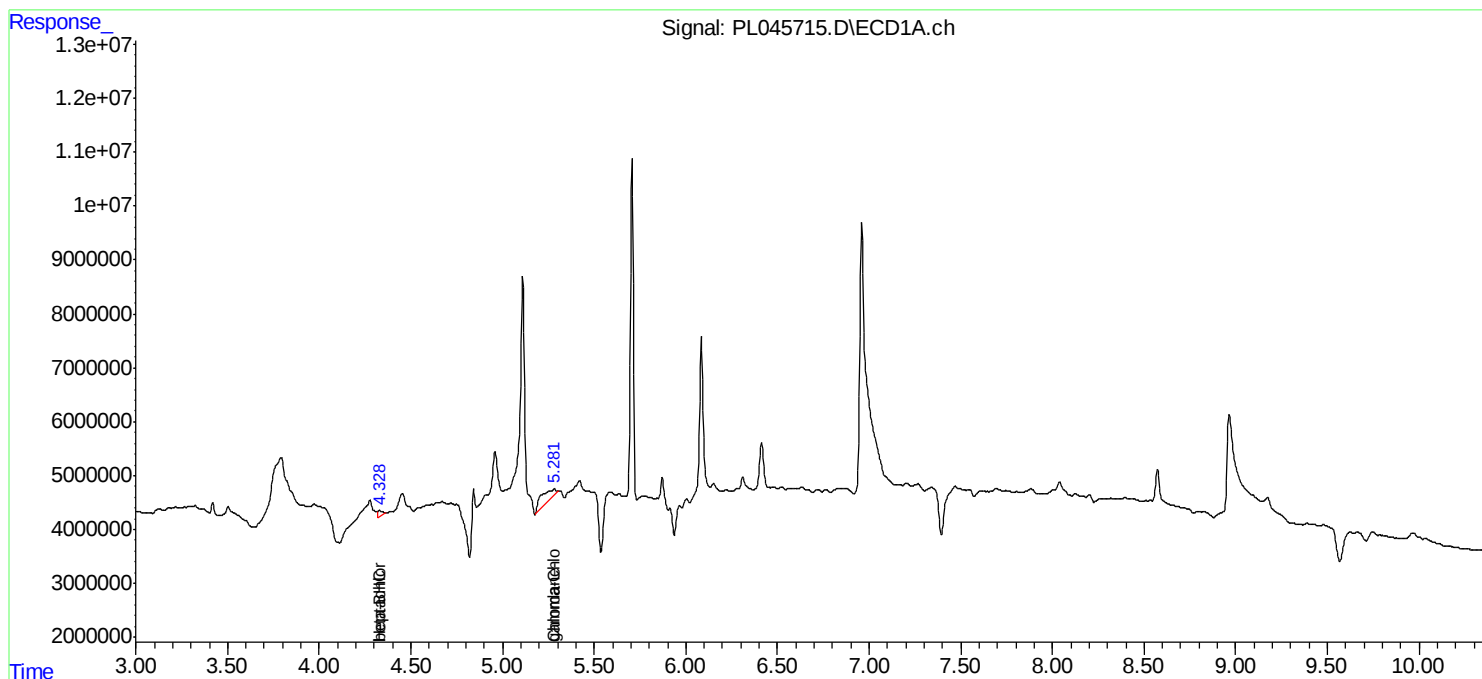


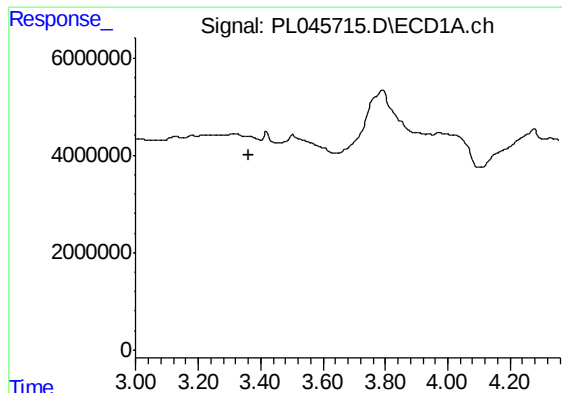

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

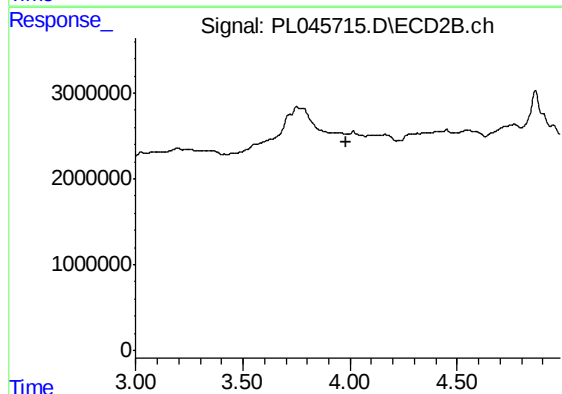


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.982 min
Response: 0
Conc: N.D.

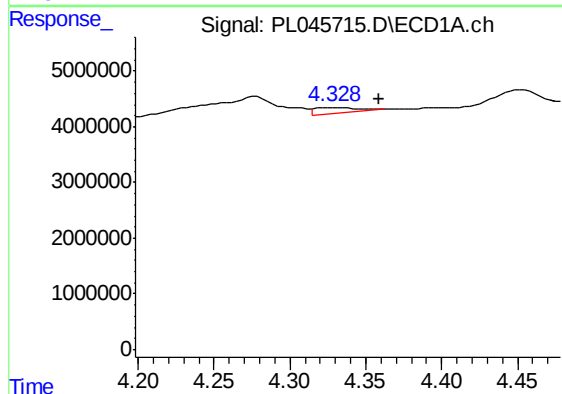


#4 Heptachlor

R.T.: 4.329 min
Delta R.T.: -0.030 min
Response: 1938397
Conc: 0.18 ng/ml

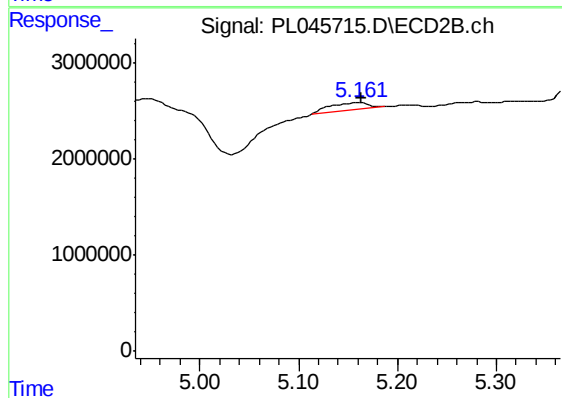

#4 Heptachlor


R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 2128383
Conc: 0.72 ng/ml

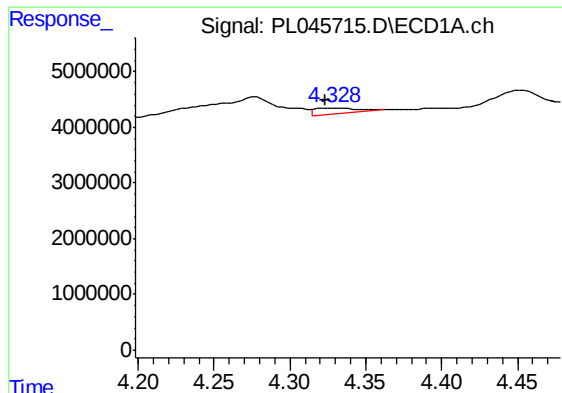

#6 beta-BHC


R.T.: 4.329 min
Delta R.T.: 0.005 min
Response: 1938397
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

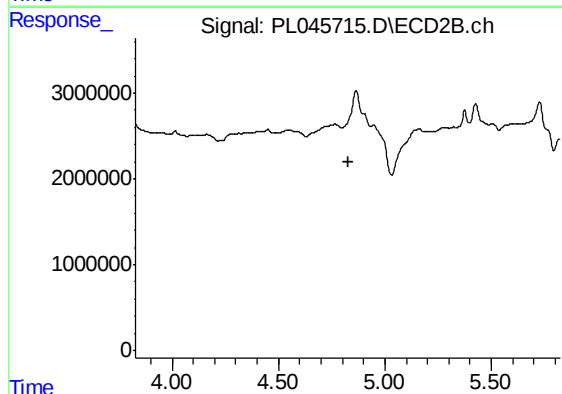


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.828 min
Response: 0
Conc: N.D.

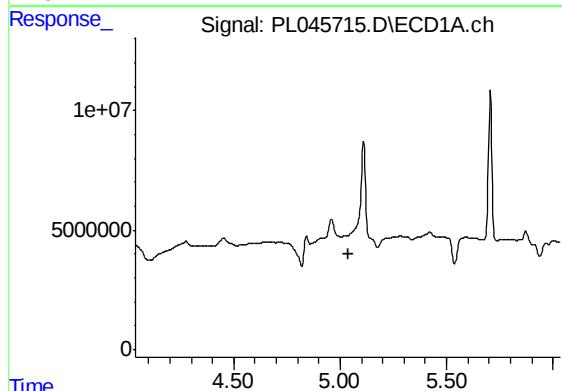


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

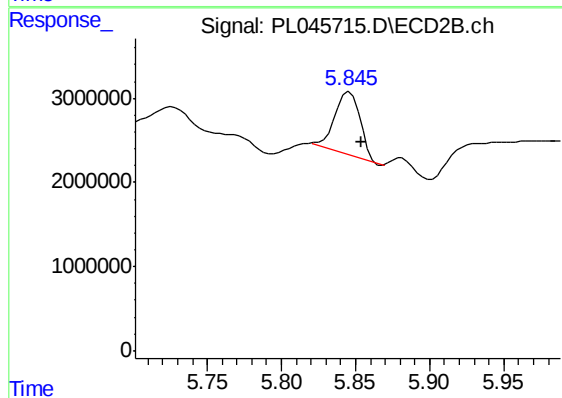

#8 Heptachlor epoxide


R.T.: 5.846 min
Delta R.T.: -0.008 min
Response: 8822779
Conc: 3.67 ng/ml

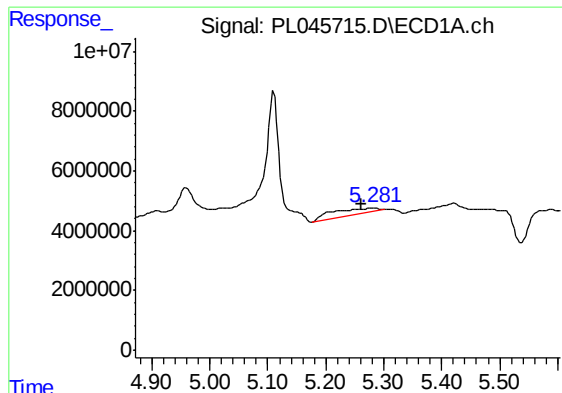

#10 gamma-Chlordane


R.T.: 5.282 min
Delta R.T.: 0.022 min
Response: 11332373
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

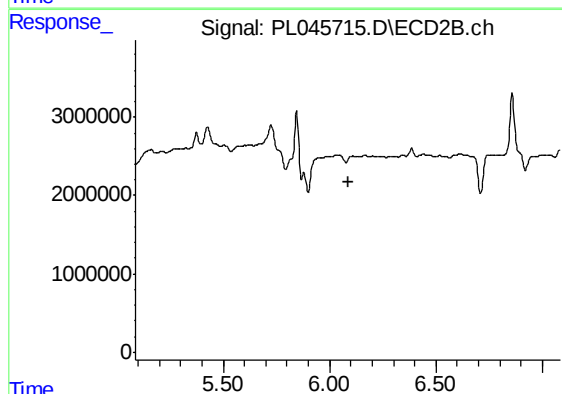


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

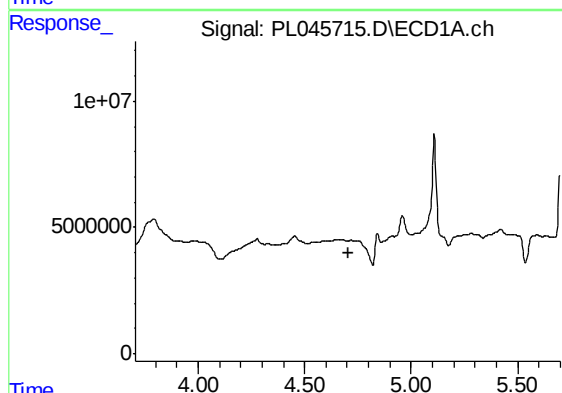


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

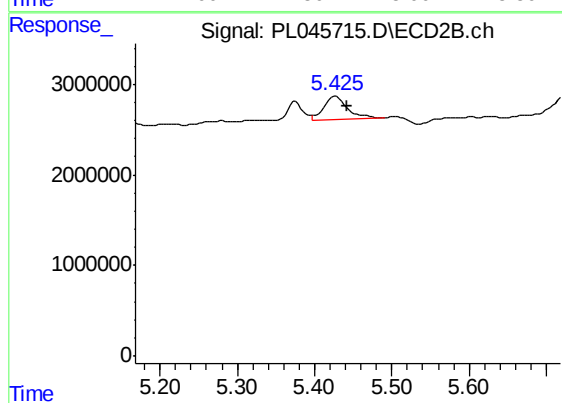

#24 Chlordane-2


R.T.: 5.427 min
Delta R.T.: -0.016 min
Response: 5360057
Conc: 44.36 ng/ml

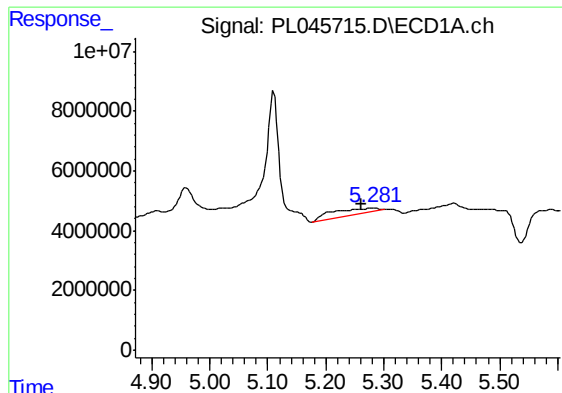

#25 Chlordane-3


R.T.: 5.282 min
Delta R.T.: 0.020 min
Response: 11332373
Conc: 9.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

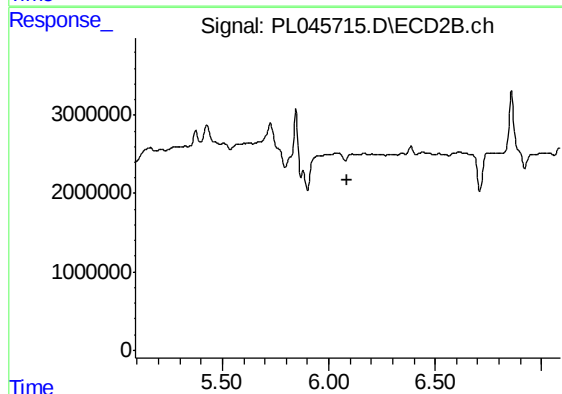


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

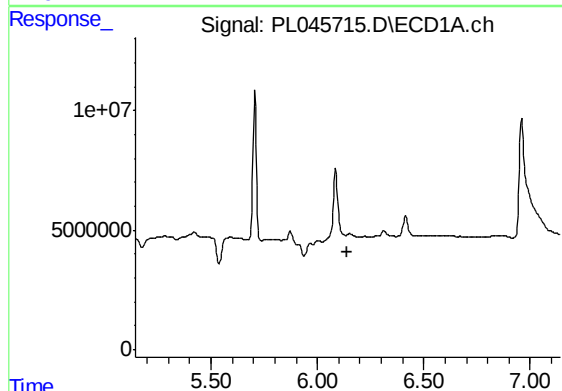


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.143 min
Response: 0
Conc: N.D.

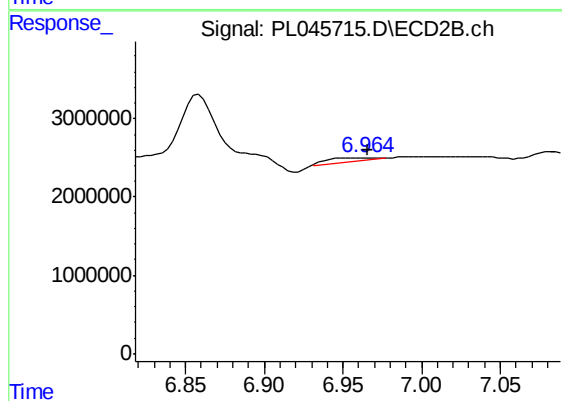

#27 Chlordane-5


R.T.: 6.965 min
Delta R.T.: -0.001 min
Response: 1050294
Conc: 11.56 ng/ml

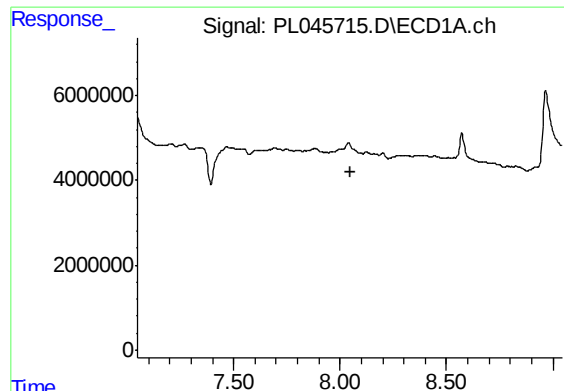

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

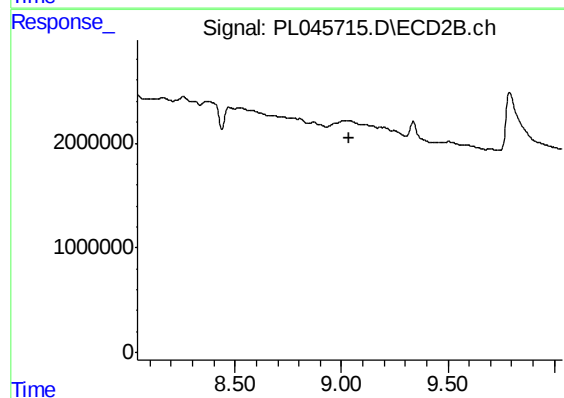

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.039 min
Response: 0
Conc: N.D.