

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031219\
 Data File : PL045732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2019 12:53
 Operator : AJ\SJ
 Sample : K1693-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 13:06:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	49584447	15353255	7.208	7.169
28)	SA Decachlor...	8.045	9.038	62361687	19204787	7.453	8.405
Target Compounds							
5)	MB Aldrin	0.000	5.465	0	1540475	N.D.	0.570 #
8)	B Heptachlo...	0.000	5.846	0	2059799	N.D.	0.858 #
10)	B gamma-Chl...	5.278f	6.088	10235300	583540	1.046	0.218 #
11)	B alpha-Chl...	0.000	6.162	0	4773422	N.D.	1.769 #
12)	B 4,4'-DDE	5.481	6.315	8346276	3528939	0.951	1.511 #
23)	Chlordane-1	4.211	0.000	5377842	0	15.961	N.D. #
24)	Chlordane-2	0.000	5.436	0	3485856	N.D.	28.849 #
25)	Chlordane-3	5.278f	6.088	10235300	583540	8.923	1.498 #
26)	Chlordane-4	0.000	6.162	0	4773422	N.D.	10.203 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031219\
Data File : PL045732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2019 12:53
Operator : AJ\SJ
Sample : K1693-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 13:06:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

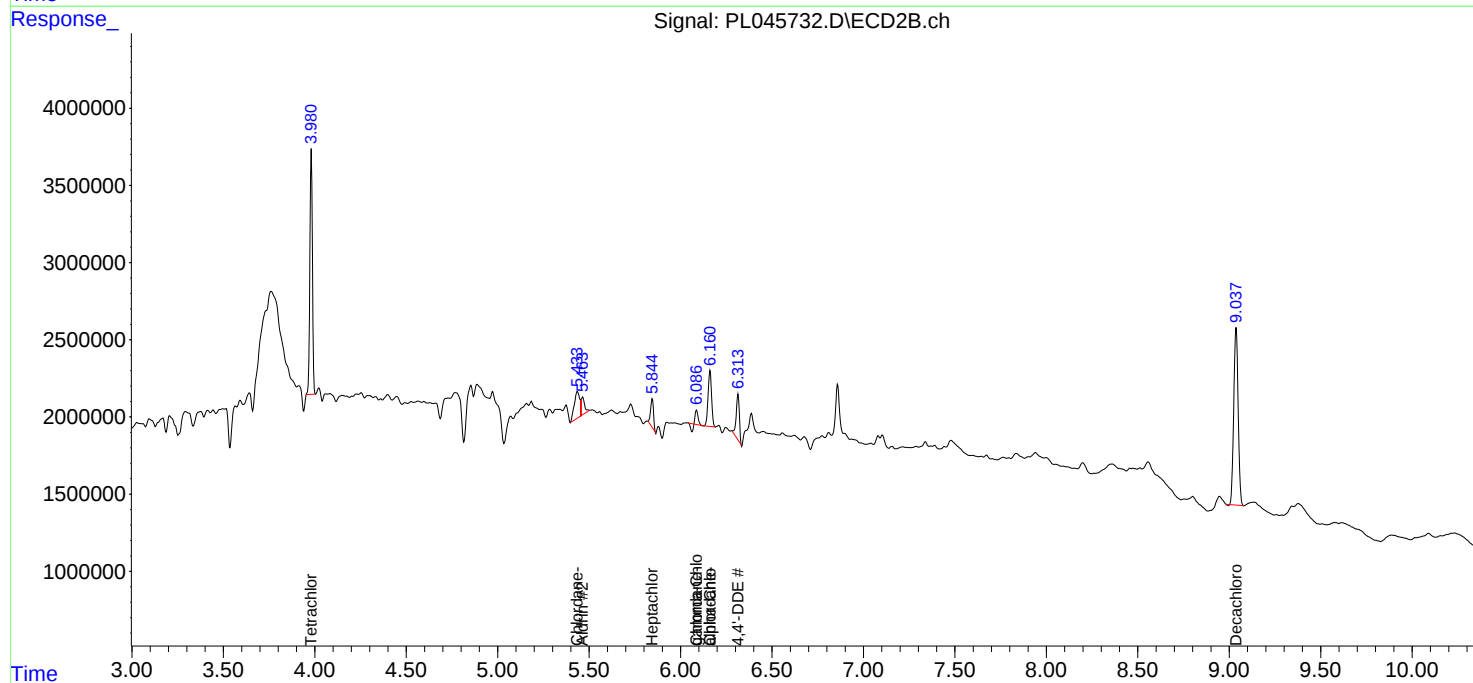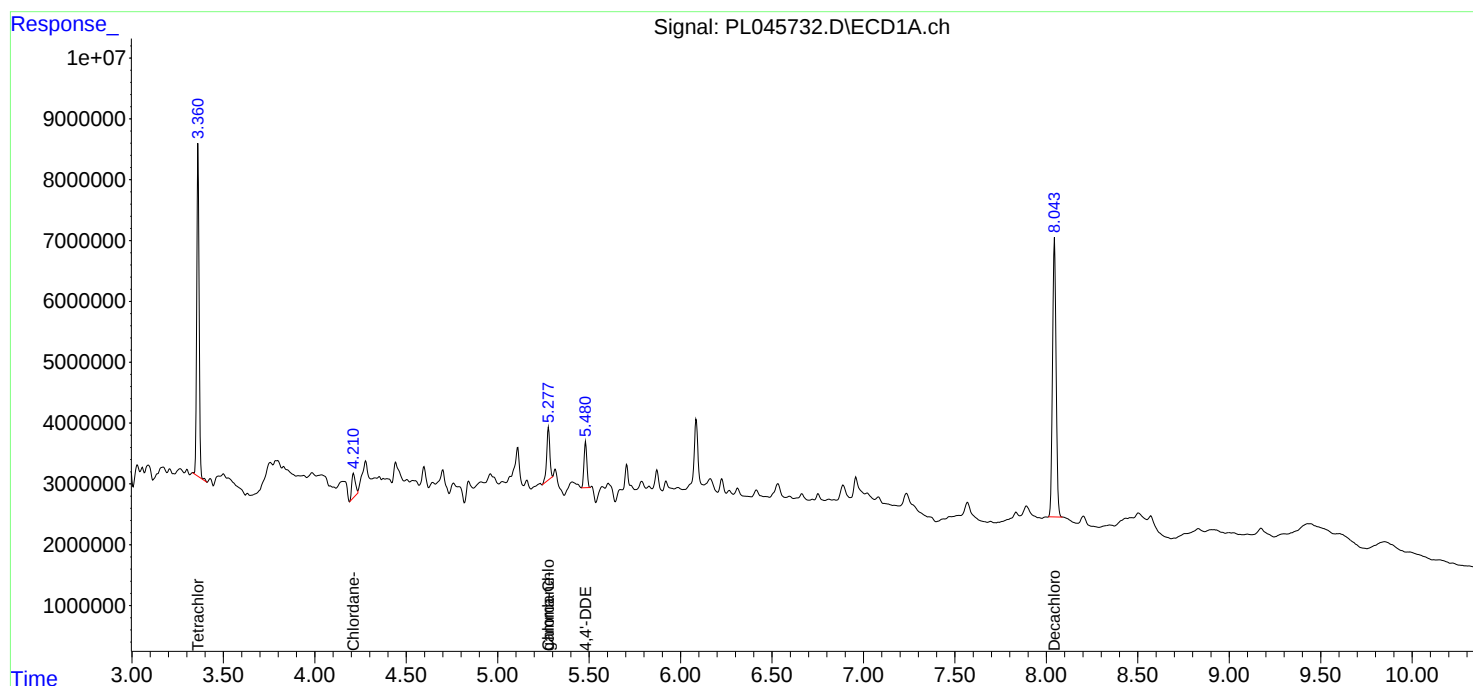


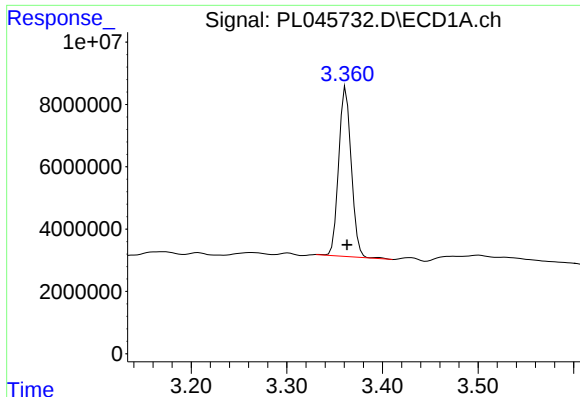

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: -0.001 min
Response: 49584447
Conc: 7.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

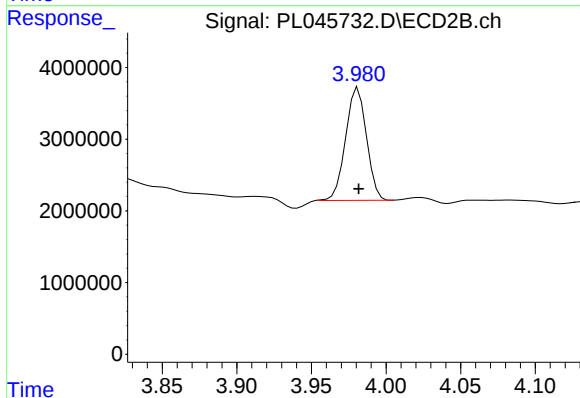


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 15353255
Conc: 7.17 ng/ml

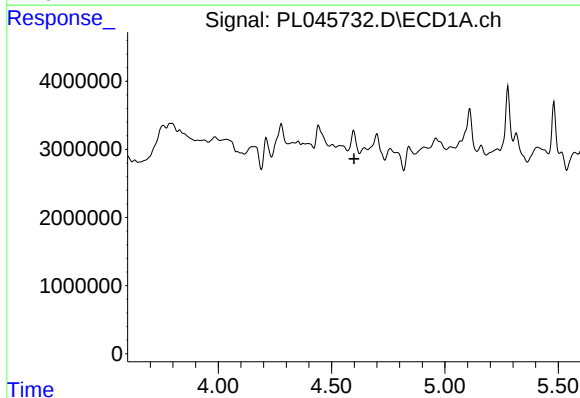


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.599 min
Response: 0
Conc: N.D.

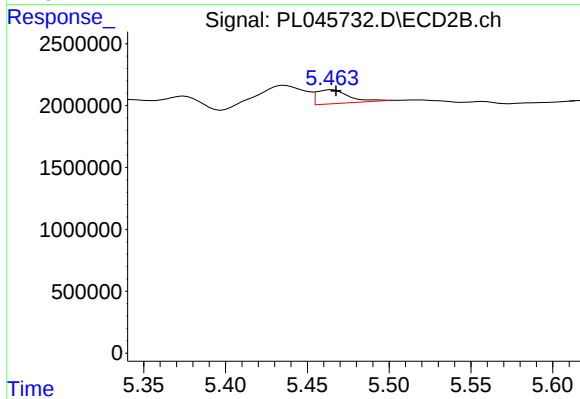

#5 Aldrin


R.T.: 5.465 min
Delta R.T.: -0.002 min
Response: 1540475
Conc: 0.57 ng/ml

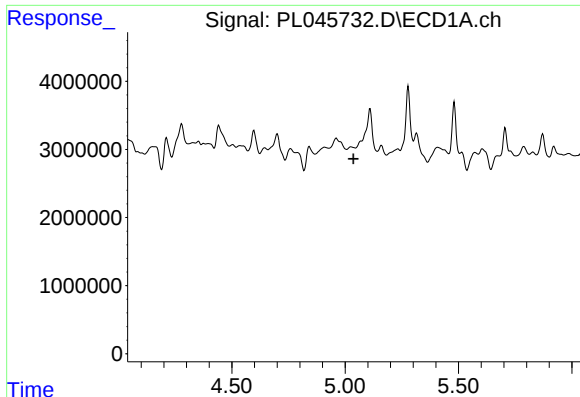

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

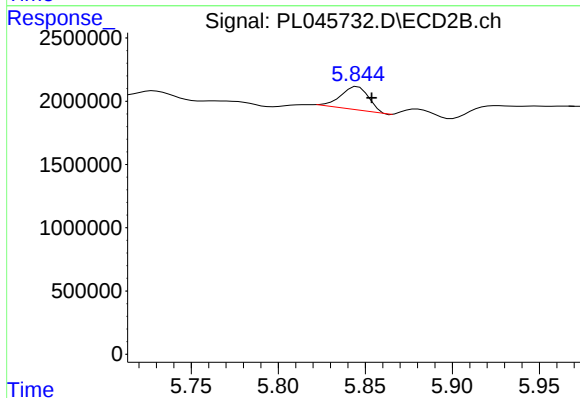


#8 Heptachlor epoxide

R.T.: 5.846 min
Delta R.T.: -0.008 min
Response: 2059799
Conc: 0.86 ng/ml

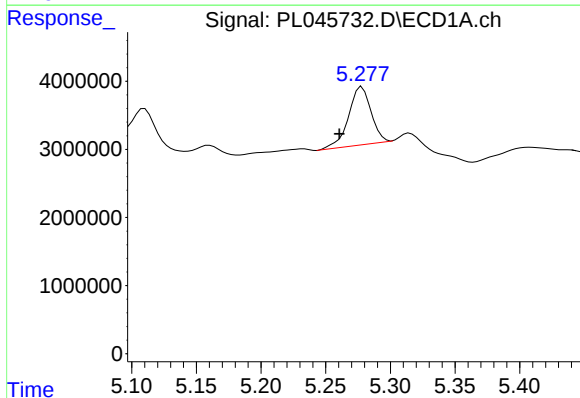


#10 gamma-Chlordane

R.T.: 5.278 min
Delta R.T.: 0.018 min
Response: 10235300
Conc: 1.05 ng/ml

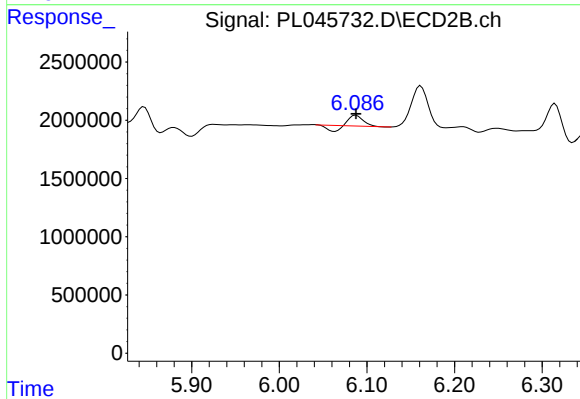

#10 gamma-Chlordane


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 583540
Conc: 0.22 ng/ml

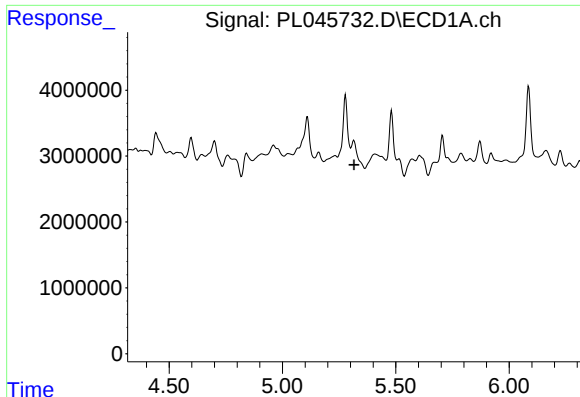

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

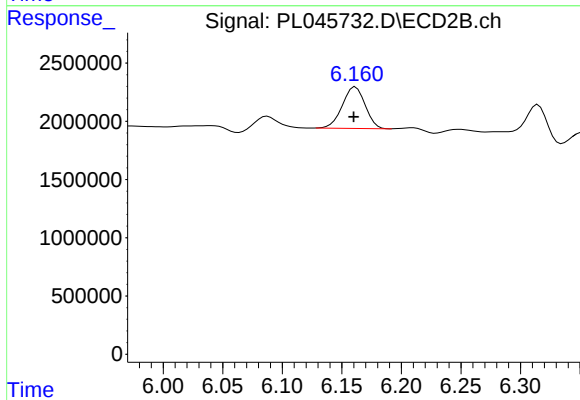


#11 alpha-Chlordane

R.T.: 6.162 min
Delta R.T.: 0.002 min
Response: 4773422
Conc: 1.77 ng/ml

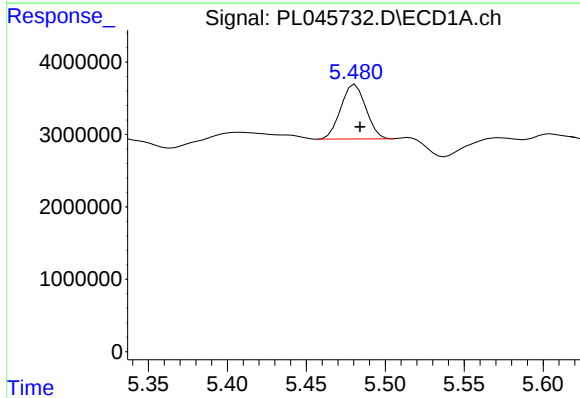


#12 4,4'-DDE

R.T.: 5.481 min
Delta R.T.: -0.003 min
Response: 8346276
Conc: 0.95 ng/ml

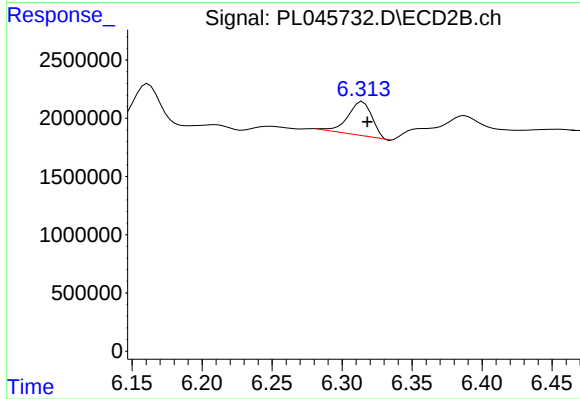

#12 4,4'-DDE


R.T.: 6.315 min
Delta R.T.: -0.003 min
Response: 3528939
Conc: 1.51 ng/ml

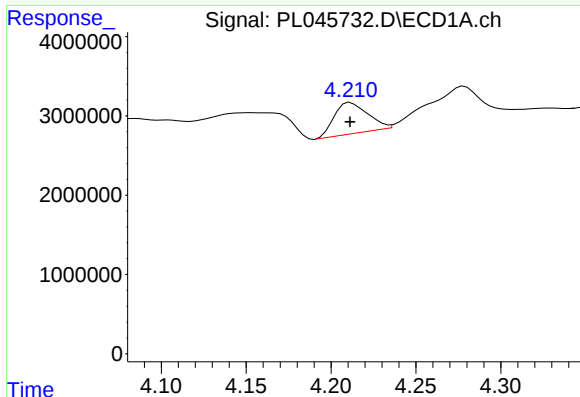

#23 Chlordane-1


R.T.: 4.211 min
Delta R.T.: 0.000 min
Response: 5377842
Conc: 15.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

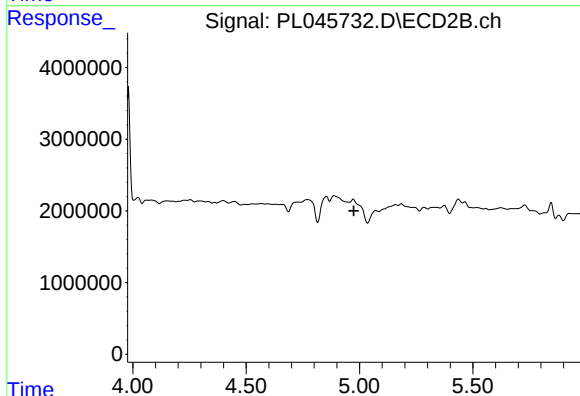


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

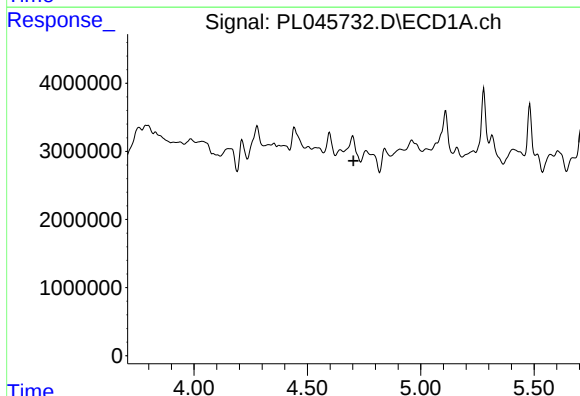


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

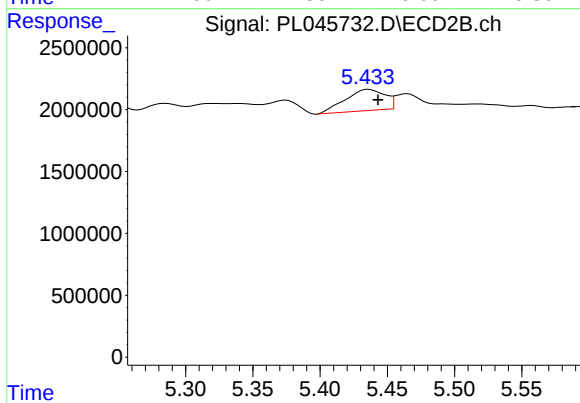

#24 Chlordane-2


R.T.: 5.436 min
Delta R.T.: -0.007 min
Response: 3485856
Conc: 28.85 ng/ml

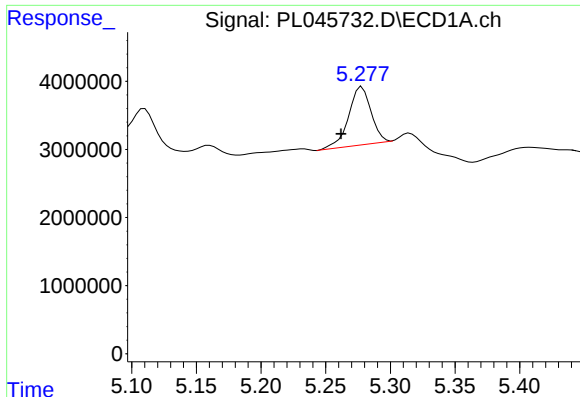

#25 Chlordane-3


R.T.: 5.278 min
Delta R.T.: 0.016 min
Response: 10235300
Conc: 8.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

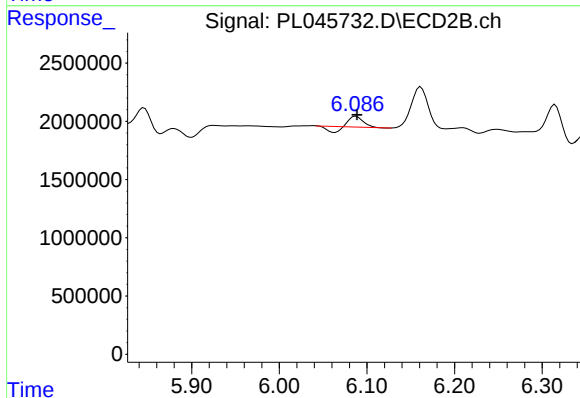


#25 Chlordane-3

R.T.: 6.088 min
Delta R.T.: -0.001 min
Response: 583540
Conc: 1.50 ng/ml

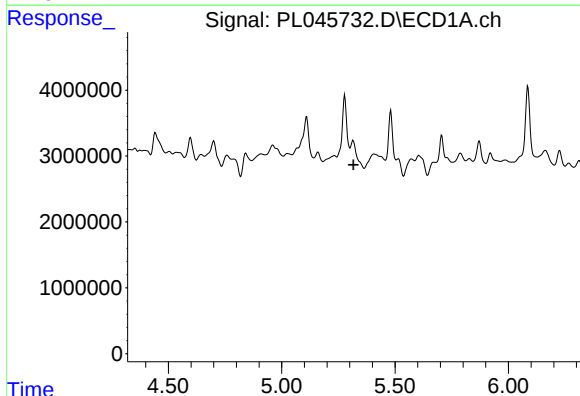


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.317 min
Response: 0
Conc: N.D.

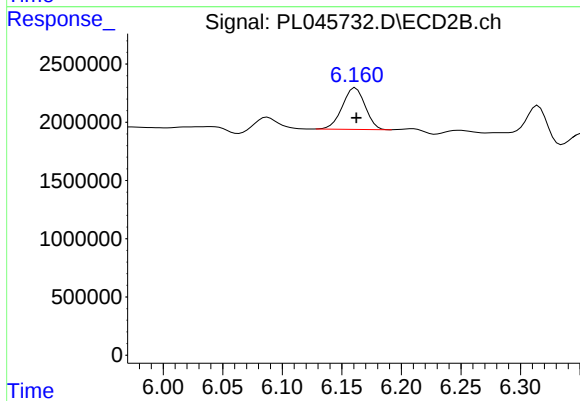

#26 Chlordane-4


R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 4773422
Conc: 10.20 ng/ml

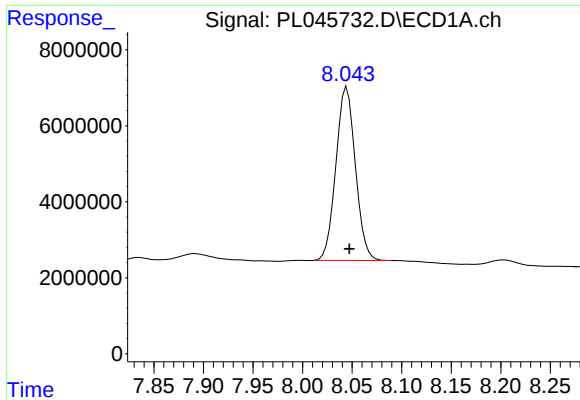

#28 Decachlorobiphenyl

R.T.: 8.045 min
Delta R.T.: -0.003 min
Response: 62361687
Conc: 7.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

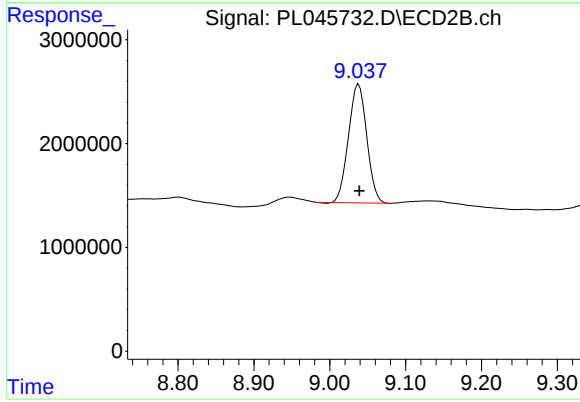

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 19204787
Conc: 8.40 ng/ml