

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031219\
 Data File : PL045776.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2019 23:44
 Operator : AJ\SJ
 Sample : K1844-09
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TOTE-1-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 01:27:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	16697141	5410843	2.427	2.527
28)	SA Decachlor...	8.043	9.037	7721954	2313712	0.923	1.013
Target Compounds							
10)	B gamma-Chl...	5.282f	6.094	16115392	1268516	1.647	0.473 #
25)	Chlordane-3	5.282f	6.094	16115392	1268516	14.050	3.256 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031219\
Data File : PL045776.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2019 23:44
Operator : AJ\SJ
Sample : K1844-09
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TOTE-1-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 01:27:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

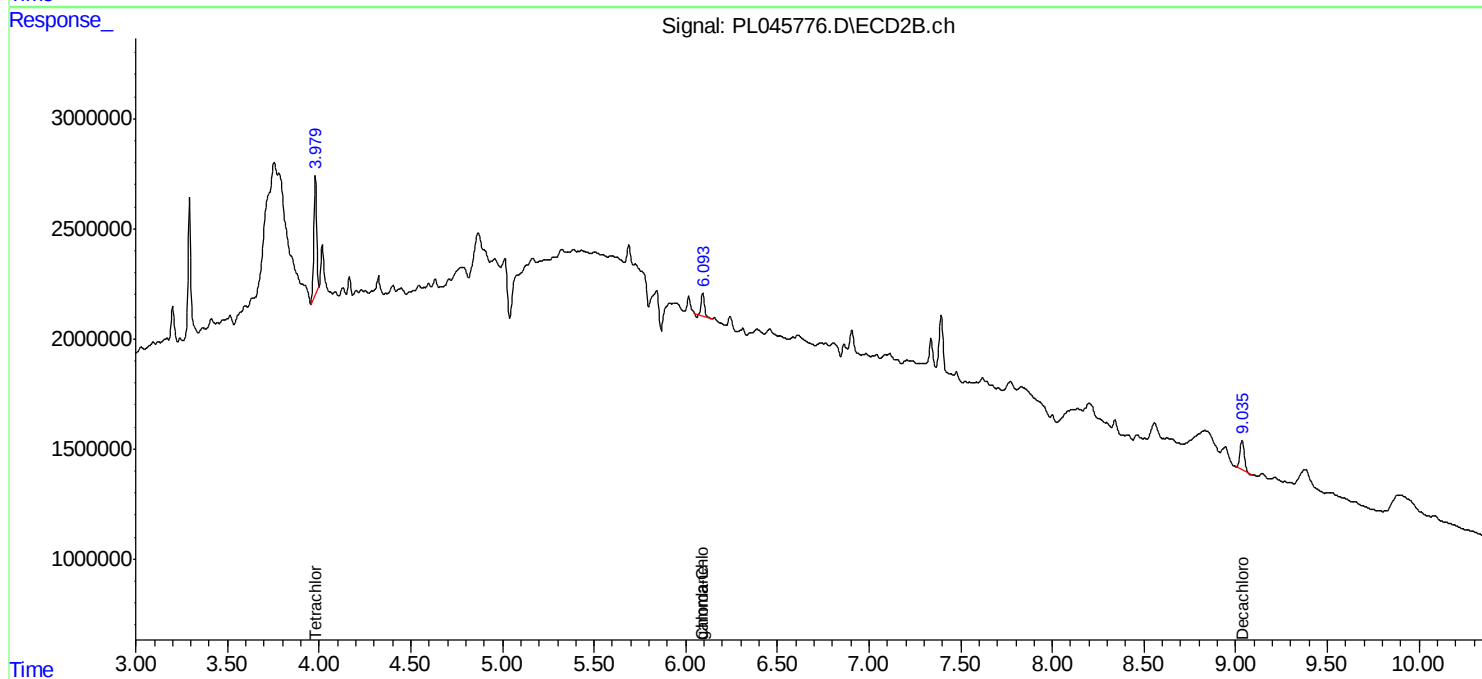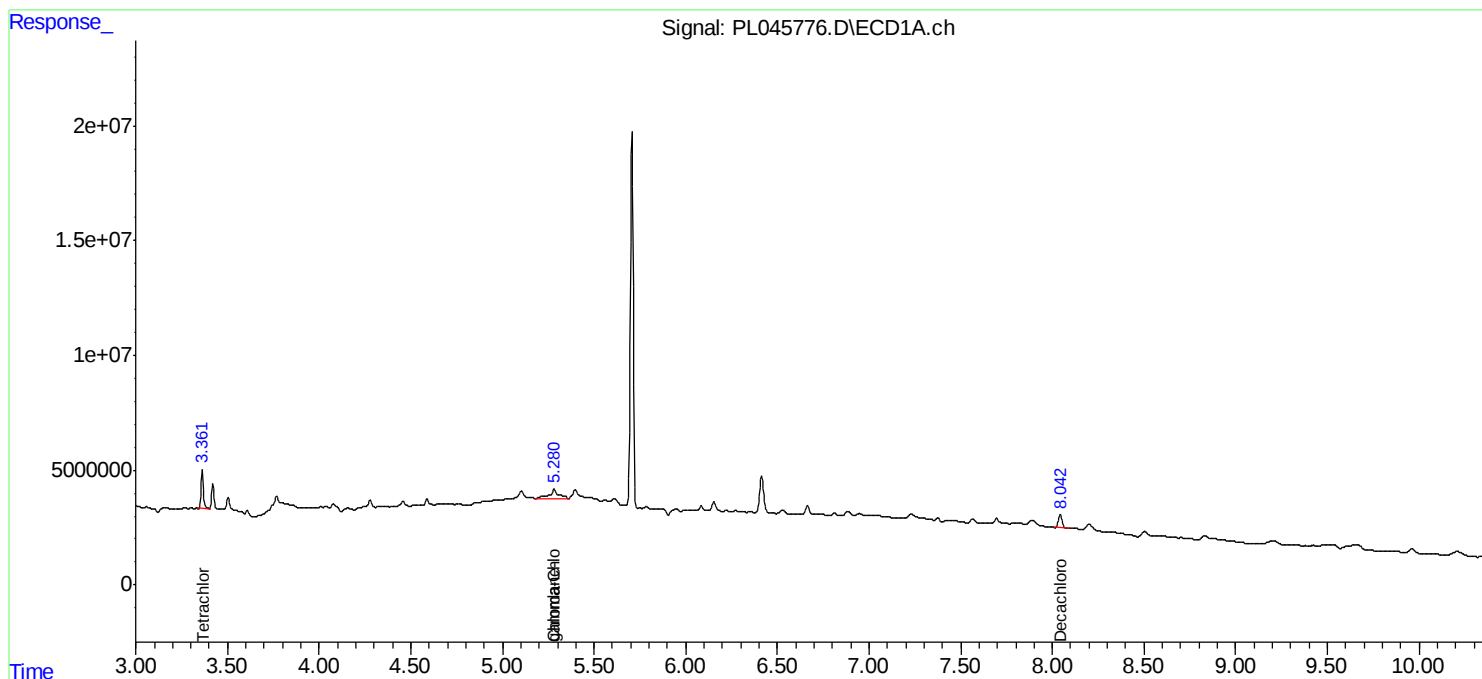


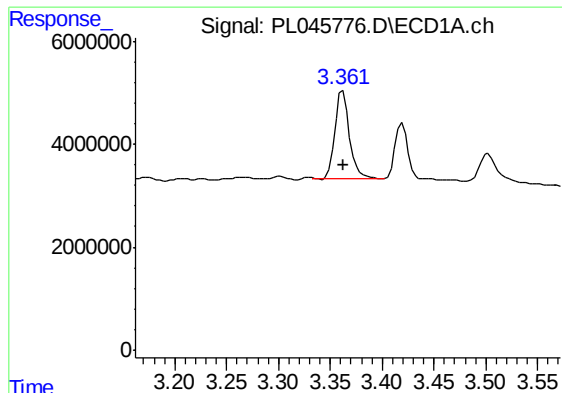

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 16697141
Conc: 2.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
TOTE-1-3

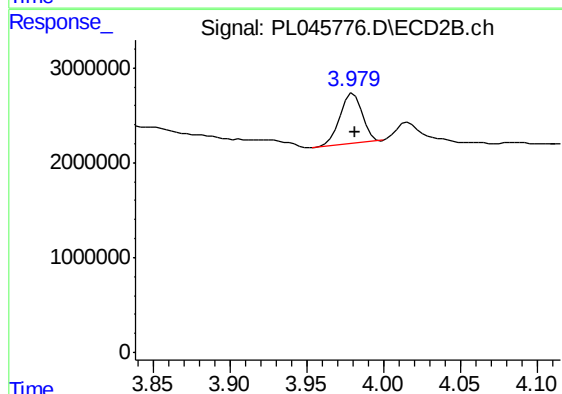


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 5410843
Conc: 2.53 ng/ml

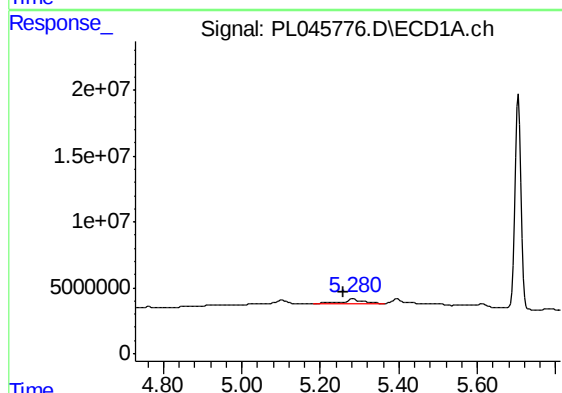


#10 gamma-Chlordane

R.T.: 5.282 min
Delta R.T.: 0.021 min
Response: 16115392
Conc: 1.65 ng/ml

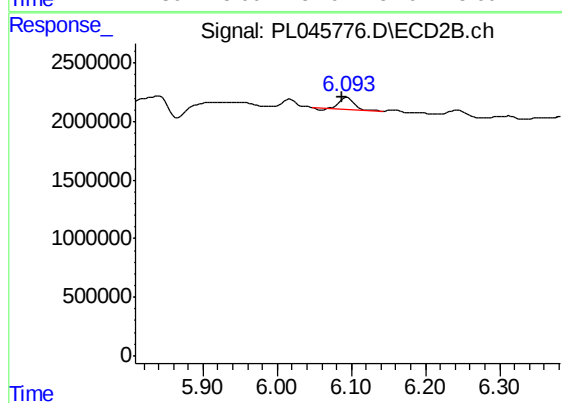

#10 gamma-Chlordane


R.T.: 6.094 min
Delta R.T.: 0.007 min
Response: 1268516
Conc: 0.47 ng/ml

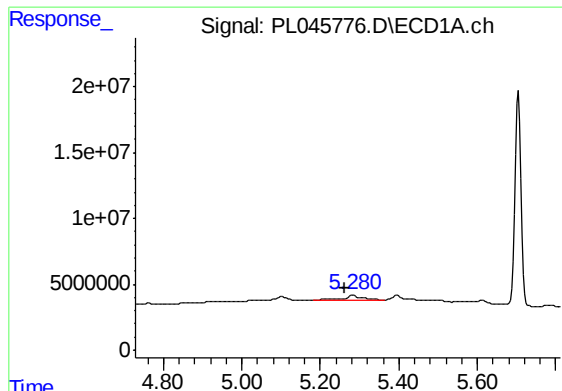

#25 Chlordane-3


R.T.: 5.282 min
Delta R.T.: 0.020 min
Response: 16115392
Conc: 14.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
TOTE-1-3

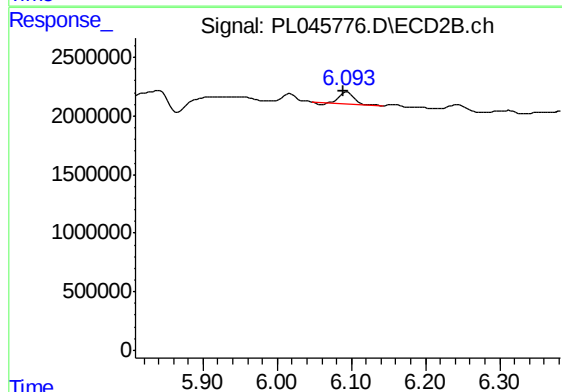


#25 Chlordane-3

R.T.: 6.094 min
Delta R.T.: 0.006 min
Response: 1268516
Conc: 3.26 ng/ml

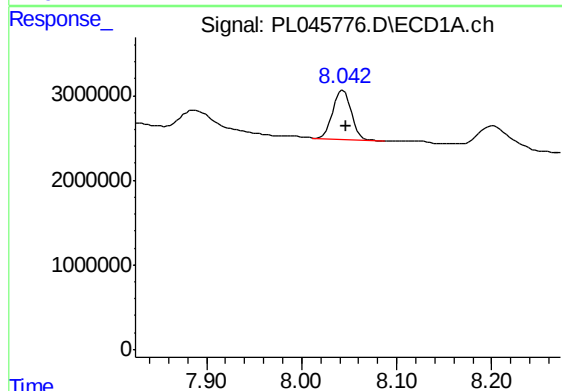

#28 Decachlorobiphenyl

R.T.: 8.043 min
Delta R.T.: -0.004 min
Response: 7721954
Conc: 0.92 ng/ml

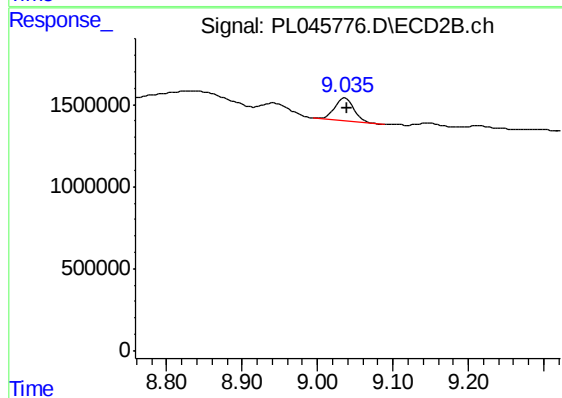

#28 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 2313712
Conc: 1.01 ng/ml