

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031219\
 Data File : PL045800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2019 06:07
 Operator : AJ\SJ
 Sample : K1849-07
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 C135-CON

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 08:01:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.363	3.981	127.4E6	40628229	18.524	18.972
28) SA Decachlor...	8.043	9.038	148.9E6	46223540	17.799	20.230
Target Compounds						
9) A Endosulfan I	0.000	6.237f	0	1581965	N.D.	0.635 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031219\
Data File : PL045800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2019 06:07
Operator : AJ\SJ
Sample : K1849-07
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
C135-CON

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 08:01:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

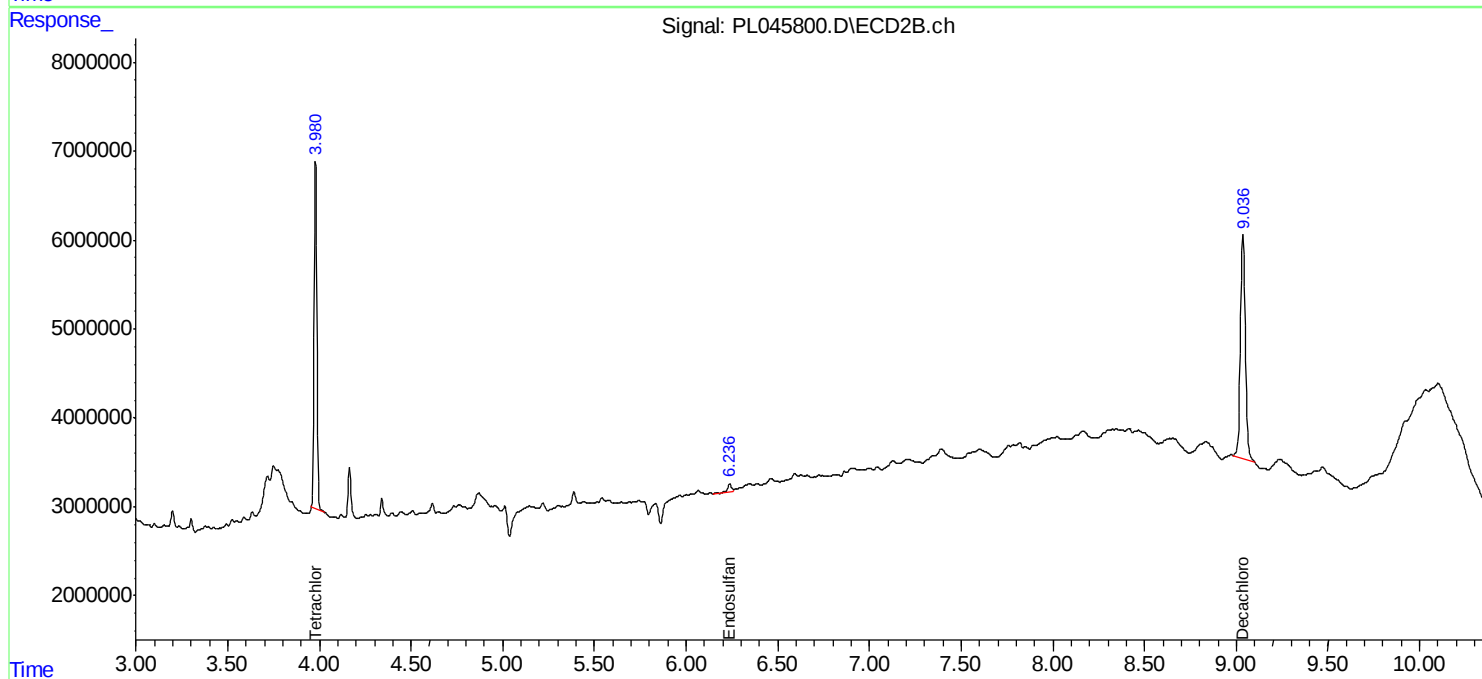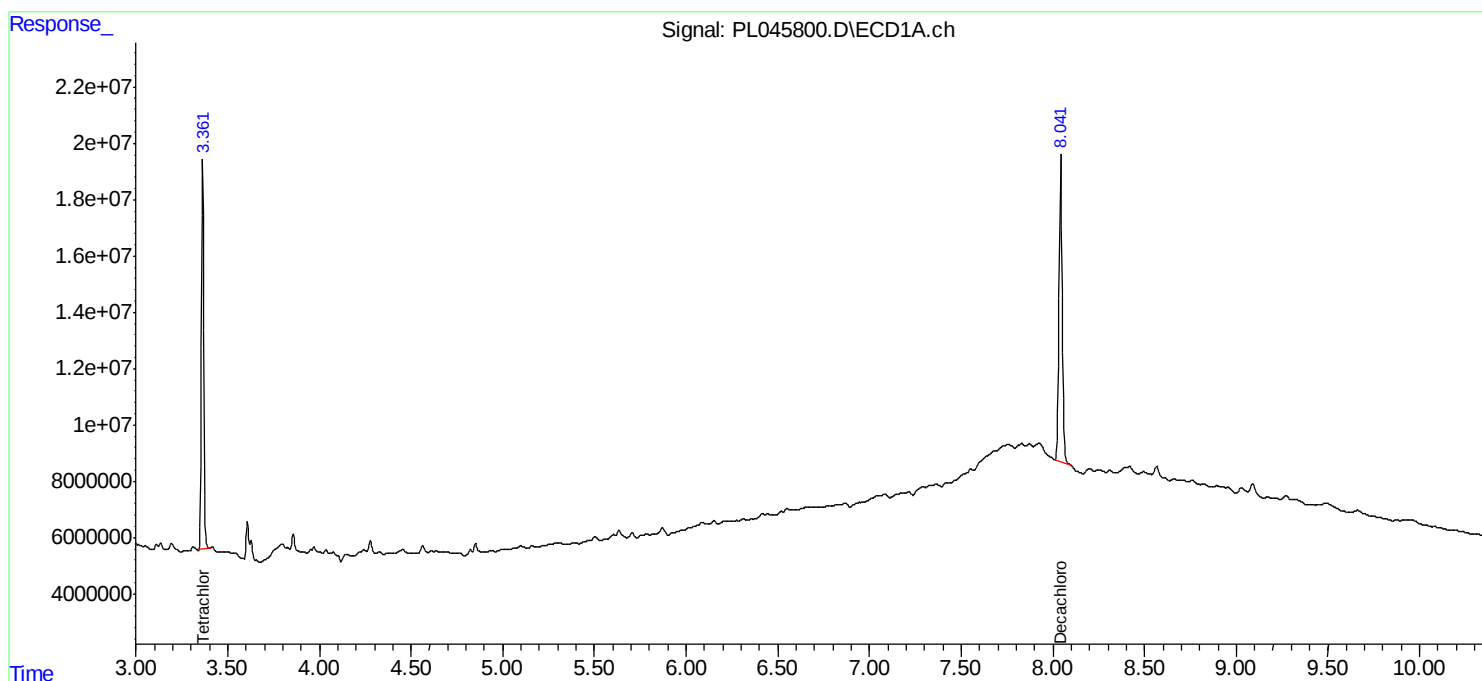


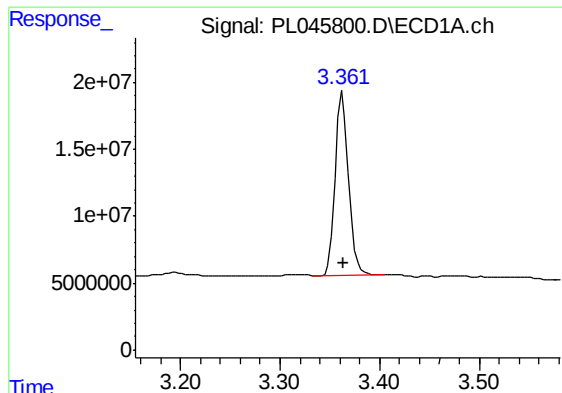

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 127428550
Conc: 18.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
C135-CON

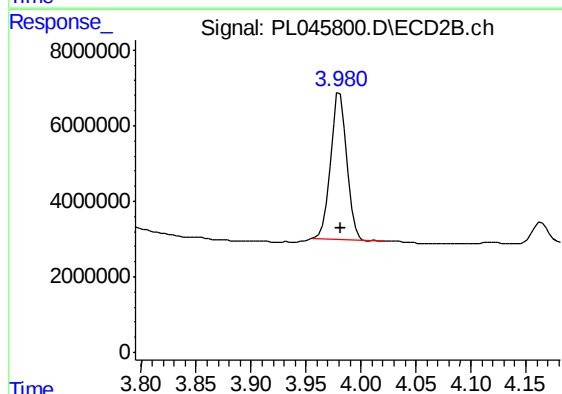


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 40628229
Conc: 18.97 ng/ml

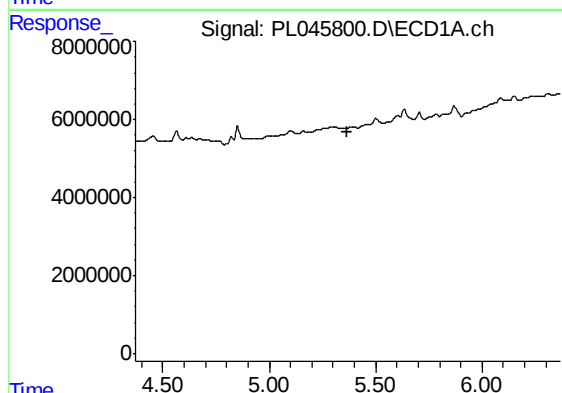


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.369 min
Response: 0
Conc: N.D.

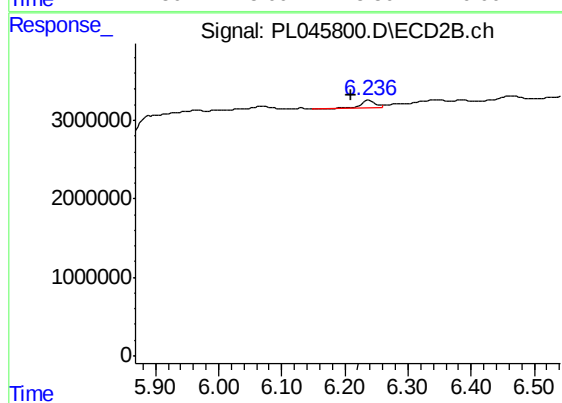

#9 Endosulfan I


R.T.: 6.237 min
Delta R.T.: 0.027 min
Response: 1581965
Conc: 0.64 ng/ml

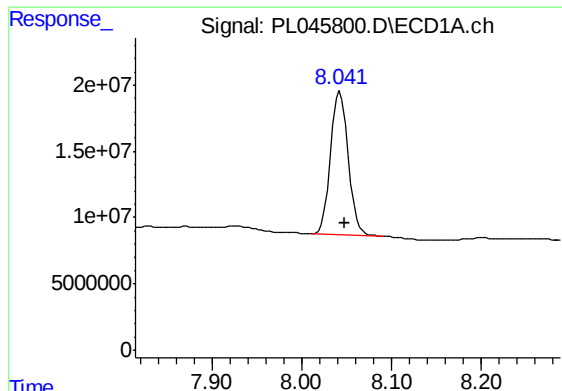

#28 Decachlorobiphenyl

R.T.: 8.043 min
Delta R.T.: -0.005 min
Response: 148931782
Conc: 17.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
C135-CON

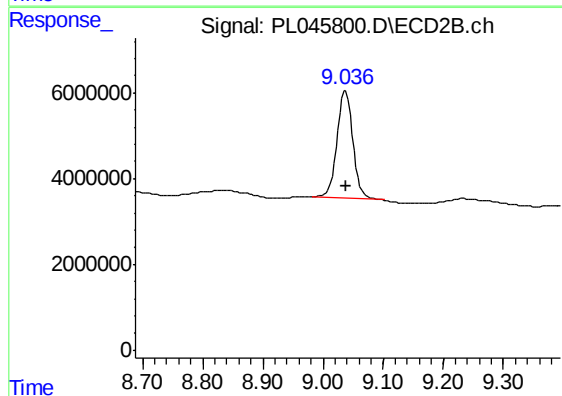

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: -0.001 min
Response: 46223540
Conc: 20.23 ng/ml