

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031219\
 Data File : PL045769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2019 22:05
 Operator : AJ\SJ
 Sample : K1808-01
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-01-AA0-BB0-AA0A-BB0A

Manual Integrations
 APPROVED

Sohil
 3/13/2019 9:37:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 01:25:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	115.6E6	36463692	16.808	17.027
28)	SA Decachlor...	8.043	9.035	114.8E6	35656389	13.716	15.605m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031219\
Data File : PL045769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2019 22:05
Operator : AJ\SJ
Sample : K1808-01
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A


Manual Integrations
APPROVED

Sohil
3/13/2019 9:37:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 01:25:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

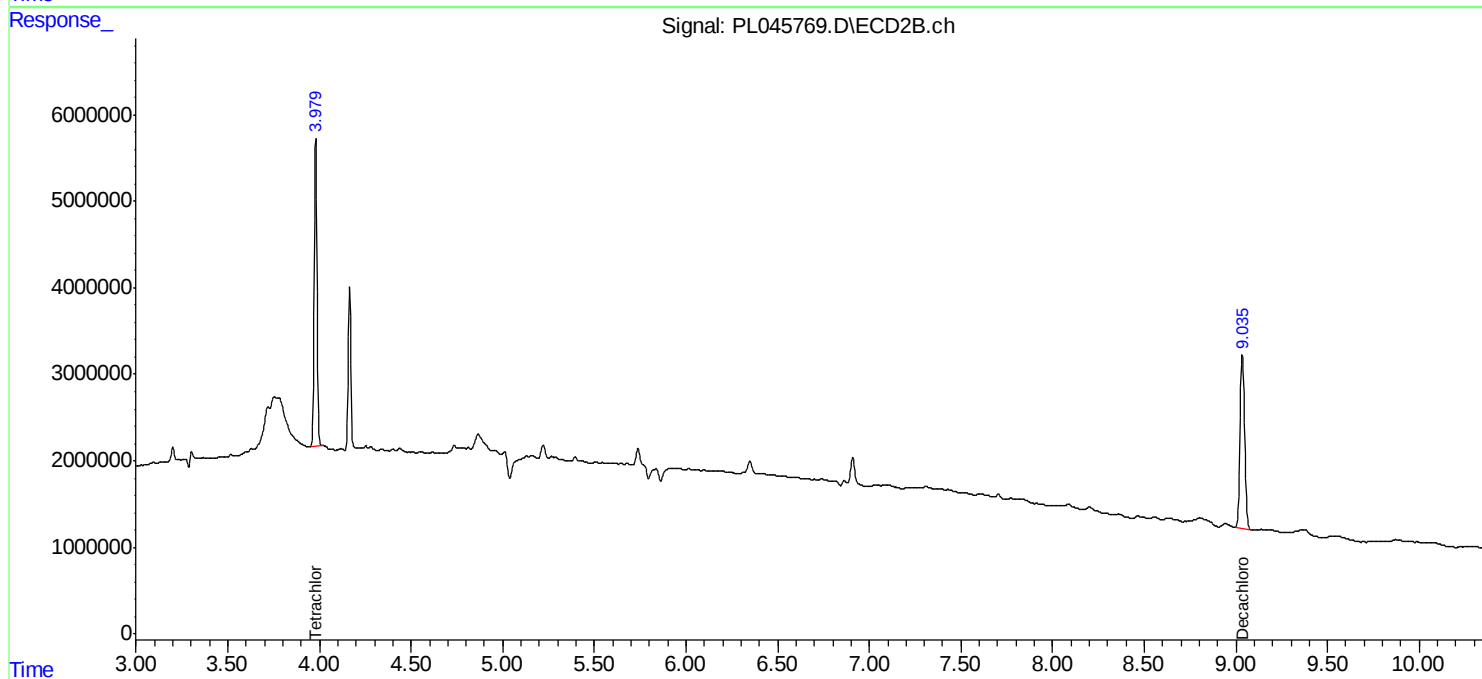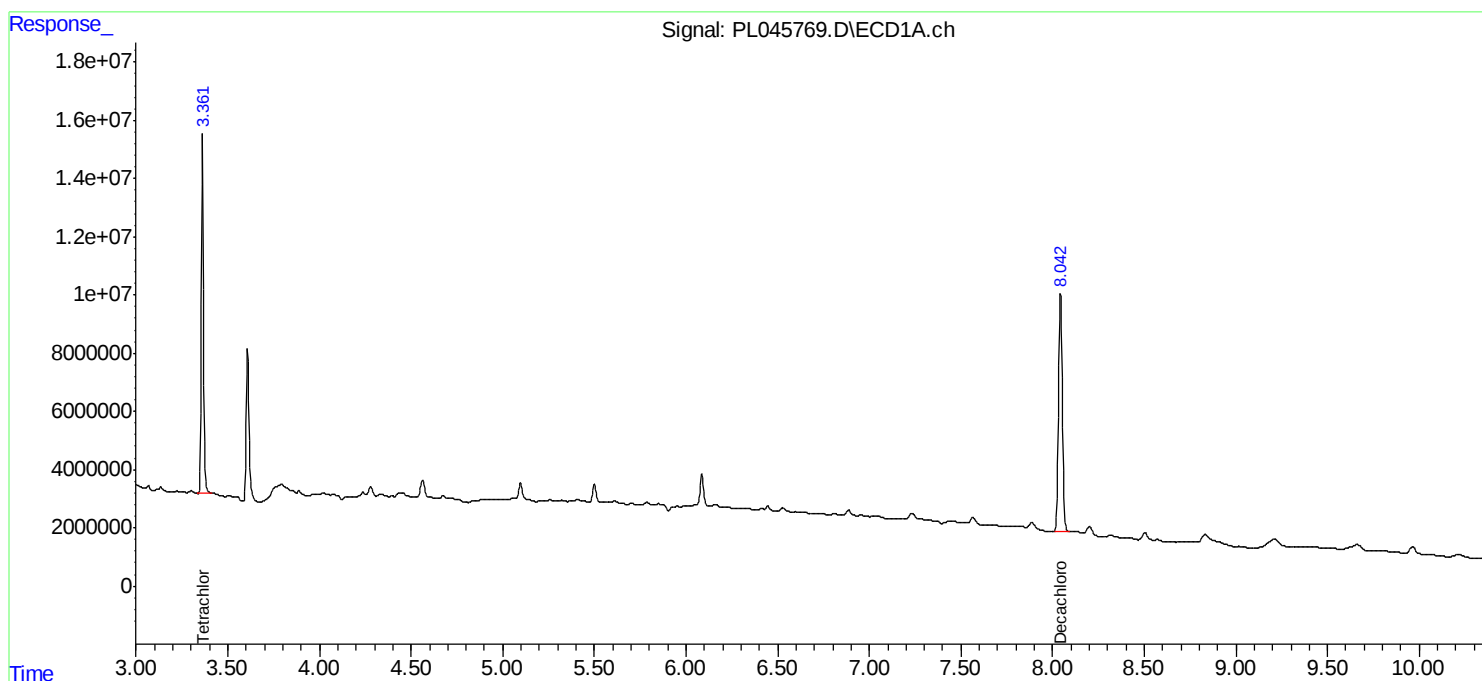

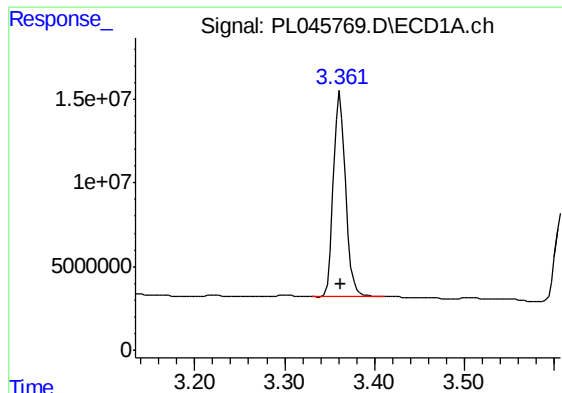


#1 Tetrachloro-m-xylene

R.T.: 3.362 min
Delta R.T.: -0.001 min
Response: 115627636
Conc: 16.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A


Manual Integrations
APPROVED

Sohil
3/13/2019 9:37:03 AM

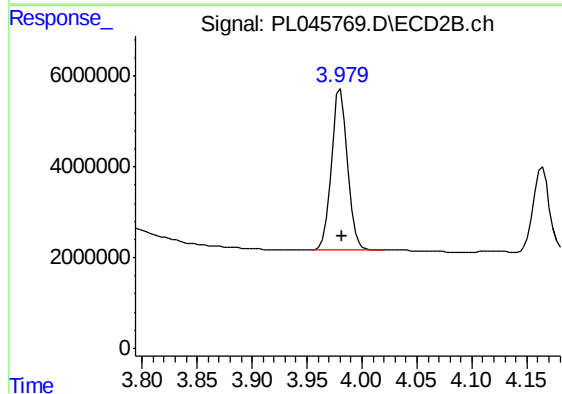


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 36463692
Conc: 17.03 ng/ml

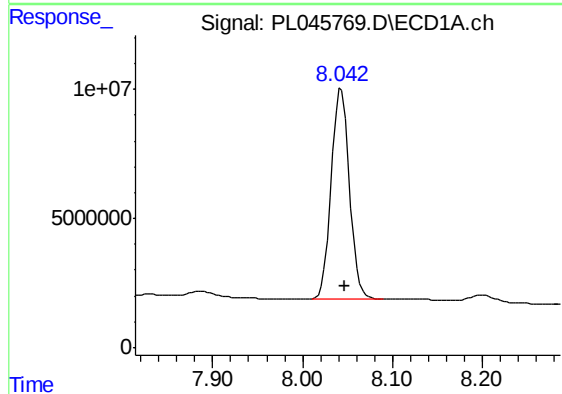

#28 Decachlorobiphenyl

R.T.: 8.043 min
Delta R.T.: -0.004 min
Response: 114767666
Conc: 13.72 ng/ml

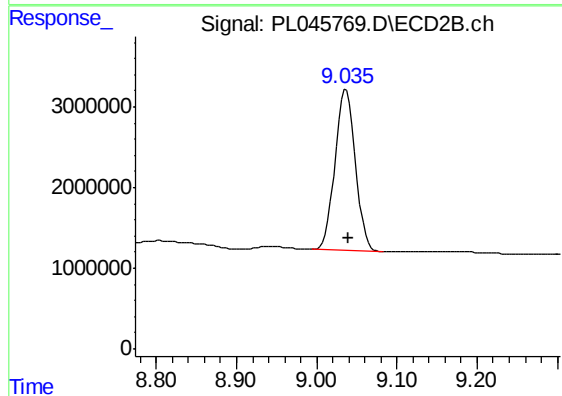

#28 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: -0.004 min
Response: 35656389
Conc: 15.61 ng/ml m