

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031220\
 Data File : PL057288.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2020 14:16
 Operator : AJ\MA
 Sample : PB127463TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB127460TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 05:56:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 11 17:44:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.958	174.3E6	40477503	20.455	18.972
28)	SA Decachlor...	8.205	8.979	194.4E6	40906561	20.116	19.252
Target Compounds							
2)	A alpha-BHC	3.898	0.000	5800638	0	0.391	N.D. #
4)	MA Heptachlor	0.000	5.135	0	10914948	N.D.	3.507 #
5)	MB Aldrin	0.000	5.442	0	3223279	N.D.	1.078 #
8)	B Heptachlo...	5.170	5.803	323251	2808034	0.027	1.013 #
14)	MA Endrin	6.012	6.664f	2589889	356503	0.238	0.138 #
15)	B Endosulfa...	0.000	6.870f	0	580864	N.D.	0.207 #
23)	Chlordane-1	4.356f	0.000	3024767	0	9.952	N.D. #
24)	Chlordane-2	0.000	5.396	0	1961928	N.D.	20.554 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031220\
Data File : PL057288.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2020 14:16
Operator : AJ\MA
Sample : PB127463TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB127460TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 05:56:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 11 17:44:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

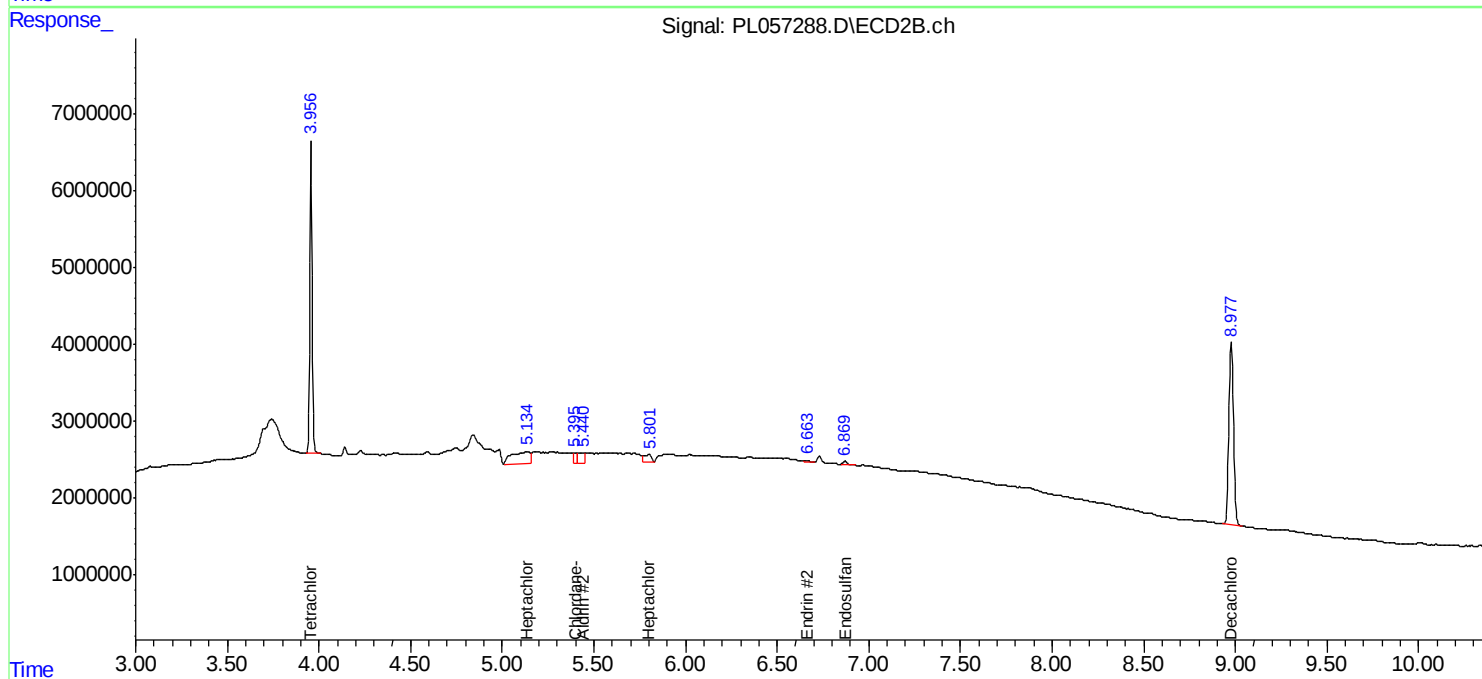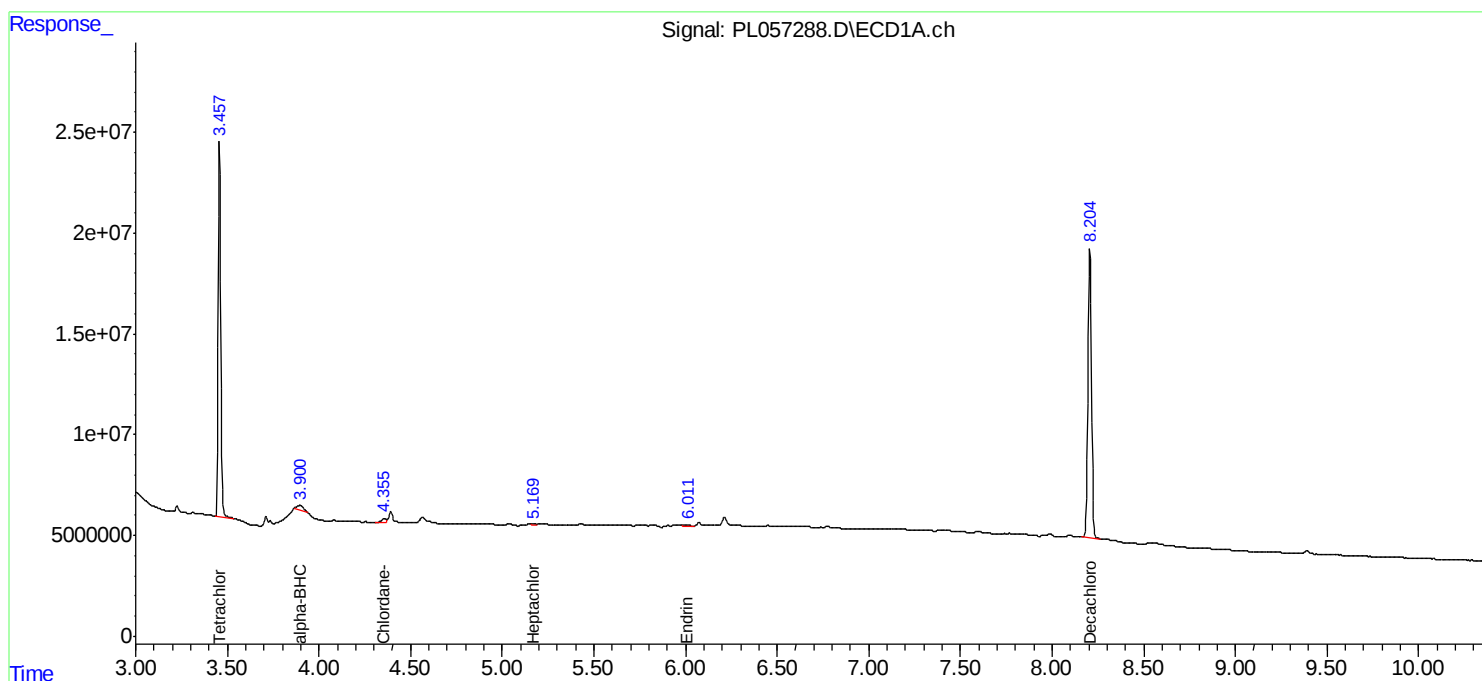


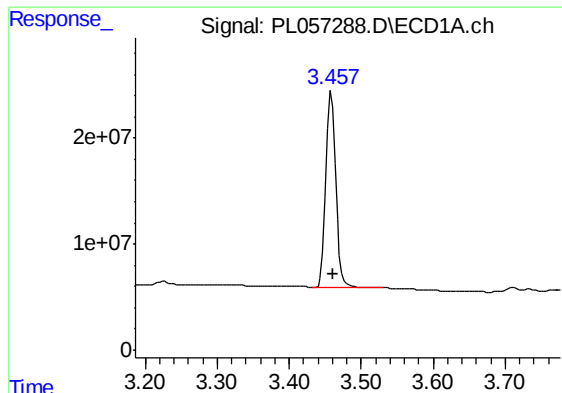

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 174321114
Conc: 20.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127460TB

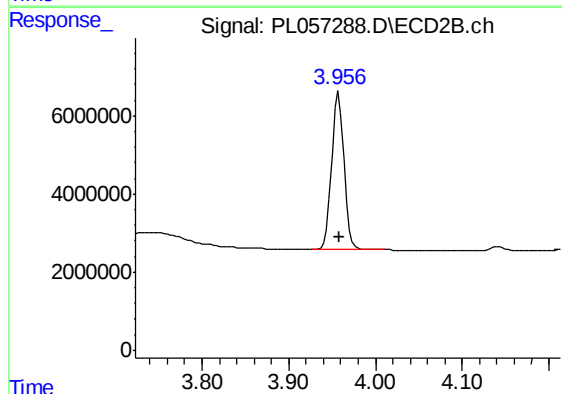


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 40477503
Conc: 18.97 ng/ml

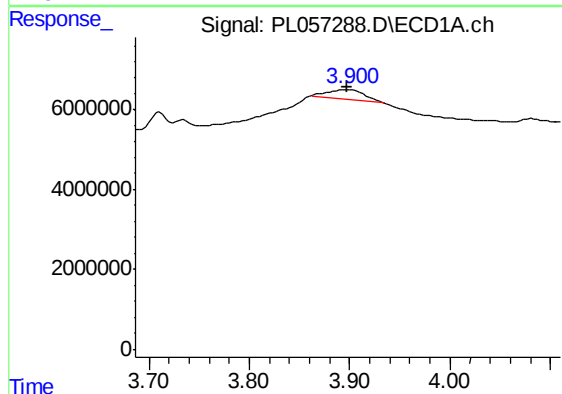


#2 alpha-BHC

R.T.: 3.898 min
Delta R.T.: 0.000 min
Response: 5800638
Conc: 0.39 ng/ml

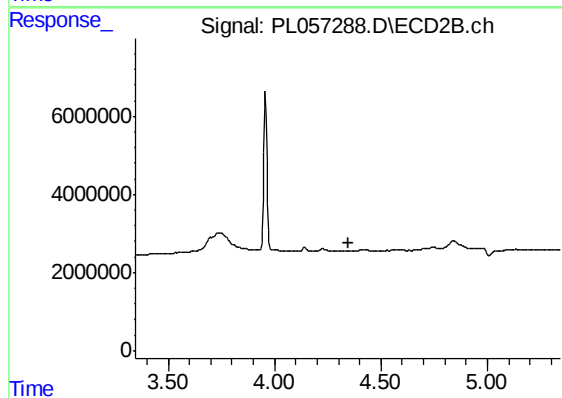

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

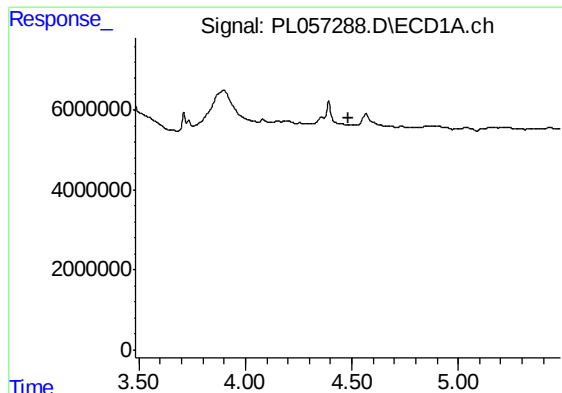

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.483 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB127460TB

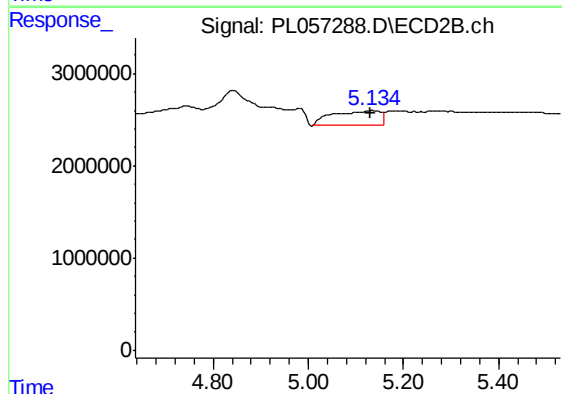


#4 Heptachlor

R.T.: 5.135 min
Delta R.T.: 0.005 min
Response: 10914948
Conc: 3.51 ng/ml

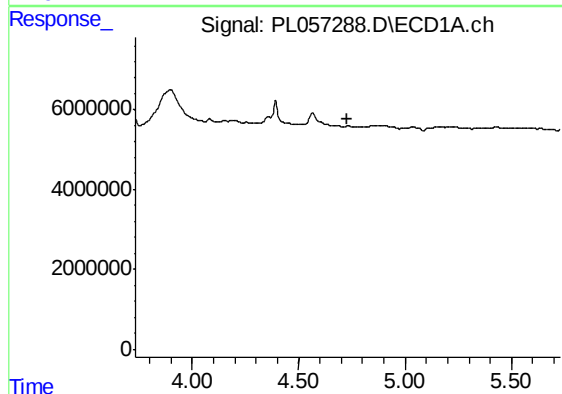


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.731 min
Response: 0
Conc: N.D.

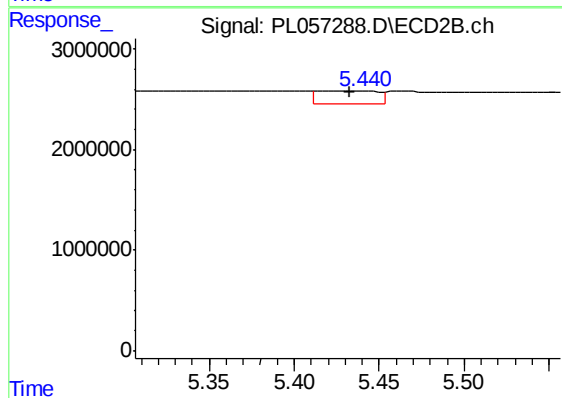

#5 Aldrin


R.T.: 5.442 min
Delta R.T.: 0.009 min
Response: 3223279
Conc: 1.08 ng/ml

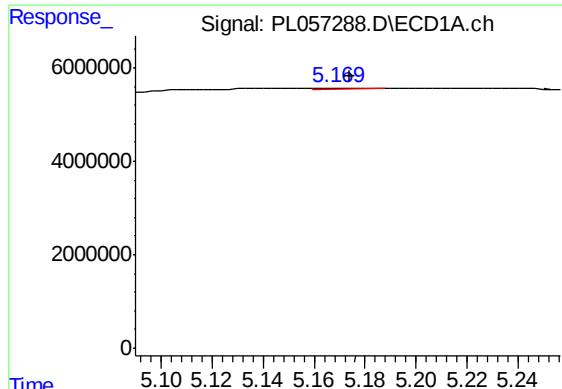

#8 Heptachlor epoxide


R.T.: 5.170 min
Delta R.T.: -0.004 min
Response: 323251
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127460TB

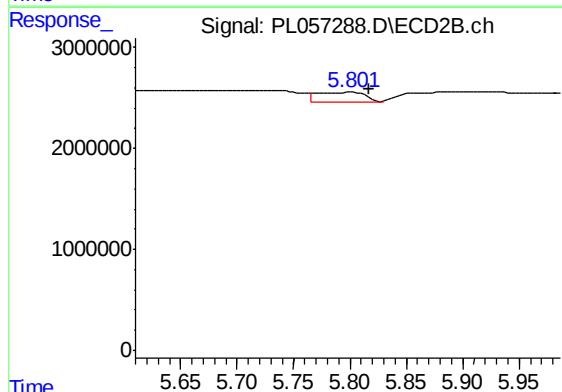


#8 Heptachlor epoxide

R.T.: 5.803 min
Delta R.T.: -0.015 min
Response: 2808034
Conc: 1.01 ng/ml

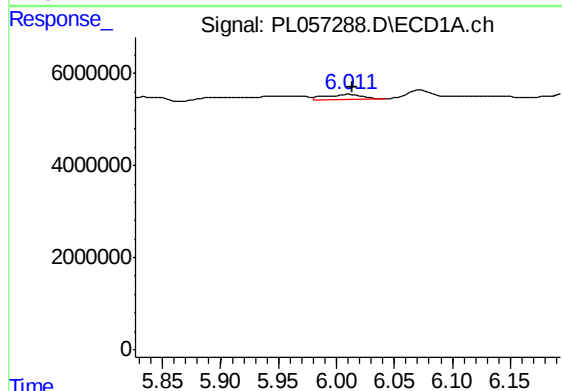


#14 Endrin

R.T.: 6.012 min
Delta R.T.: -0.002 min
Response: 2589889
Conc: 0.24 ng/ml

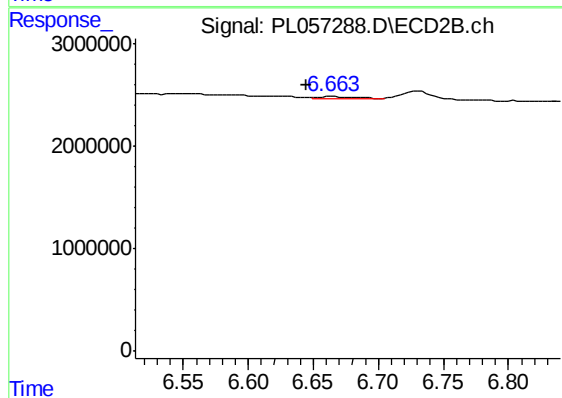

#14 Endrin


R.T.: 6.664 min
Delta R.T.: 0.019 min
Response: 356503
Conc: 0.14 ng/ml

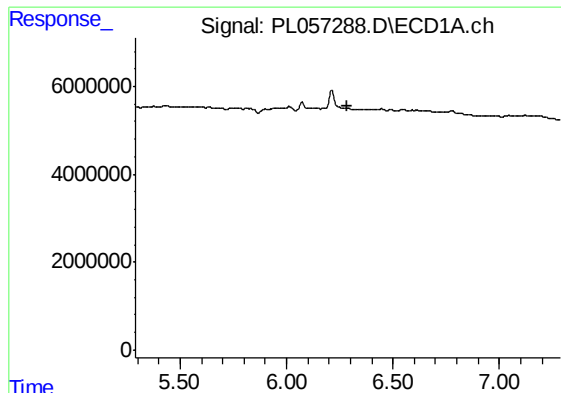

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.287 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB127460TB

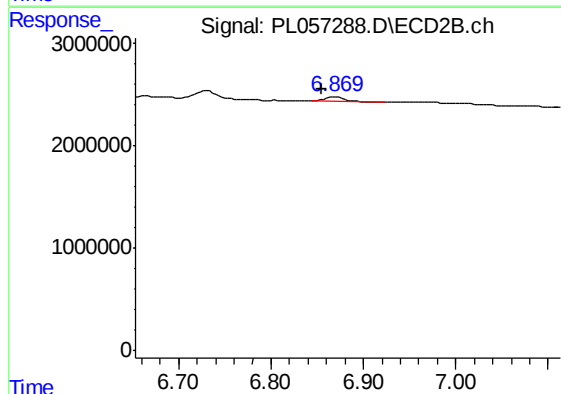


#15 Endosulfan II

R.T.: 6.870 min
Delta R.T.: 0.015 min
Response: 580864
Conc: 0.21 ng/ml

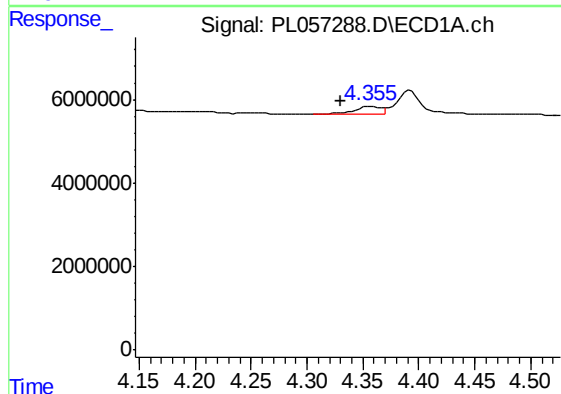


#23 Chlordane-1

R.T.: 4.356 min
Delta R.T.: 0.026 min
Response: 3024767
Conc: 9.95 ng/ml

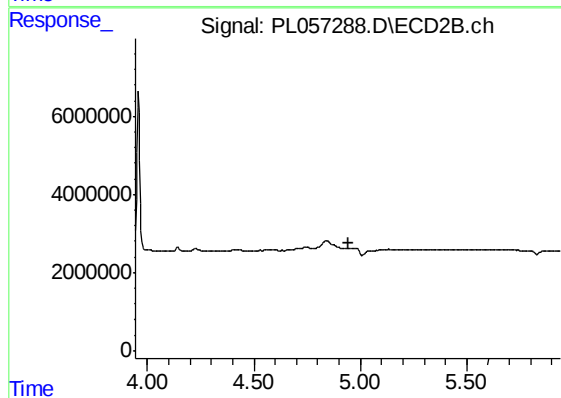

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

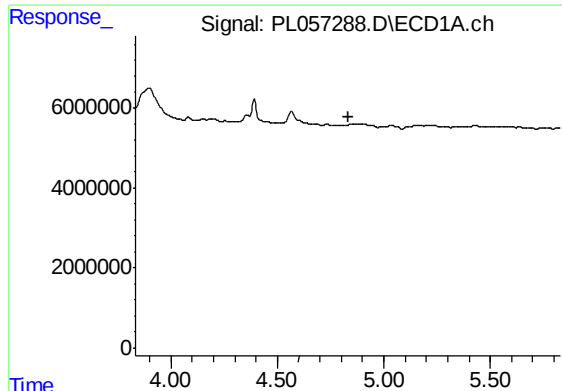

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 4.832 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB127460TB

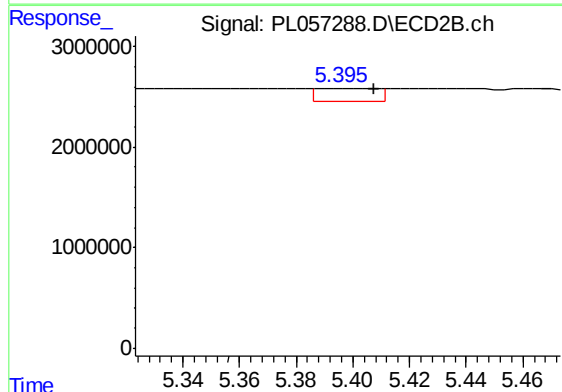


#24 Chlordane-2

R.T.: 5.396 min
Delta R.T.: -0.011 min
Response: 1961928
Conc: 20.55 ng/ml

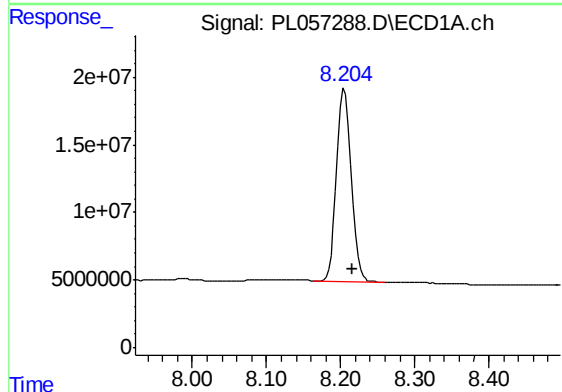

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.010 min
Response: 194419326
Conc: 20.12 ng/ml

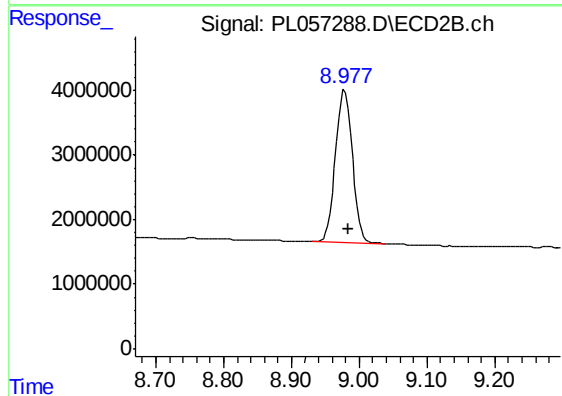

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.006 min
Response: 40906561
Conc: 19.25 ng/ml