

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031220\
 Data File : PL057307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2020 19:06
 Operator : AJ\MA
 Sample : PB127489BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB127489BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 06:05:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 11 17:44:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	184.9E6	43339855	21.699	20.314
28)	SA Decachlor...	8.206	8.979	195.9E6	43182401	20.264	20.324
Target Compounds							
2)	A alpha-BHC	3.899	0.000	7073664	0	0.477	N.D. #
4)	MA Heptachlor	0.000	5.138	0	19156463	N.D.	6.155 #
5)	MB Aldrin	0.000	5.451f	0	7225791	N.D.	2.417 #
8)	B Heptachlo...	5.155f	5.801f	1522947	5408877	0.126	1.952 #
14)	MA Endrin	6.013	6.667f	1471479	510439	0.135	0.198 #
15)	B Endosulfa...	0.000	6.869	0	534176	N.D.	0.190 #
23)	Chlordane-1	4.356f	0.000	3337718	0	10.981	N.D. #
24)	Chlordane-2	4.852f	0.000	2035400	0	5.772	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031220\
Data File : PL057307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2020 19:06
Operator : AJ\MA
Sample : PB127489BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB127489BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 06:05:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 11 17:44:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

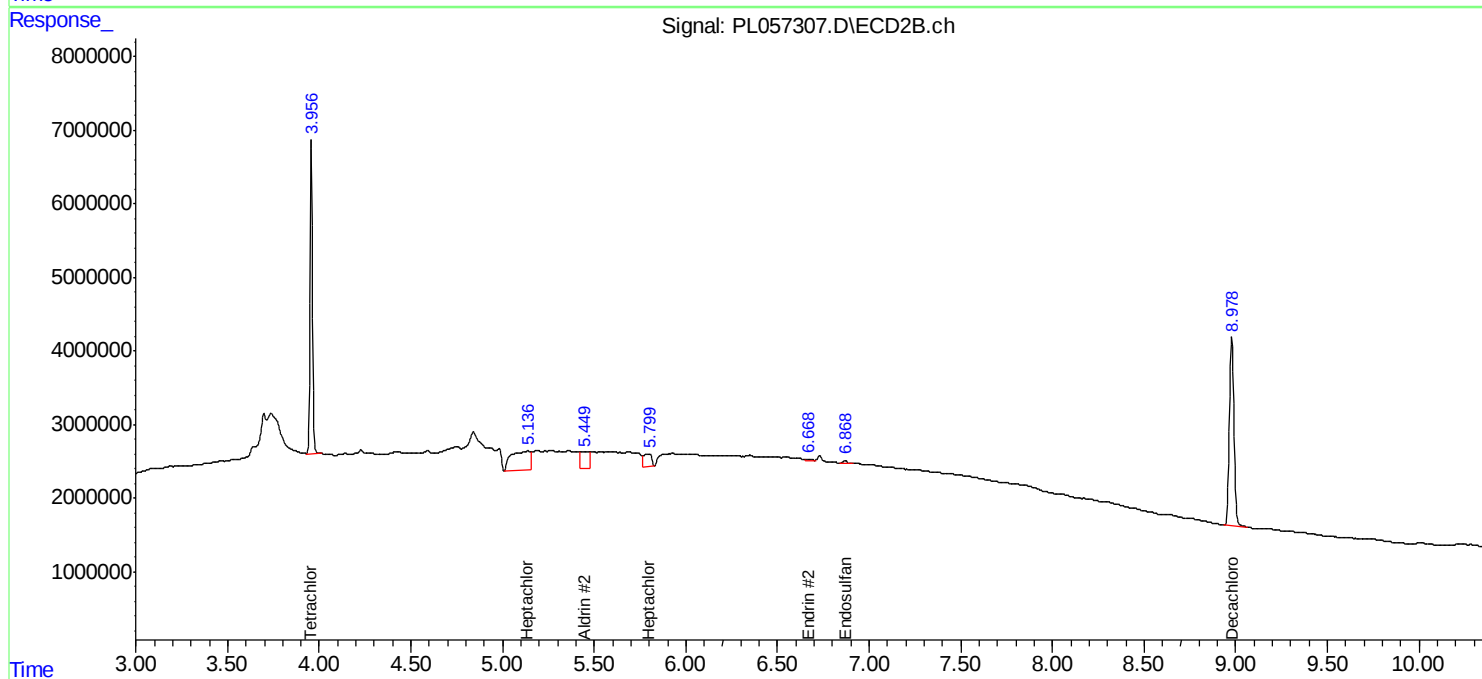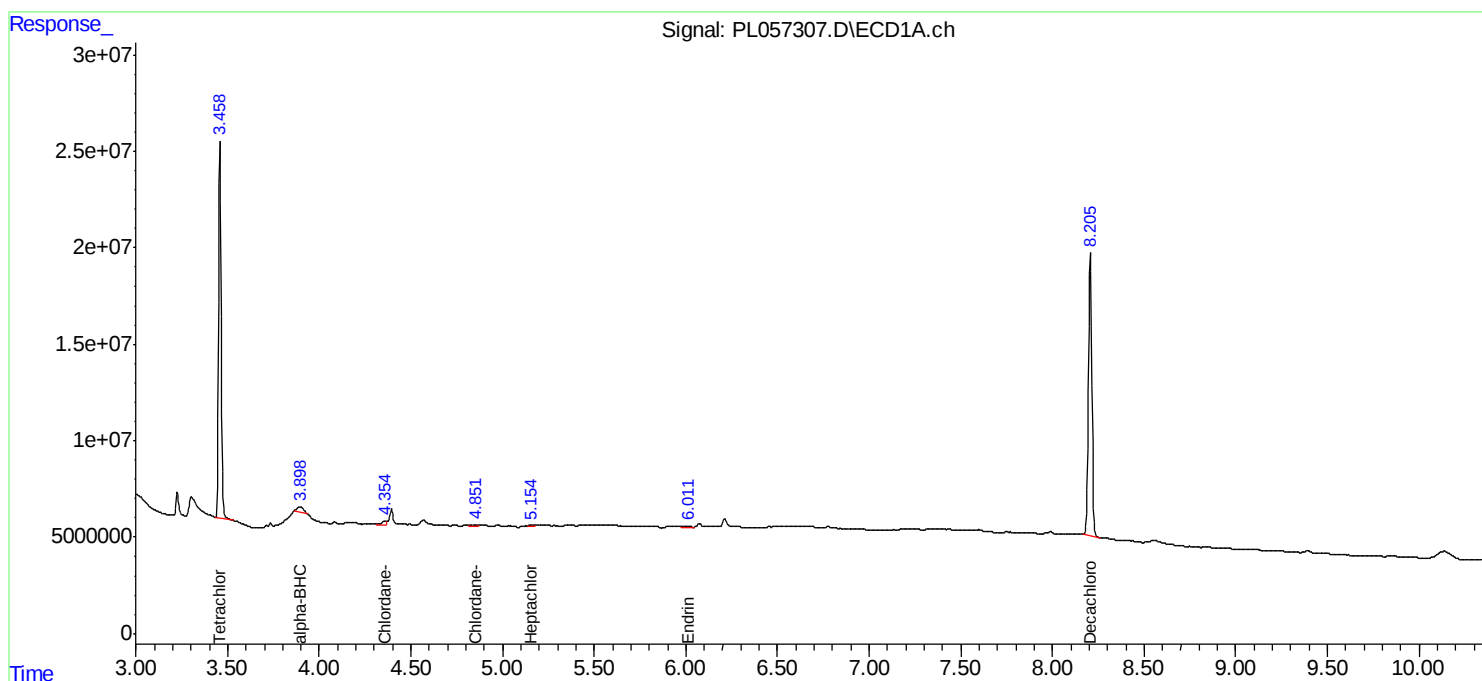


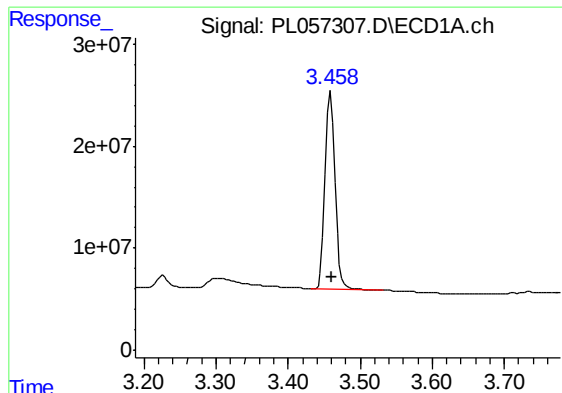

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 184926398
Conc: 21.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127489BL

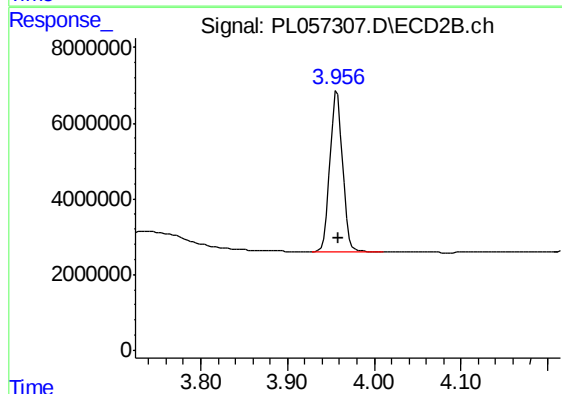


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 43339855
Conc: 20.31 ng/ml

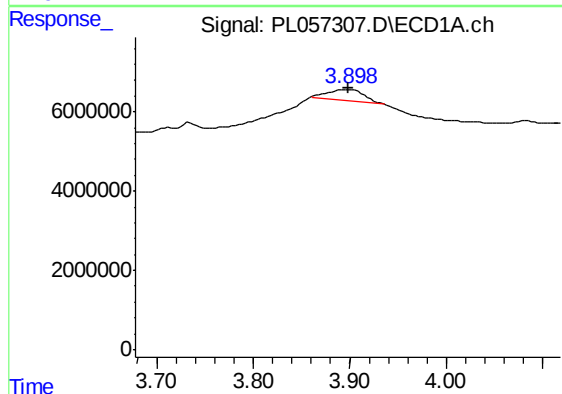


#2 alpha-BHC

R.T.: 3.899 min
Delta R.T.: 0.001 min
Response: 7073664
Conc: 0.48 ng/ml

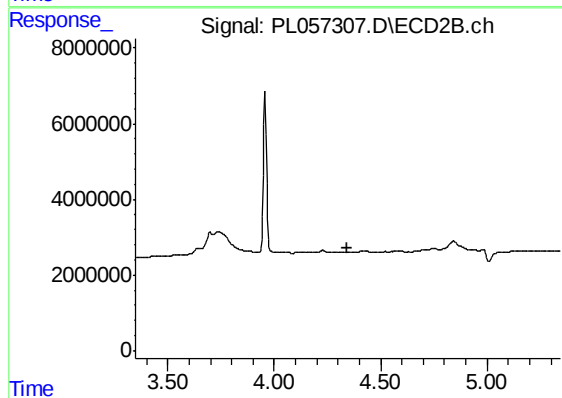

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

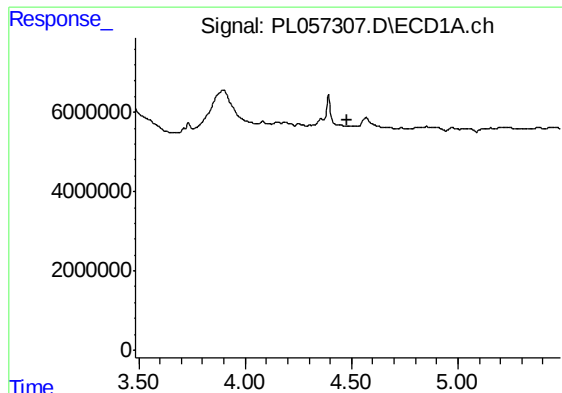

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.483 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB127489BL

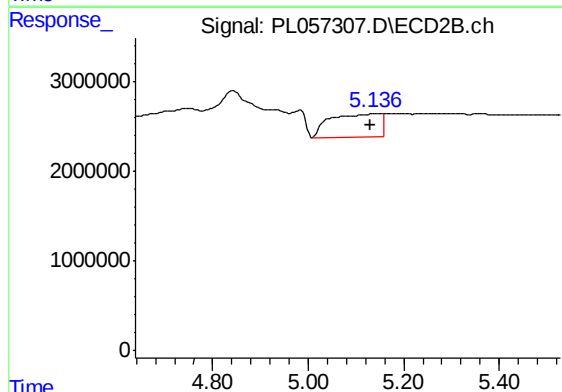


#4 Heptachlor

R.T.: 5.138 min
Delta R.T.: 0.008 min
Response: 19156463
Conc: 6.15 ng/ml

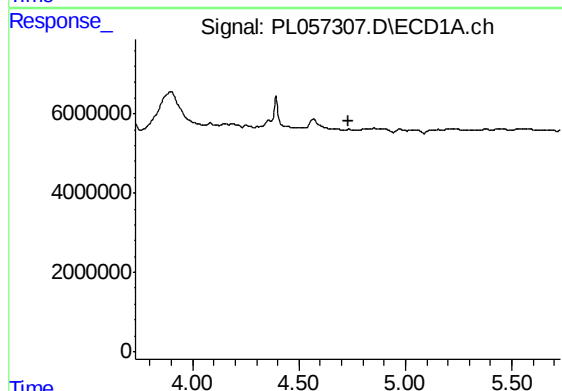


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 4.731 min
Response: 0
Conc: N.D.

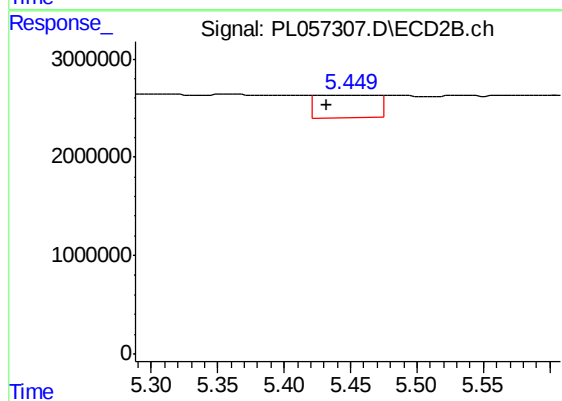

#5 Aldrin


R.T.: 5.451 min
Delta R.T.: 0.018 min
Response: 7225791
Conc: 2.42 ng/ml

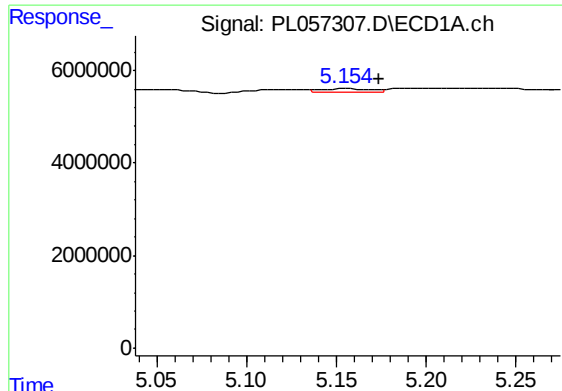

#8 Heptachlor epoxide


R.T.: 5.155 min
Delta R.T.: -0.019 min
Response: 1522947
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127489BL

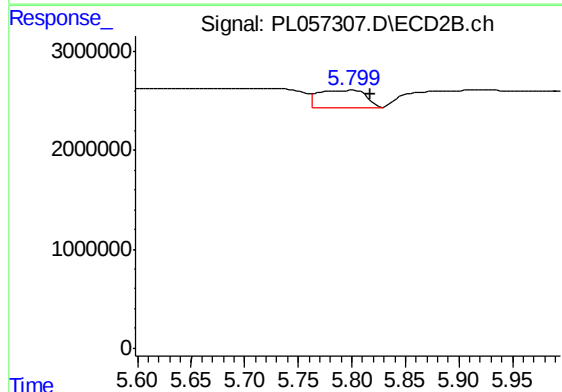


#8 Heptachlor epoxide

R.T.: 5.801 min
Delta R.T.: -0.017 min
Response: 5408877
Conc: 1.95 ng/ml

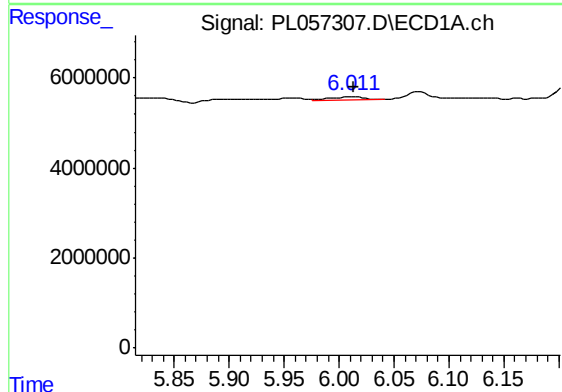


#14 Endrin

R.T.: 6.013 min
Delta R.T.: 0.000 min
Response: 1471479
Conc: 0.14 ng/ml

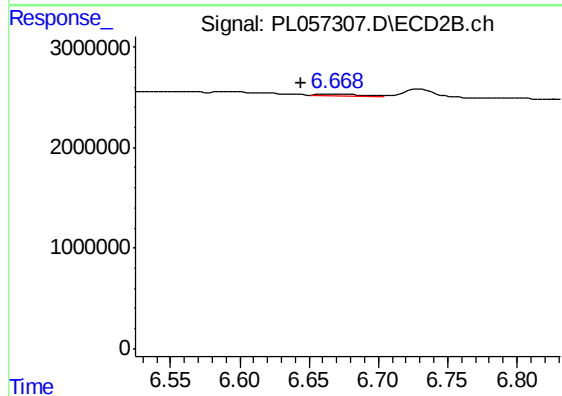

#14 Endrin


R.T.: 6.667 min
Delta R.T.: 0.023 min
Response: 510439
Conc: 0.20 ng/ml

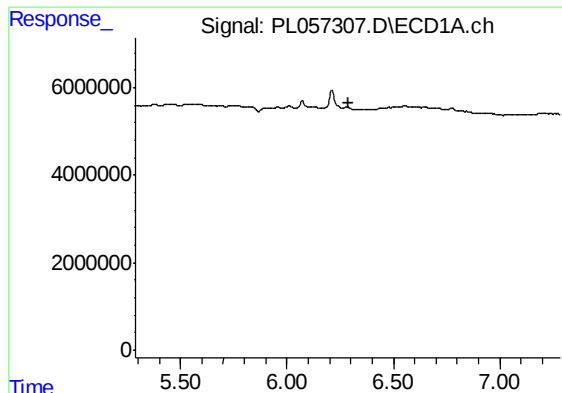

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.287 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB127489BL

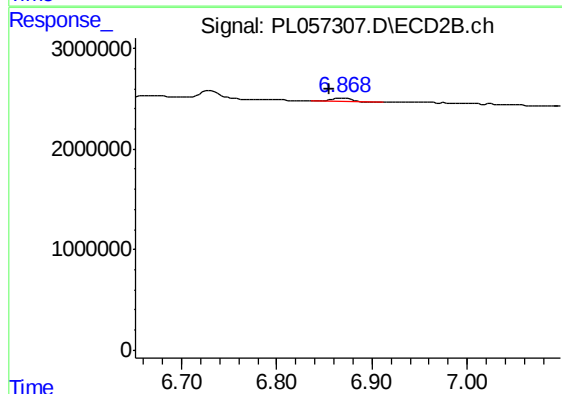


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.014 min
Response: 534176
Conc: 0.19 ng/ml

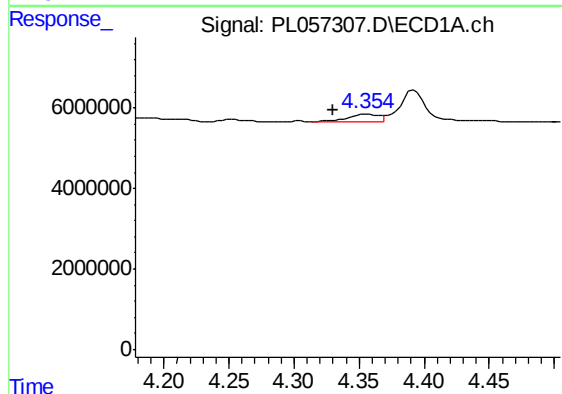


#23 Chlordane-1

R.T.: 4.356 min
Delta R.T.: 0.025 min
Response: 3337718
Conc: 10.98 ng/ml

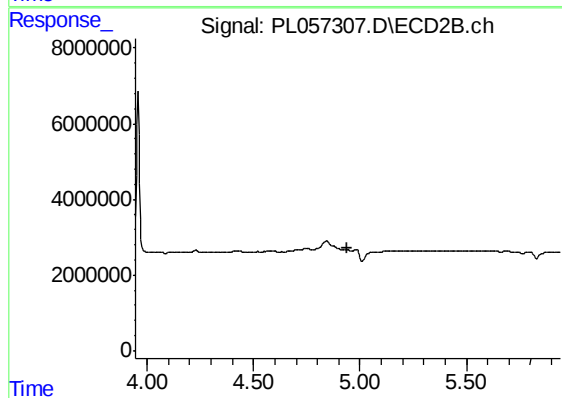

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

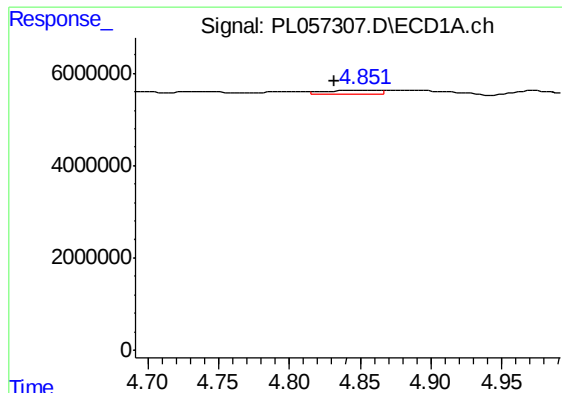

#24 Chlordane-2


R.T.: 4.852 min
Delta R.T.: 0.020 min
Response: 2035400
Conc: 5.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127489BL

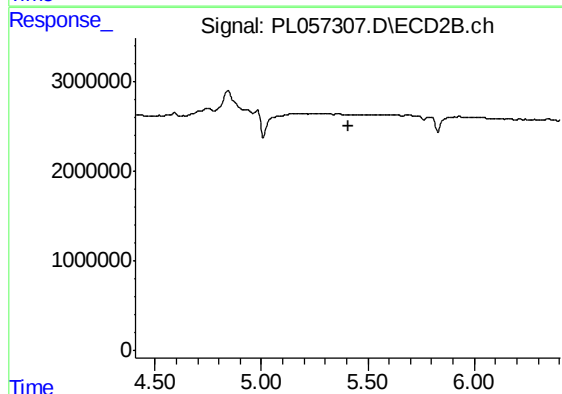


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

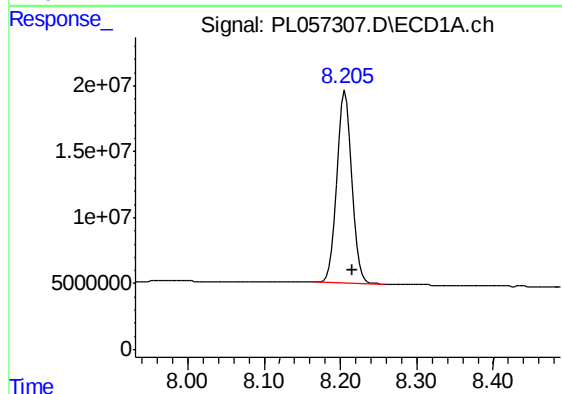

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.010 min
Response: 195854110
Conc: 20.26 ng/ml

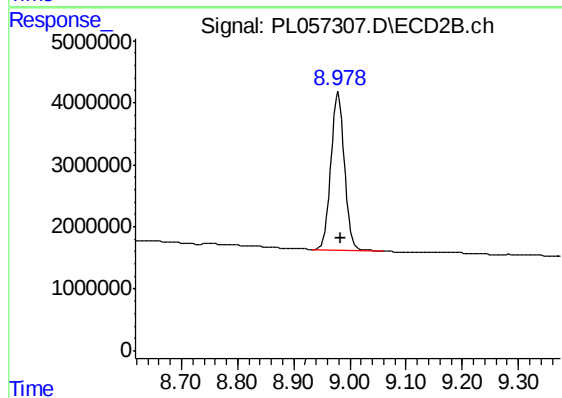

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.005 min
Response: 43182401
Conc: 20.32 ng/ml