

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031220\
 Data File : PL057279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2020 12:08
 Operator : AJ\MA
 Sample : L1853-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CB-EC-52-G

Manual Integrations
 APPROVED

mohammad
 3/16/2020 2:56:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 05:52:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 11 17:44:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.458	3.956	181.6E6	47323950	21.304m	22.181m
28) SA Decachlor...	8.206	8.979	195.4E6	42131885	20.220	19.829

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031220\
Data File : PL057279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2020 12:08
Operator : AJ\MA
Sample : L1853-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CB-EC-52-G


Manual Integrations
APPROVED

mohammad
3/16/2020 2:56:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 05:52:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 11 17:44:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

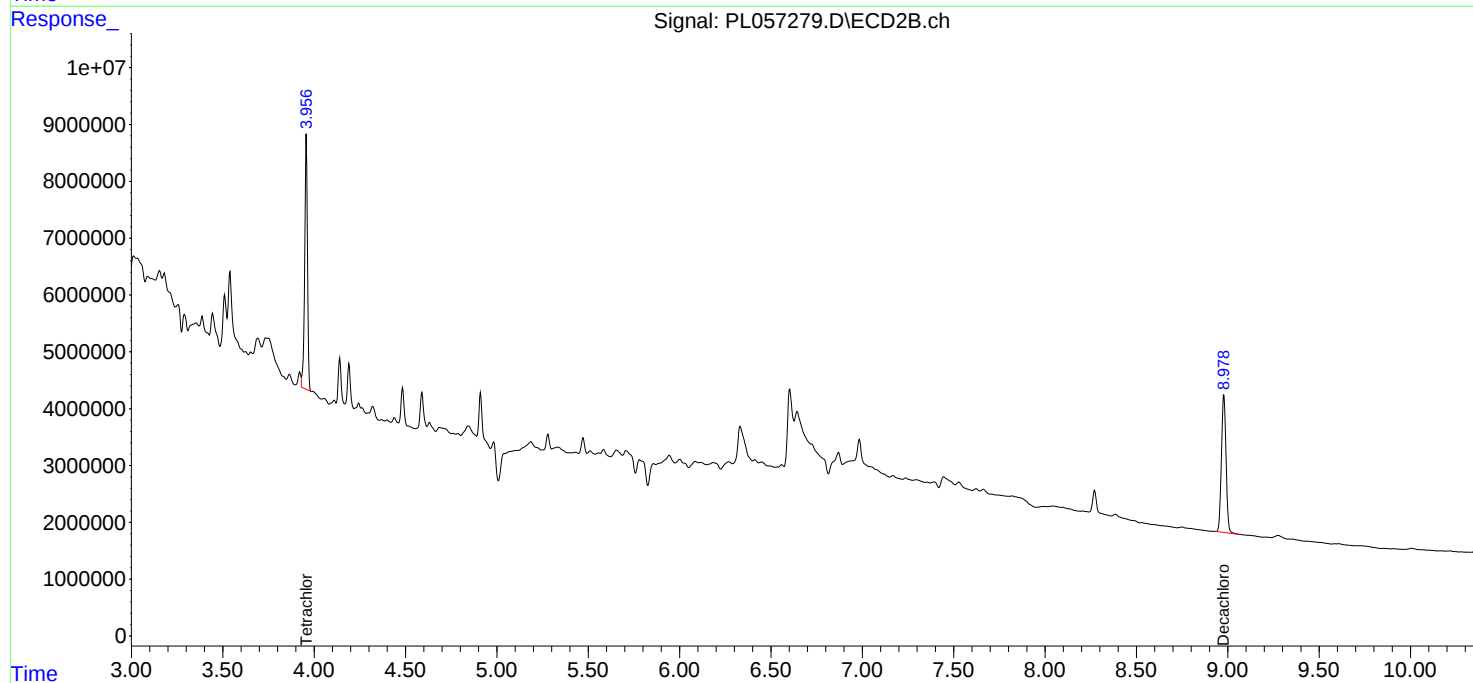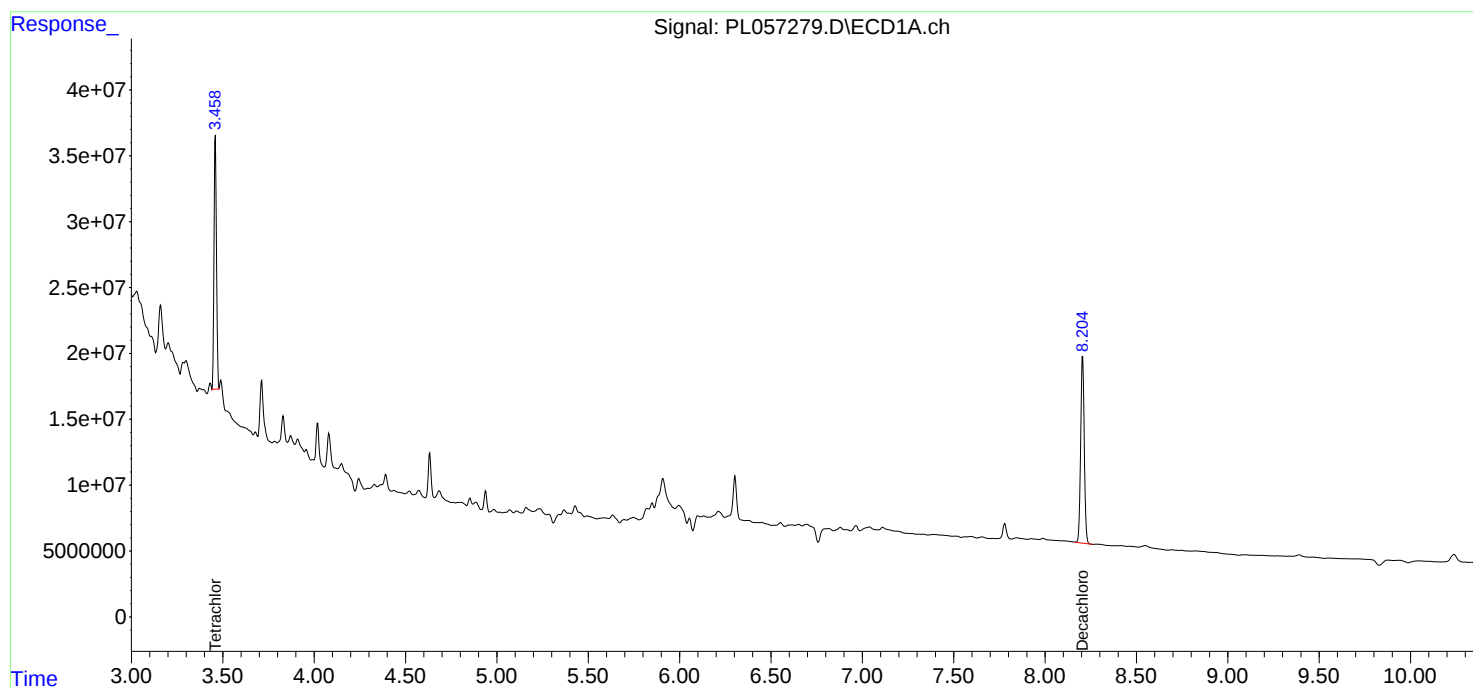

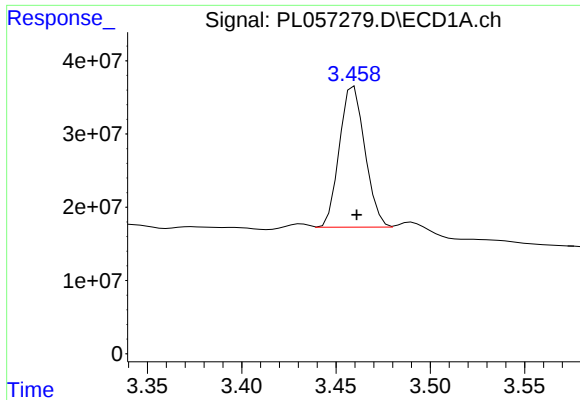


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: -0.003 min
Response: 181554504
Conc: 21.30 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CB-EC-52-G


Manual Integrations
APPROVED

mohammad
3/16/2020 2:56:40 PM

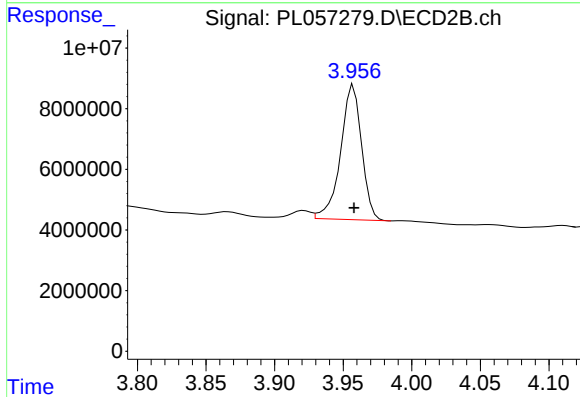


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.002 min
Response: 47323950
Conc: 22.18 ng/ml m

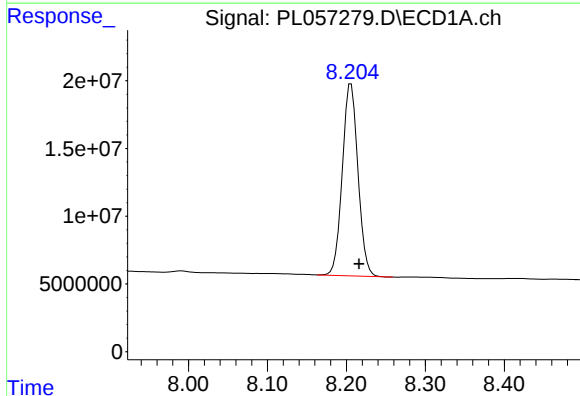

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.010 min
Response: 195432422
Conc: 20.22 ng/ml

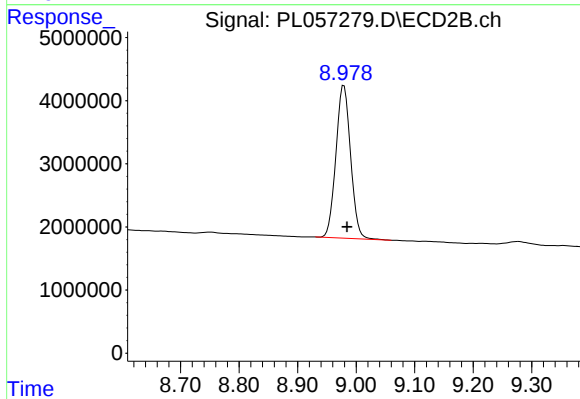

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.005 min
Response: 42131885
Conc: 19.83 ng/ml