

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031220\
 Data File : PL057280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2020 12:22
 Operator : AJ\MA
 Sample : L1853-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CB-EC-52-S

Manual Integrations
 APPROVED

mohammad
 3/16/2020 2:56:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 05:52:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 11 17:44:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.958	192.6E6	46153272	22.596m	21.633
28)	SA Decachlor...	8.205	8.980	194.5E6	40555294	20.120	19.087

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031220\
Data File : PL057280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2020 12:22
Operator : AJ\MA
Sample : L1853-06
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CB-EC-52-S


Manual Integrations
APPROVED

mohammad
3/16/2020 2:56:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 05:52:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 11 17:44:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

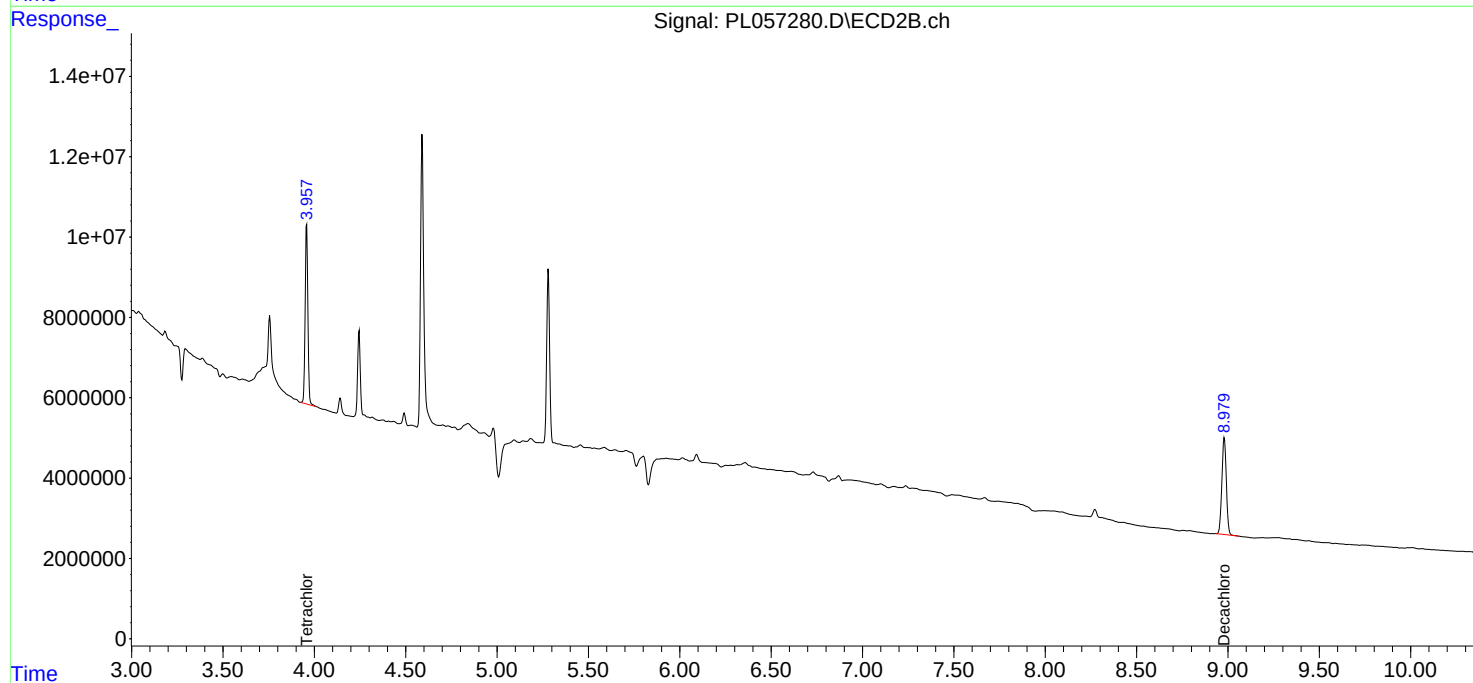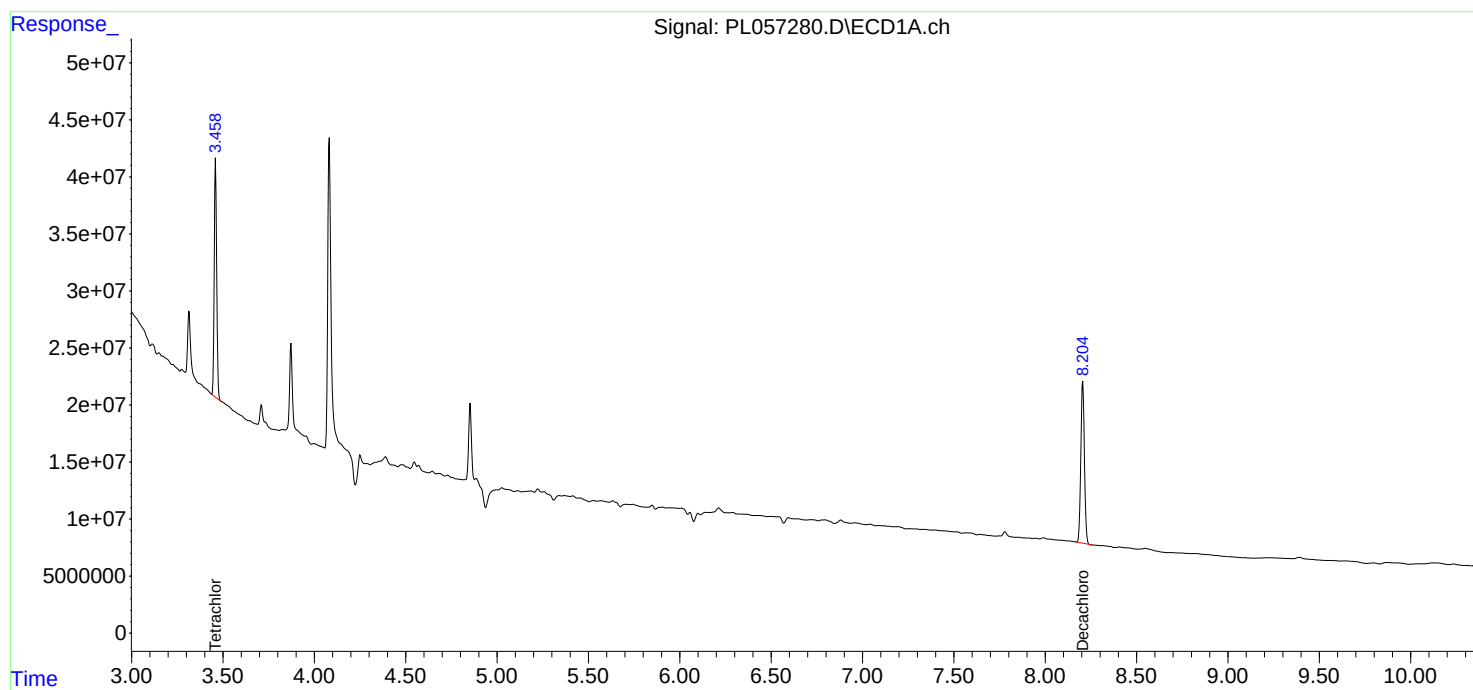

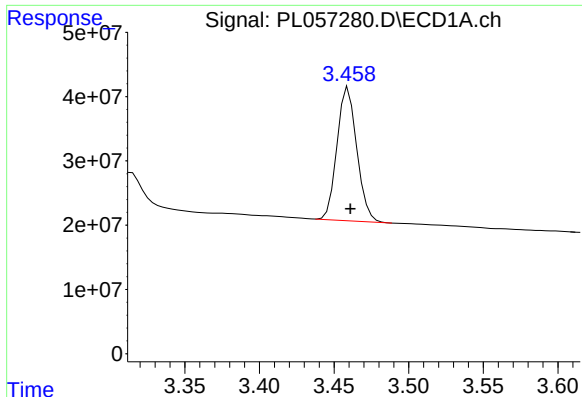


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: -0.003 min
Response: 192573550
Conc: 22.60 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CB-EC-52-S


Manual Integrations
APPROVED

mohammad
3/16/2020 2:56:43 PM

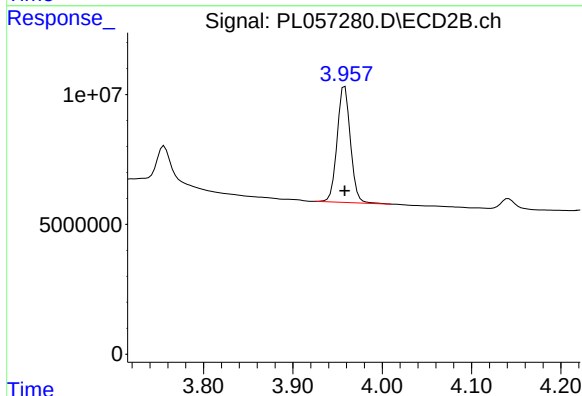


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 46153272
Conc: 21.63 ng/ml

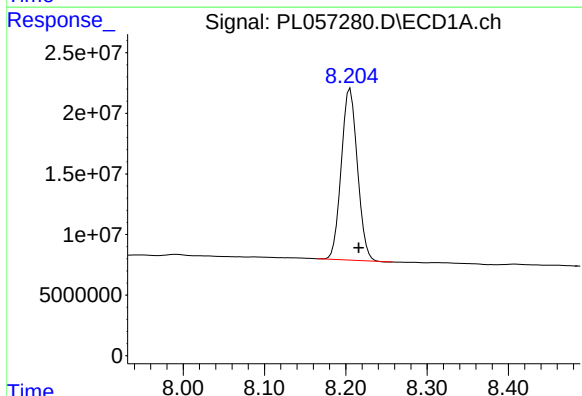

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.010 min
Response: 194462839
Conc: 20.12 ng/ml

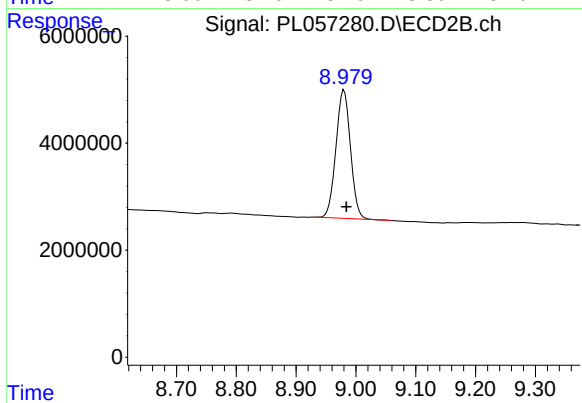

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: -0.004 min
Response: 40555294
Conc: 19.09 ng/ml