

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031220\
 Data File : PL057298.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2020 16:59
 Operator : AJ\MA
 Sample : L1893-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2-DA

Manual Integrations
 APPROVED

mohammad
 3/17/2020 2:34:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 06:00:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 11 17:44:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	220.5E6	50541251	25.879	23.689
28)	SA Decachlor...	8.206	8.979	189.4E6	42611392	19.593	20.055
Target Compounds							
12)	B 4,4'-DDE	5.618	6.278	58494579	13001992	4.992	4.582
17)	MA 4,4'-DDT	6.374	7.063	67094623	16511154	6.857	6.712m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031220\
Data File : PL057298.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2020 16:59
Operator : AJ\MA
Sample : L1893-10
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
TP-2-DA


Manual Integrations
APPROVED

mohammad
3/17/2020 2:34:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 06:00:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 11 17:44:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

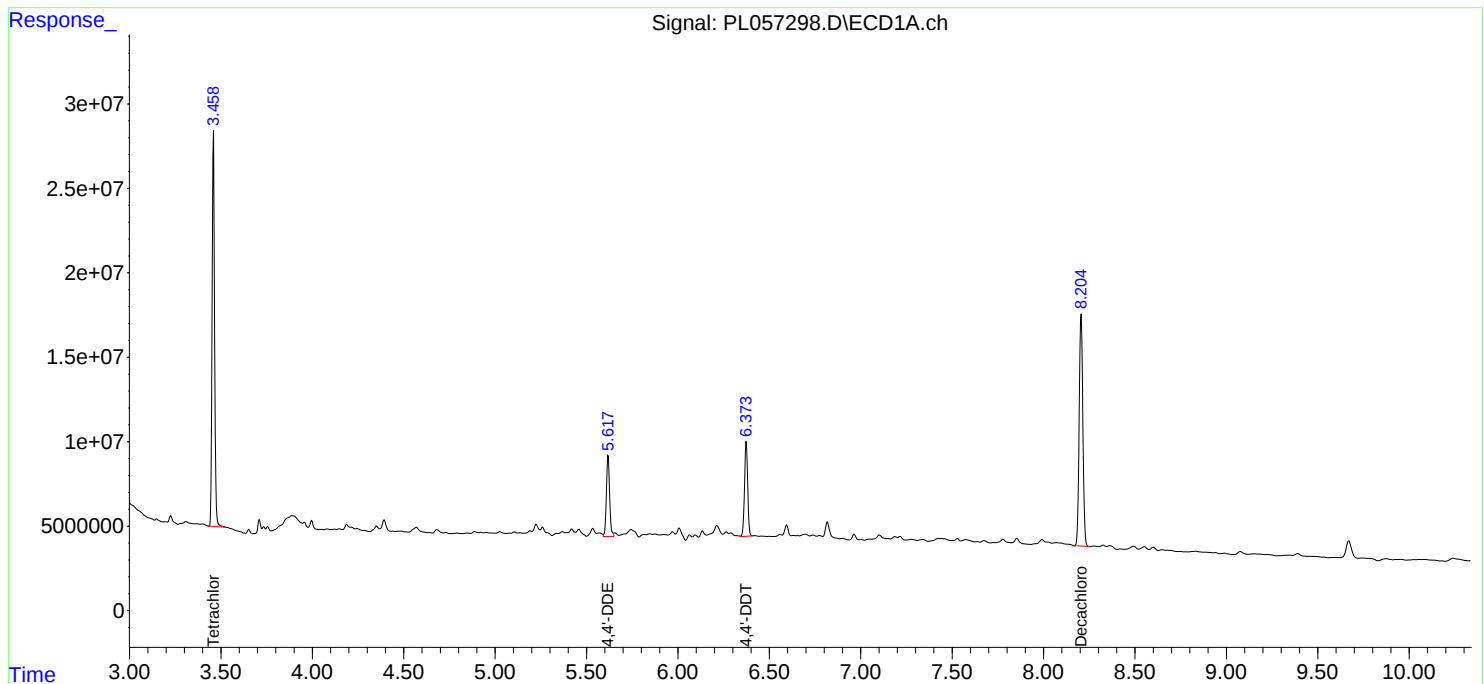

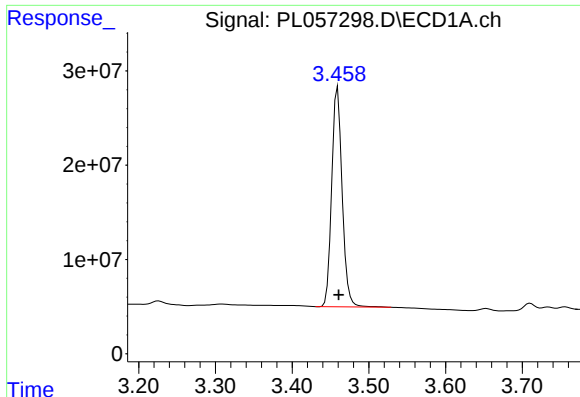


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 220545506
Conc: 25.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-DA


Manual Integrations
APPROVED

mohammad
3/17/2020 2:34:01 PM

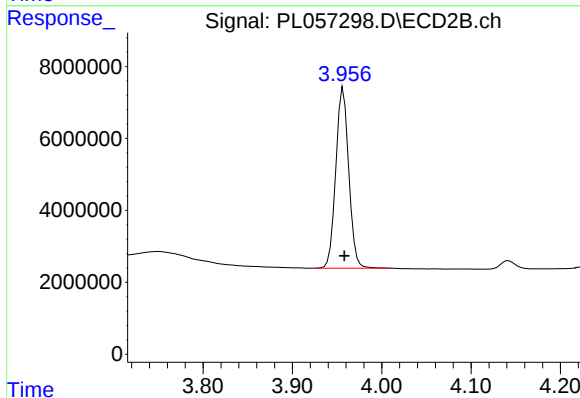


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.001 min
Response: 50541251
Conc: 23.69 ng/ml

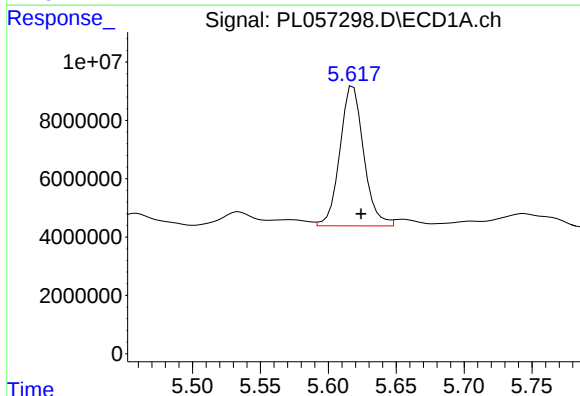


#12 4,4'-DDE

R.T.: 5.618 min
Delta R.T.: -0.006 min
Response: 58494579
Conc: 4.99 ng/ml

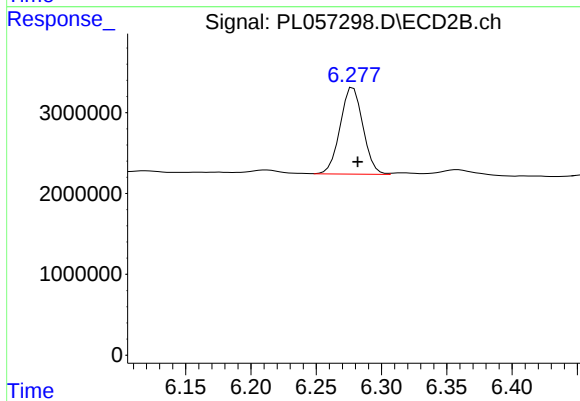

#12 4,4'-DDE

R.T.: 6.278 min
Delta R.T.: -0.003 min
Response: 13001992
Conc: 4.58 ng/ml

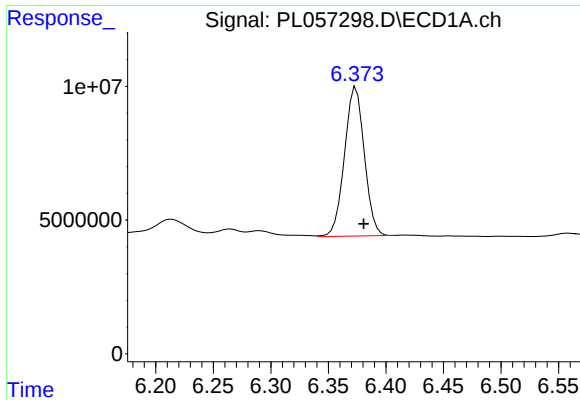


#17 4,4'-DDT

R.T.: 6.374 min
Delta R.T.: -0.007 min
Response: 67094623
Conc: 6.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-DA


Manual Integrations
APPROVED

mohammad
3/17/2020 2:34:01 PM

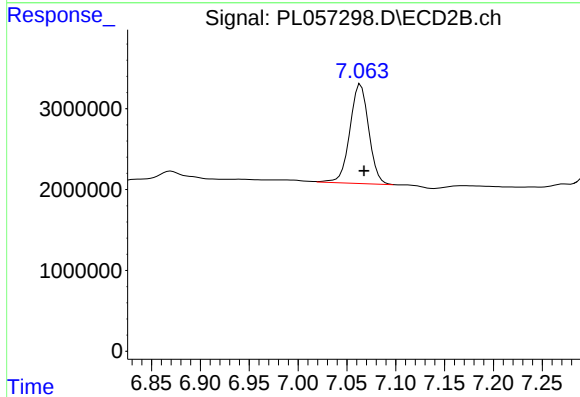


#17 4,4'-DDT

R.T.: 7.063 min
Delta R.T.: -0.005 min
Response: 16511154
Conc: 6.71 ng/ml m

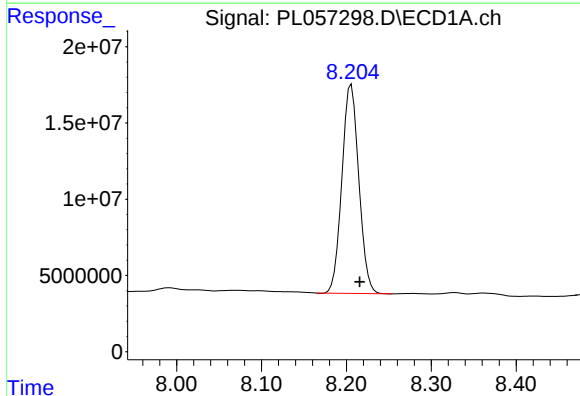

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.010 min
Response: 189364848
Conc: 19.59 ng/ml

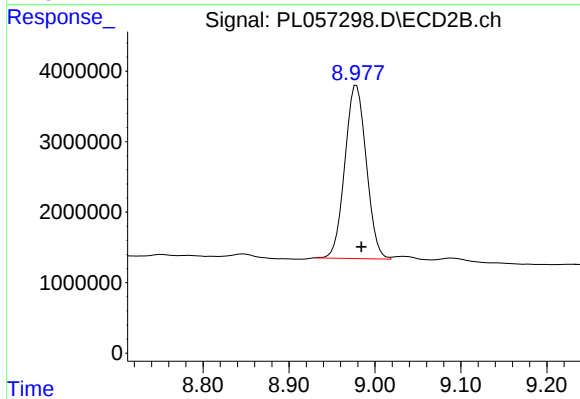

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.006 min
Response: 42611392
Conc: 20.05 ng/ml