

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031225\
 Data File : PL094623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2025 09:44
 Operator : AR\AJ
 Sample : Q1494-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PURGE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 13:25:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.772	59597808	70666438	21.054	19.799
28)	SA Decachlor...	9.062	7.907	48083632	87759174	22.816	21.726
Target Compounds							
7)	B delta-BHC	4.770	0.000	15583469	0	4.002	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031225\
Data File : PL094623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2025 09:44
Operator : AR\AJ
Sample : Q1494-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PURGE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 13:25:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

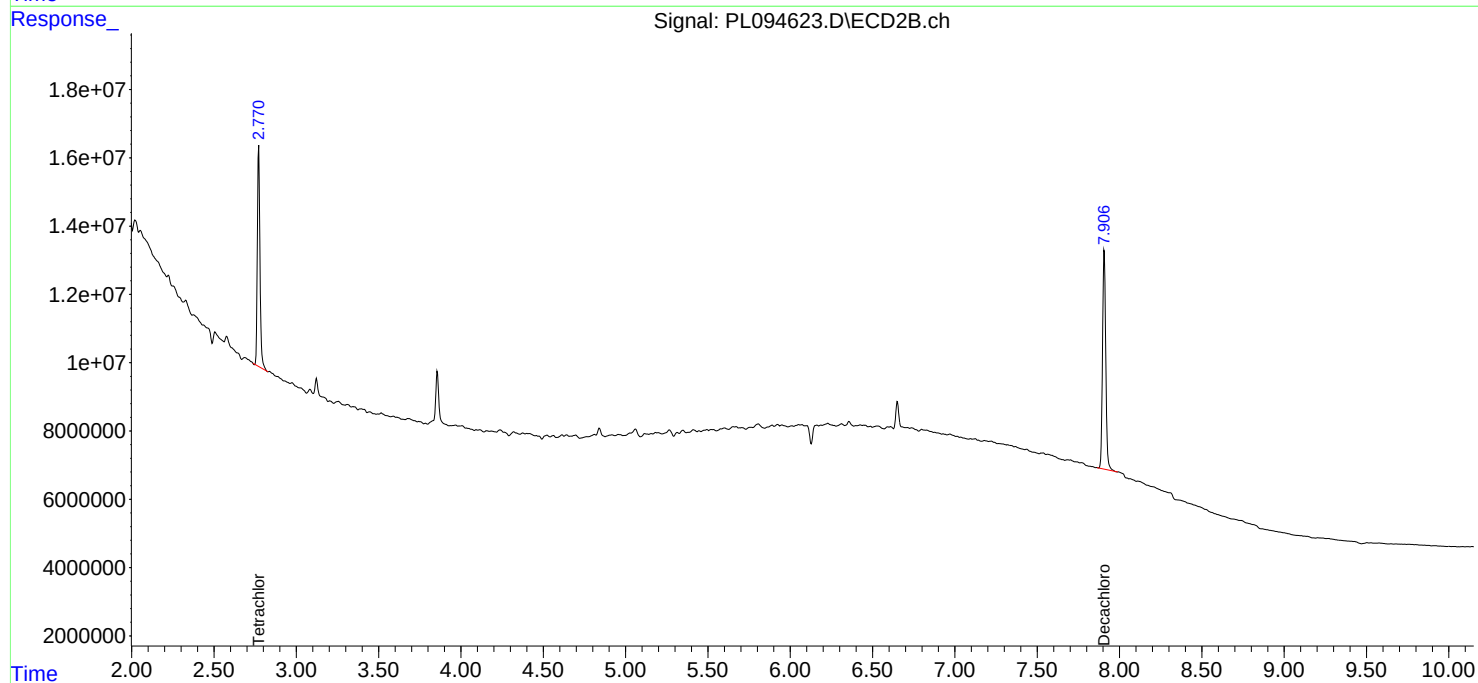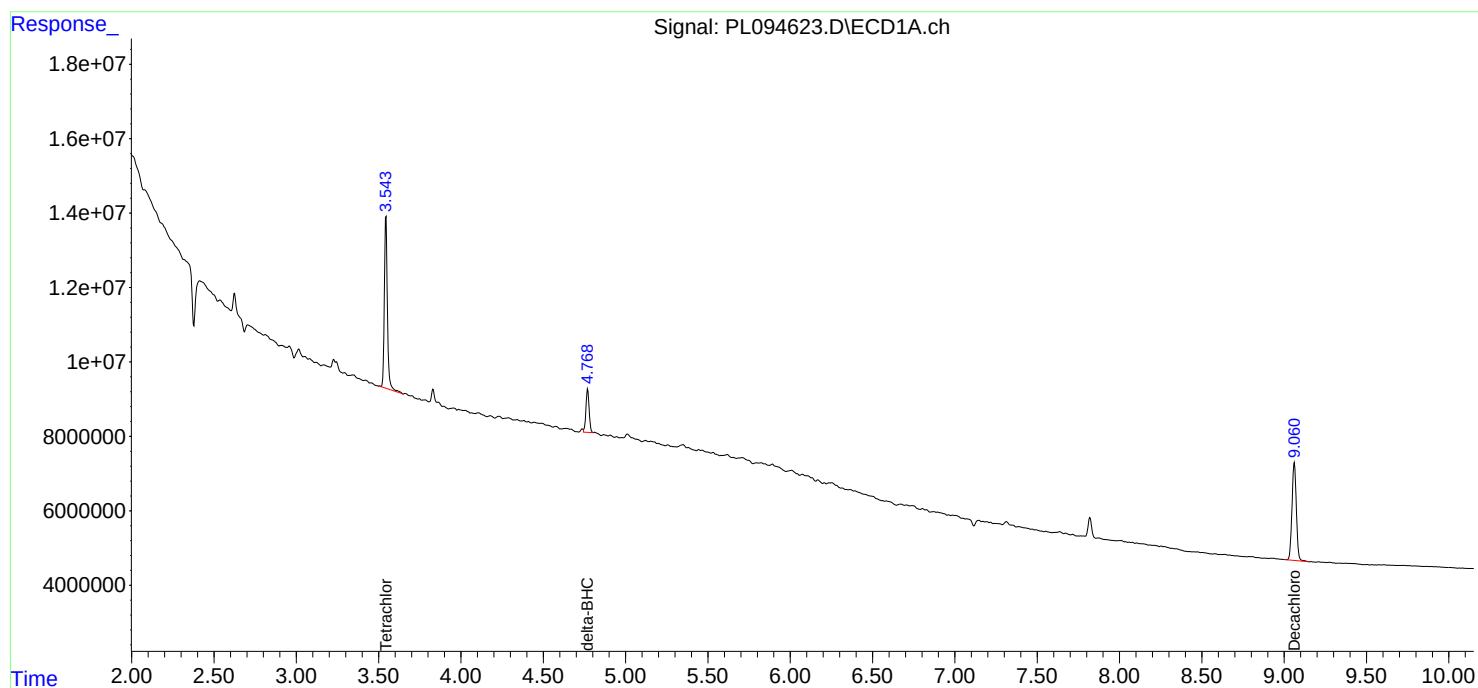


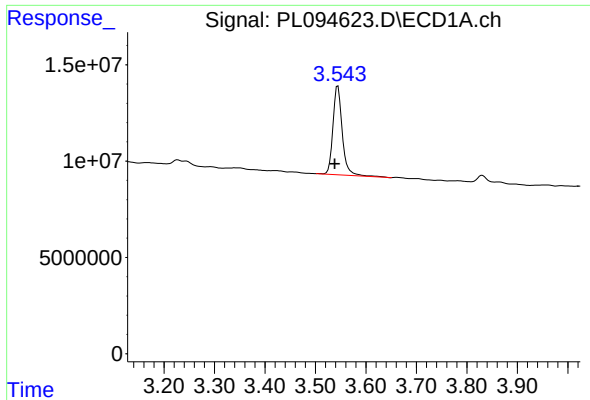

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.006 min
Response: 59597808
Conc: 21.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PURGE-WATER

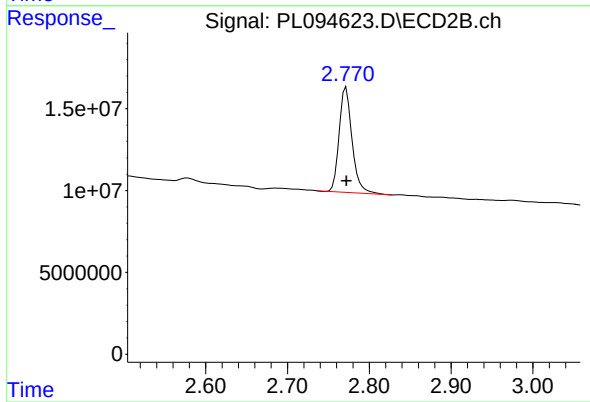


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 70666438
Conc: 19.80 ng/ml

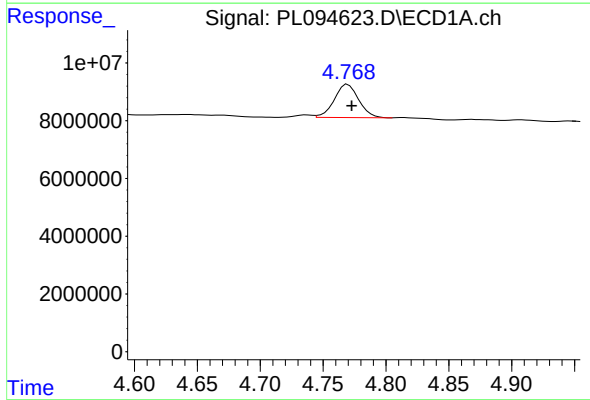


#7 delta-BHC

R.T.: 4.770 min
Delta R.T.: -0.003 min
Response: 15583469
Conc: 4.00 ng/ml

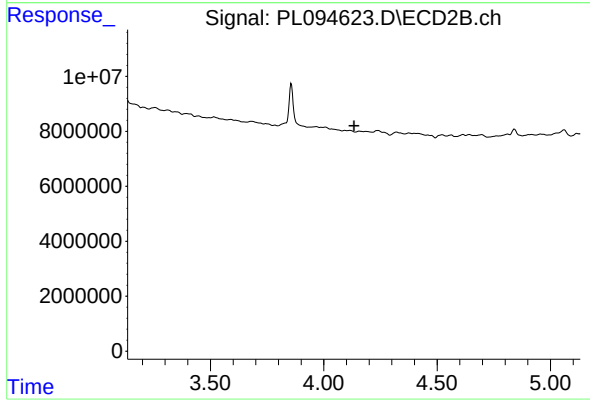

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.133 min
Response: 0
Conc: N.D.

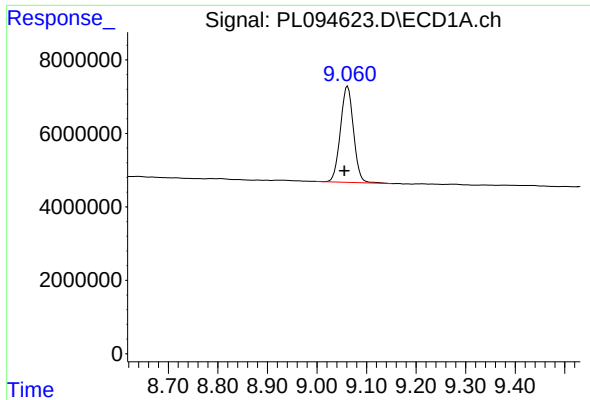

#28 Decachlorobiphenyl

R.T.: 9.062 min
Delta R.T.: 0.006 min
Response: 48083632
Conc: 22.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PURGE-WATER

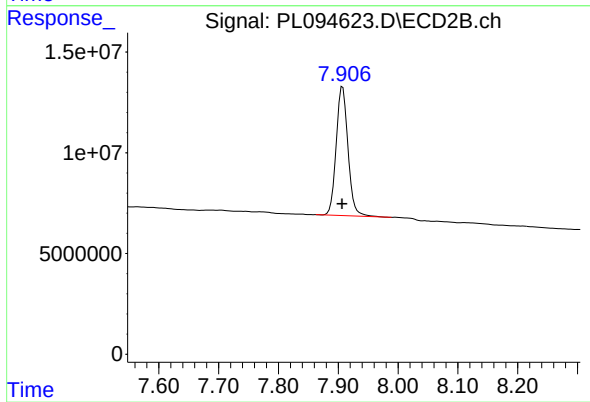

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 87759174
Conc: 21.73 ng/ml