

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031225\
 Data File : PL094643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2025 17:20
 Operator : AR\AJ
 Sample : PB167091BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB167091BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/13/2025
 Supervised By : mohammad ahmed 03/28/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 05:34:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.771	64844707	78576282	22.908m	22.015
28) SA Decachlor...	9.061	7.906	60778441	100.7E6	28.840	24.931

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031225\
Data File : PL094643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2025 17:20
Operator : AR\AJ
Sample : PB167091BL
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB167091BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/13/2025
Supervised By : mohammad ahmed 03/28/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 05:34:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

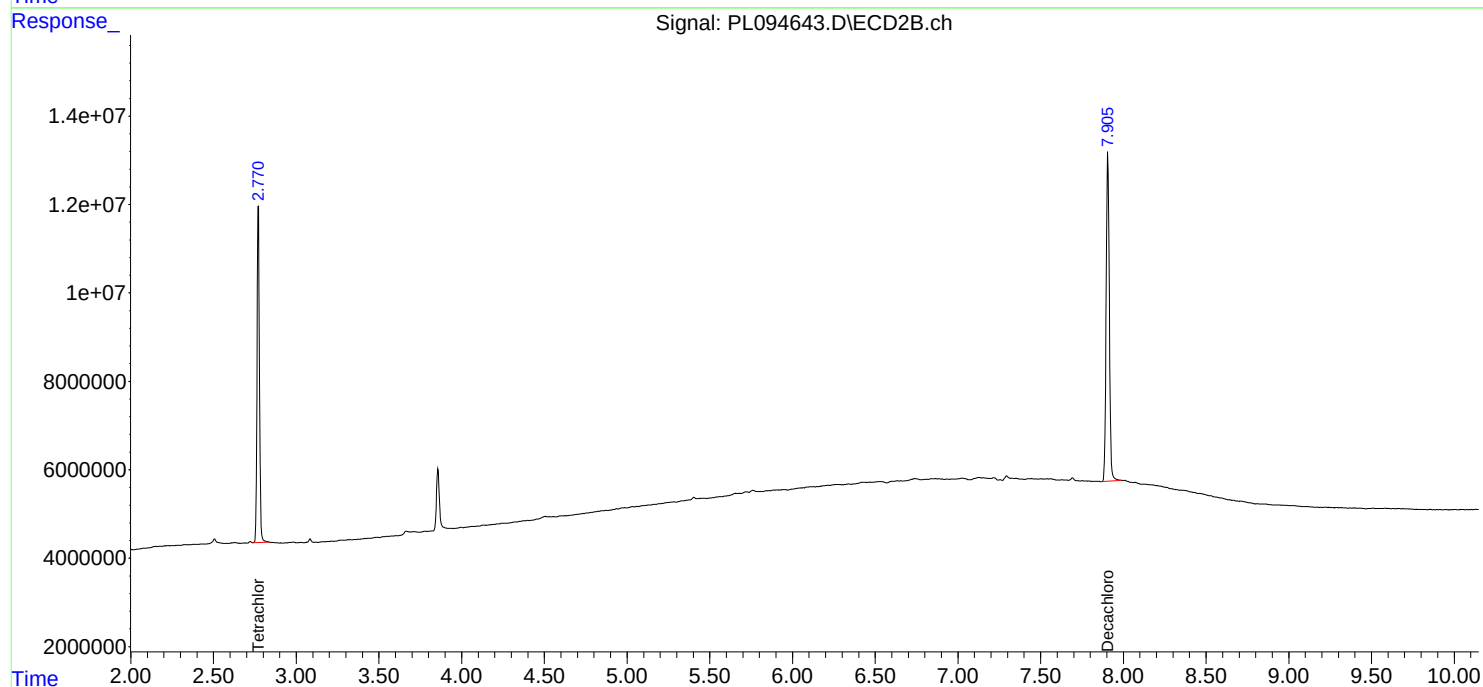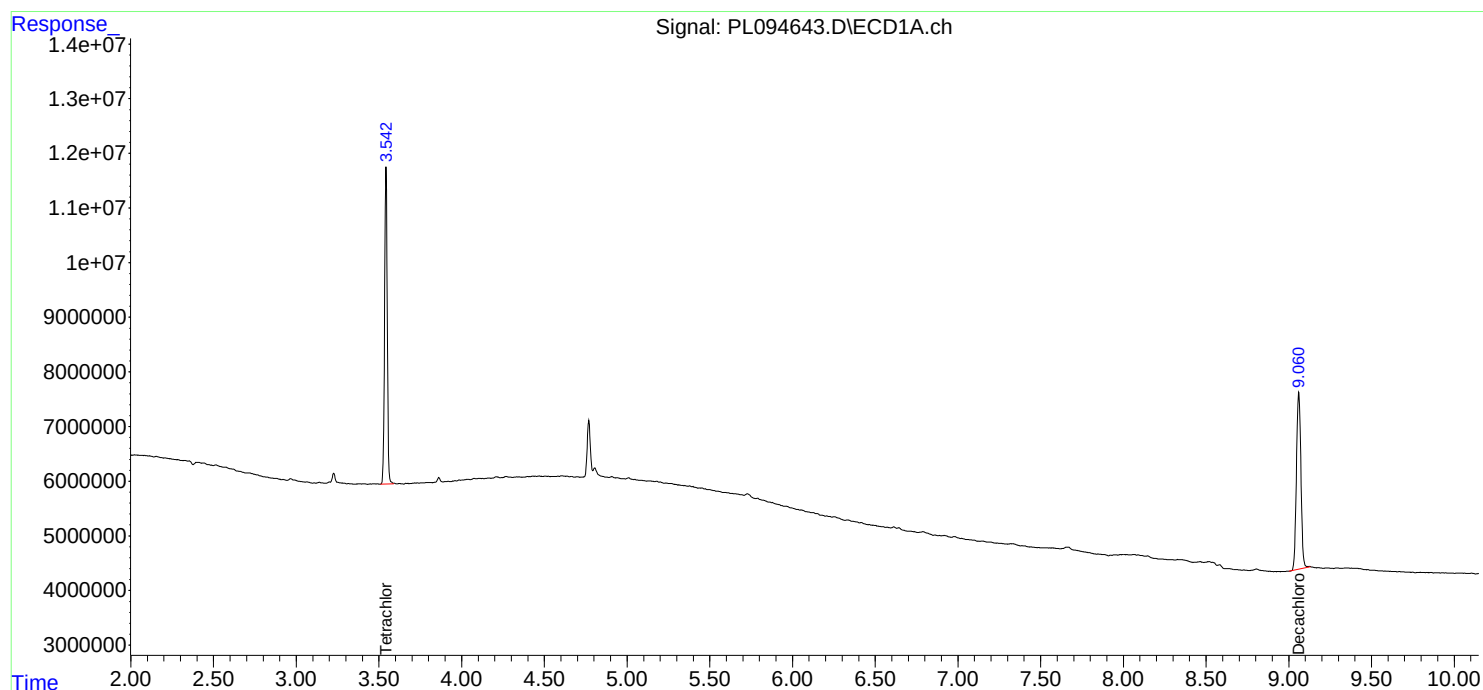

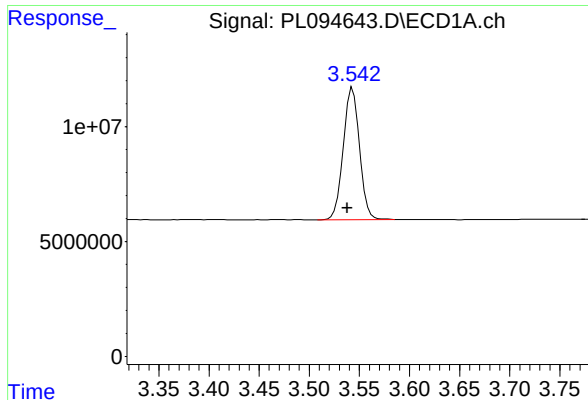

#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: 0.004 min
Response: 64844707
Conc: 22.91 ng/ml

Instrument :


ECD_L

ClientSampleId :

PB167091BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/13/2025
Supervised By :mohammad ahmed 03/28/2025

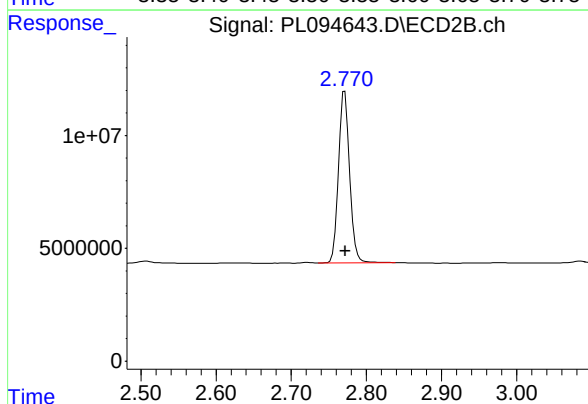


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 78576282
Conc: 22.01 ng/ml

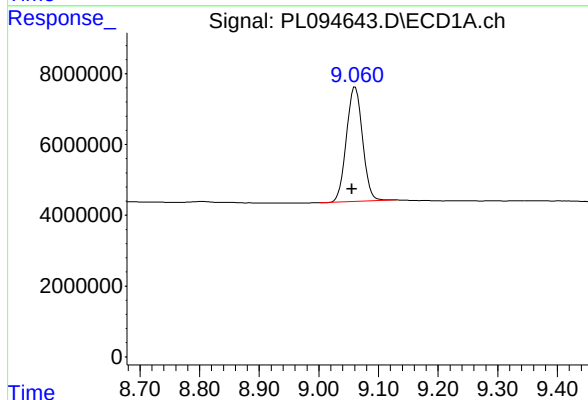

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.005 min
Response: 60778441
Conc: 28.84 ng/ml

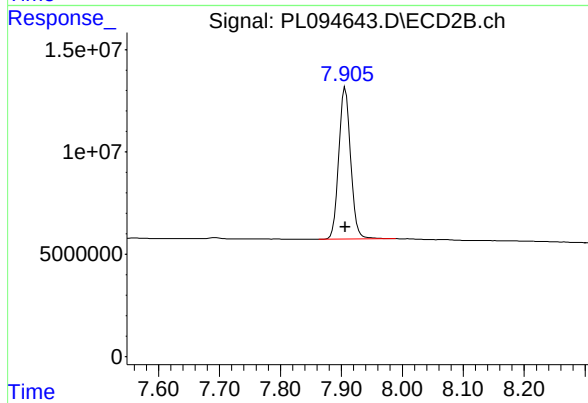

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: 0.000 min
Response: 100703923
Conc: 24.93 ng/ml