

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL031319\  
 Data File : PL045809.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 13 Mar 2019 09:13  
 Operator : AJ\SJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 HEXANE

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 13 10:38:38 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL022719.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Feb 27 17:00:03 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |              |        |        |          |          |               |
|------------------|--------------|--------|--------|----------|----------|---------------|
| 8) B             | Heptachlo... | 0.000  | 5.849  | 0        | 43434601 | N.D. 18.083 # |
| 14) MA           | Endrin       | 5.881f | 0.000  | 11545277 | 0        | 1.282 N.D. #  |
| 16) A            | 4,4'-DDD     | 0.000  | 6.829f | 0        | 1395340  | N.D. 0.726 #  |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL031319\  
Data File : PL045809.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 13 Mar 2019 09:13  
Operator : AJ\SJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 13 10:38:38 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL022719.M  
Quant Title : GC Extractables  
QLast Update : Wed Feb 27 17:00:03 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

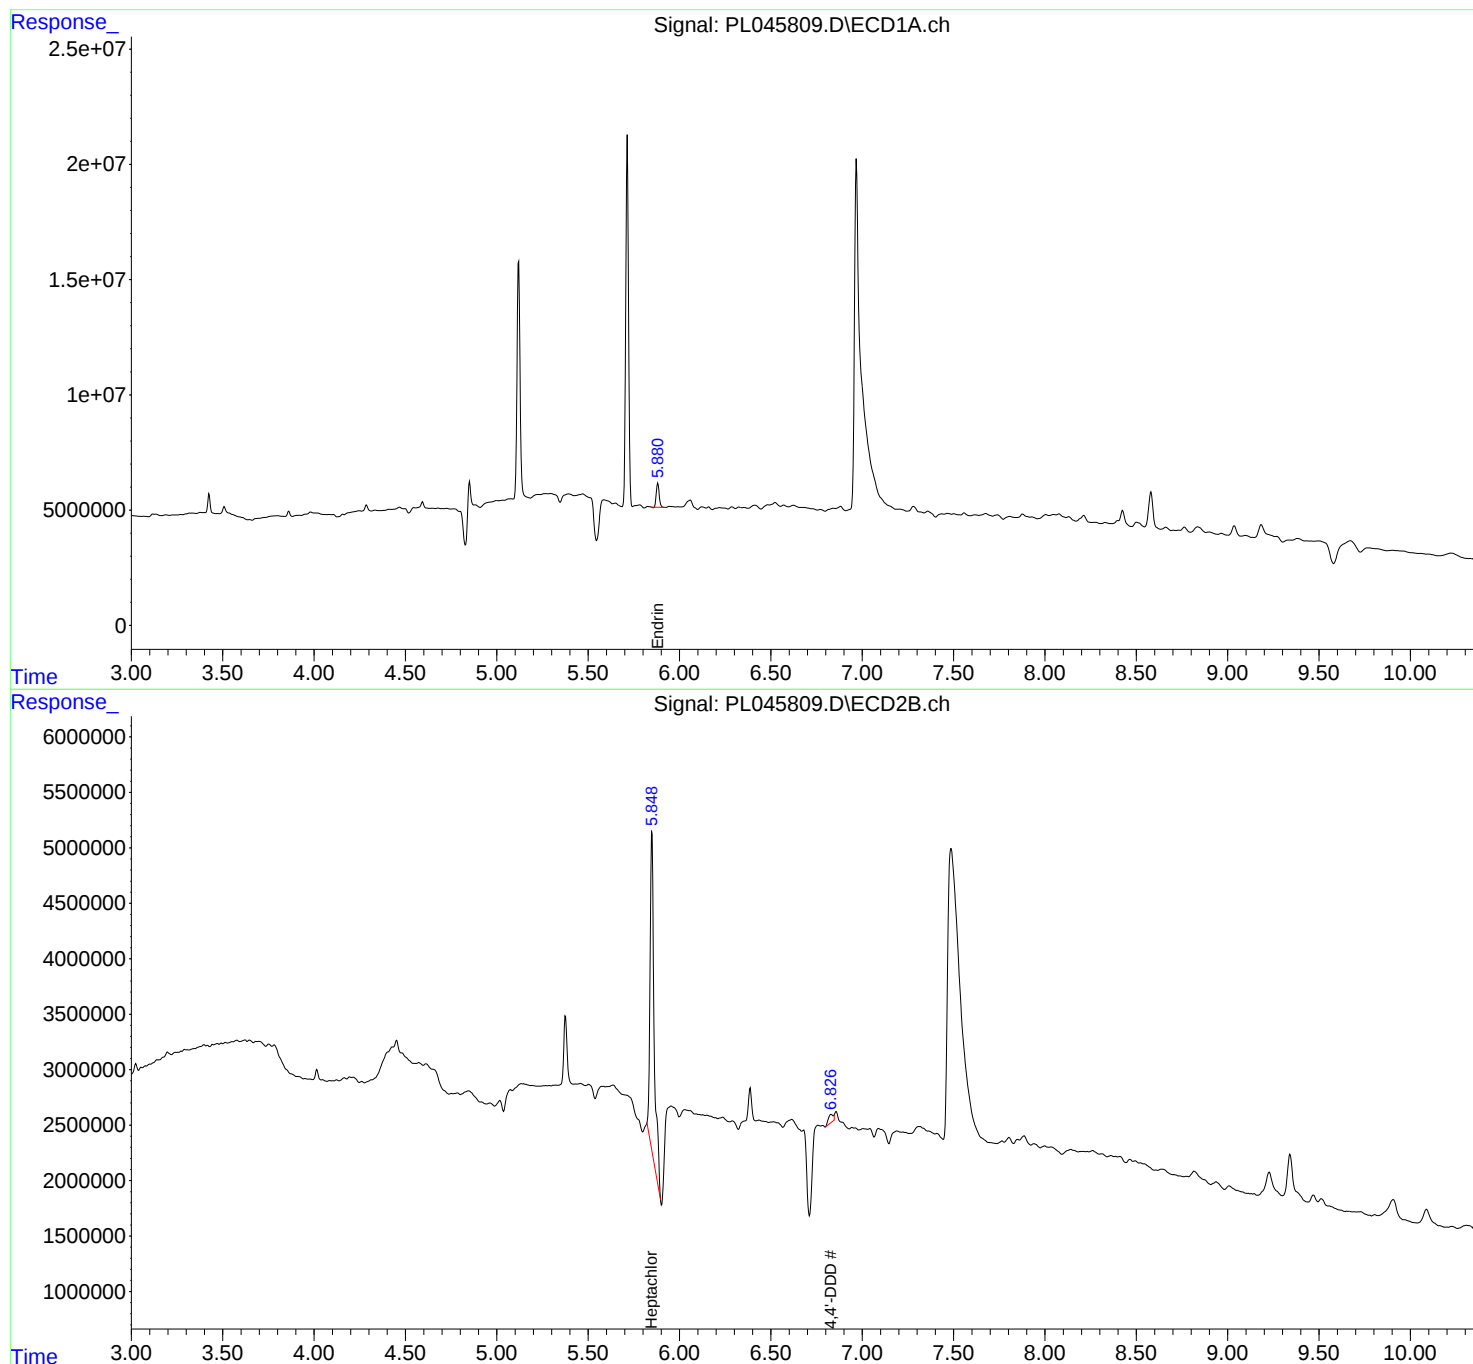


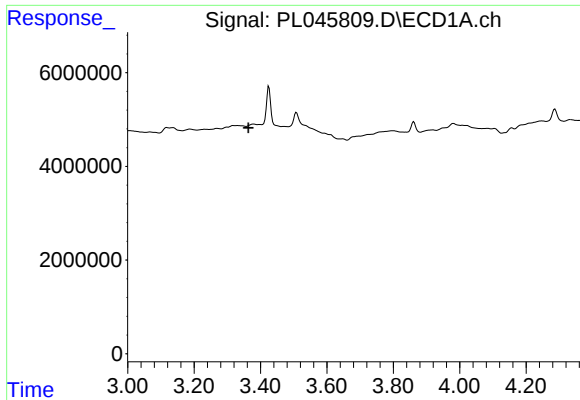

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 3.363 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

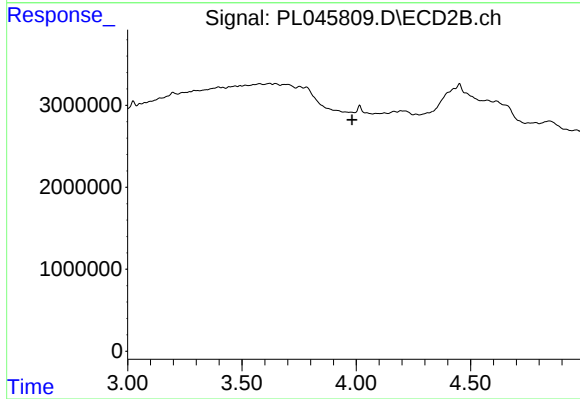


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 3.982 min  
Response: 0  
Conc: N.D.

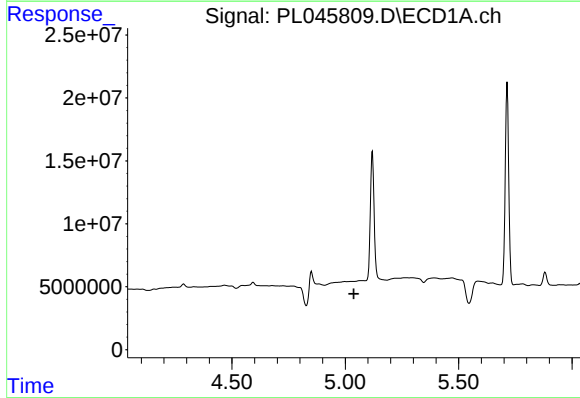


#8 Heptachlor epoxide

R.T.: 0.000 min  
Exp R.T. : 5.037 min  
Response: 0  
Conc: N.D.

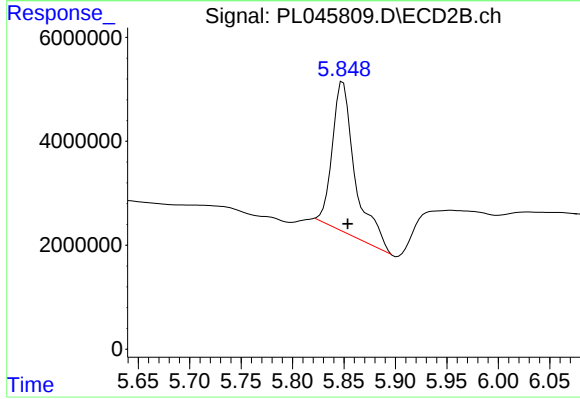

#8 Heptachlor epoxide


R.T.: 5.849 min  
Delta R.T.: -0.005 min  
Response: 43434601  
Conc: 18.08 ng/ml

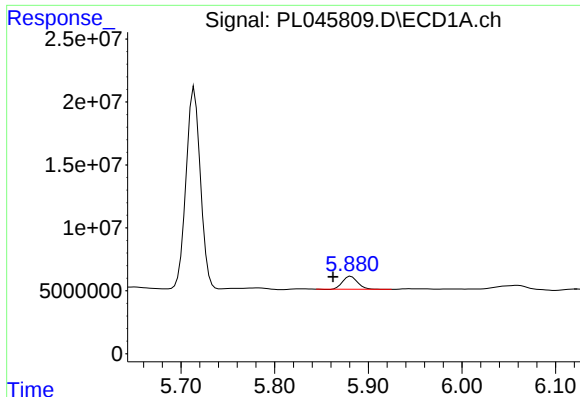

#14 Endrin


R.T.: 5.881 min  
Delta R.T.: 0.019 min  
Response: 11545277  
Conc: 1.28 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

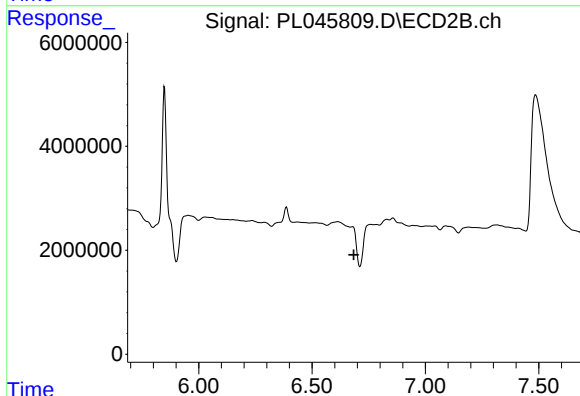


#14 Endrin

R.T.: 0.000 min  
Exp R.T. : 6.684 min  
Response: 0  
Conc: N.D.

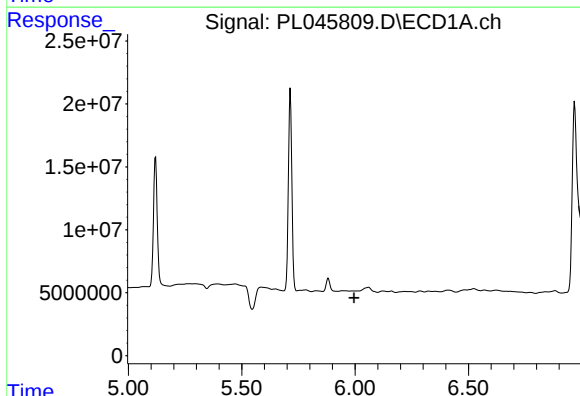


#16 4,4'-DDD

R.T.: 0.000 min  
Exp R.T. : 5.996 min  
Response: 0  
Conc: N.D.

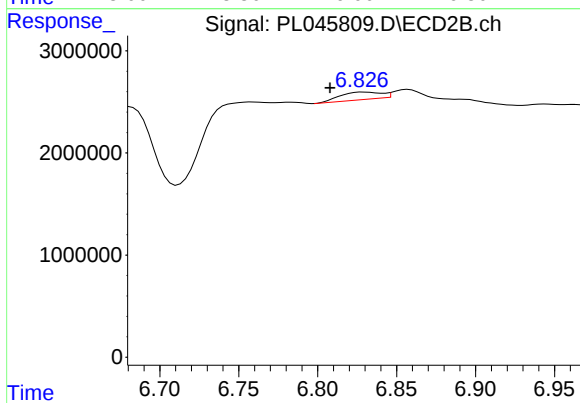

#16 4,4'-DDD


R.T.: 6.829 min  
Delta R.T.: 0.022 min  
Response: 1395340  
Conc: 0.73 ng/ml

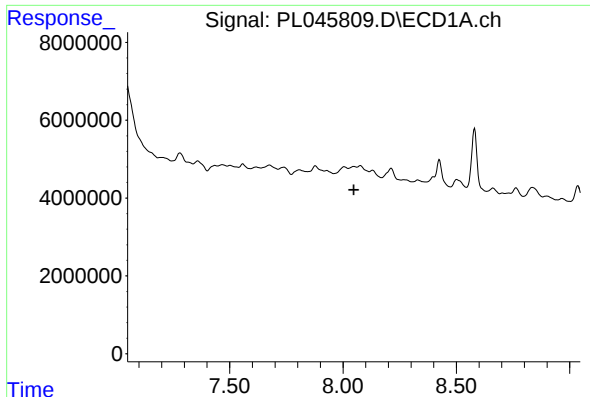

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.047 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

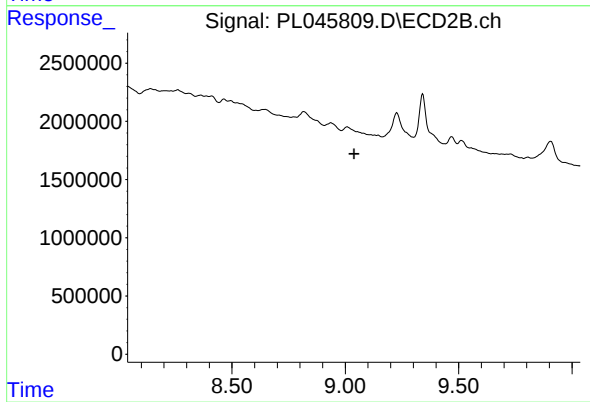

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 9.039 min  
Response: 0  
Conc: N.D.