

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031319\
 Data File : PL045830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2019 16:16
 Operator : AJ\SJ
 Sample : K1824-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-28

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:05:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.362	3.980	134.2E6	42526452	19.510	19.858
28) SA Decachlor...	8.042	9.035	143.5E6	41990658	17.146	18.377
Target Compounds						
12) B 4,4'-DDE	0.000	6.315	0	1541570	N.D.	0.660 #
17) MA 4,4'-DDT	0.000	7.104	0	1828779	N.D.	0.927 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031319\
Data File : PL045830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2019 16:16
Operator : AJ\SJ
Sample : K1824-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-28

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:05:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

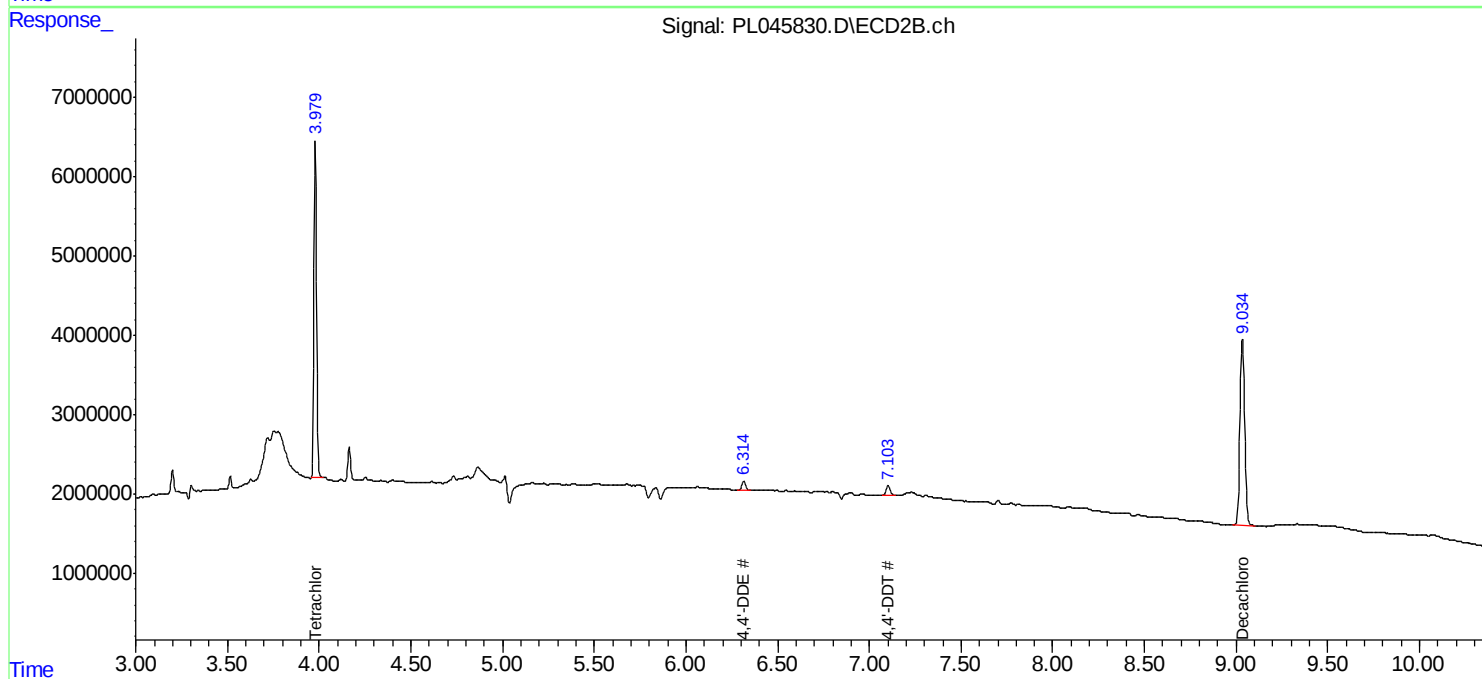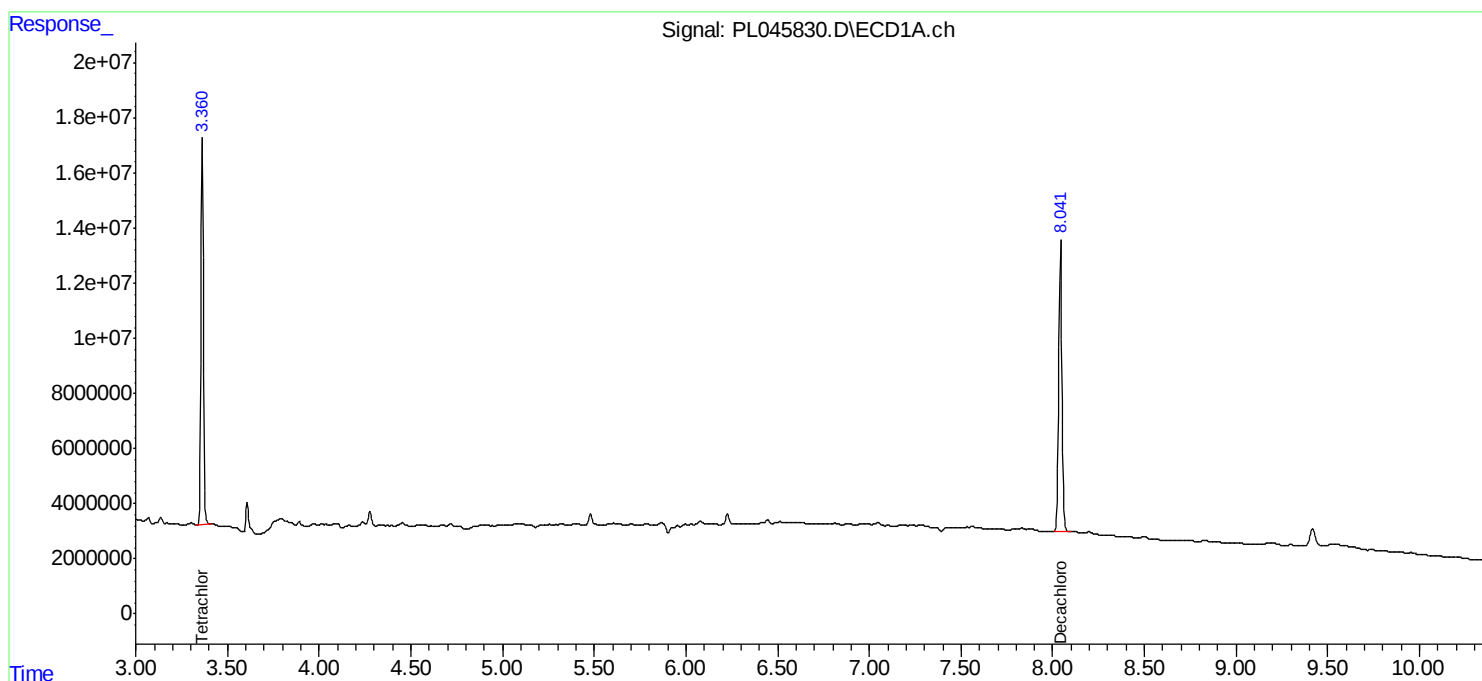


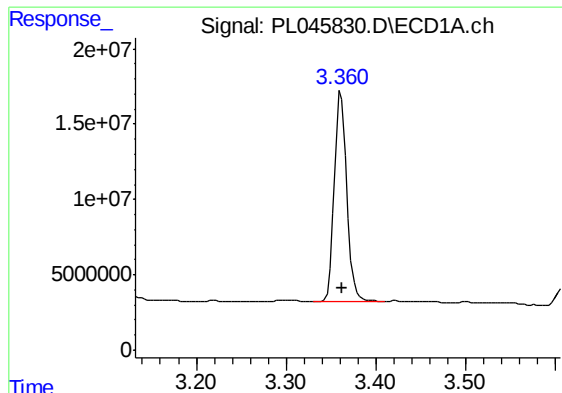

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: -0.001 min
Response: 134214678
Conc: 19.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-28

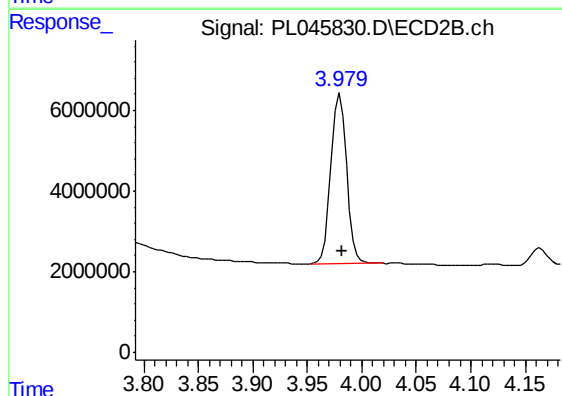


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 42526452
Conc: 19.86 ng/ml

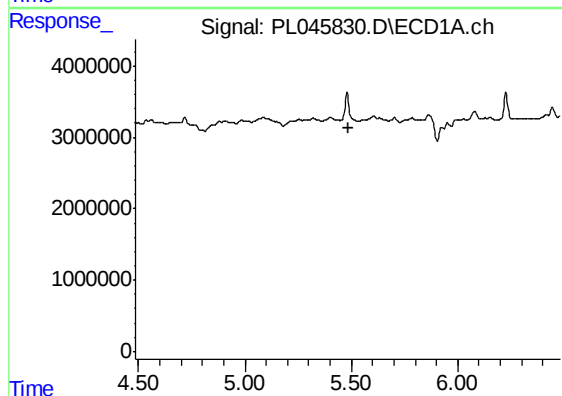


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.484 min
Response: 0
Conc: N.D.

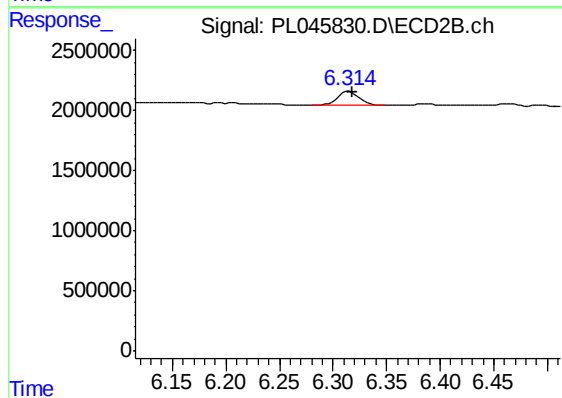

#12 4,4'-DDE


R.T.: 6.315 min
Delta R.T.: -0.003 min
Response: 1541570
Conc: 0.66 ng/ml

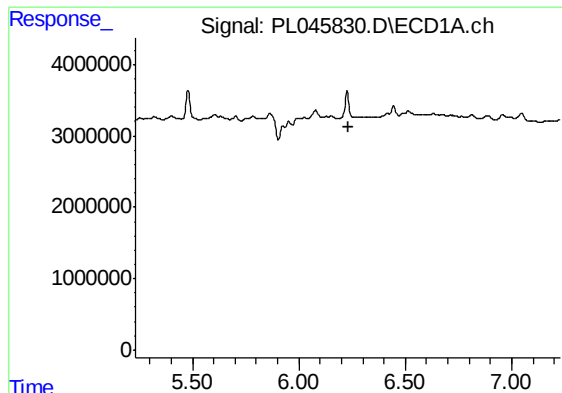

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-28

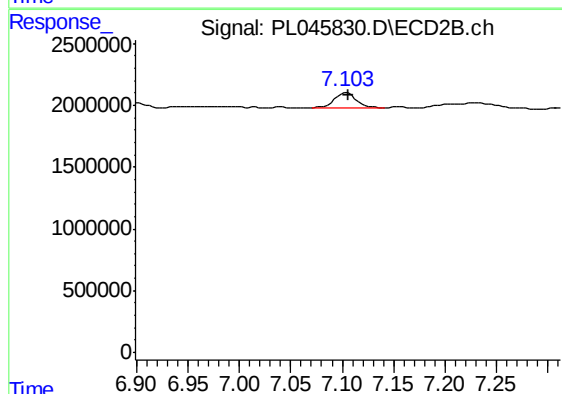


#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: -0.002 min
Response: 1828779
Conc: 0.93 ng/ml

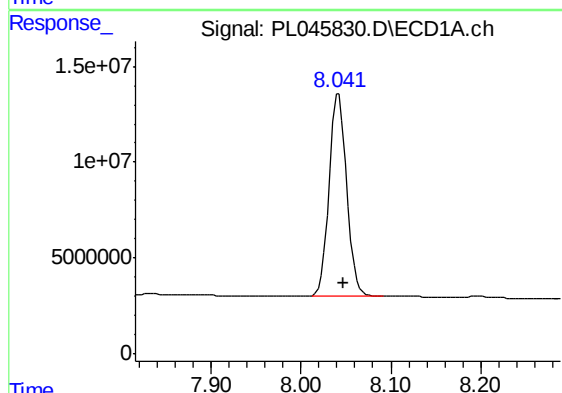

#28 Decachlorobiphenyl

R.T.: 8.042 min
Delta R.T.: -0.005 min
Response: 143465563
Conc: 17.15 ng/ml

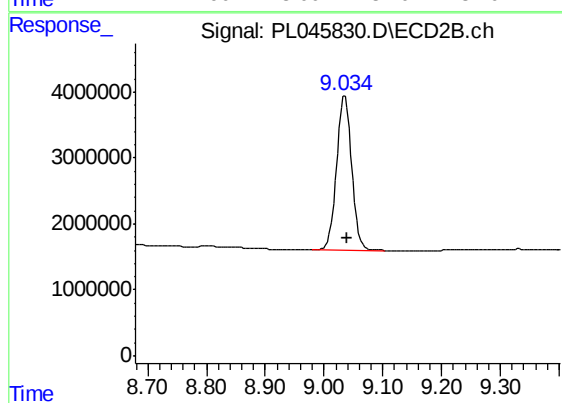

#28 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: -0.004 min
Response: 41990658
Conc: 18.38 ng/ml