

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031319\
 Data File : PL045846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2019 20:25
 Operator : AJ\SJ
 Sample : K1869-09
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:08:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	107.2E6	34873567	15.587	16.284
28)	SA Decachlor...	8.042	9.036	86902594	25674679	10.386	11.237
Target Compounds							
15)	B Endosulfa...	0.000	6.908	0	3139709	N.D.	1.335 #
19)	B Endosulfa...	6.531f	0.000	8141184	0	1.002	N.D. #
23)	Chlordane-1	4.219	0.000	6001239	0	17.811	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031319\
Data File : PL045846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2019 20:25
Operator : AJ\SJ
Sample : K1869-09
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:08:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

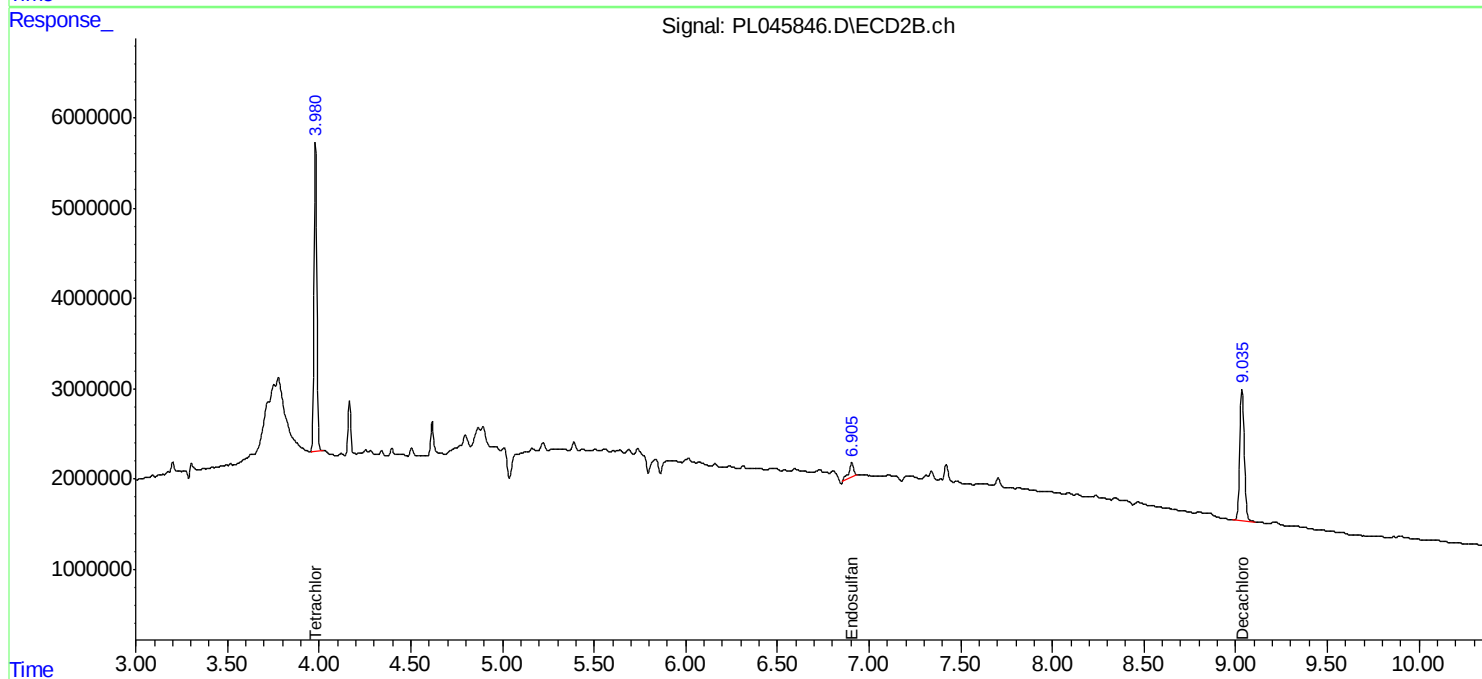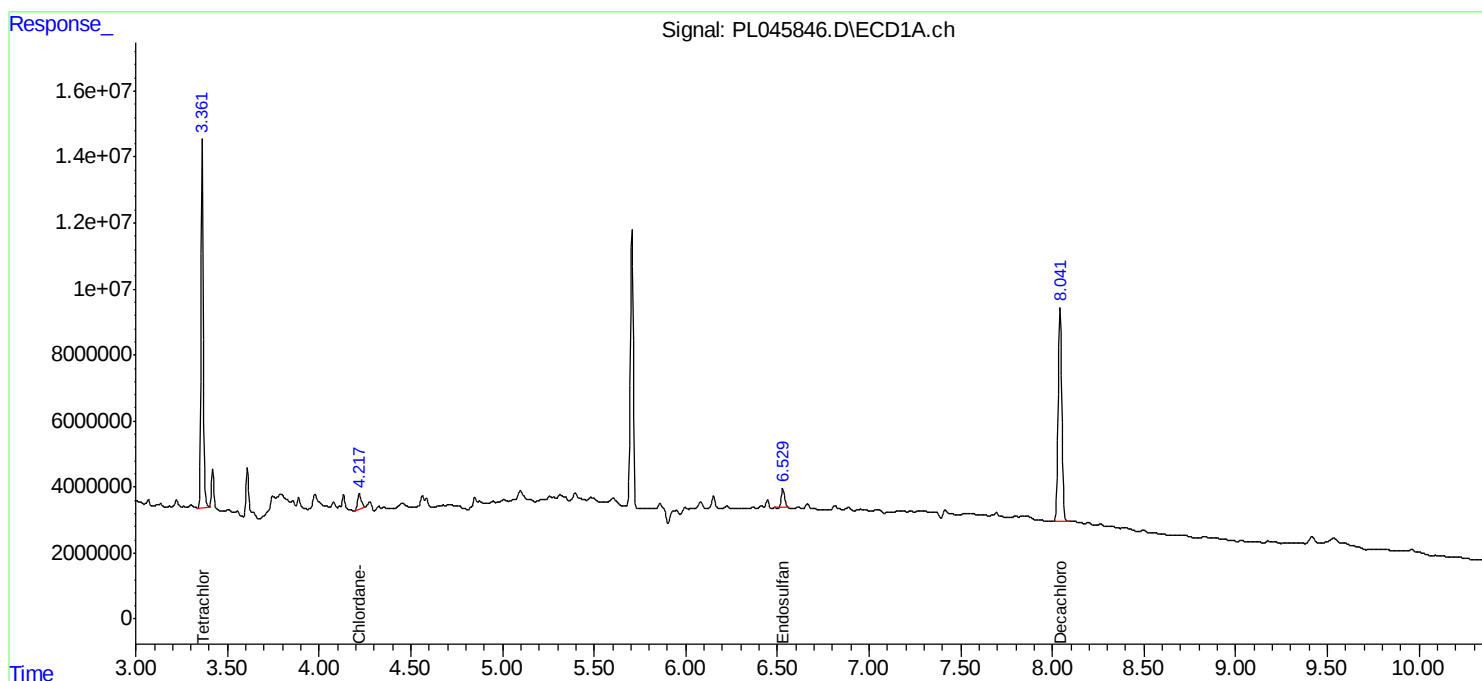


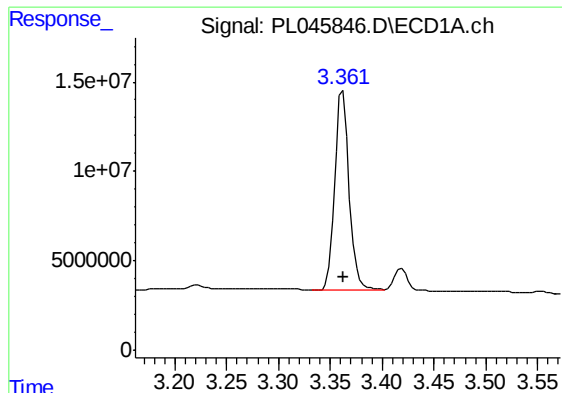

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 107227993
Conc: 15.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-2

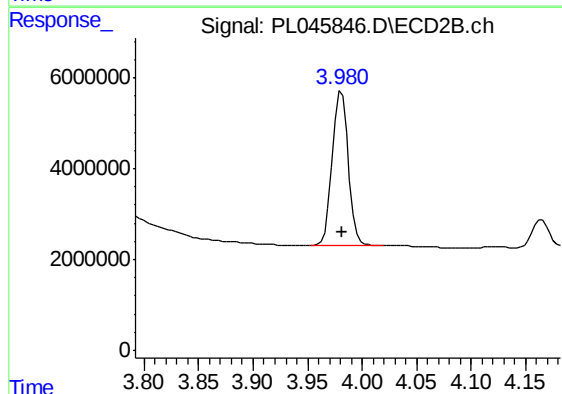


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 34873567
Conc: 16.28 ng/ml

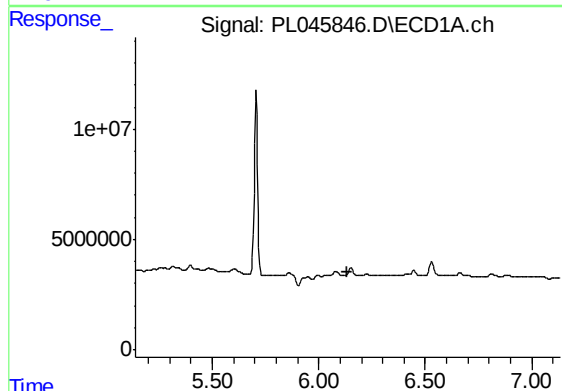


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.137 min
Response: 0
Conc: N.D.

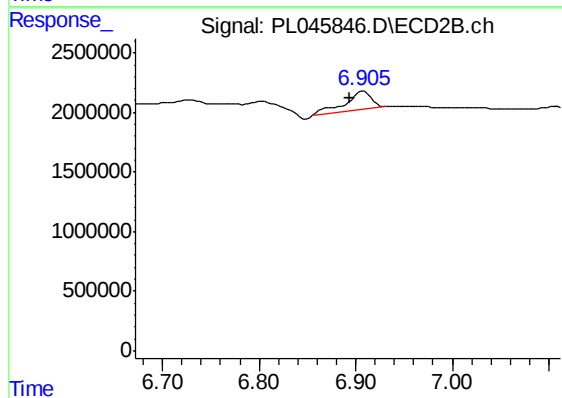

#15 Endosulfan II


R.T.: 6.908 min
Delta R.T.: 0.014 min
Response: 3139709
Conc: 1.34 ng/ml

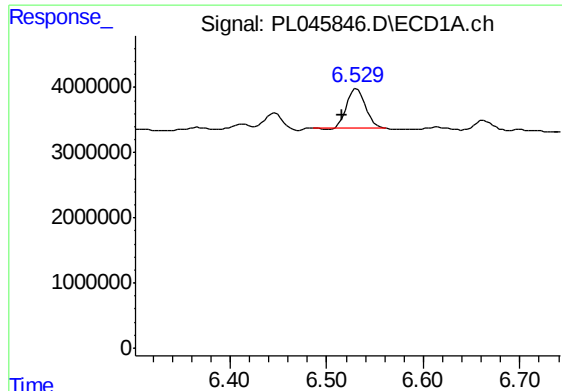

#19 Endosulfan Sulfate


R.T.: 6.531 min
Delta R.T.: 0.015 min
Response: 8141184
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-2

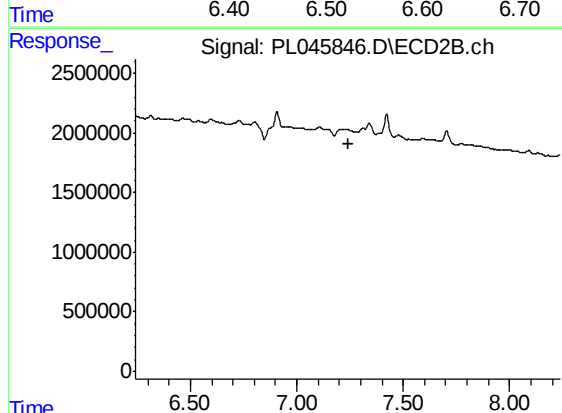


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.241 min
Response: 0
Conc: N.D.

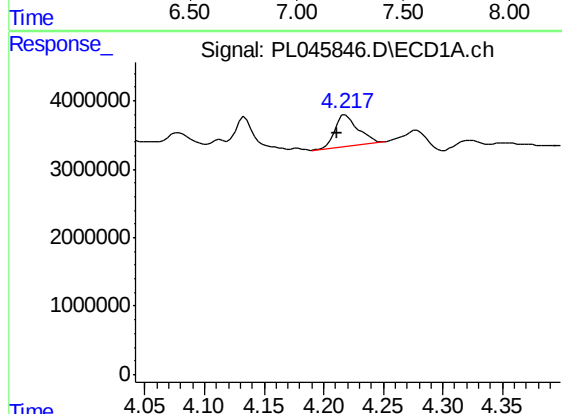


#23 Chlordane-1

R.T.: 4.219 min
Delta R.T.: 0.008 min
Response: 6001239
Conc: 17.81 ng/ml

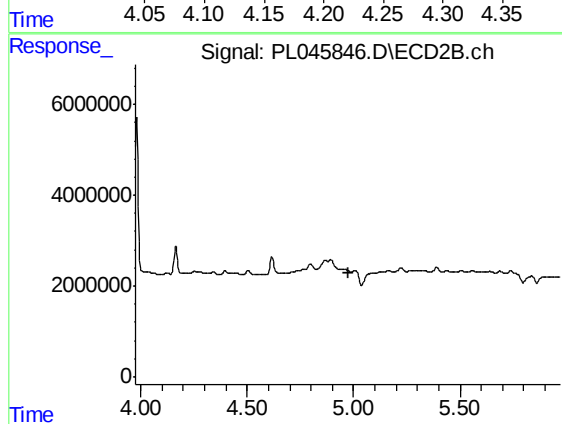

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

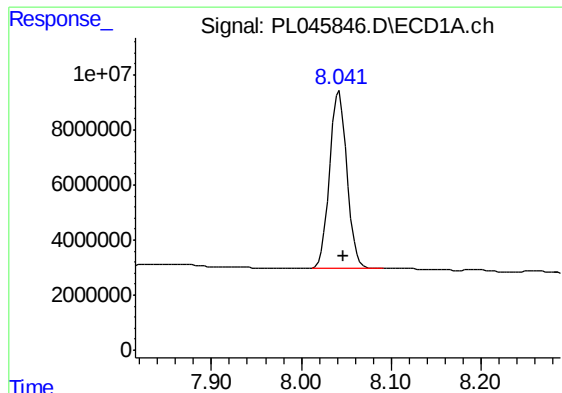

#28 Decachlorobiphenyl

R.T.: 8.042 min
Delta R.T.: -0.005 min
Response: 86902594
Conc: 10.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-2

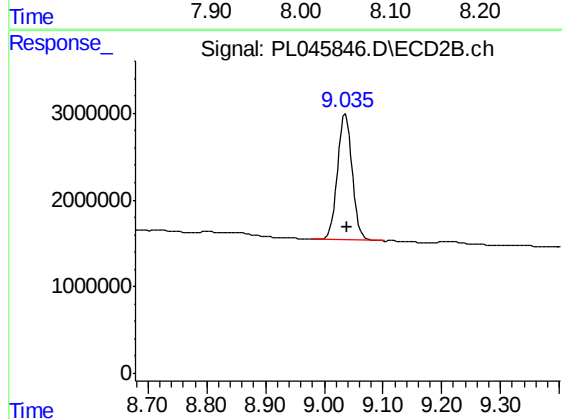

#28 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: -0.003 min
Response: 25674679
Conc: 11.24 ng/ml