

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031319\
 Data File : PL045877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2019 04:13
 Operator : AJ\SJ
 Sample : K1871-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 06:05:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.981	49992178	16488818	7.267	7.700
28)	SA Decachlor...	8.043	9.036	101.5E6	30922119	12.127	13.533
Target Compounds							
8)	B Heptachlo...	0.000	5.845	0	1468806	N.D.	0.612 #
10)	B gamma-Chl...	5.234f	0.000	6609143	0	0.675	N.D. #
13)	MA Dieldrin	5.623	6.458	7383263	2733806	0.772	1.064 #
14)	MA Endrin	0.000	6.676	0	1516600	N.D.	0.667 #
16)	A 4,4'-DDD	0.000	6.813	0	6299271	N.D.	3.276 #
17)	MA 4,4'-DDT	6.223	0.000	17674968	0	2.357	N.D. #
18)	B Endrin al...	6.315	0.000	6937577	0	0.949	N.D. #
19)	B Endosulfa...	6.506	0.000	14029001	0	1.726	N.D. #
20)	A Methoxychlor	6.751f	0.000	13116553	0	2.987	N.D. #
21)	B Endrin ke...	7.022f	0.000	7121714	0	0.773	N.D. #
25)	Chlordane-3	5.234f	0.000	6609143	0	5.762	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031319\
Data File : PL045877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2019 04:13
Operator : AJ\SJ
Sample : K1871-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 06:05:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

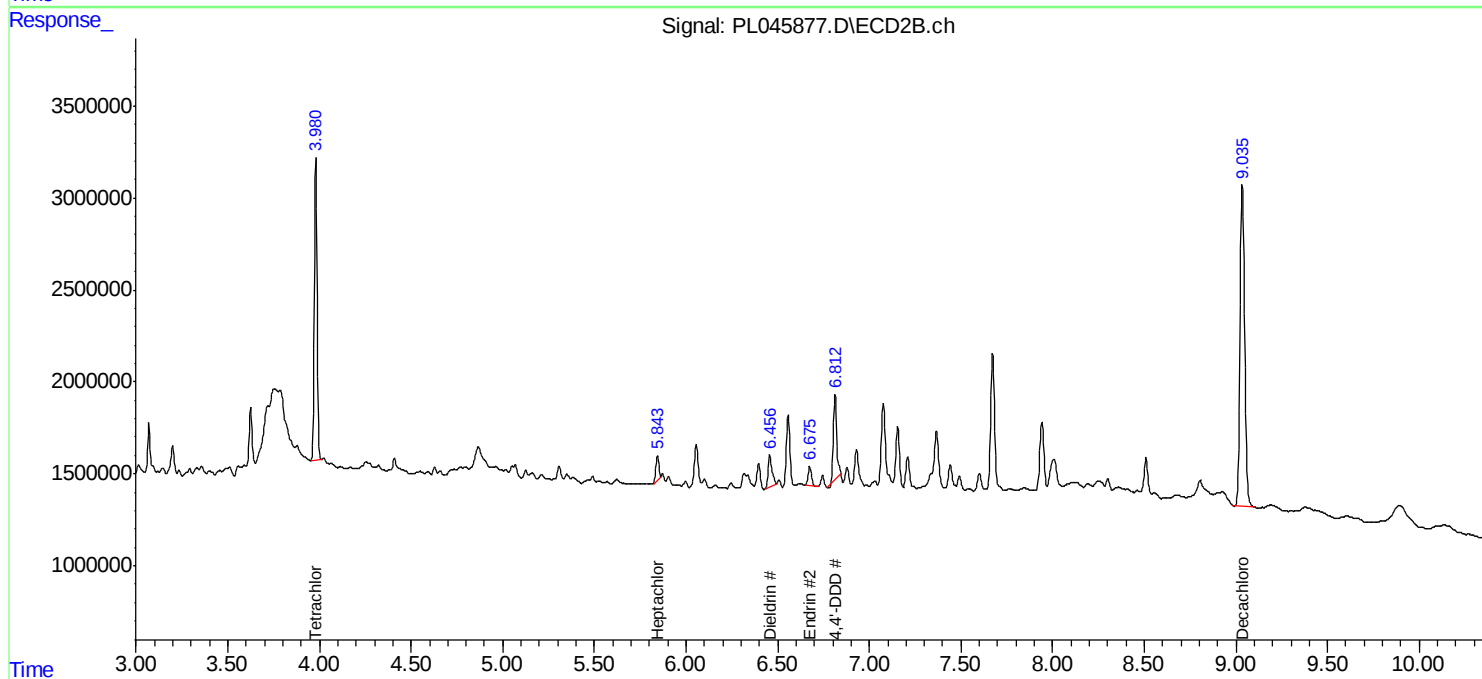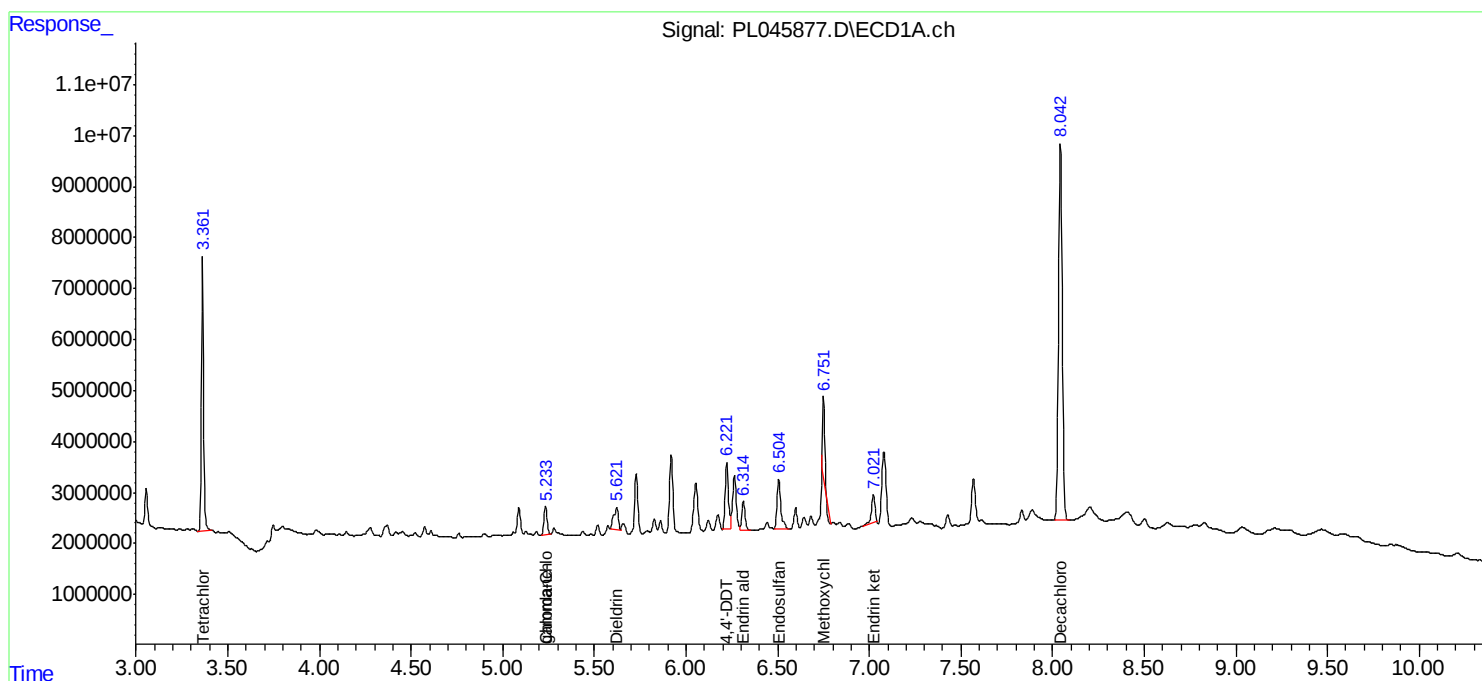


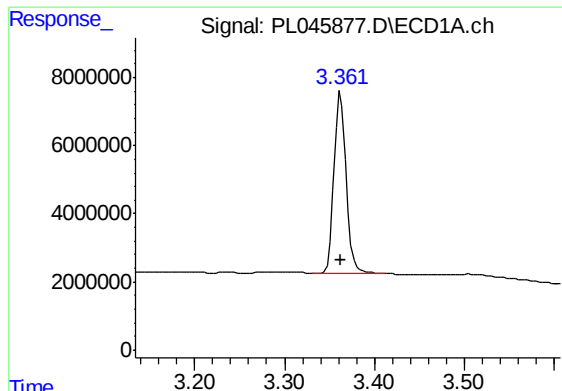

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 49992178
Conc: 7.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

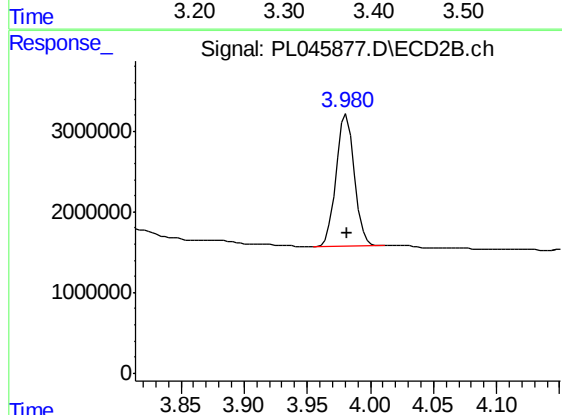


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 16488818
Conc: 7.70 ng/ml

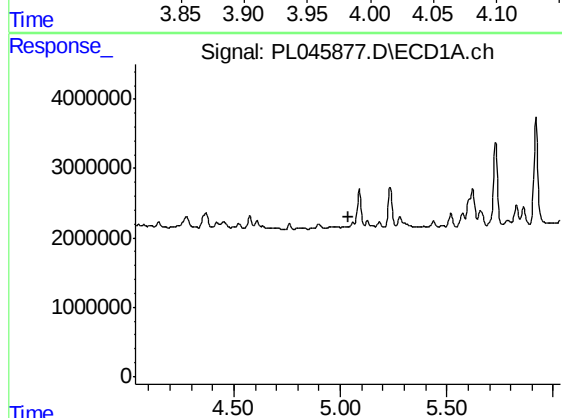


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

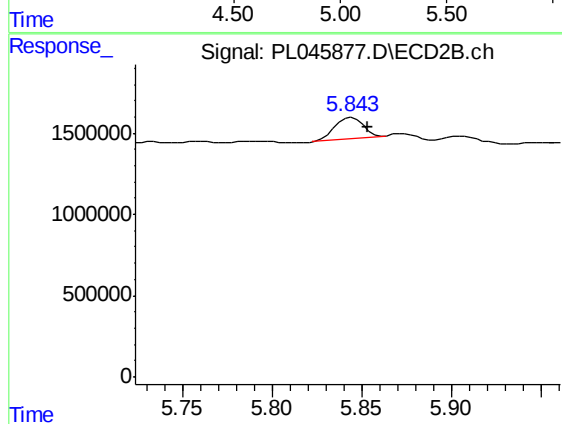

#8 Heptachlor epoxide


R.T.: 5.845 min
Delta R.T.: -0.009 min
Response: 1468806
Conc: 0.61 ng/ml

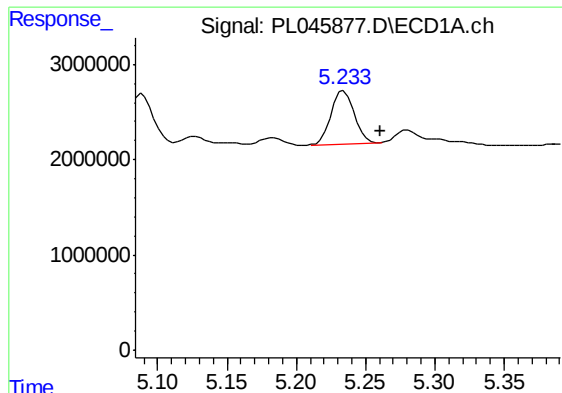

#10 gamma-Chlordane


R.T.: 5.234 min
Delta R.T.: -0.026 min
Response: 6609143
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

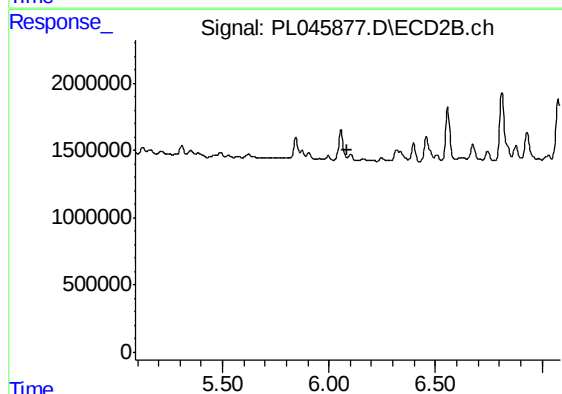


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

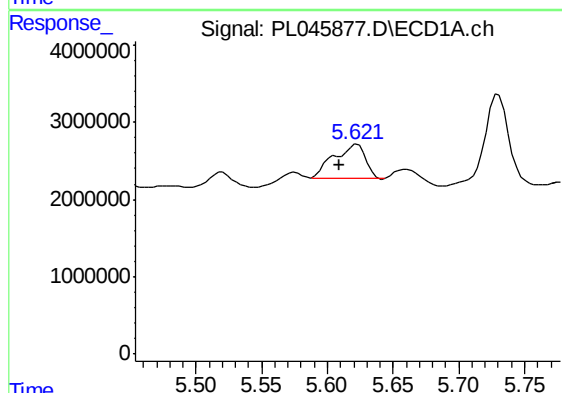


#13 Dieldrin

R.T.: 5.623 min
Delta R.T.: 0.014 min
Response: 7383263
Conc: 0.77 ng/ml

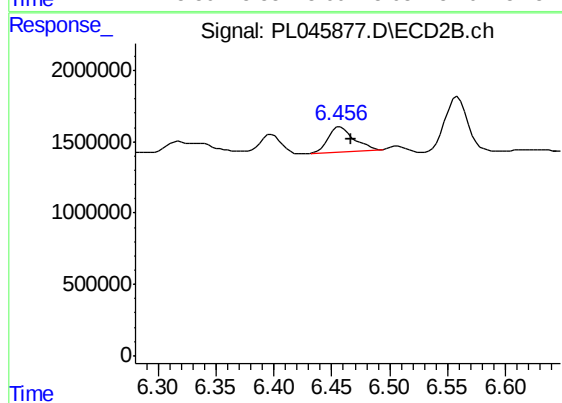

#13 Dieldrin


R.T.: 6.458 min
Delta R.T.: -0.009 min
Response: 2733806
Conc: 1.06 ng/ml

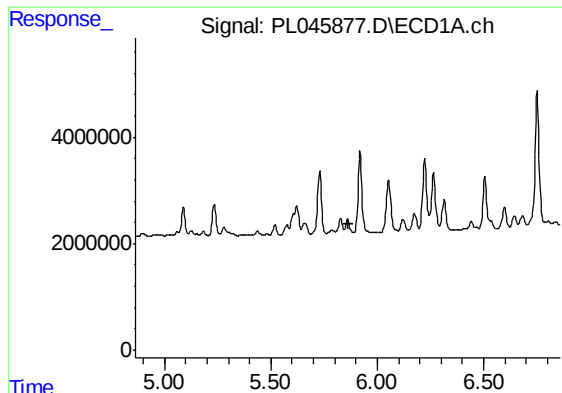

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.862 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

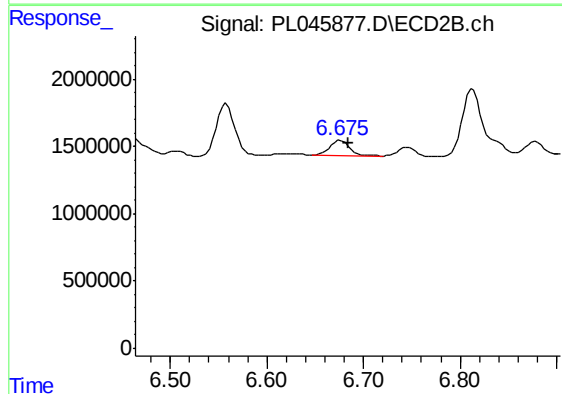


#14 Endrin

R.T.: 6.676 min
Delta R.T.: -0.008 min
Response: 1516600
Conc: 0.67 ng/ml

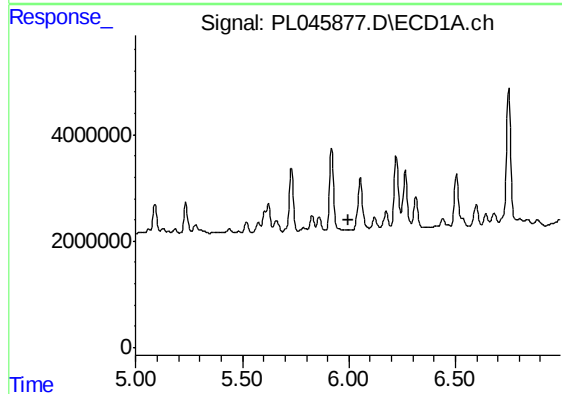


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

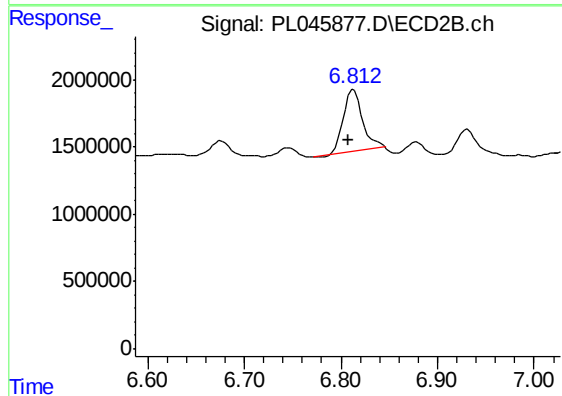

#16 4,4'-DDD


R.T.: 6.813 min
Delta R.T.: 0.005 min
Response: 6299271
Conc: 3.28 ng/ml

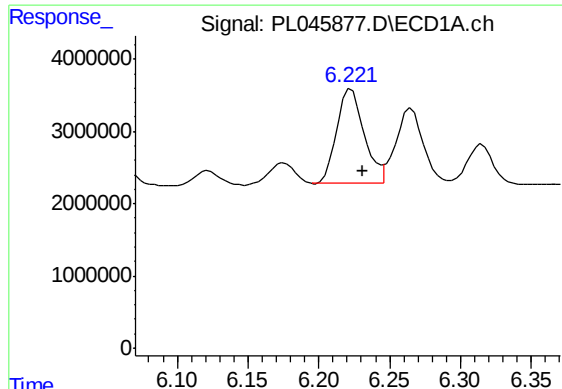

#17 4,4'-DDT


R.T.: 6.223 min
Delta R.T.: -0.008 min
Response: 17674968
Conc: 2.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

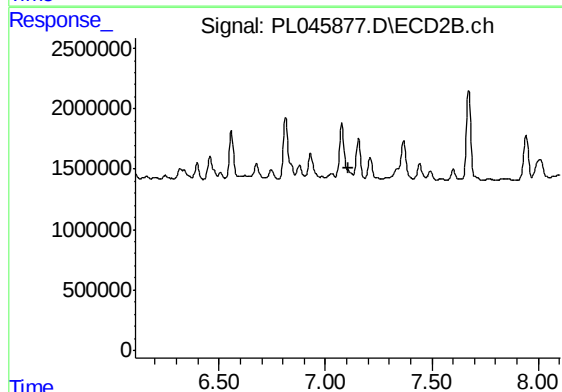


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.106 min
Response: 0
Conc: N.D.

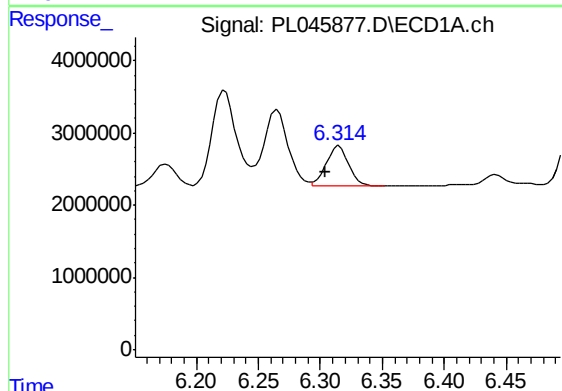


#18 Endrin aldehyde

R.T.: 6.315 min
Delta R.T.: 0.011 min
Response: 6937577
Conc: 0.95 ng/ml

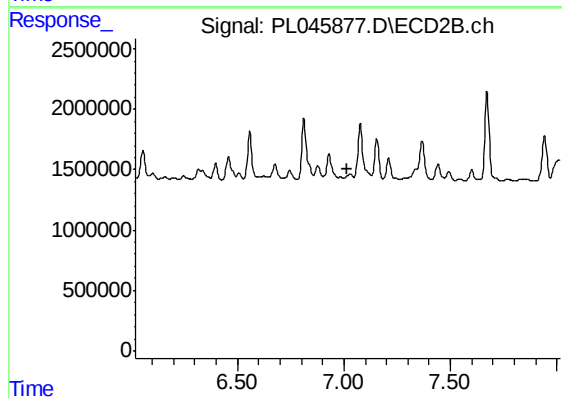

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.017 min
Response: 0
Conc: N.D.

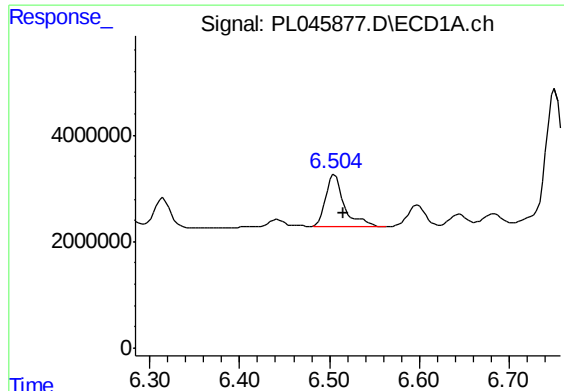

#19 Endosulfan Sulfate


R.T.: 6.506 min
Delta R.T.: -0.010 min
Response: 14029001
Conc: 1.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

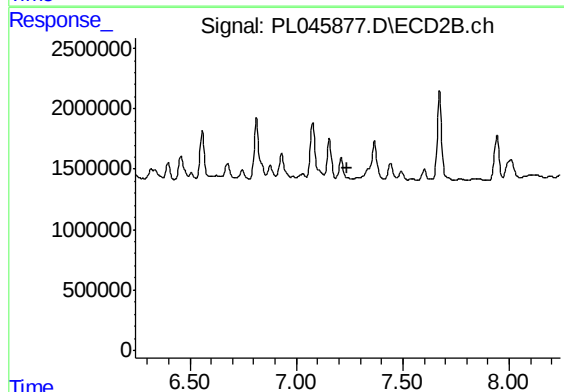


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.241 min
Response: 0
Conc: N.D.

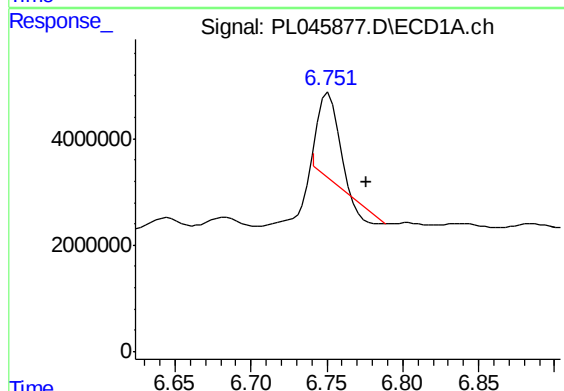


#20 Methoxychlor

R.T.: 6.751 min
Delta R.T.: -0.025 min
Response: 13116553
Conc: 2.99 ng/ml

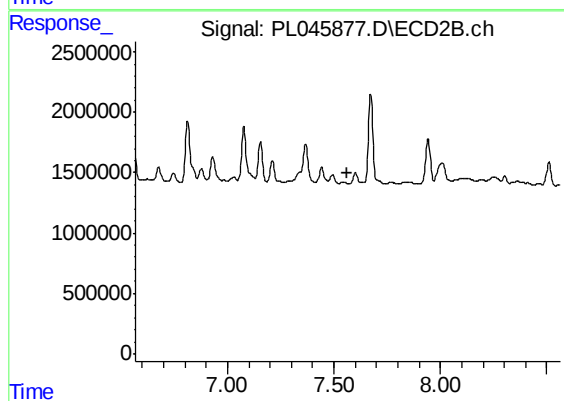

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.564 min
Response: 0
Conc: N.D.

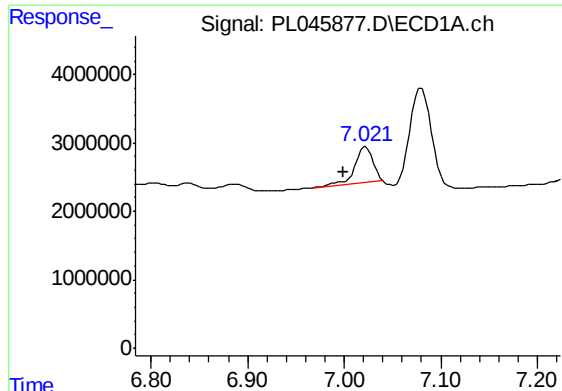

#21 Endrin ketone


R.T.: 7.022 min
Delta R.T.: 0.023 min
Response: 7121714
Conc: 0.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

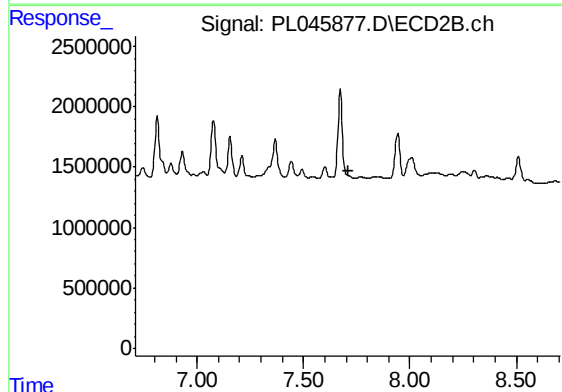


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

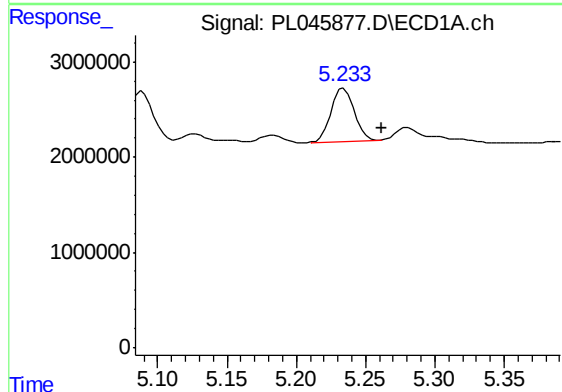


#25 Chlordane-3

R.T.: 5.234 min
Delta R.T.: -0.027 min
Response: 6609143
Conc: 5.76 ng/ml

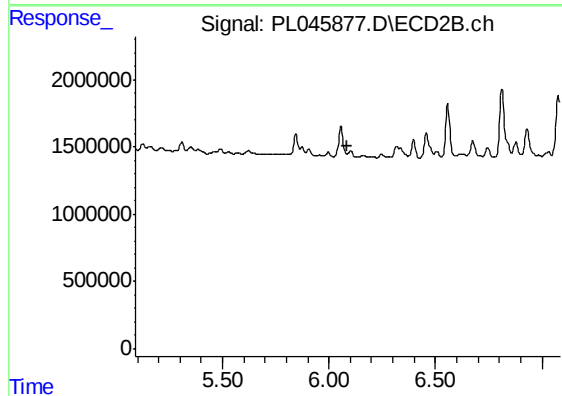

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

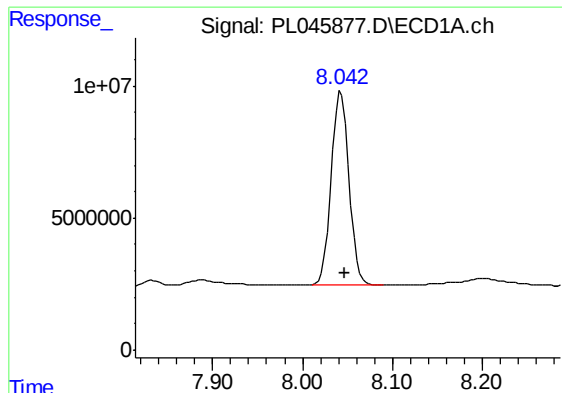

#28 Decachlorobiphenyl

R.T.: 8.043 min
Delta R.T.: -0.004 min
Response: 101472285
Conc: 12.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

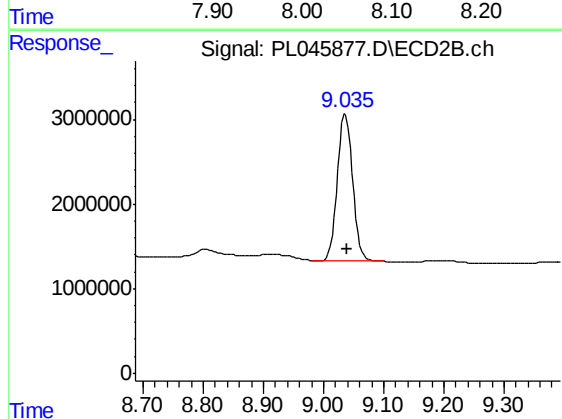

#28 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: -0.002 min
Response: 30922119
Conc: 13.53 ng/ml