

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031319\
 Data File : PL045891.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2019 08:00
 Operator : AJ\SJ
 Sample : K1866-09
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MR-MH-15-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 08:24:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	132.6E6	41372891	19.280	19.319
28)	SA Decachlor...	8.042	9.037	158.4E6	43385707	18.925	18.988
Target Compounds							
8)	B Heptachlo...	0.000	5.880f	0	3636910	N.D.	1.514 #
9)	A Endosulfan I	5.395f	0.000	13139679	0	1.470	N.D. #
10)	B gamma-Chl...	0.000	6.073	0	7116703	N.D.	2.653 #
13)	MA Dieldrin	5.614	6.494f	15333034	1485669	1.604	0.578 #
15)	B Endosulfa...	0.000	6.905	0	3473352	N.D.	1.477 #
16)	A 4,4'-DDD	0.000	6.803	0	4648246	N.D.	2.417 #
21)	B Endrin ke...	0.000	7.706	0	2171078	N.D.	0.913 #
23)	Chlordane-1	4.219	0.000	12935937	0	38.392	N.D. #
25)	Chlordane-3	0.000	6.073f	0	7116703	N.D.	18.265 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031319\
Data File : PL045891.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2019 08:00
Operator : AJ\SJ
Sample : K1866-09
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MR-MH-15-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 08:24:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

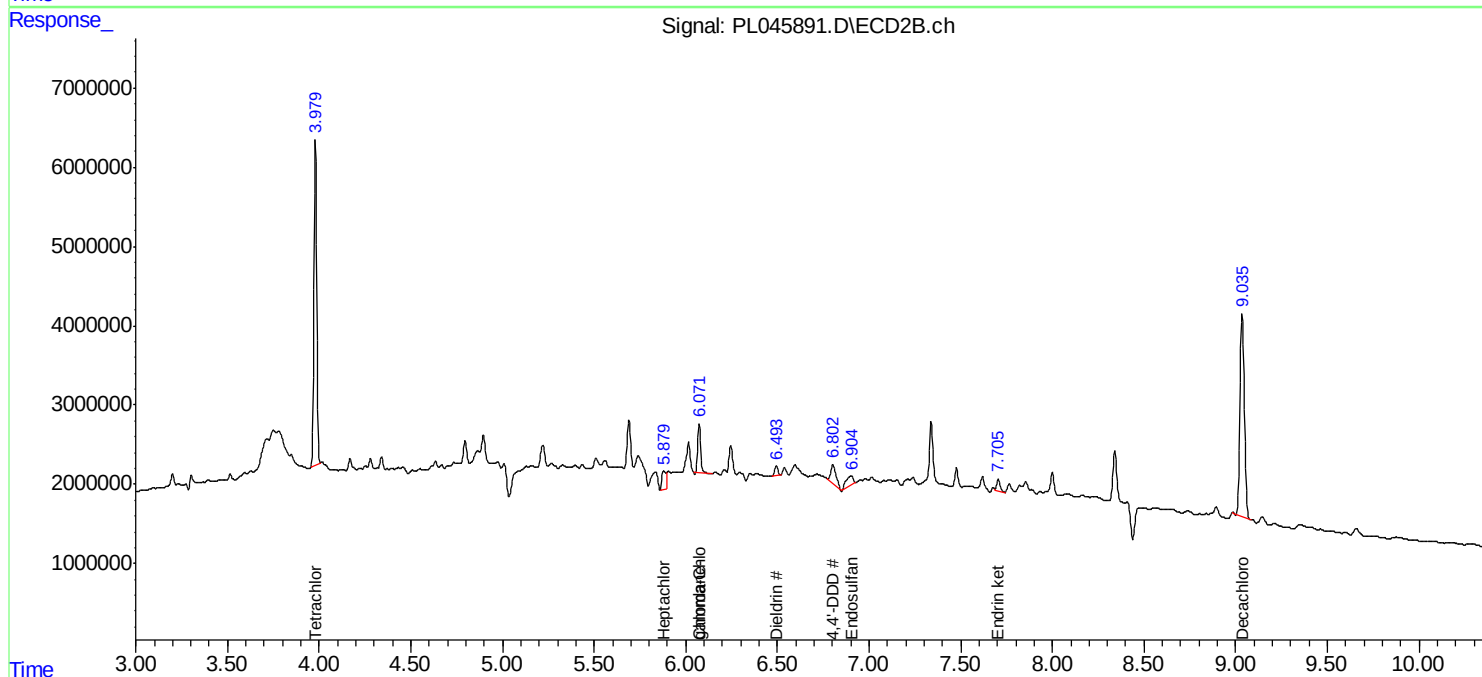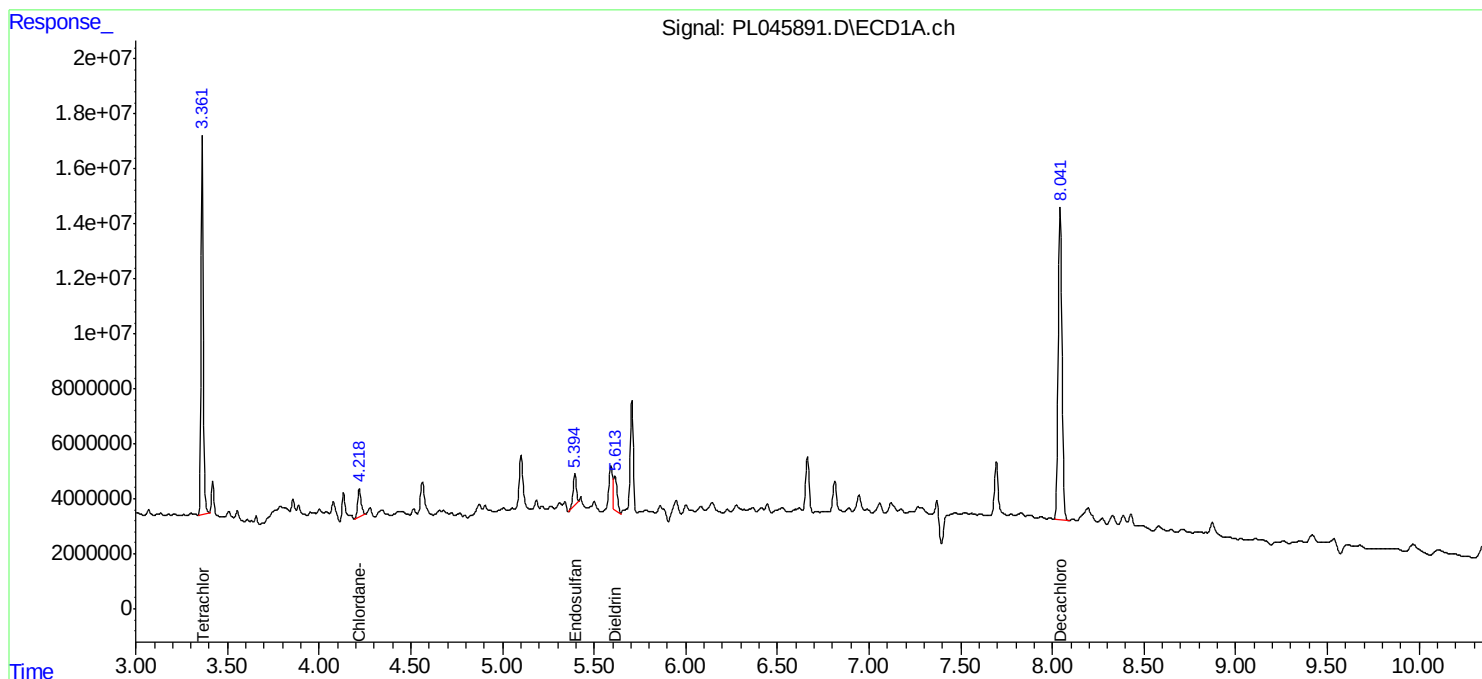


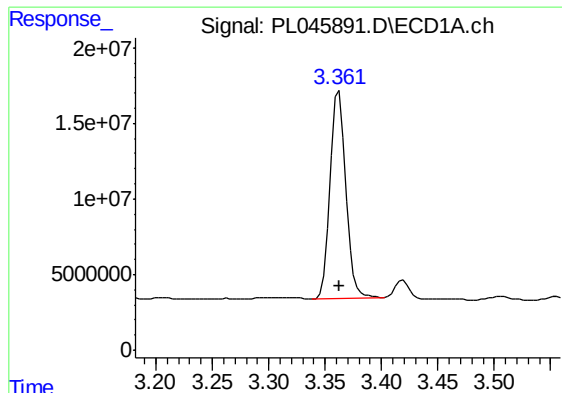

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 132634243
Conc: 19.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
MR-MH-15-COMP

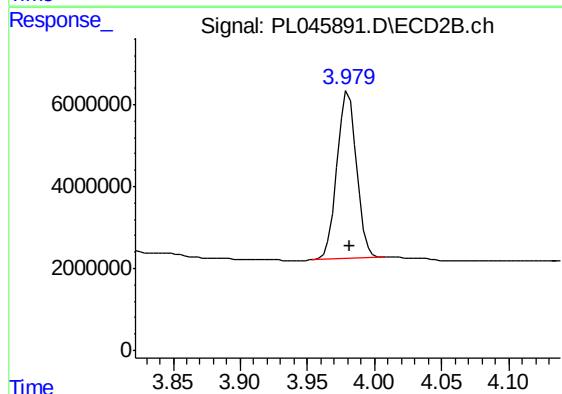


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 41372891
Conc: 19.32 ng/ml

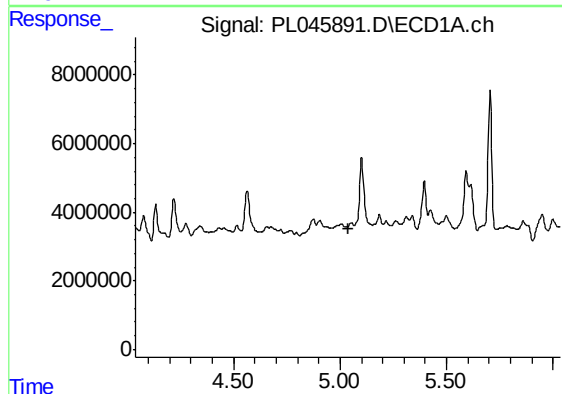


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

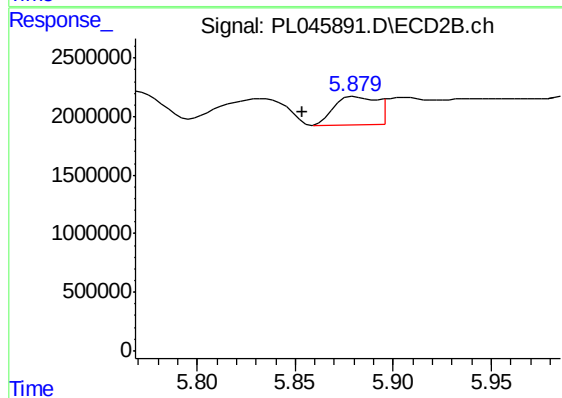

#8 Heptachlor epoxide


R.T.: 5.880 min
Delta R.T.: 0.027 min
Response: 3636910
Conc: 1.51 ng/ml

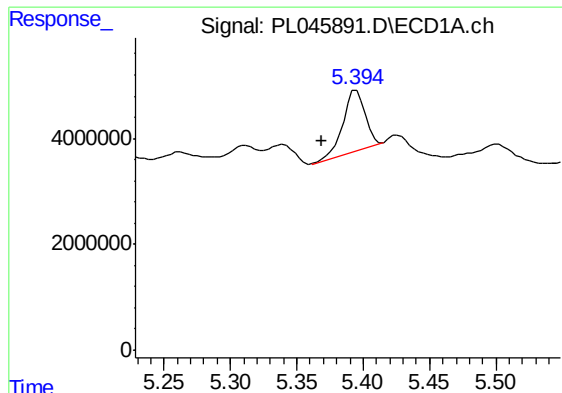

#9 Endosulfan I


R.T.: 5.395 min
Delta R.T.: 0.026 min
Response: 13139679
Conc: 1.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
MR-MH-15-COMP

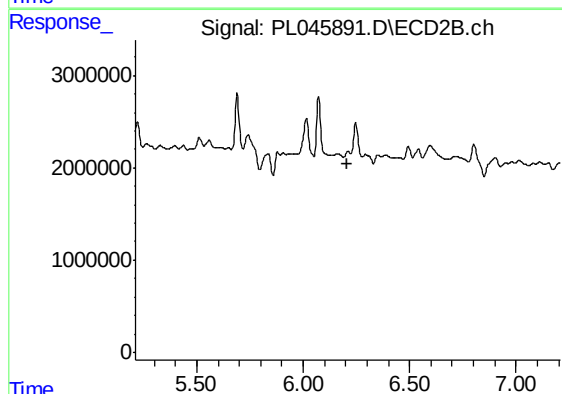


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

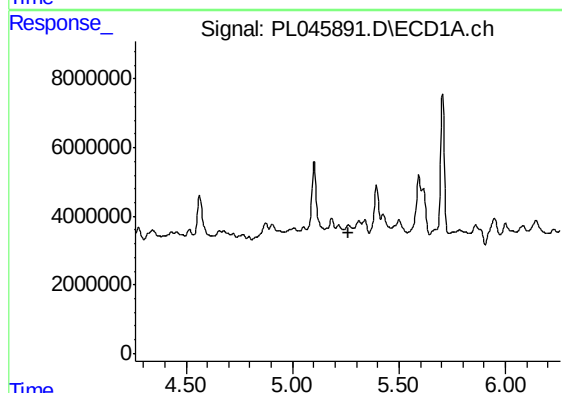


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

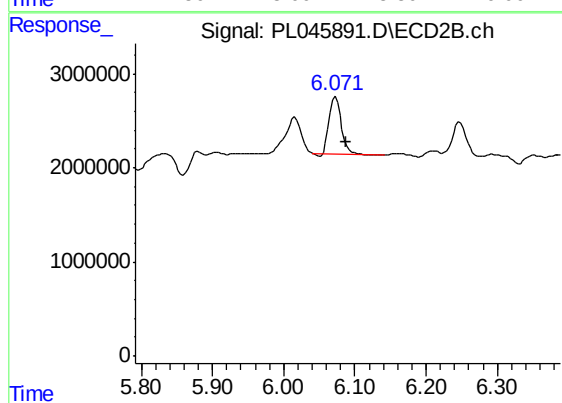

#10 gamma-Chlordane


R.T.: 6.073 min
Delta R.T.: -0.015 min
Response: 7116703
Conc: 2.65 ng/ml

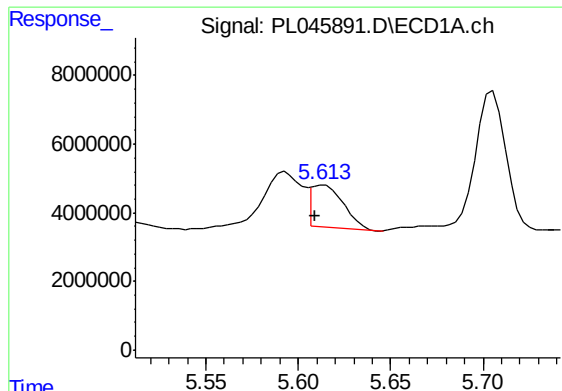

#13 Dielddrin


R.T.: 5.614 min
Delta R.T.: 0.005 min
Response: 15333034
Conc: 1.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
MR-MH-15-COMP

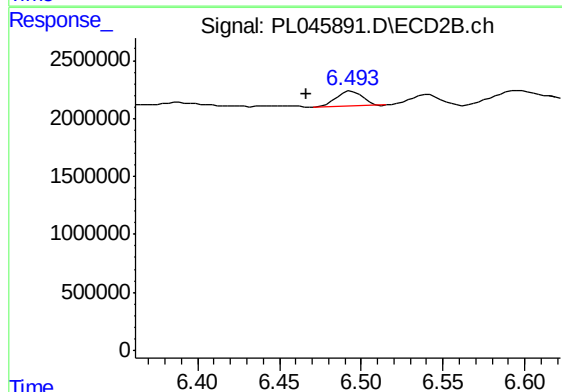


#13 Dielddrin

R.T.: 6.494 min
Delta R.T.: 0.028 min
Response: 1485669
Conc: 0.58 ng/ml

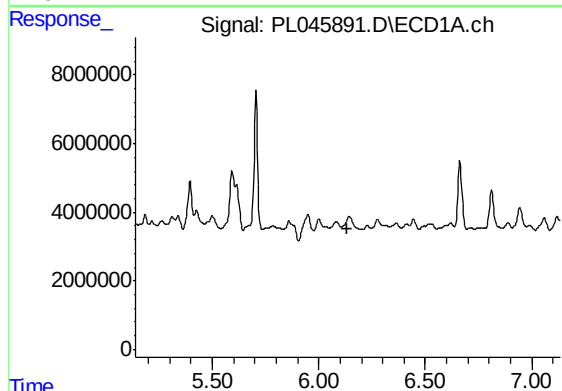


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.137 min
Response: 0
Conc: N.D.

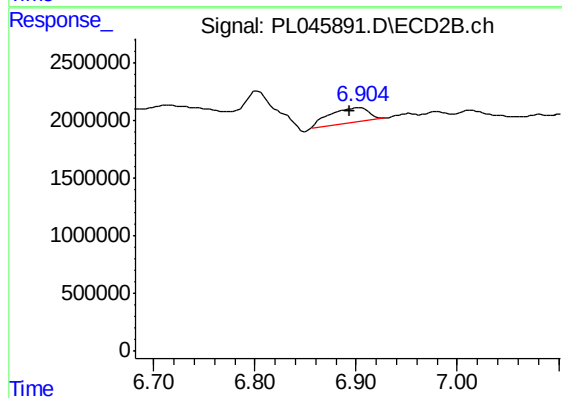

#15 Endosulfan II


R.T.: 6.905 min
Delta R.T.: 0.011 min
Response: 3473352
Conc: 1.48 ng/ml

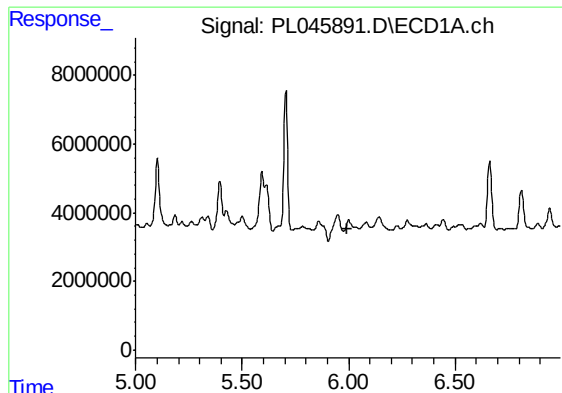

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MR-MH-15-COMP

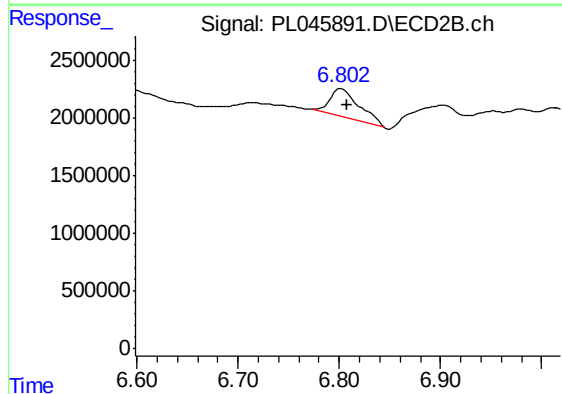


#16 4,4'-DDD

R.T.: 6.803 min
Delta R.T.: -0.005 min
Response: 4648246
Conc: 2.42 ng/ml

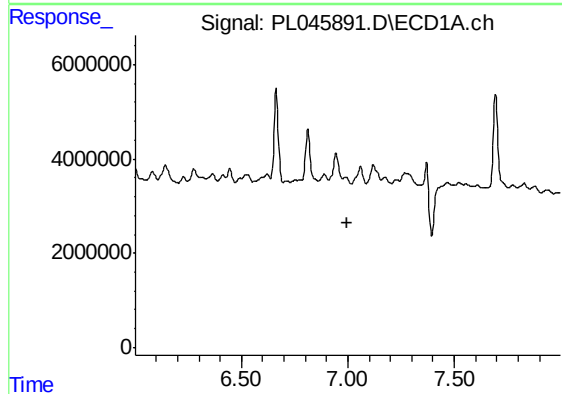


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

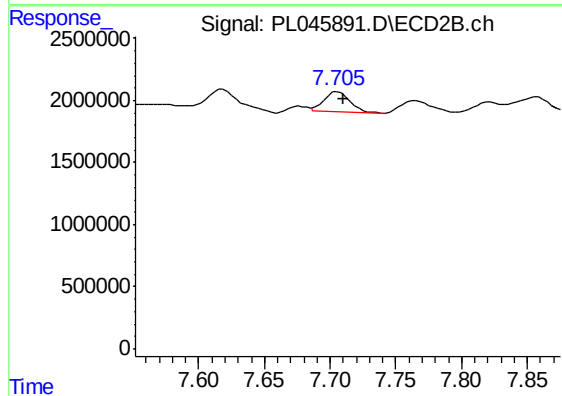

#21 Endrin ketone


R.T.: 7.706 min
Delta R.T.: -0.004 min
Response: 2171078
Conc: 0.91 ng/ml

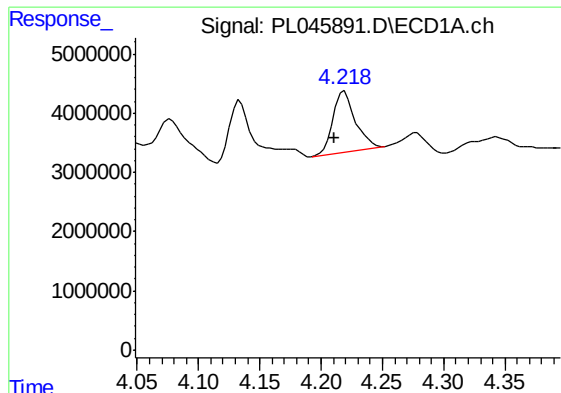

#23 Chlordane-1


R.T.: 4.219 min
Delta R.T.: 0.008 min
Response: 12935937
Conc: 38.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
MR-MH-15-COMP

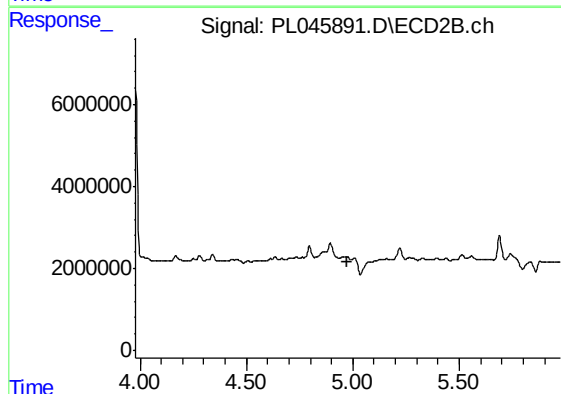


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

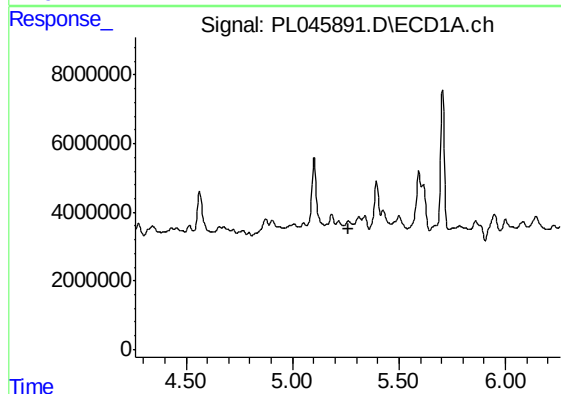


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.262 min
Response: 0
Conc: N.D.

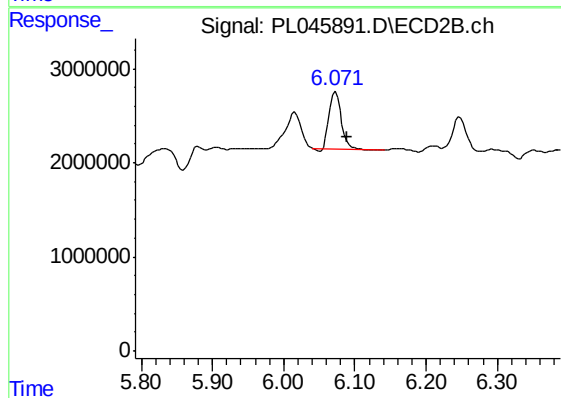

#25 Chlordane-3


R.T.: 6.073 min
Delta R.T.: -0.016 min
Response: 7116703
Conc: 18.27 ng/ml

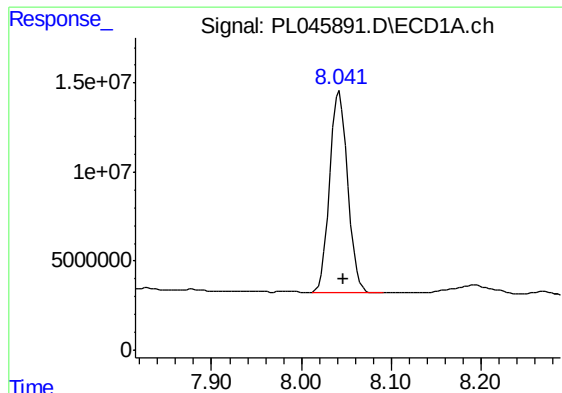

#28 Decachlorobiphenyl

R.T.: 8.042 min
Delta R.T.: -0.005 min
Response: 158354397
Conc: 18.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
MR-MH-15-COMP

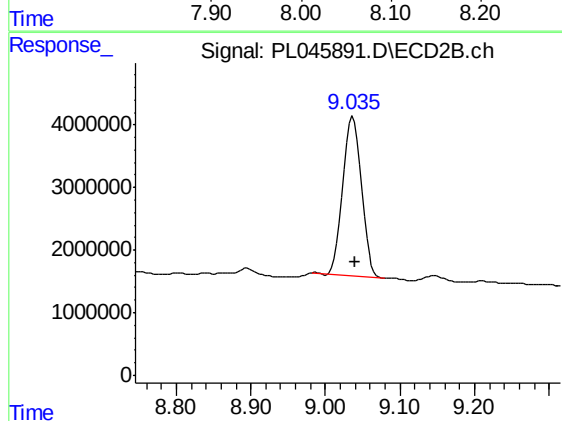

#28 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 43385707
Conc: 18.99 ng/ml