

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031319\
 Data File : PL045826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2019 15:19
 Operator : AJ\SJ
 Sample : K1824-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-24

Manual Integrations
 APPROVED

Sohil
 3/14/2019 12:12:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:04:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.980	123.3E6	38636666	17.919	18.042
28)	SA Decachlor...	8.043	9.036	108.0E6	31898978	12.911	13.961
Target Compounds							
12)	B 4,4'-DDE	5.479	6.314	2366161	863497	0.270m	0.370m#
17)	MA 4,4'-DDT	6.226	7.103	1590157	967279	0.212m	0.490m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031319\
Data File : PL045826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2019 15:19
Operator : AJ\SJ
Sample : K1824-02
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-24


Manual Integrations
APPROVED

Sohil
3/14/2019 12:12:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:04:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

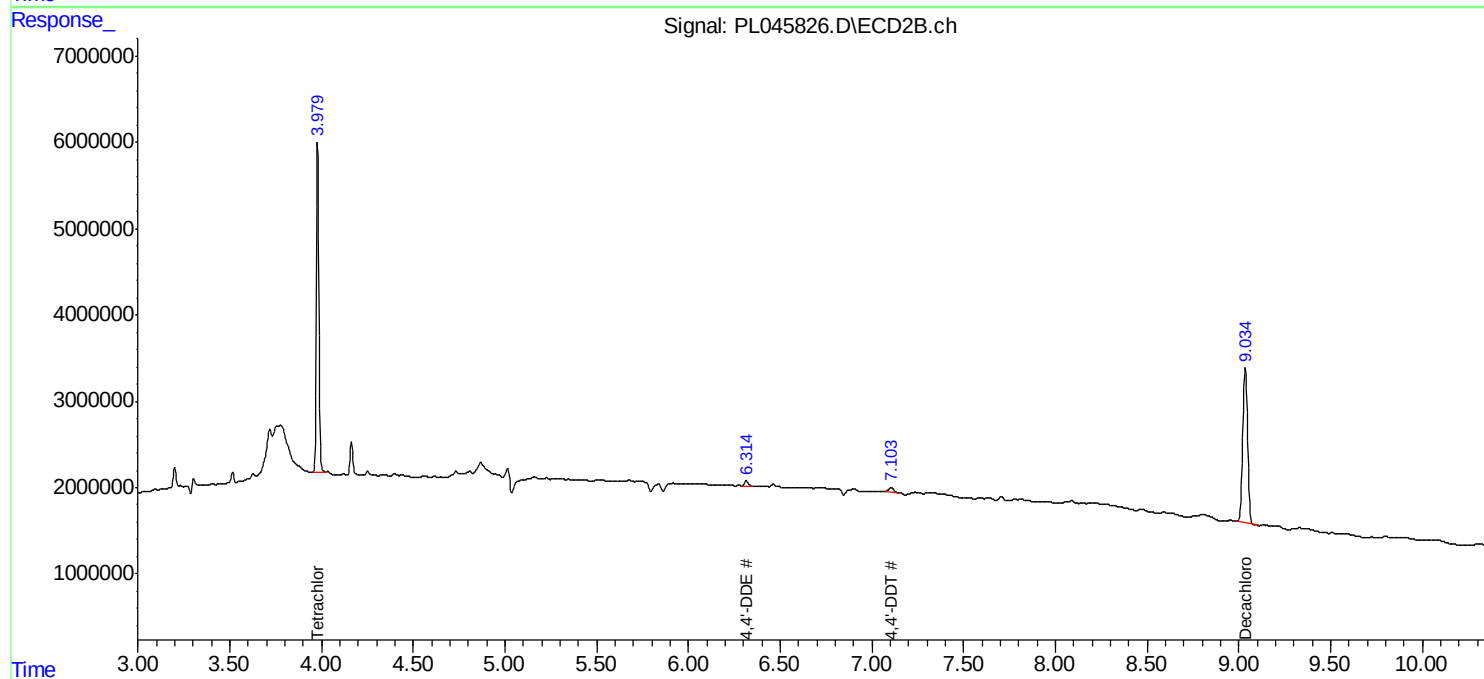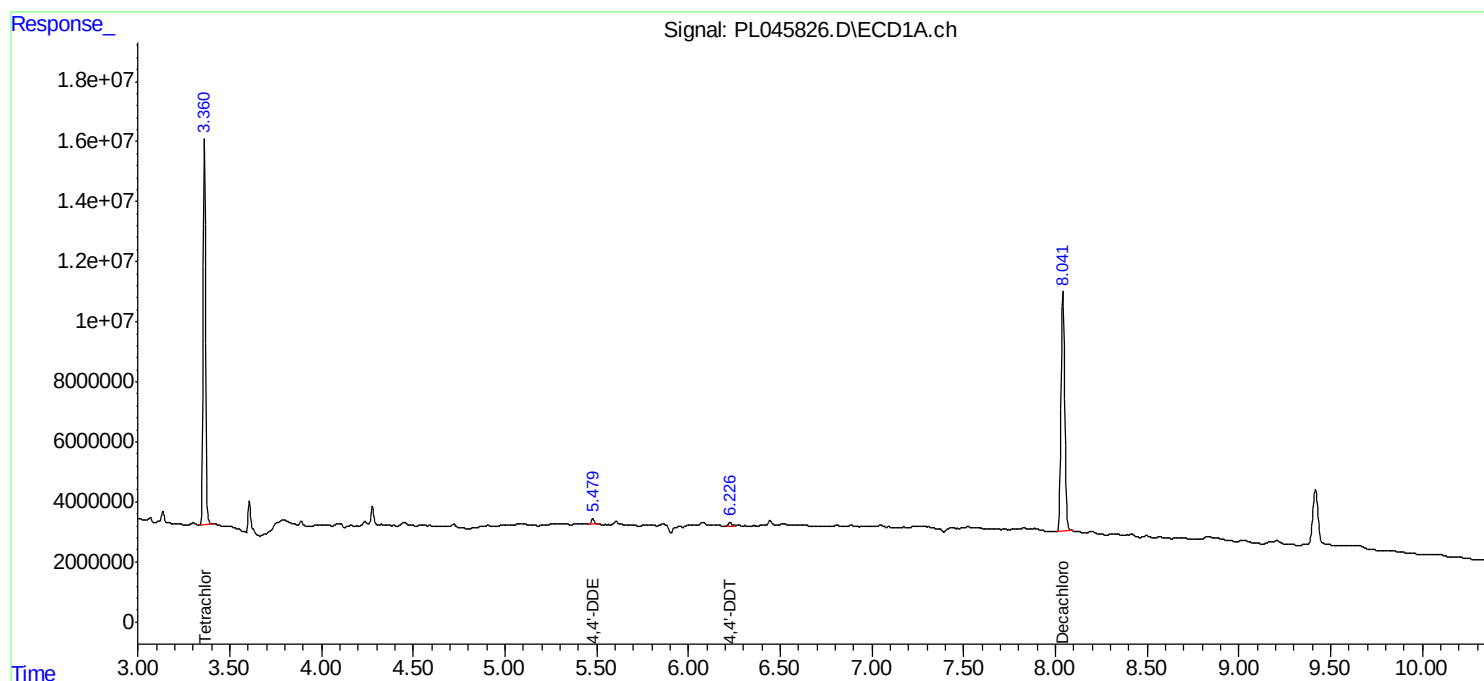

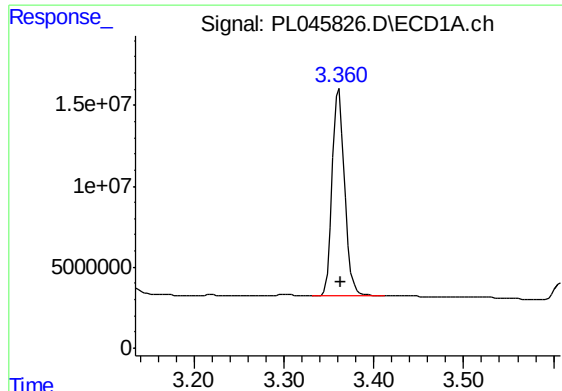


#1 Tetrachloro-m-xylene

R.T.: 3.361 min
Delta R.T.: -0.002 min
Response: 123266664
Conc: 17.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-24


Manual Integrations
APPROVED

Sohil
3/14/2019 12:12:15 PM

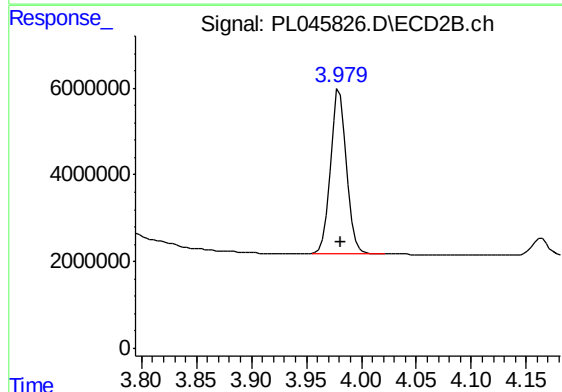


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.001 min
Response: 38636666
Conc: 18.04 ng/ml

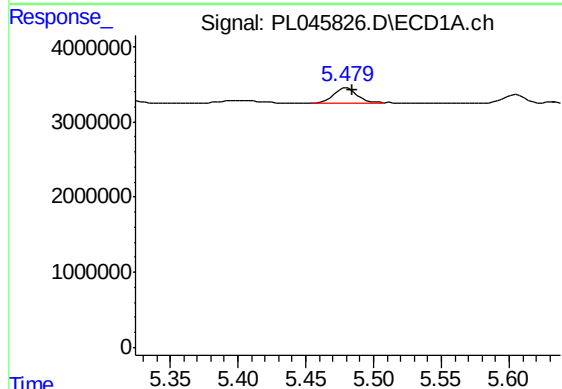


#12 4,4'-DDE

R.T.: 5.479 min
Delta R.T.: -0.005 min
Response: 2366161
Conc: 0.27 ng/ml m

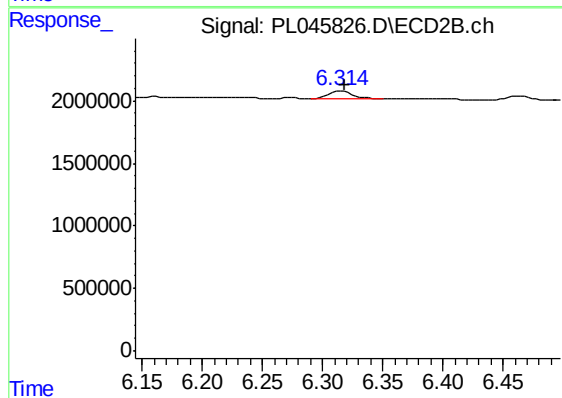

#12 4,4'-DDE

R.T.: 6.314 min
Delta R.T.: -0.004 min
Response: 863497
Conc: 0.37 ng/ml m

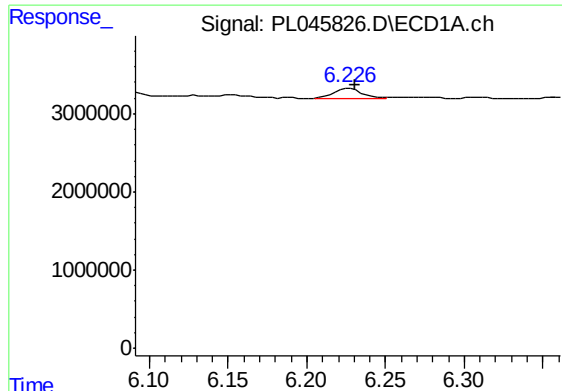


#17 4,4'-DDT

R.T.: 6.226 min
Delta R.T.: -0.005 min
Response: 1590157
Conc: 0.21 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-24


Manual Integrations
APPROVED

Sohil
3/14/2019 12:12:15 PM

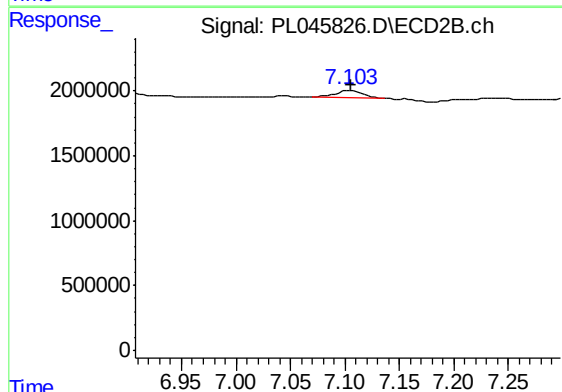


#17 4,4'-DDT

R.T.: 7.103 min
Delta R.T.: -0.003 min
Response: 967279
Conc: 0.49 ng/ml m

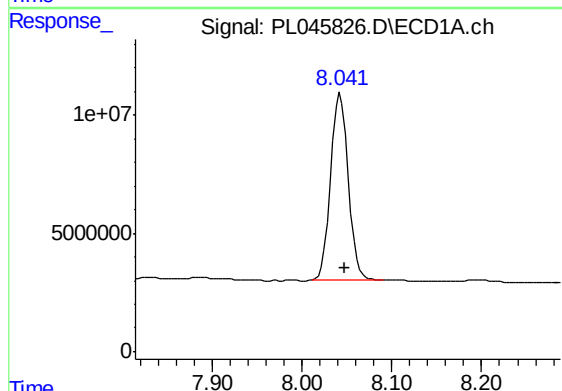

#28 Decachlorobiphenyl

R.T.: 8.043 min
Delta R.T.: -0.005 min
Response: 108035748
Conc: 12.91 ng/ml

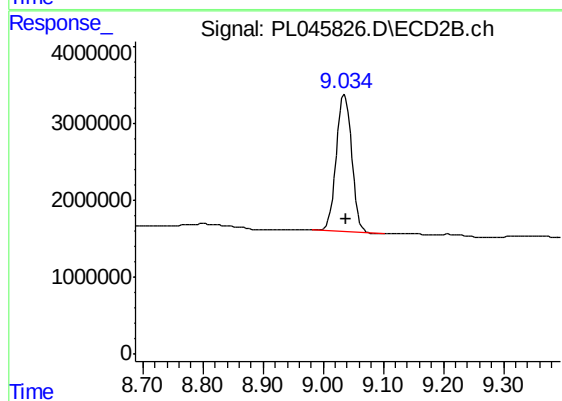

#28 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: -0.003 min
Response: 31898978
Conc: 13.96 ng/ml