

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
 Data File : PL065253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2021 17:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 02:41:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 01:11:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.295	3.884	50257860	59370778	21.332	21.554
28)	SA Decachlor...	7.941	8.895	47790440	38936924	22.177	21.194
Target Compounds							
16)	A 4,4'-DDD	0.000	6.671f	0	18371048	N.D.	7.568 #
23)	Chlordane-1	4.102f	0.000	6605400	0	63.733	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
Data File : PL065253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2021 17:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 02:41:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 01:11:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

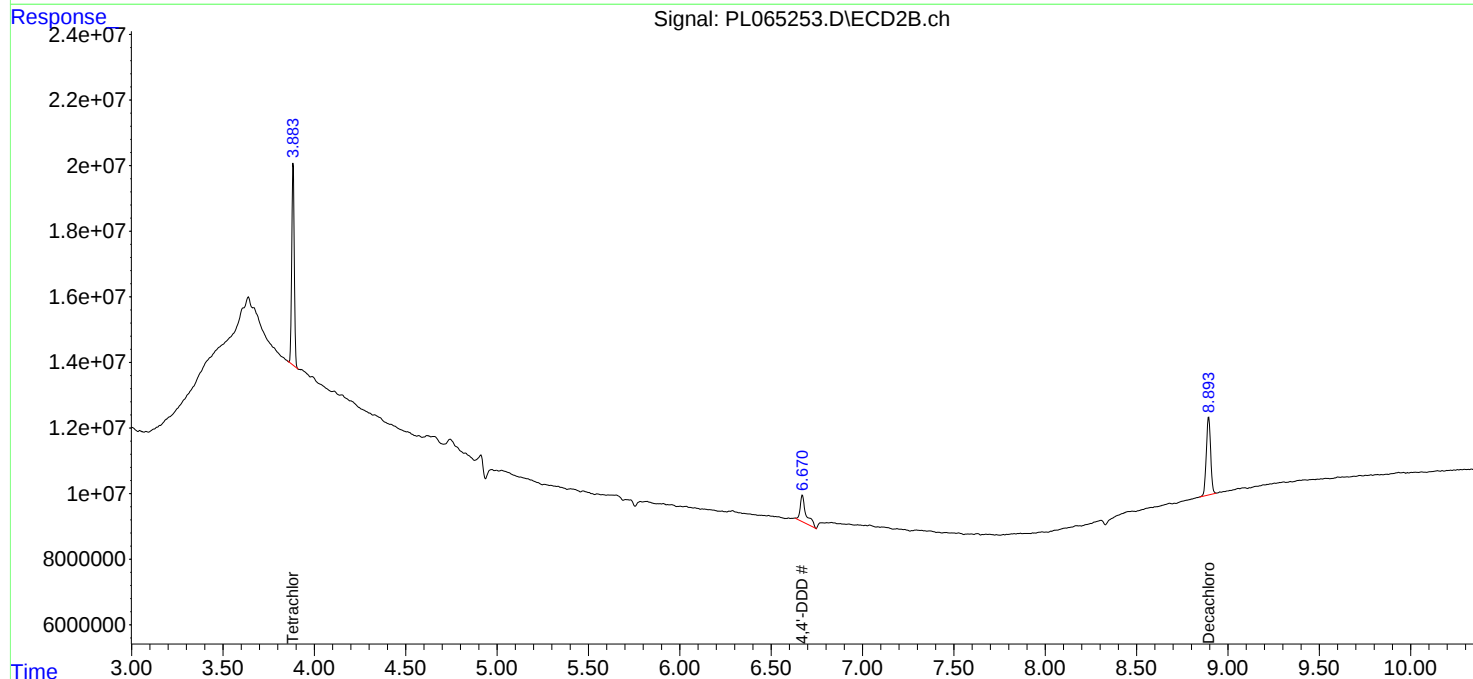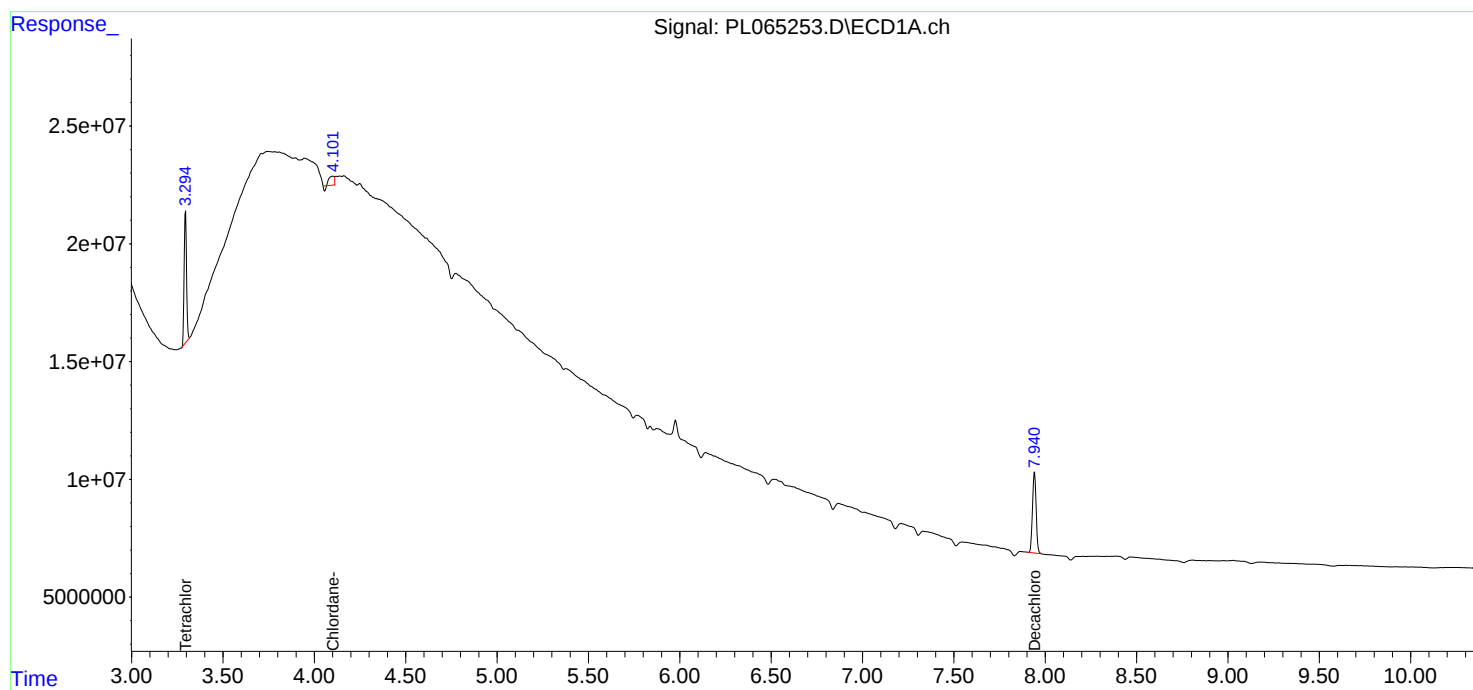


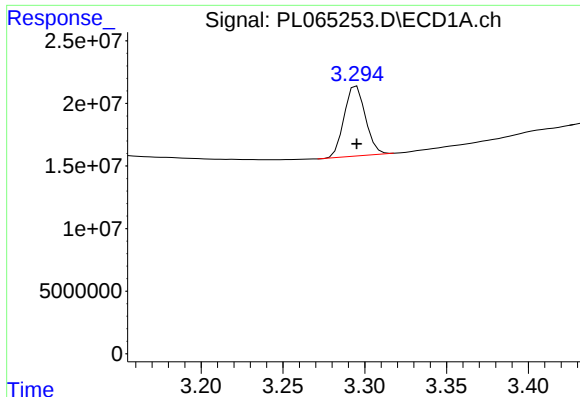

#1 Tetrachloro-m-xylene


R.T.: 3.295 min
Delta R.T.: 0.000 min
Response: 50257860
Conc: 21.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

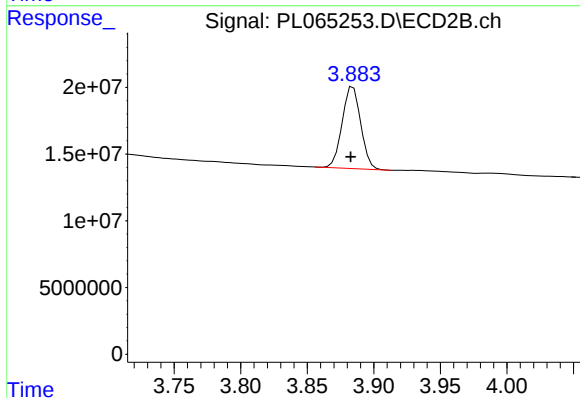


#1 Tetrachloro-m-xylene

R.T.: 3.884 min
Delta R.T.: 0.002 min
Response: 59370778
Conc: 21.55 ng/ml

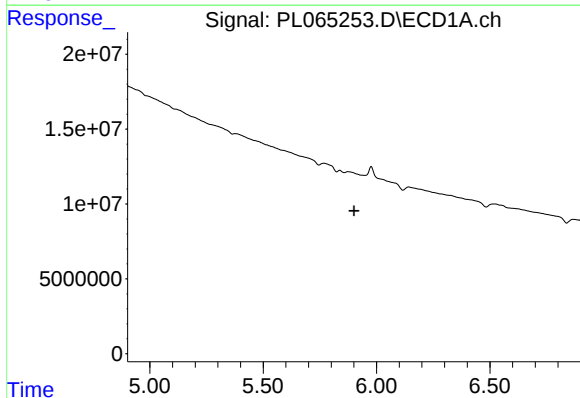


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.900 min
Response: 0
Conc: N.D.

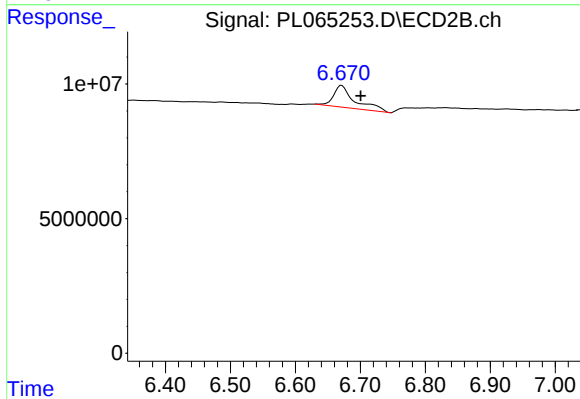

#16 4,4'-DDD


R.T.: 6.671 min
Delta R.T.: -0.029 min
Response: 18371048
Conc: 7.57 ng/ml

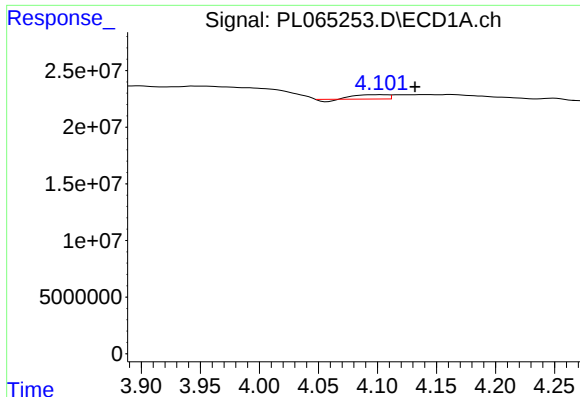

#23 Chlordane-1


R.T.: 4.102 min
Delta R.T.: -0.029 min
Response: 6605400
Conc: 63.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

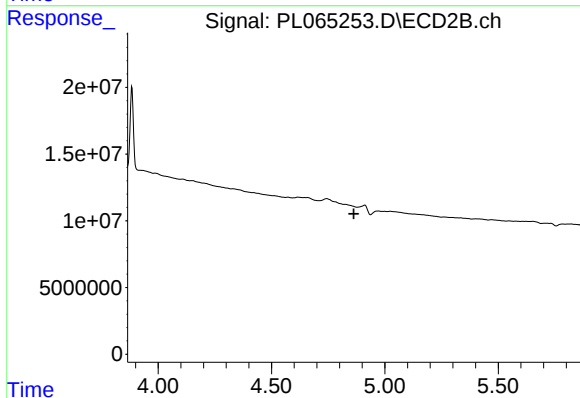


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.864 min
Response: 0
Conc: N.D.

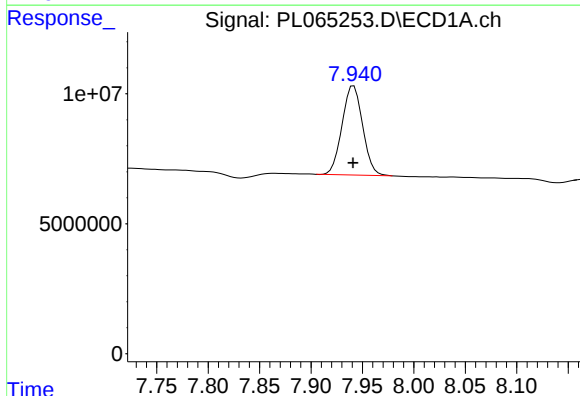

#28 Decachlorobiphenyl

R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 47790440
Conc: 22.18 ng/ml

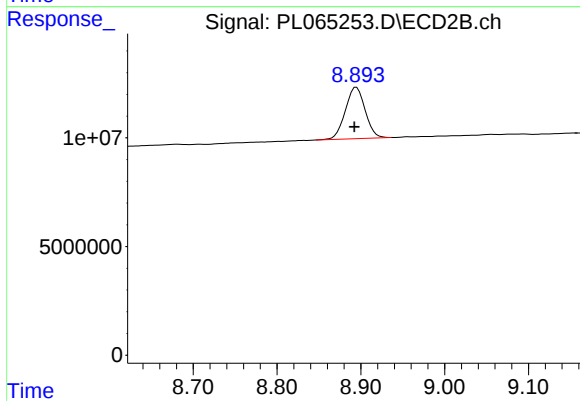

#28 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: 0.002 min
Response: 38936924
Conc: 21.19 ng/ml