

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
 Data File : PL065255.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2021 18:24
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 02:41:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 01:11:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.883	53003240	61526552	22.497	22.337
28)	SA Decachlor...	7.941	8.893	48442984	39911228	22.480	21.724
Target Compounds							
9)	A Endosulfan I	5.277	6.097	28991199	30421613	10.333	10.920
10)	B gamma-Chl...	5.170	5.975	31951433	31964507	10.102	10.708
12)	B 4,4'-DDE	5.394	6.208	61274973	61235189	20.703	22.074
13)	MA Dieldrin	5.515	6.355	64618162	65654396	21.675	22.327
19)	B Endosulfa...	6.416	7.136	52710369	48619069	20.652	20.713
20)	A Methoxychlor	6.681	7.462	109.7E6	103.5E6	117.378	111.587
21)	B Endrin ke...	6.895	7.607	56030420	51685448	19.687	19.769
23)	Chlordane-1	4.122	0.000	4411987	0	42.570	N.D. #
25)	Chlordane-3	5.170	5.975	31951433	31964507	106.239	78.206 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
Data File : PL065255.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2021 18:24
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 02:41:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 01:11:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

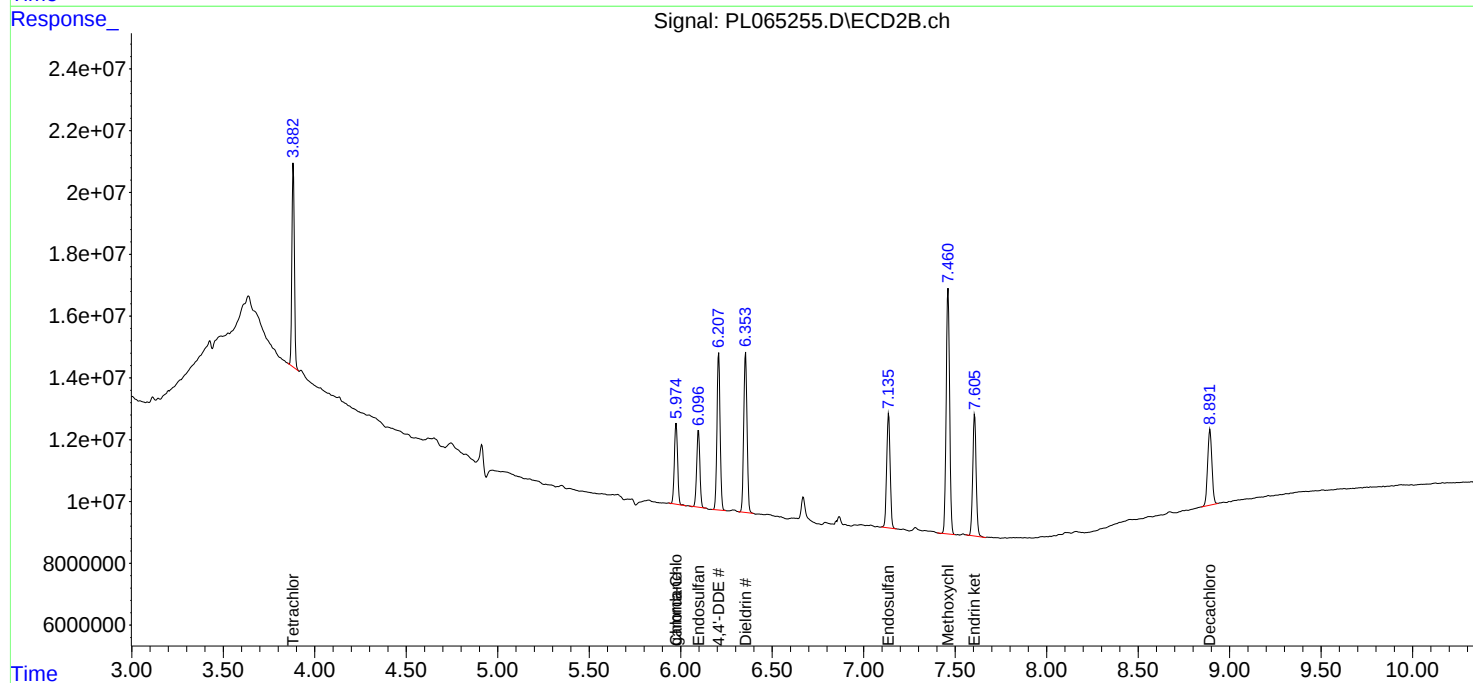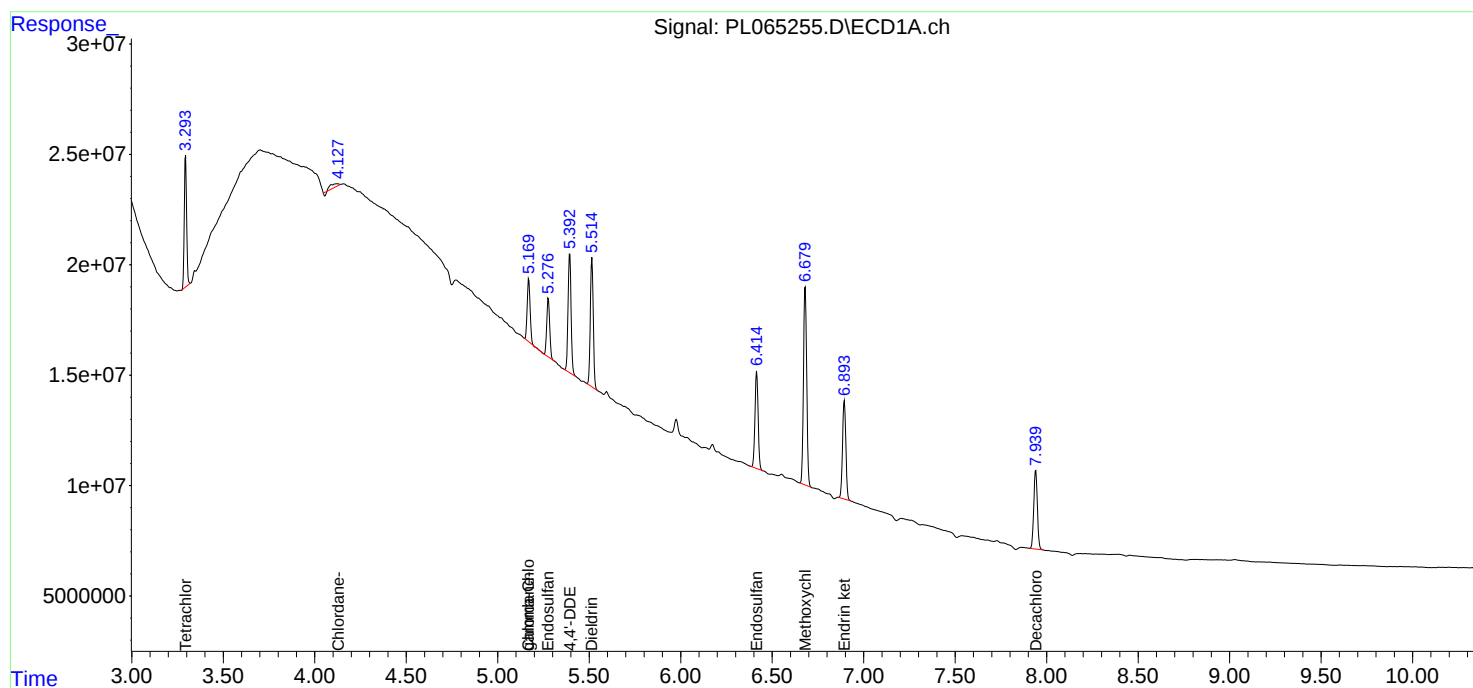


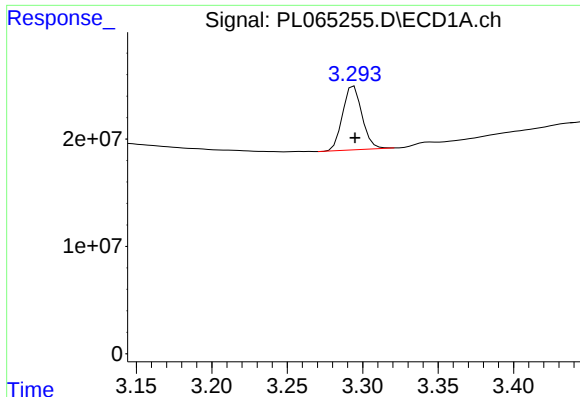

#1 Tetrachloro-m-xylene


R.T.: 3.294 min
Delta R.T.: 0.000 min
Response: 53003240
Conc: 22.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

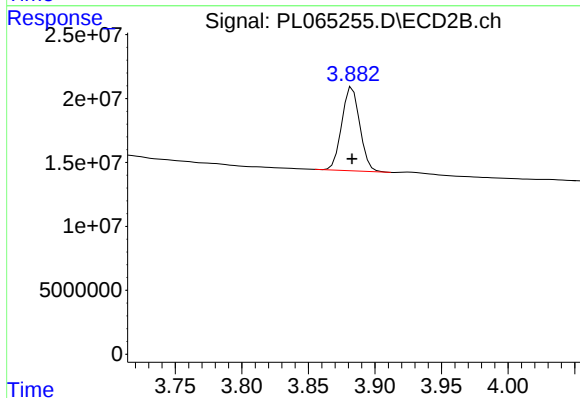


#1 Tetrachloro-m-xylene

R.T.: 3.883 min
Delta R.T.: 0.000 min
Response: 61526552
Conc: 22.34 ng/ml

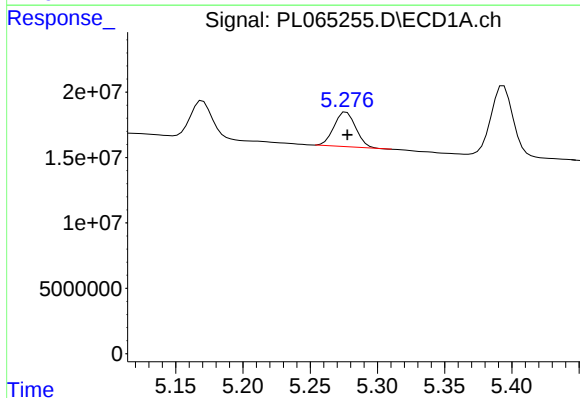


#9 Endosulfan I

R.T.: 5.277 min
Delta R.T.: 0.000 min
Response: 28991199
Conc: 10.33 ng/ml

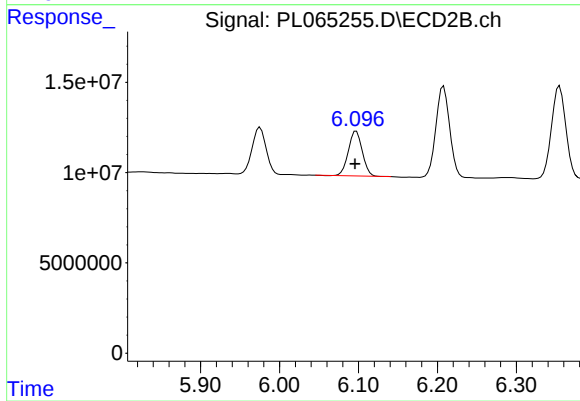

#9 Endosulfan I


R.T.: 6.097 min
Delta R.T.: 0.001 min
Response: 30421613
Conc: 10.92 ng/ml

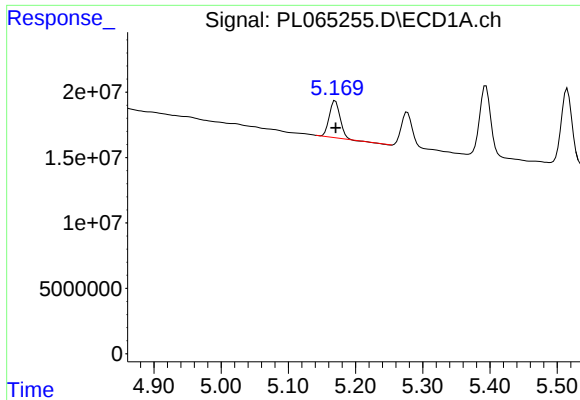

#10 gamma-Chlordane


R.T.: 5.170 min
Delta R.T.: 0.000 min
Response: 31951433
Conc: 10.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

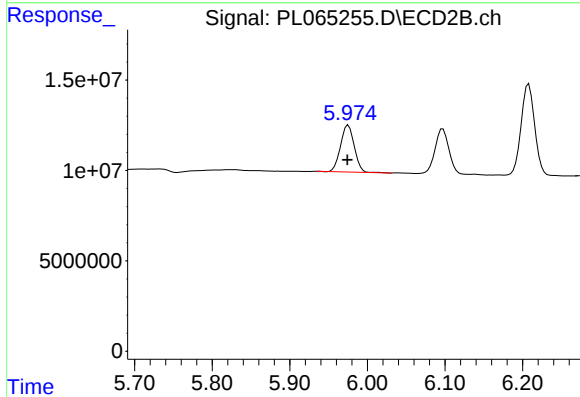


#10 gamma-Chlordane

R.T.: 5.975 min
Delta R.T.: 0.001 min
Response: 31964507
Conc: 10.71 ng/ml

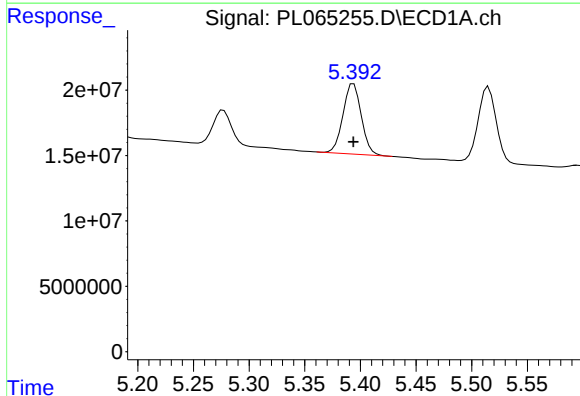


#12 4,4'-DDE

R.T.: 5.394 min
Delta R.T.: 0.000 min
Response: 61274973
Conc: 20.70 ng/ml

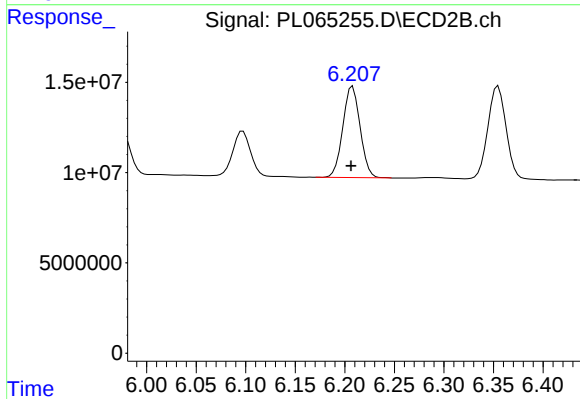

#12 4,4'-DDE


R.T.: 6.208 min
Delta R.T.: 0.002 min
Response: 61235189
Conc: 22.07 ng/ml

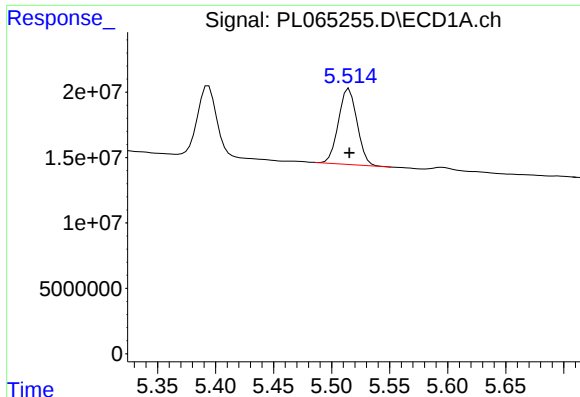

#13 Dieldrin


R.T.: 5.515 min
Delta R.T.: 0.000 min
Response: 64618162
Conc: 21.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

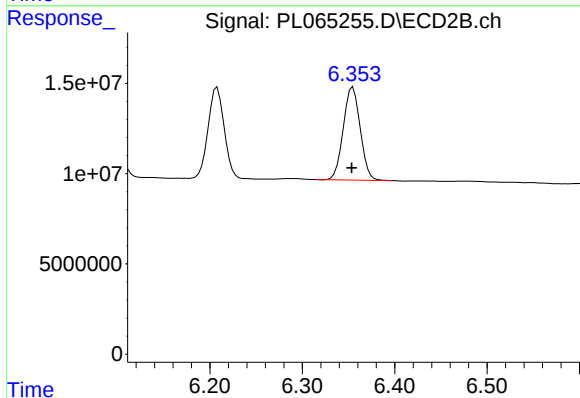


#13 Dieldrin

R.T.: 6.355 min
Delta R.T.: 0.001 min
Response: 65654396
Conc: 22.33 ng/ml

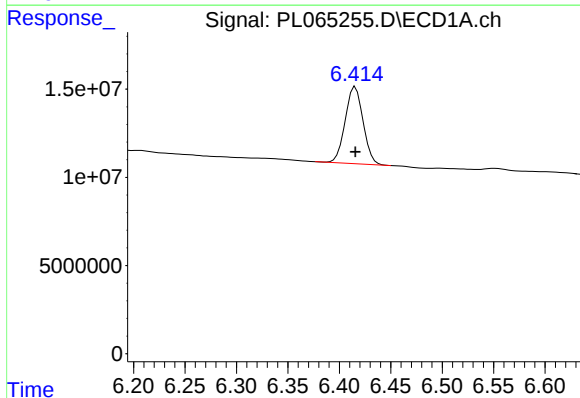


#19 Endosulfan Sulfate

R.T.: 6.416 min
Delta R.T.: 0.000 min
Response: 52710369
Conc: 20.65 ng/ml

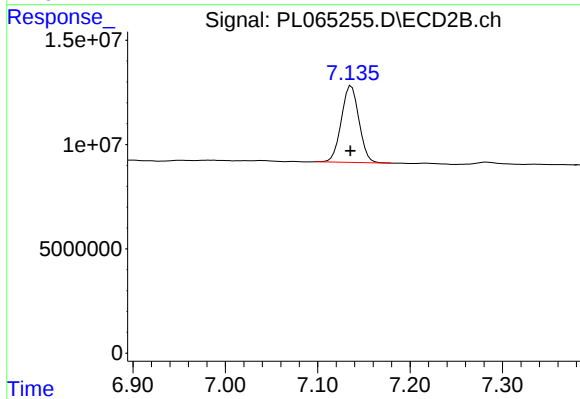

#19 Endosulfan Sulfate


R.T.: 7.136 min
Delta R.T.: 0.001 min
Response: 48619069
Conc: 20.71 ng/ml

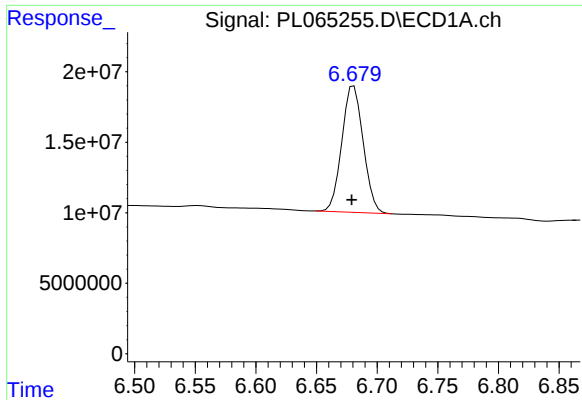

#20 Methoxychlor


R.T.: 6.681 min
Delta R.T.: 0.002 min
Response: 109700574
Conc: 117.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

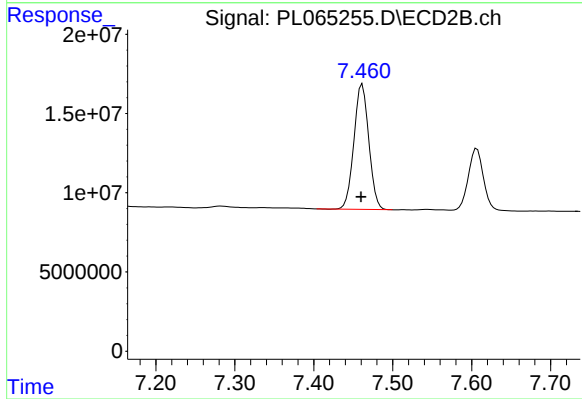


#20 Methoxychlor

R.T.: 7.462 min
Delta R.T.: 0.002 min
Response: 103517085
Conc: 111.59 ng/ml

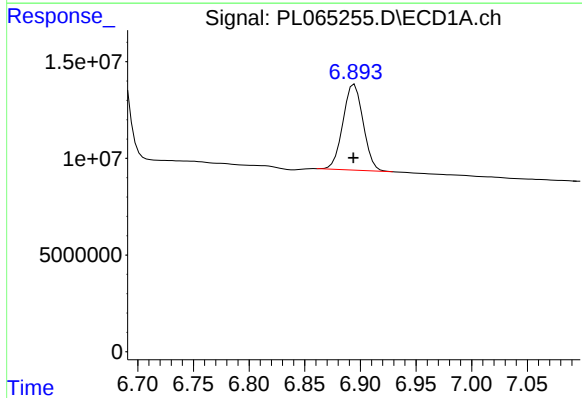


#21 Endrin ketone

R.T.: 6.895 min
Delta R.T.: 0.000 min
Response: 56030420
Conc: 19.69 ng/ml

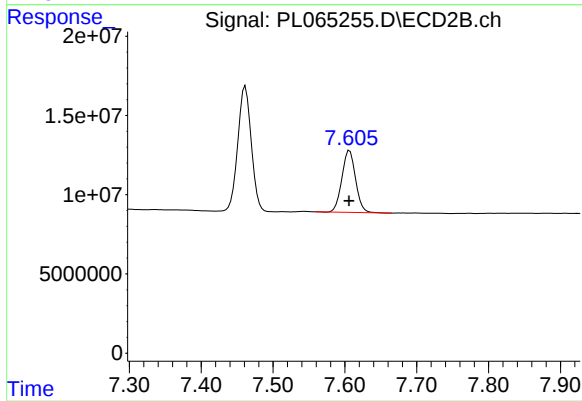

#21 Endrin ketone


R.T.: 7.607 min
Delta R.T.: 0.000 min
Response: 51685448
Conc: 19.77 ng/ml

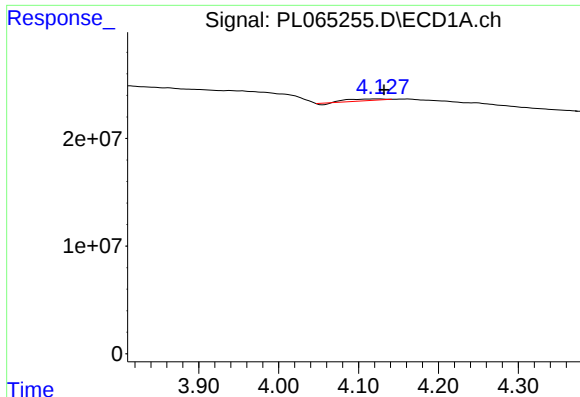

#23 Chlordane-1


R.T.: 4.122 min
Delta R.T.: -0.010 min
Response: 4411987
Conc: 42.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

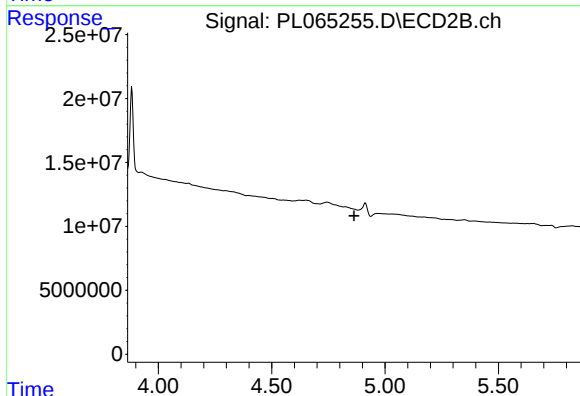


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.864 min
Response: 0
Conc: N.D.

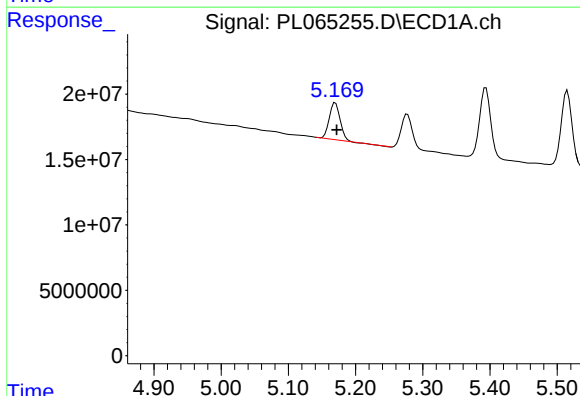


#25 Chlordane-3

R.T.: 5.170 min
Delta R.T.: -0.002 min
Response: 31951433
Conc: 106.24 ng/ml

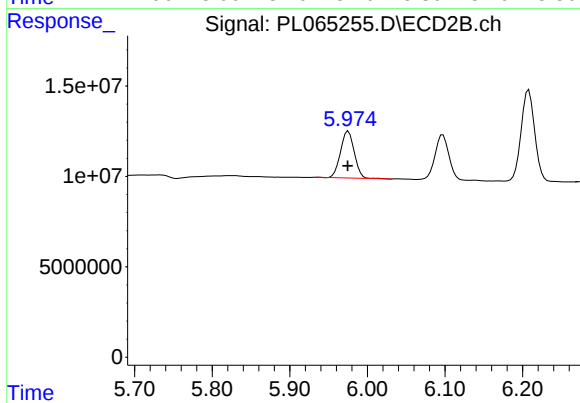

#25 Chlordane-3


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 31964507
Conc: 78.21 ng/ml

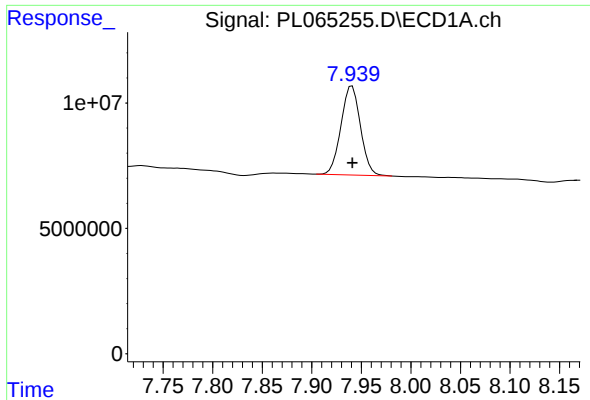

#28 Decachlorobiphenyl

R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 48442984
Conc: 22.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

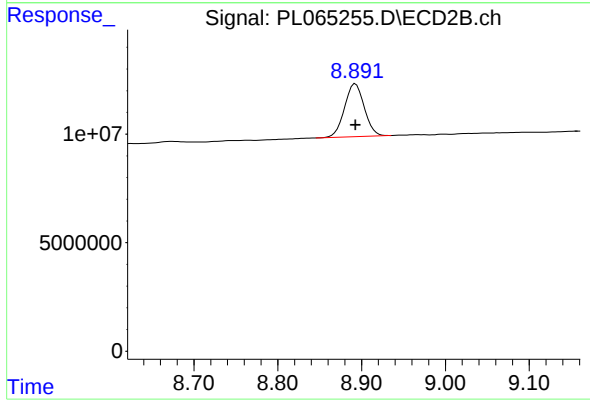

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: 0.000 min
Response: 39911228
Conc: 21.72 ng/ml