

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
 Data File : PL065264.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2021 20:33
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 00:56:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 00:55:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.882	61794891	66095840	23.700	24.795
28)	SA Decachlor...	7.941	8.892	52026063	44576909	24.995	25.318
Target Compounds							
23)	Chlordane-1	4.131	4.863	24721296	24394187	218.576	243.348
24)	Chlordane-2	4.619	5.331	23095766	26087484	232.871	253.431
25)	Chlordane-3	5.171	5.974	73611493	103.6E6	240.429	253.286
26)	Chlordane-4	5.227	6.045	63889449	119.6E6	235.646	254.645
27)	Chlordane-5	6.041	6.850	21889897	20115980	228.161	250.197



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
Data File : PL065264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2021 20:33
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 00:56:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 00:55:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

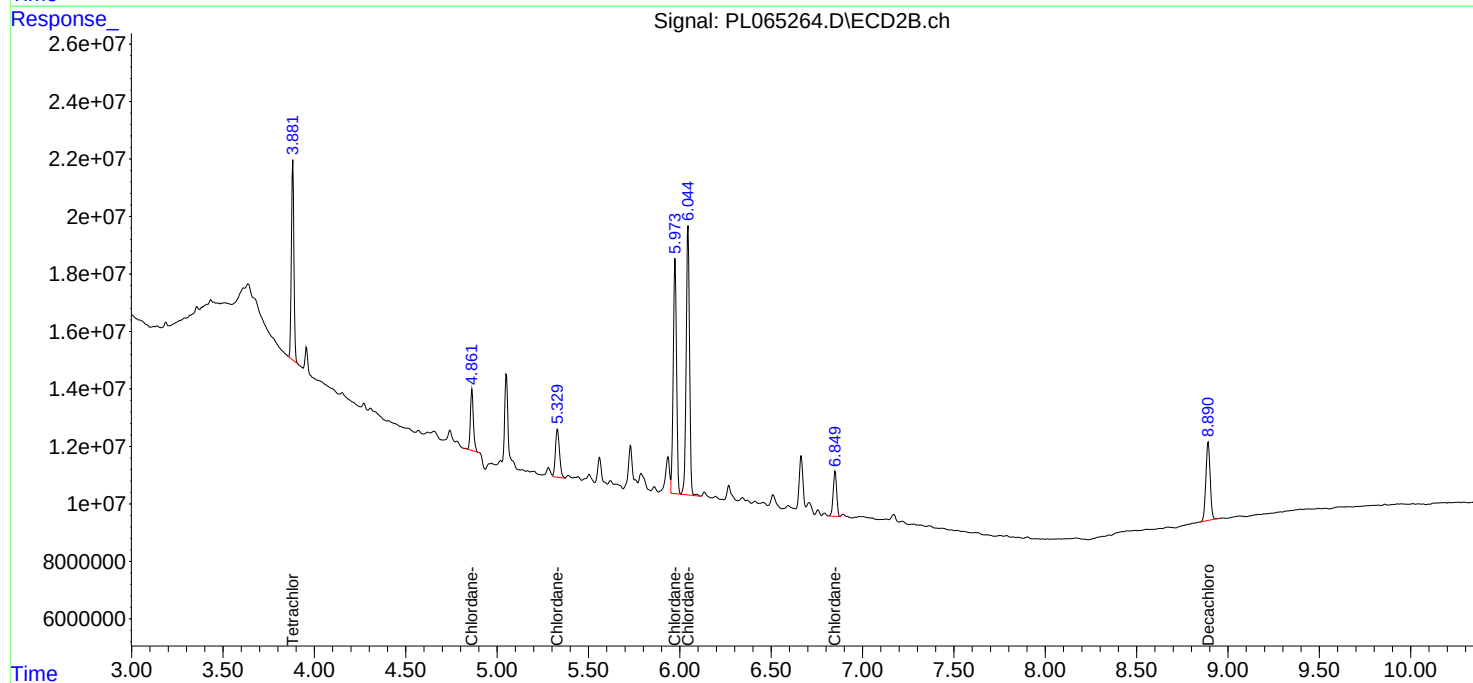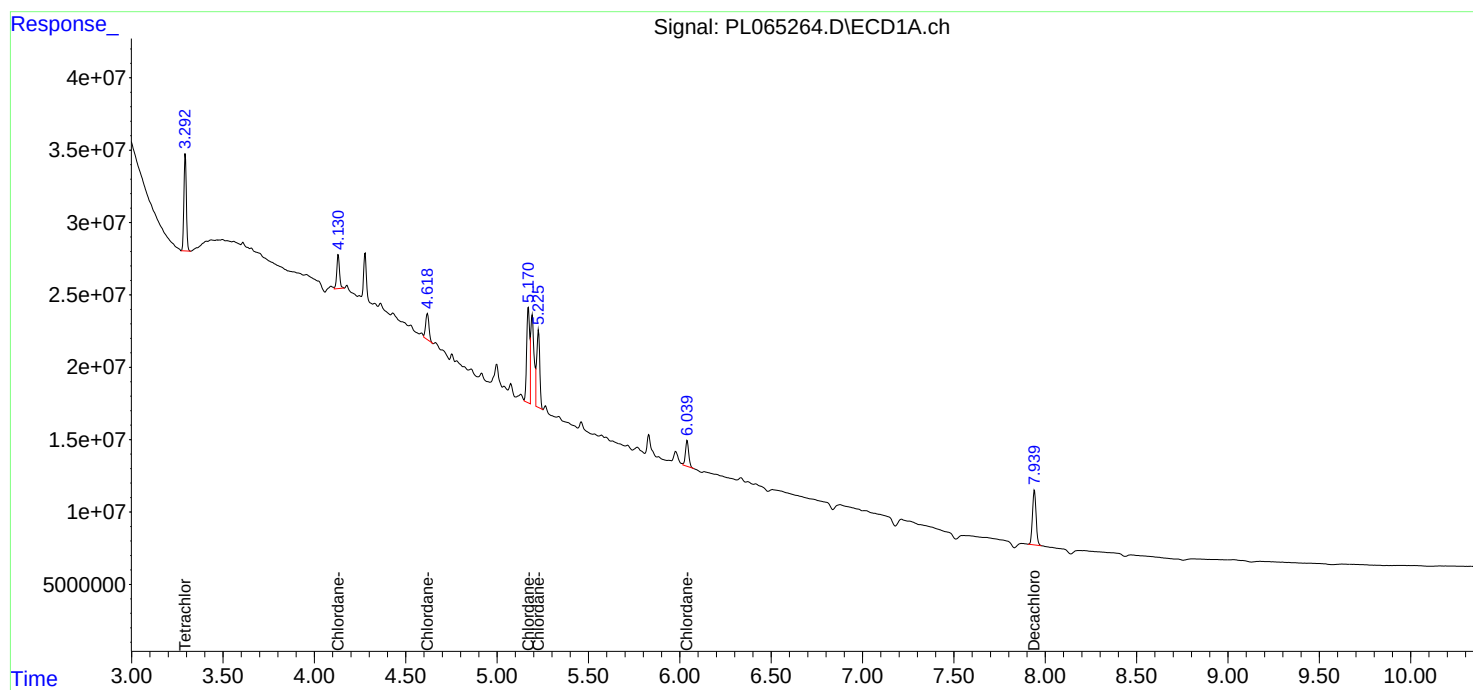


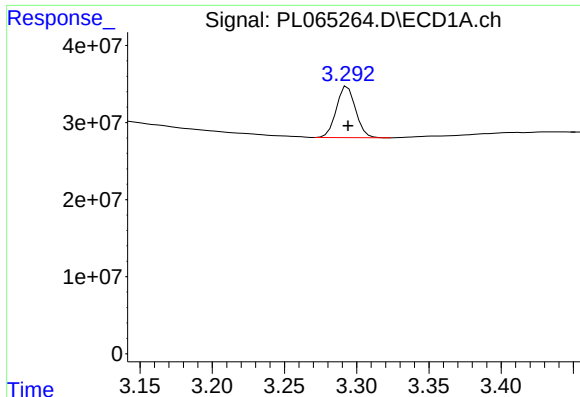

#1 Tetrachloro-m-xylene


R.T.: 3.294 min
Delta R.T.: 0.000 min
Response: 61794891
Conc: 23.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

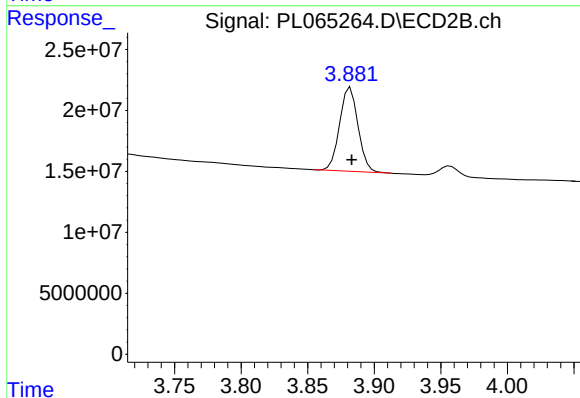


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.000 min
Response: 66095840
Conc: 24.80 ng/ml

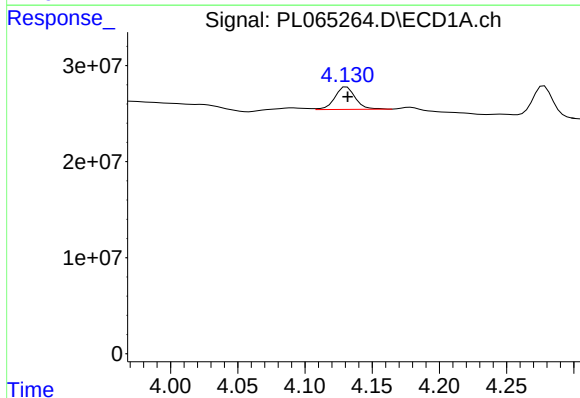


#23 Chlordane-1

R.T.: 4.131 min
Delta R.T.: 0.000 min
Response: 24721296
Conc: 218.58 ng/ml

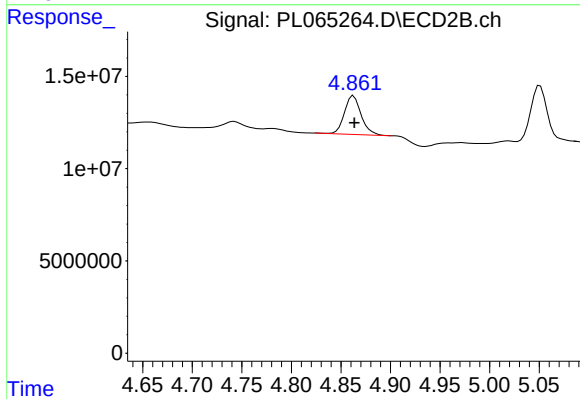

#23 Chlordane-1


R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 24394187
Conc: 243.35 ng/ml

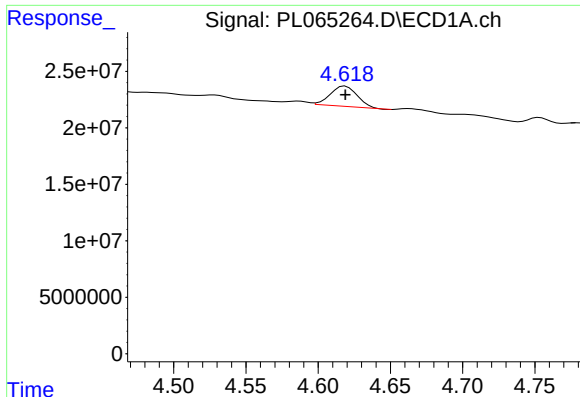

#24 Chlordane-2


R.T.: 4.619 min
Delta R.T.: 0.000 min
Response: 23095766
Conc: 232.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

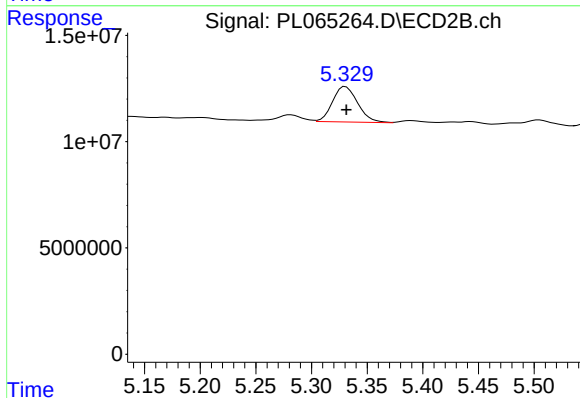


#24 Chlordane-2

R.T.: 5.331 min
Delta R.T.: 0.000 min
Response: 26087484
Conc: 253.43 ng/ml

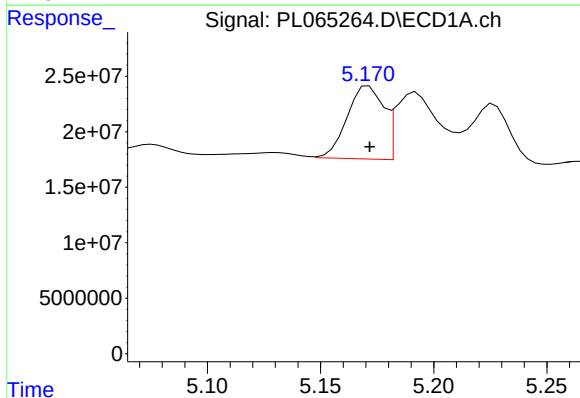


#25 Chlordane-3

R.T.: 5.171 min
Delta R.T.: 0.000 min
Response: 73611493
Conc: 240.43 ng/ml

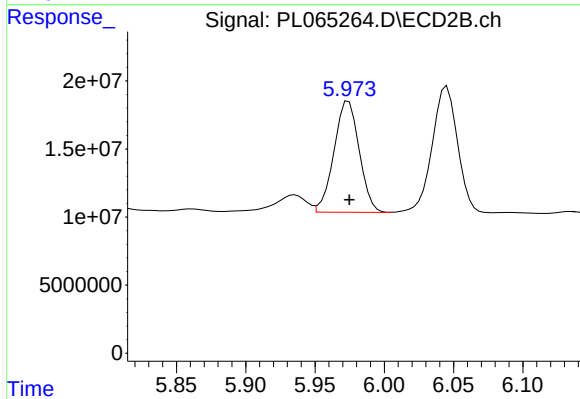

#25 Chlordane-3


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 103598117
Conc: 253.29 ng/ml

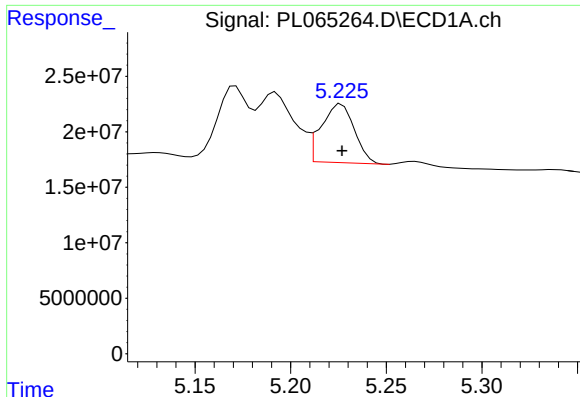

#26 Chlordane-4


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 63889449
Conc: 235.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

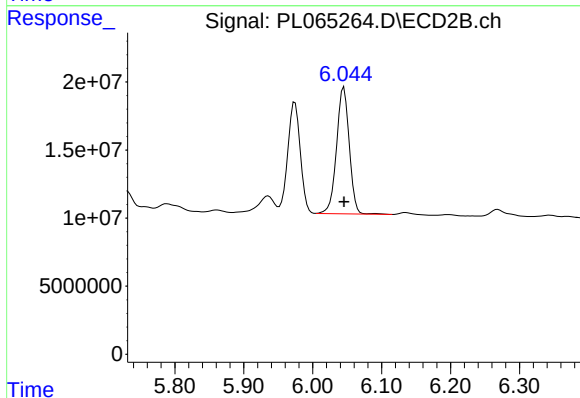


#26 Chlordane-4

R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 119592703
Conc: 254.65 ng/ml

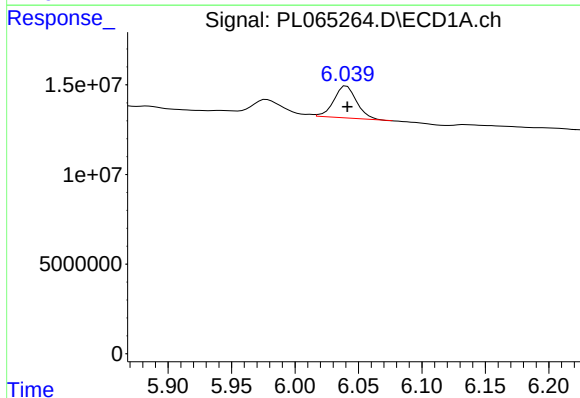


#27 Chlordane-5

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 21889897
Conc: 228.16 ng/ml

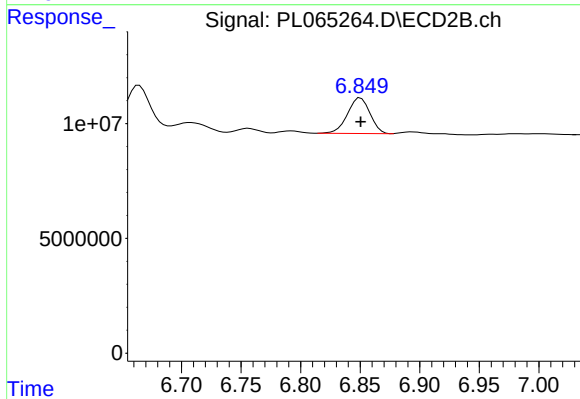

#27 Chlordane-5


R.T.: 6.850 min
Delta R.T.: 0.000 min
Response: 20115980
Conc: 250.20 ng/ml

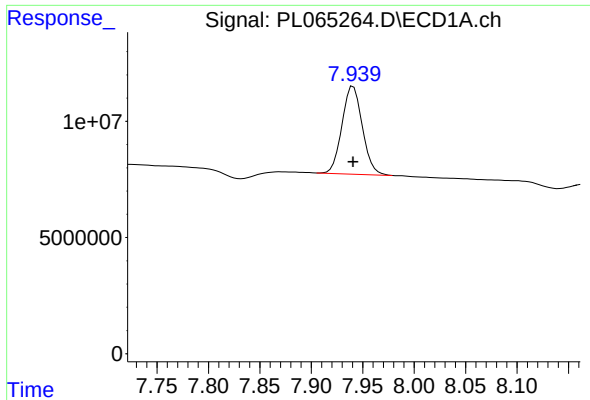

#28 Decachlorobiphenyl

R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 52026063
Conc: 25.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

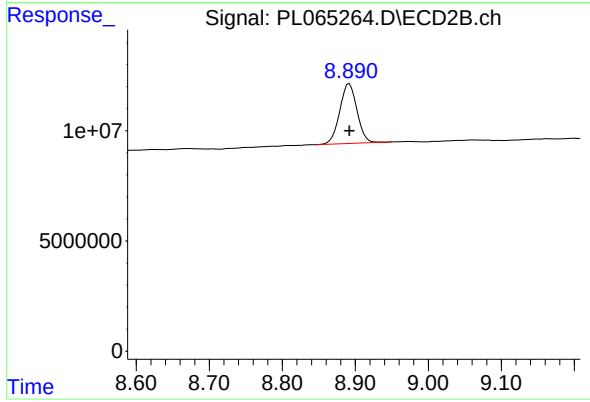

#28 Decachlorobiphenyl

R.T.: 8.892 min
Delta R.T.: 0.000 min
Response: 44576909
Conc: 25.32 ng/ml