

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
 Data File : PL065261.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2021 19:50
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 01:05:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 00:55:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.883	255.6E6	250.2E6	98.019	93.845
28)	SA Decachlor...	7.941	8.893	201.1E6	168.0E6	96.634	95.411
Target Compounds							
23)	Chlordane-1	4.132	4.864	102.5E6	99150412	906.215	989.089
24)	Chlordane-2	4.620	5.332	98123966	99804678	989.370	969.568
25)	Chlordane-3	5.172	5.975	296.7E6	387.4E6	969.167	947.105
26)	Chlordane-4	5.227	6.046	264.3E6	444.4E6	974.775	946.227
27)	Chlordane-5	6.041	6.851	94433099	77067670	984.289	958.547



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
Data File : PL065261.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2021 19:50
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 01:05:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 00:55:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

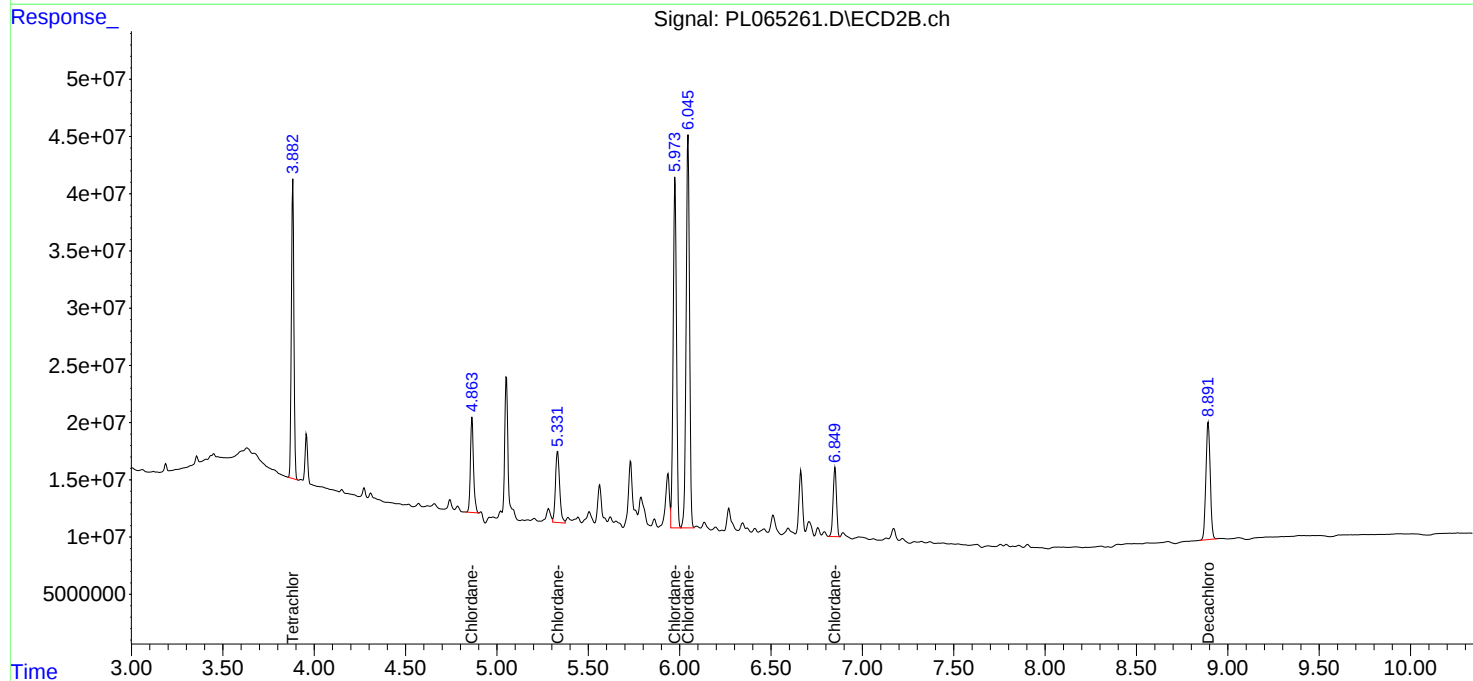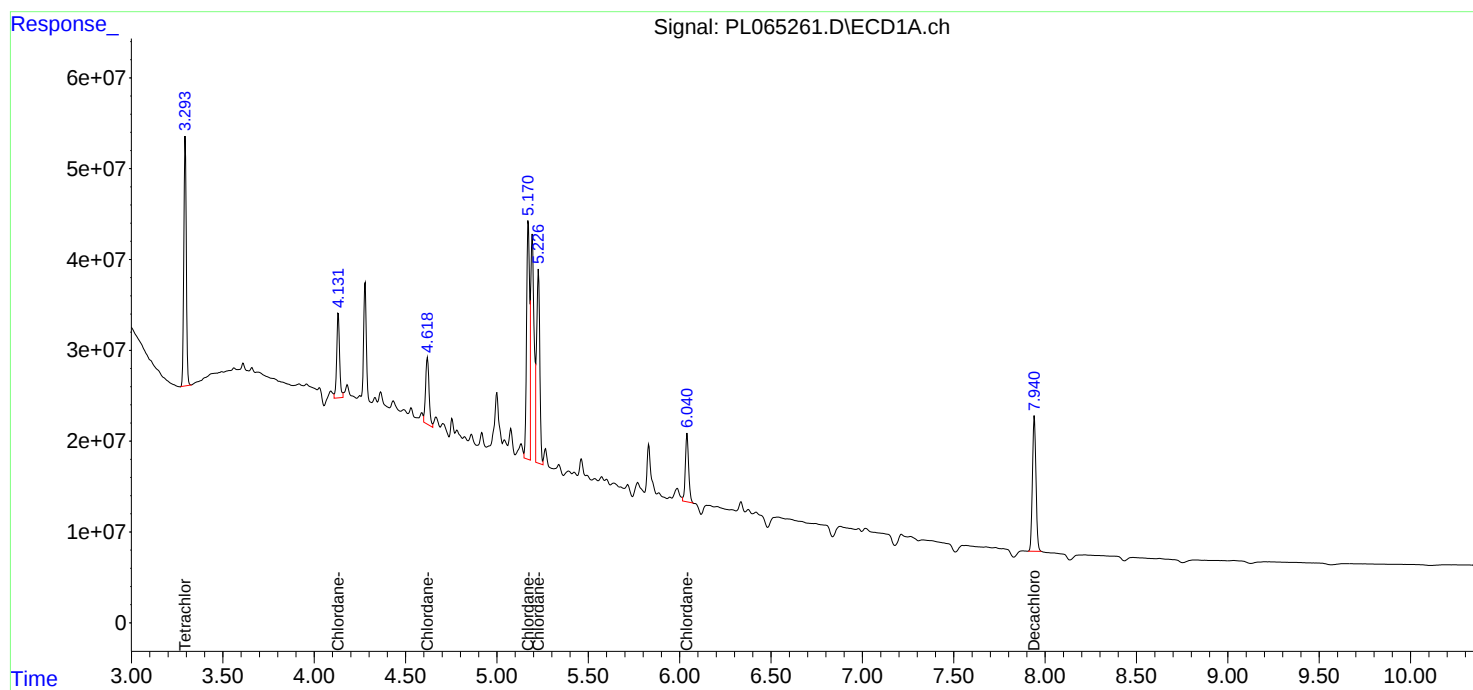


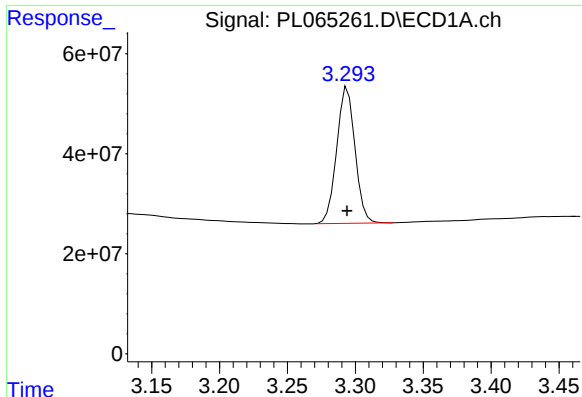

#1 Tetrachloro-m-xylene


R.T.: 3.294 min
Delta R.T.: 0.000 min
Response: 255570002
Conc: 98.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

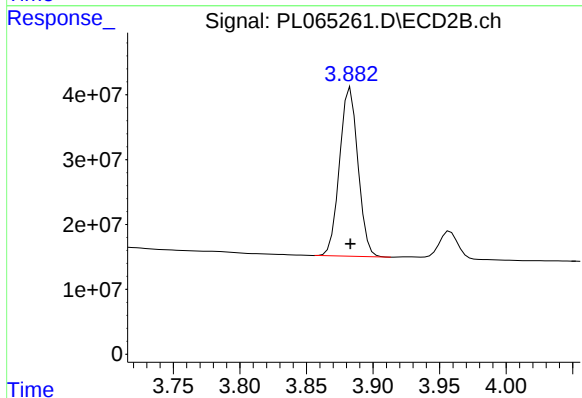


#1 Tetrachloro-m-xylene

R.T.: 3.883 min
Delta R.T.: 0.000 min
Response: 250161197
Conc: 93.85 ng/ml

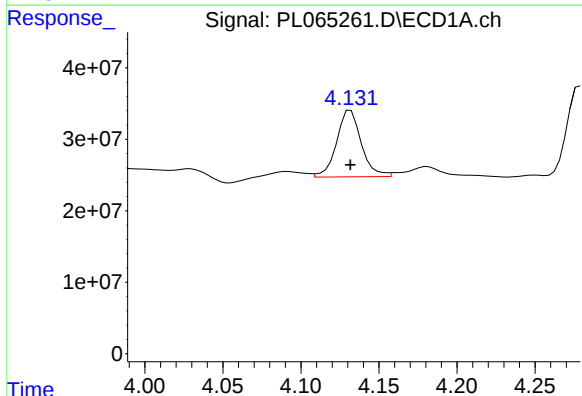


#23 Chlordane-1

R.T.: 4.132 min
Delta R.T.: 0.000 min
Response: 102494167
Conc: 906.21 ng/ml

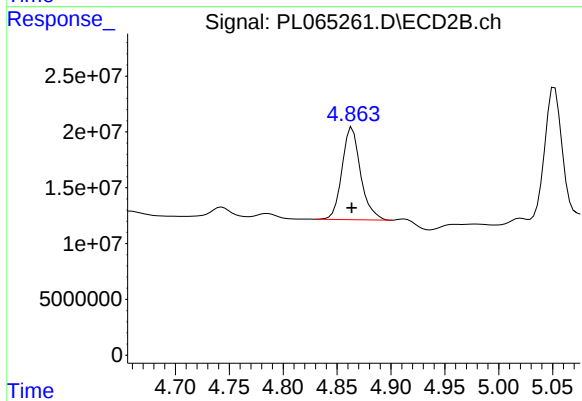

#23 Chlordane-1


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 99150412
Conc: 989.09 ng/ml

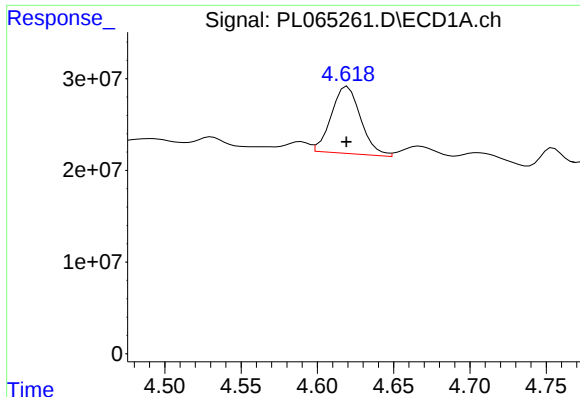

#24 Chlordane-2


R.T.: 4.620 min
Delta R.T.: 0.000 min
Response: 98123966
Conc: 989.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

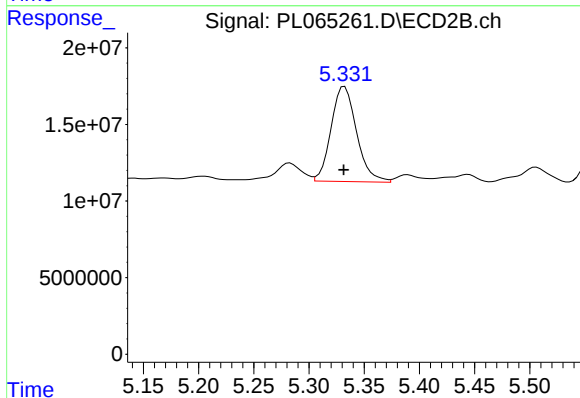


#24 Chlordane-2

R.T.: 5.332 min
Delta R.T.: 0.000 min
Response: 99804678
Conc: 969.57 ng/ml

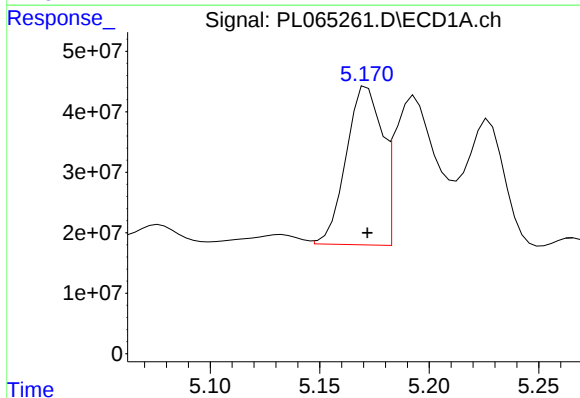


#25 Chlordane-3

R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 296726708
Conc: 969.17 ng/ml

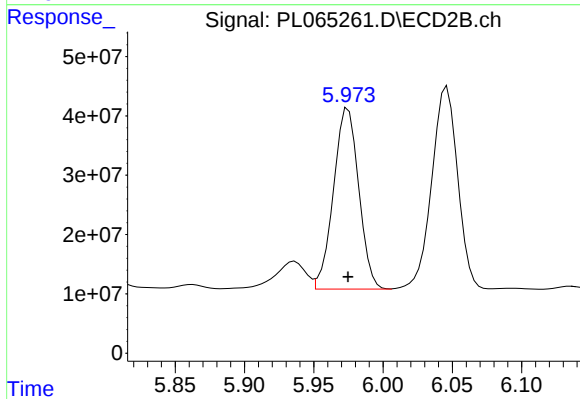

#25 Chlordane-3


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 387380953
Conc: 947.11 ng/ml

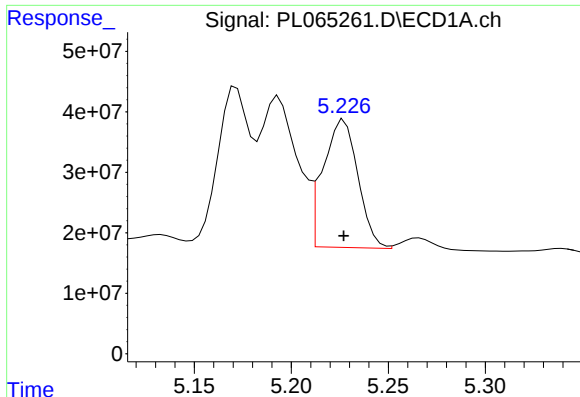

#26 Chlordane-4


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 264285291
Conc: 974.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

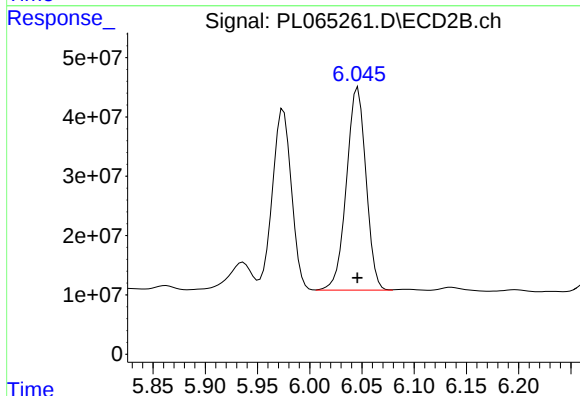


#26 Chlordane-4

R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 444390259
Conc: 946.23 ng/ml

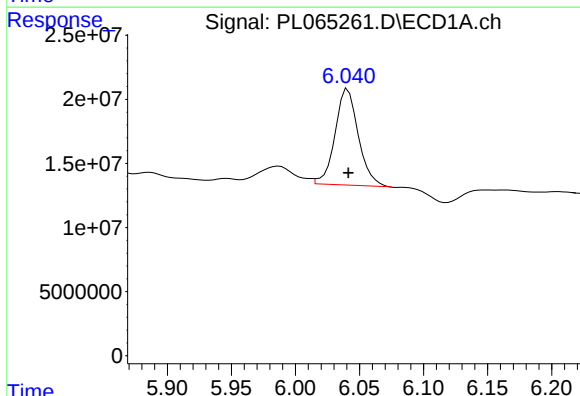


#27 Chlordane-5

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 94433099
Conc: 984.29 ng/ml

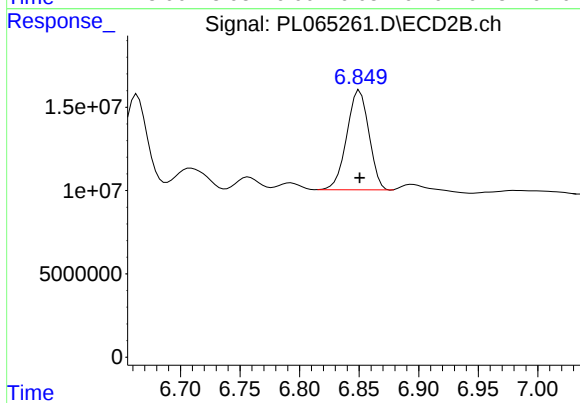

#27 Chlordane-5


R.T.: 6.851 min
Delta R.T.: 0.000 min
Response: 77067670
Conc: 958.55 ng/ml

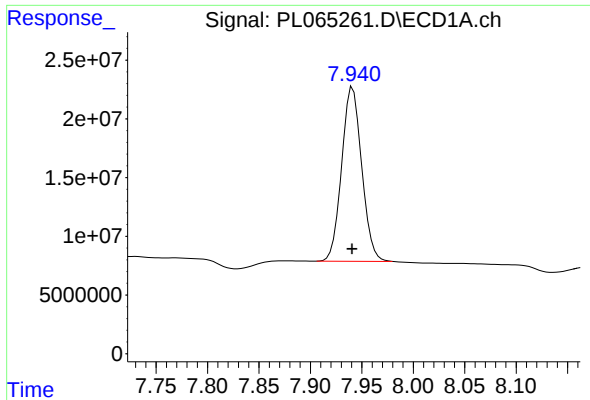

#28 Decachlorobiphenyl

R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 201137119
Conc: 96.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

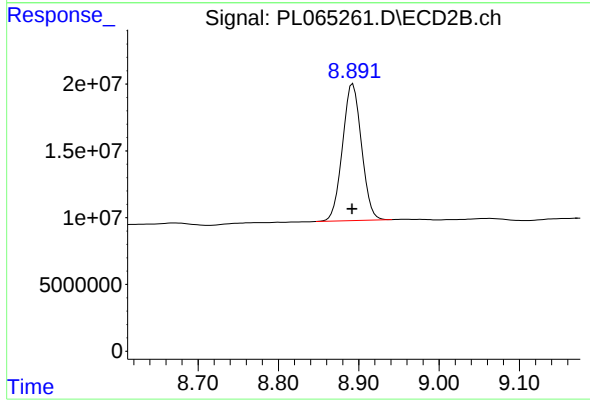

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: 0.001 min
Response: 167988789
Conc: 95.41 ng/ml