

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
 Data File : PL065262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2021 20:04
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 00:55:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 00:55:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.882	194.2E6	192.9E6	74.469	72.346
28)	SA Decachlor...	7.940	8.891	153.6E6	130.1E6	73.779	73.869
Target Compounds							
23)	Chlordane-1	4.131	4.863	81921984	77650173	724.323	774.610
24)	Chlordane-2	4.619	5.332	73787916	77743117	743.993	755.247
25)	Chlordane-3	5.171	5.974	223.9E6	301.2E6	731.445	736.381
26)	Chlordane-4	5.227	6.045	199.0E6	344.7E6	733.804	733.962
27)	Chlordane-5	6.040	6.850	73000991	58313979	760.899	725.294


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
Data File : PL065262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2021 20:04
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 00:55:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 00:55:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

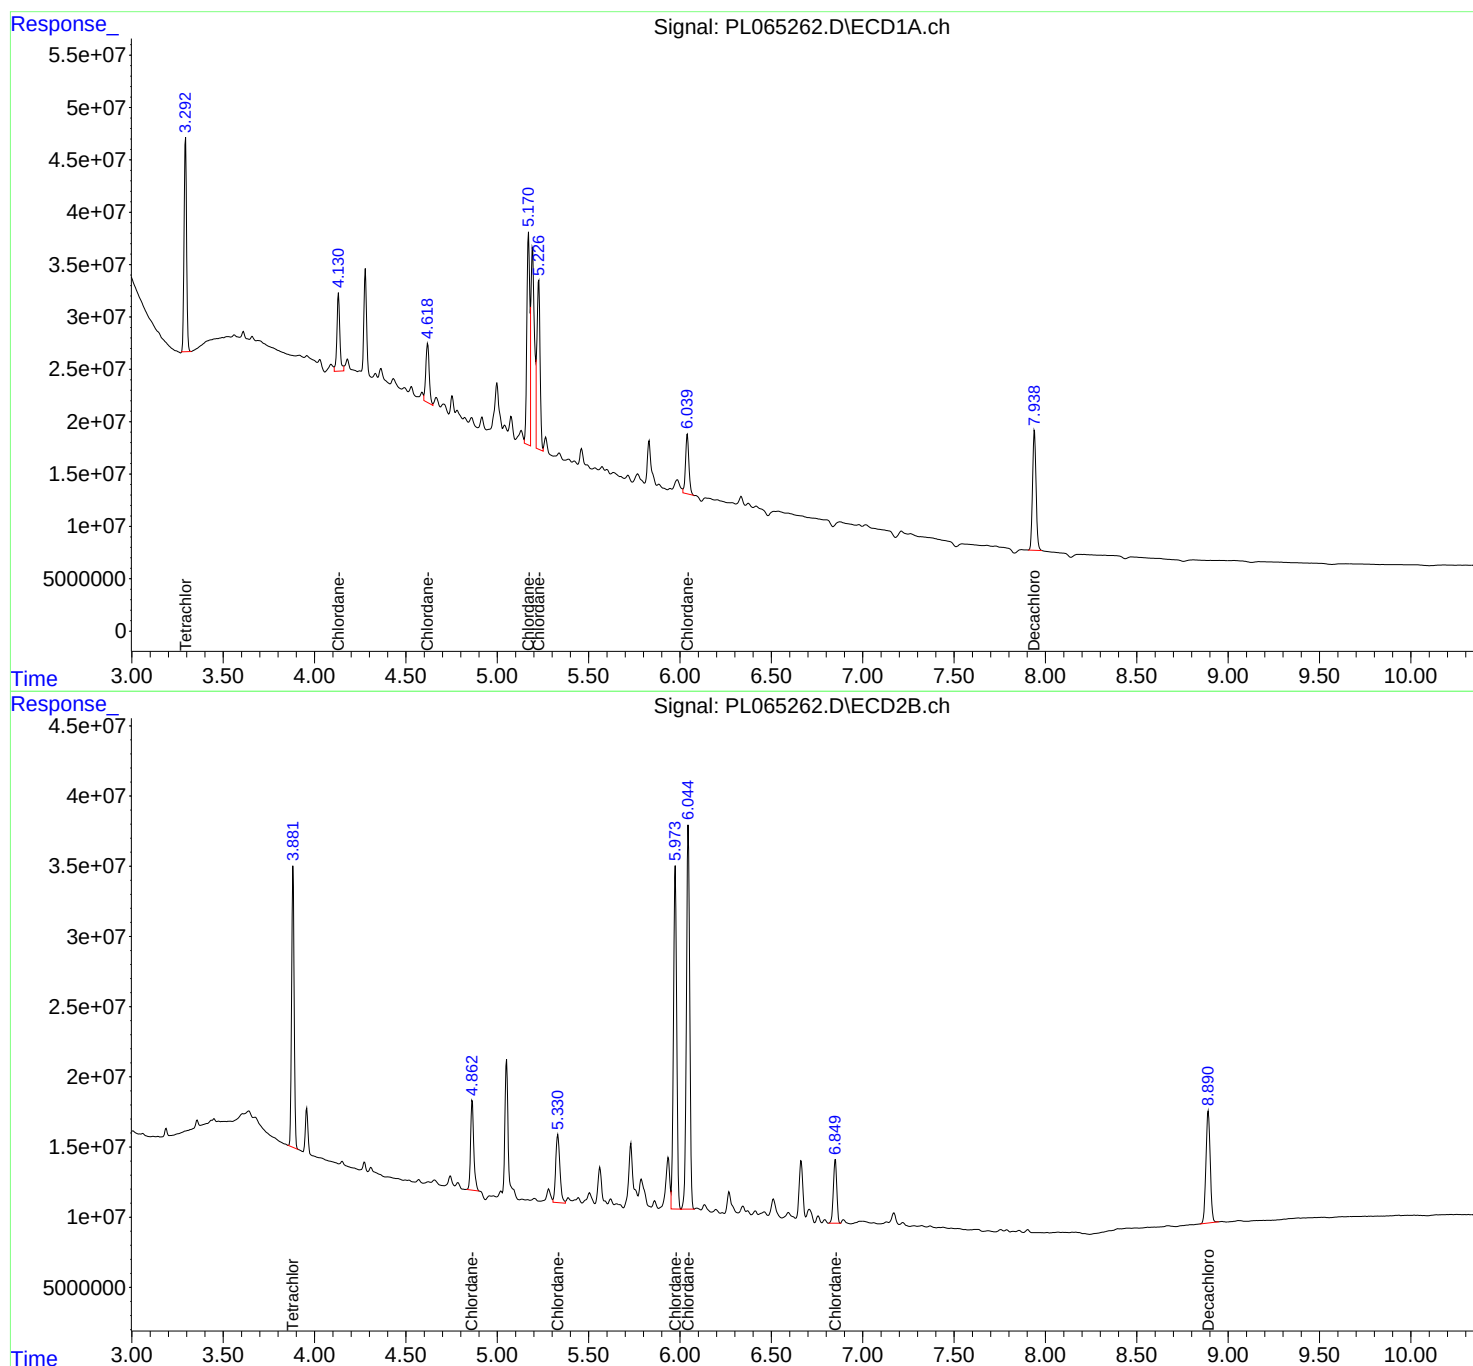


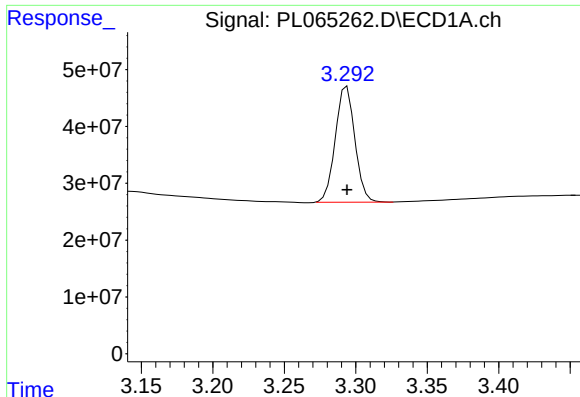

#1 Tetrachloro-m-xylene


R.T.: 3.294 min
Delta R.T.: 0.000 min
Response: 194167325
Conc: 74.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

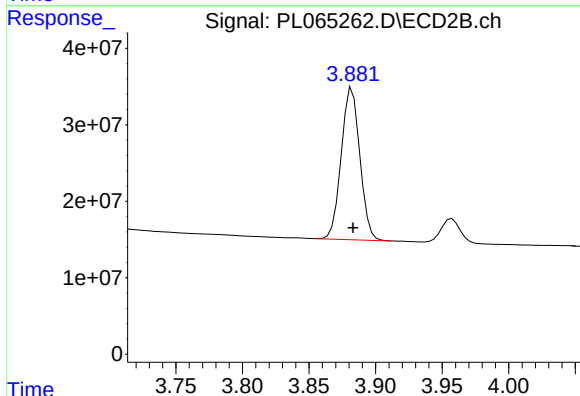


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.000 min
Response: 192850765
Conc: 72.35 ng/ml

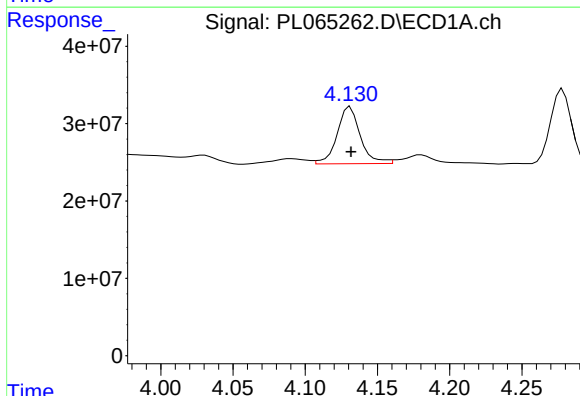


#23 Chlordane-1

R.T.: 4.131 min
Delta R.T.: 0.000 min
Response: 81921984
Conc: 724.32 ng/ml

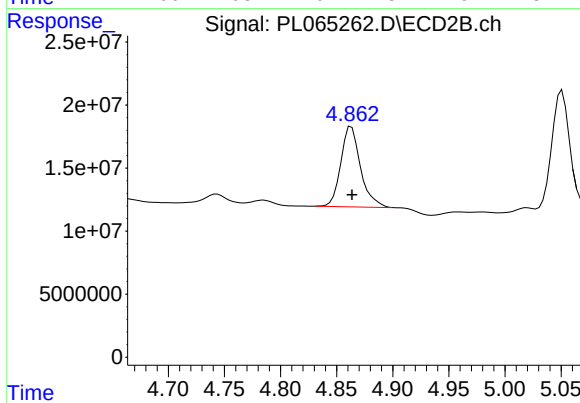

#23 Chlordane-1


R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 77650173
Conc: 774.61 ng/ml

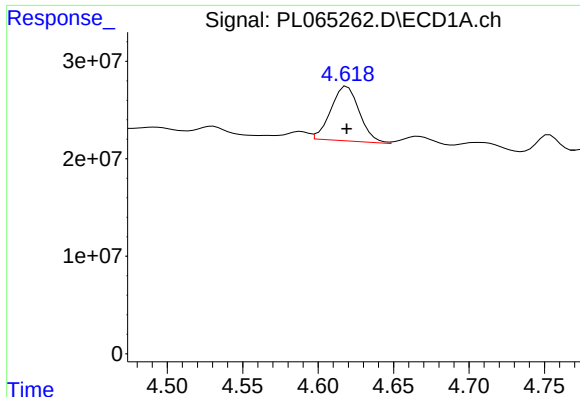

#24 Chlordane-2


R.T.: 4.619 min
Delta R.T.: 0.000 min
Response: 73787916
Conc: 743.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

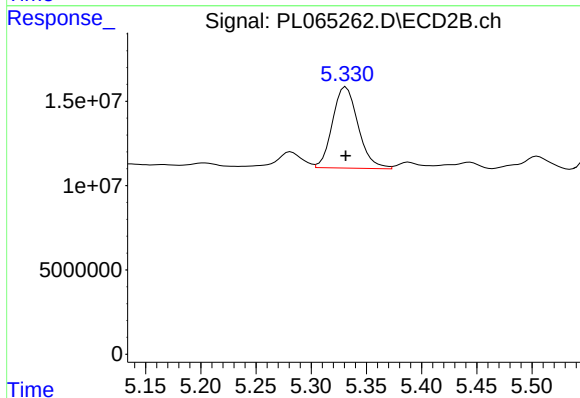


#24 Chlordane-2

R.T.: 5.332 min
Delta R.T.: 0.000 min
Response: 77743117
Conc: 755.25 ng/ml

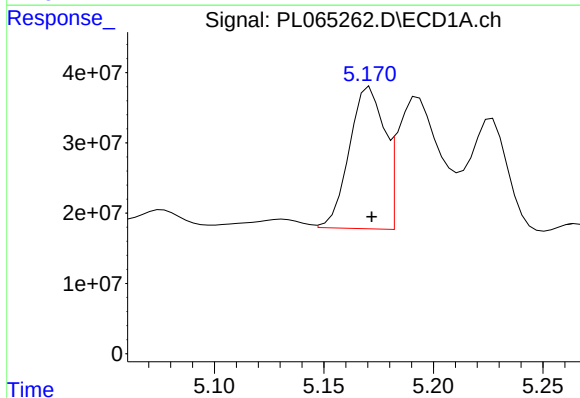


#25 Chlordane-3

R.T.: 5.171 min
Delta R.T.: 0.000 min
Response: 223944235
Conc: 731.45 ng/ml

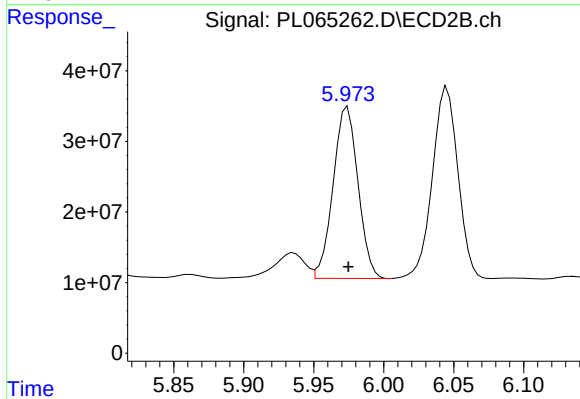

#25 Chlordane-3


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 301191451
Conc: 736.38 ng/ml

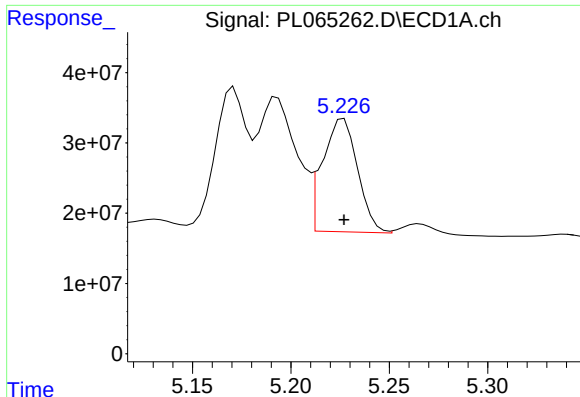

#26 Chlordane-4


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 198952108
Conc: 733.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

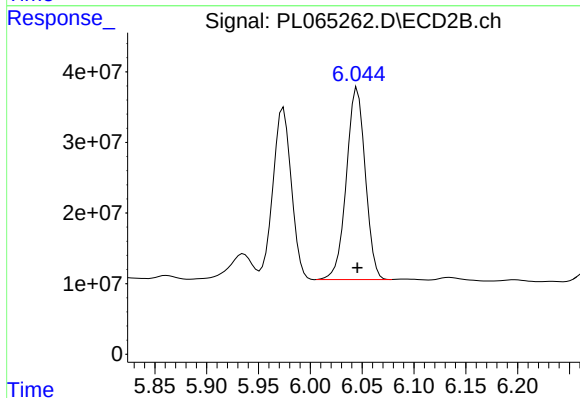


#26 Chlordane-4

R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 344701341
Conc: 733.96 ng/ml

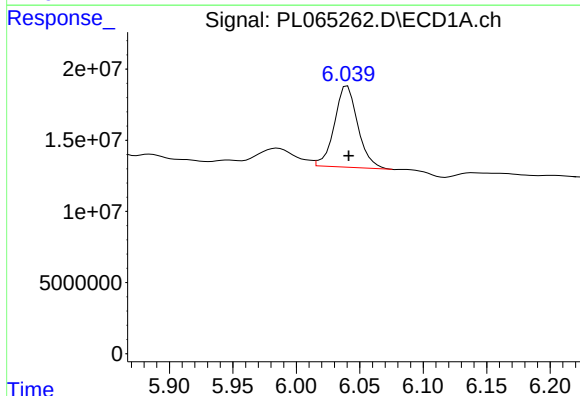


#27 Chlordane-5

R.T.: 6.040 min
Delta R.T.: 0.000 min
Response: 73000991
Conc: 760.90 ng/ml

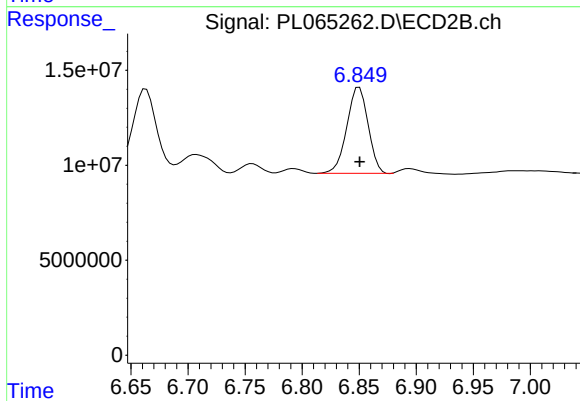

#27 Chlordane-5


R.T.: 6.850 min
Delta R.T.: 0.000 min
Response: 58313979
Conc: 725.29 ng/ml

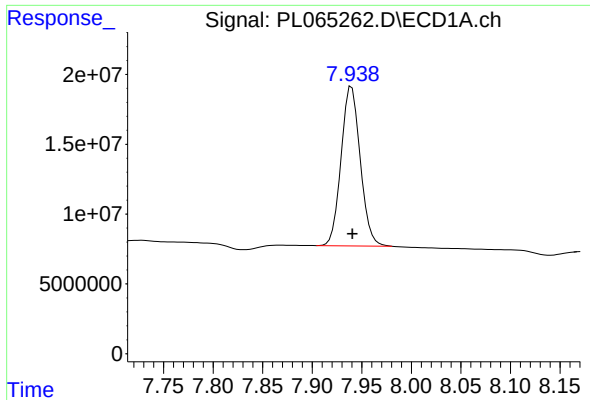

#28 Decachlorobiphenyl

R.T.: 7.940 min
Delta R.T.: 0.000 min
Response: 153567328
Conc: 73.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

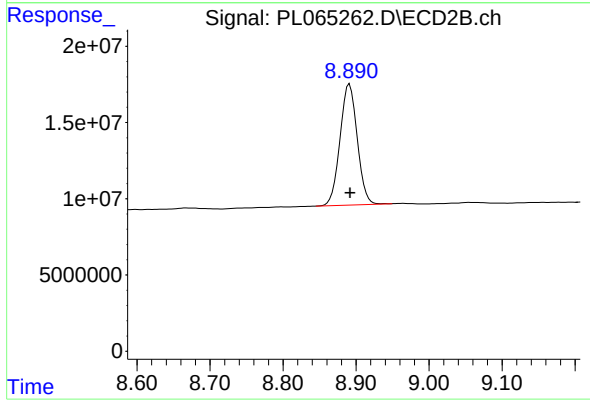

#28 Decachlorobiphenyl

R.T.: 8.891 min
Delta R.T.: 0.000 min
Response: 130060973
Conc: 73.87 ng/ml