

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
 Data File : PL065263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2021 20:18
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 00:56:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 00:55:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.883	130.4E6	133.3E6	50.000	50.000
28)	SA Decachlor...	7.940	8.892	104.1E6	88034301	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.132	4.864	56550694	50122100	500.000	500.000
24)	Chlordane-2	4.619	5.331	49589095	51468652	500.000	500.000
25)	Chlordane-3	5.172	5.975	153.1E6	204.5E6	500.000	500.000
26)	Chlordane-4	5.227	6.046	135.6E6	234.8E6	500.000	500.000
27)	Chlordane-5	6.041	6.850	47970219	40200245	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
Data File : PL065263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2021 20:18
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 00:56:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 00:55:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

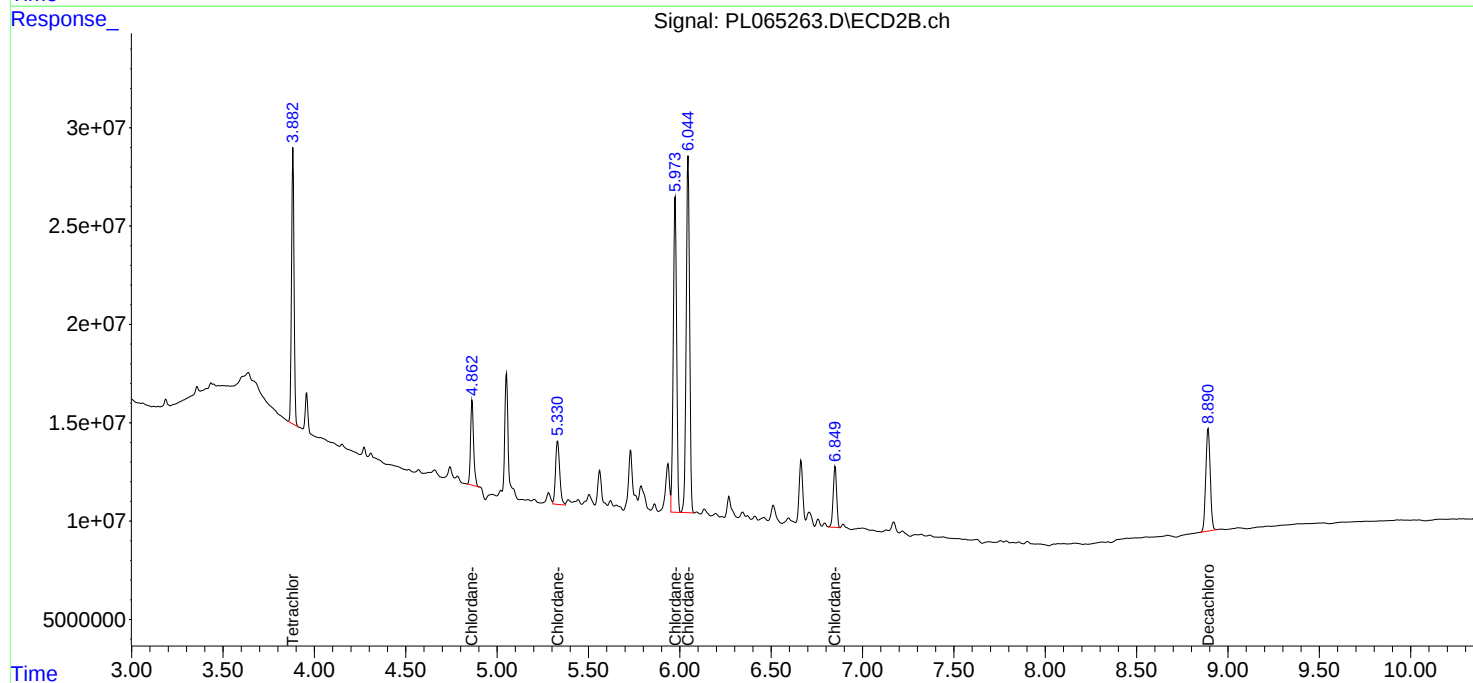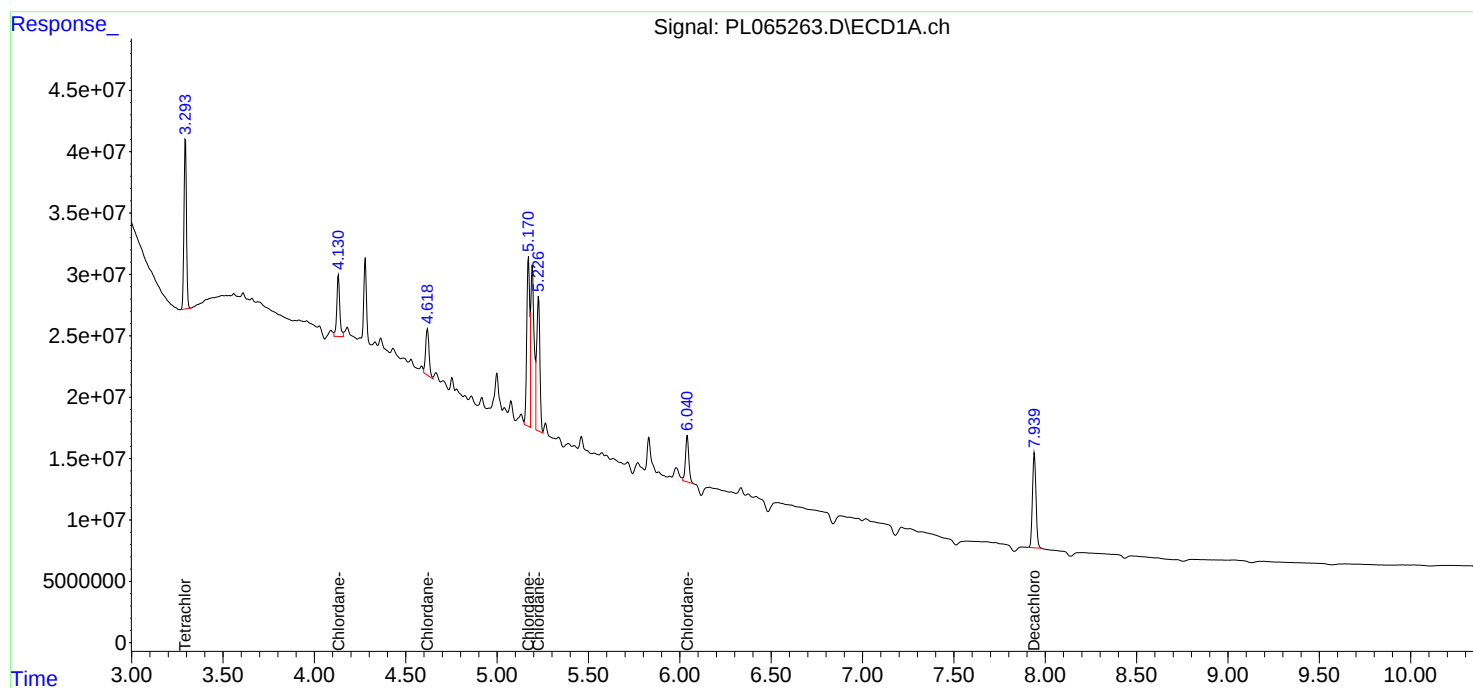


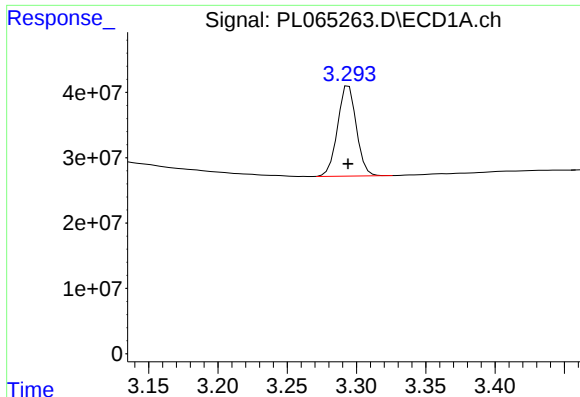

#1 Tetrachloro-m-xylene


R.T.: 3.294 min
Delta R.T.: 0.000 min
Response: 130367305
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

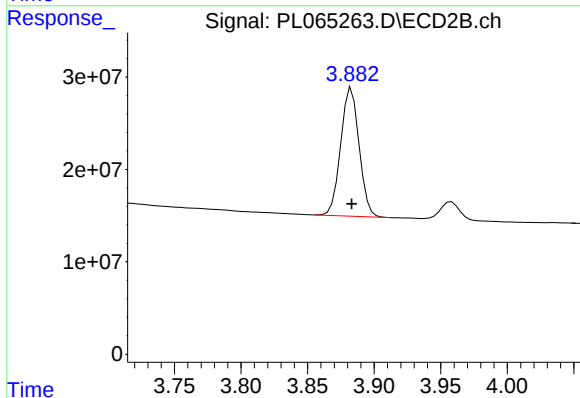


#1 Tetrachloro-m-xylene

R.T.: 3.883 min
Delta R.T.: 0.000 min
Response: 133283812
Conc: 50.00 ng/ml

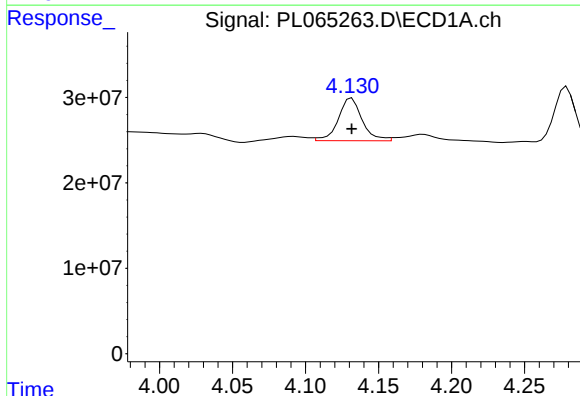


#23 Chlordane-1

R.T.: 4.132 min
Delta R.T.: 0.000 min
Response: 56550694
Conc: 500.00 ng/ml

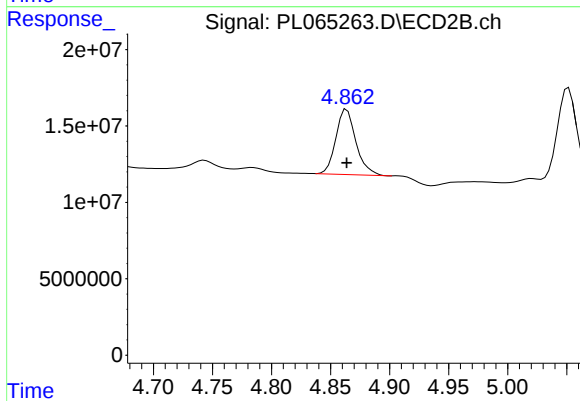

#23 Chlordane-1


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 50122100
Conc: 500.00 ng/ml

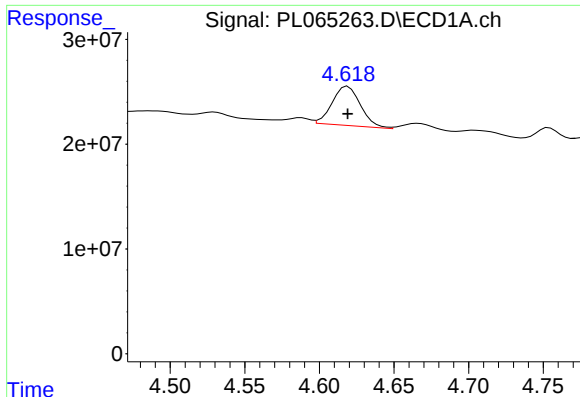

#24 Chlordane-2


R.T.: 4.619 min
Delta R.T.: 0.000 min
Response: 49589095
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

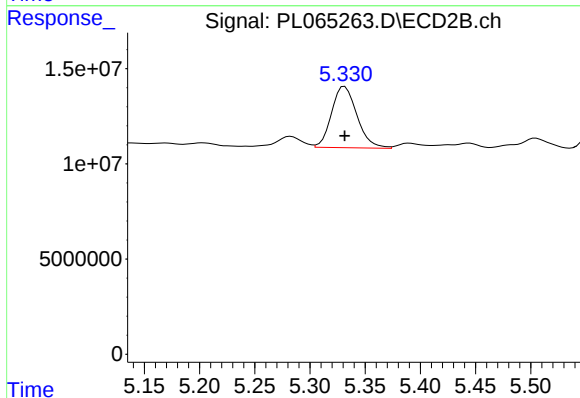


#24 Chlordane-2

R.T.: 5.331 min
Delta R.T.: 0.000 min
Response: 51468652
Conc: 500.00 ng/ml

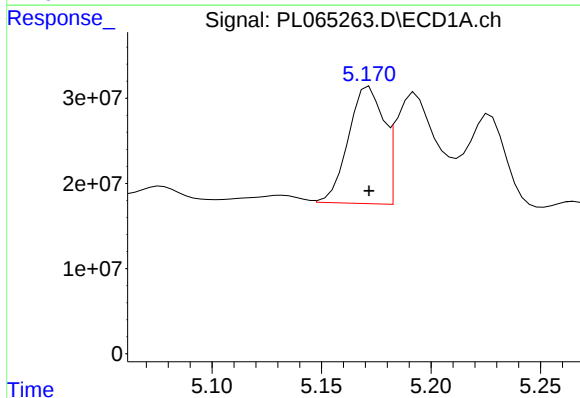


#25 Chlordane-3

R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 153083380
Conc: 500.00 ng/ml

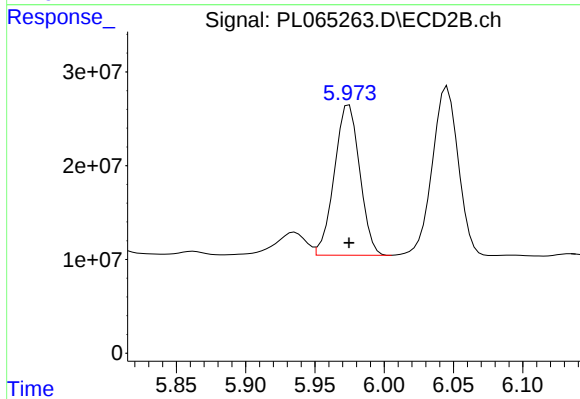

#25 Chlordane-3


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 204507853
Conc: 500.00 ng/ml

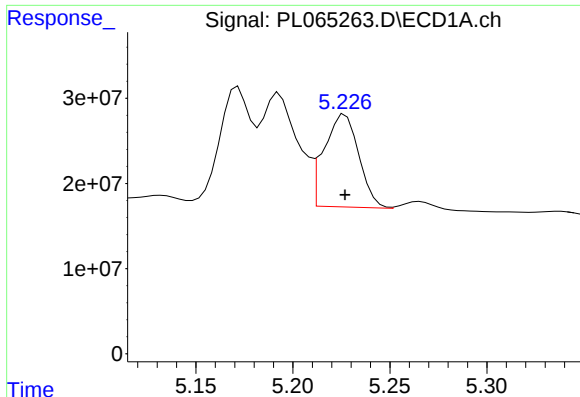

#26 Chlordane-4


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 135562144
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

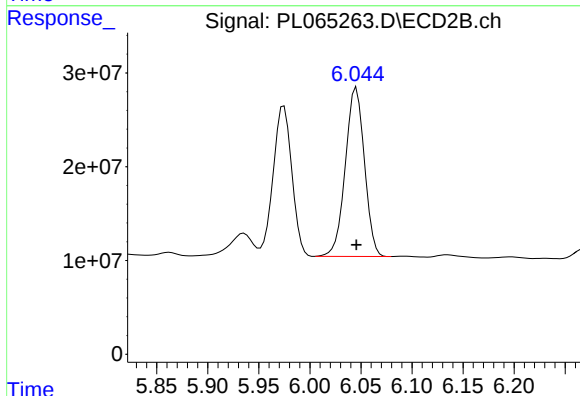


#26 Chlordane-4

R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 234822205
Conc: 500.00 ng/ml

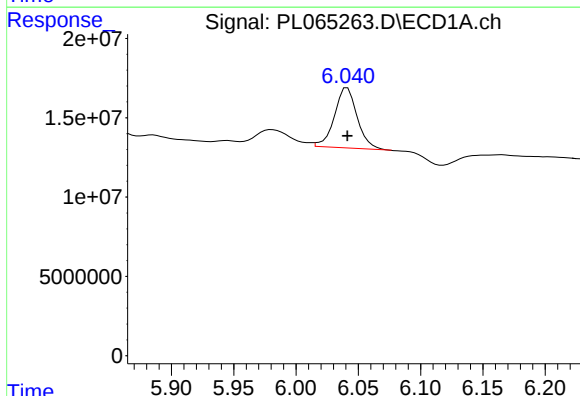


#27 Chlordane-5

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 47970219
Conc: 500.00 ng/ml

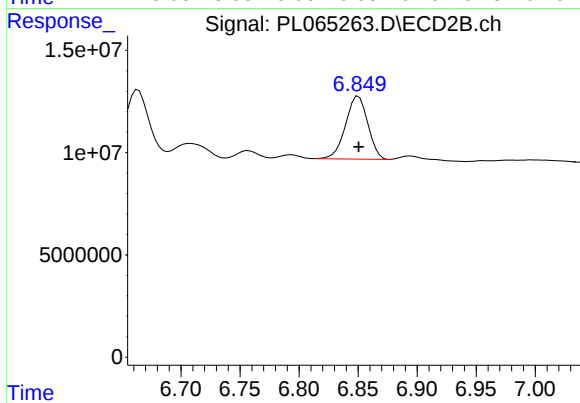

#27 Chlordane-5

R.T.: 6.850 min
Delta R.T.: 0.000 min
Response: 40200245
Conc: 500.00 ng/ml

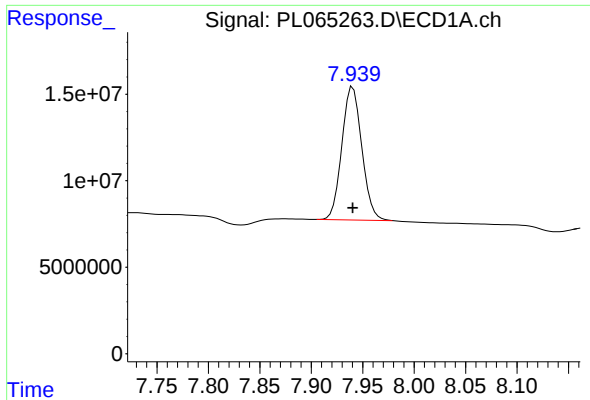

#28 Decachlorobiphenyl


R.T.: 7.940 min

Delta R.T.: 0.000 min

Response: 104072016

Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

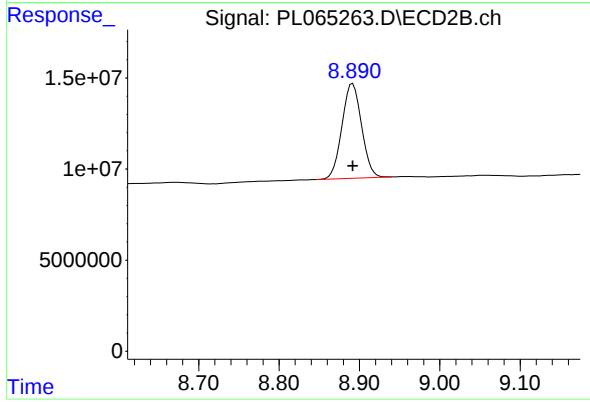

#28 Decachlorobiphenyl

R.T.: 8.892 min

Delta R.T.: 0.000 min

Response: 88034301

Conc: 50.00 ng/ml