

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
 Data File : PL065277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2021 23:40
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:49:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 01:11:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.883	128.6E6	132.9E6	54.590	48.265
28)	SA Decachlor...	7.940	8.897	105.5E6	91916076	48.978	50.031
Target Compounds							
23)	Chlordane-1	4.131	4.863	60273637	52435442	581.557	536.580
24)	Chlordane-2	4.619	5.331	49791282	51745868	501.632	502.767
25)	Chlordane-3	5.171	5.975	153.4E6	208.5E6	510.053	510.119
26)	Chlordane-4	5.226	6.046	137.2E6	238.7E6	504.366	503.517
27)	Chlordane-5	6.041	6.852	48133452	44189717	530.208	557.096



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
Data File : PL065277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2021 23:40
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:49:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 01:11:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

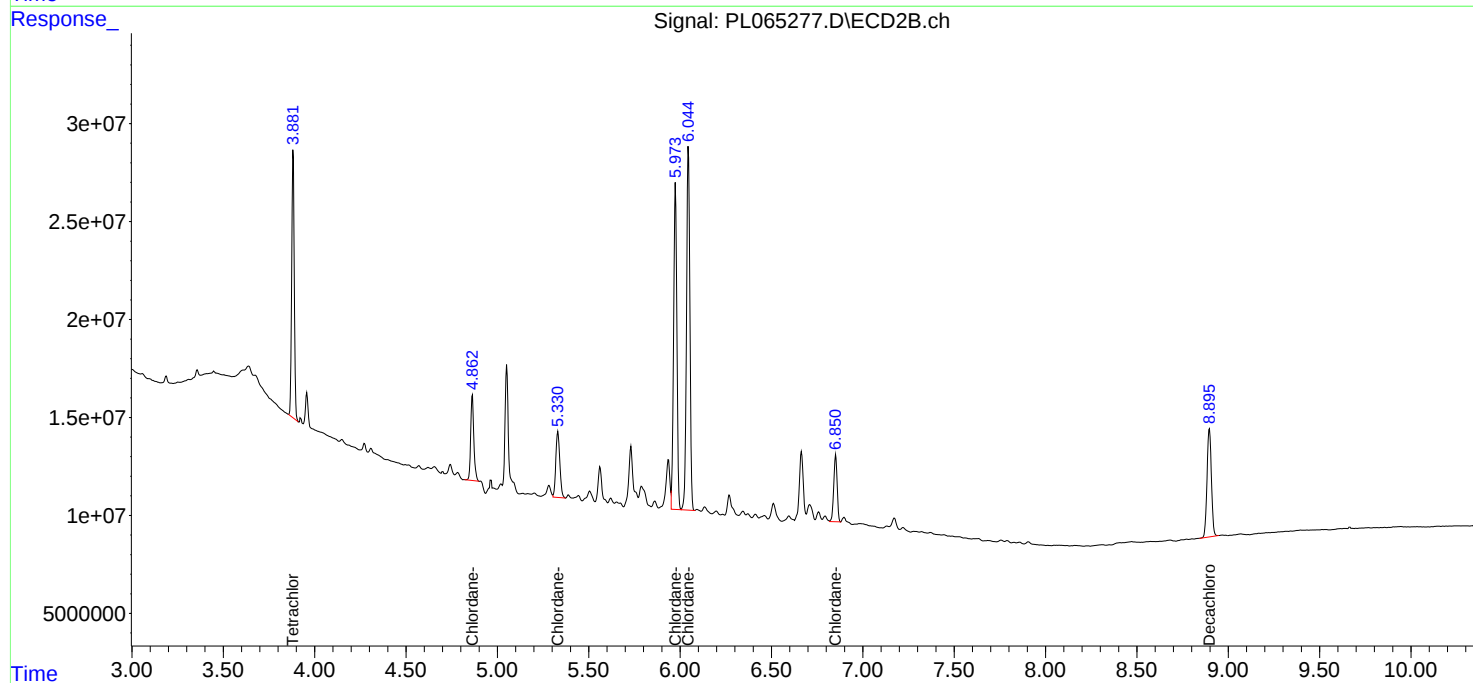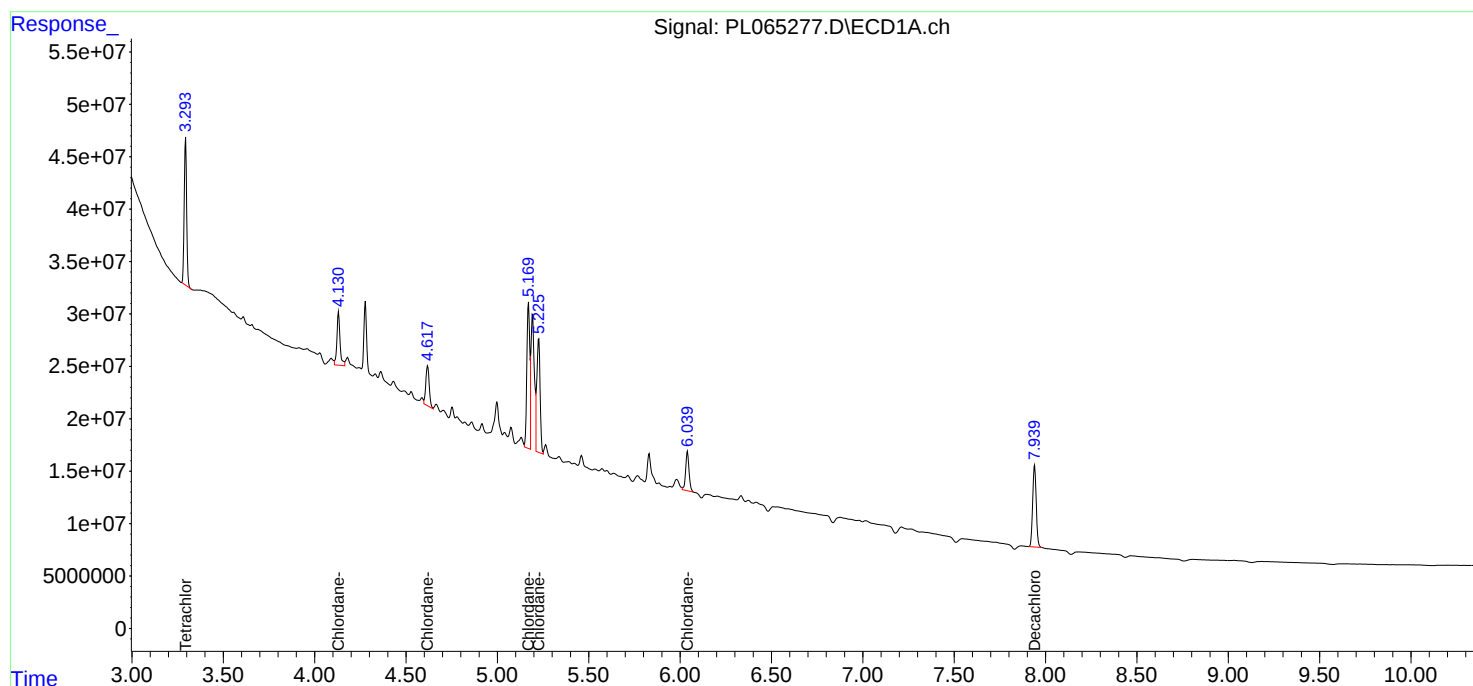


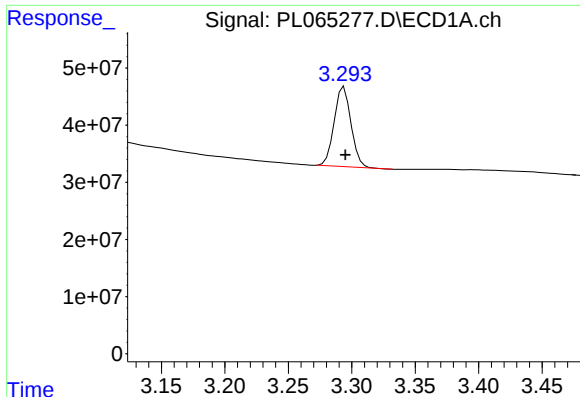

#1 Tetrachloro-m-xylene


R.T.: 3.294 min
Delta R.T.: -0.001 min
Response: 128612838
Conc: 54.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

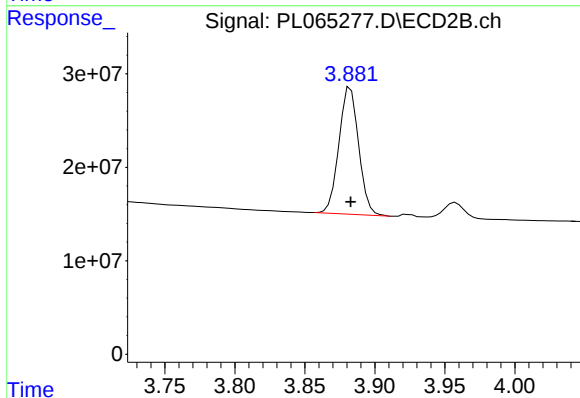


#1 Tetrachloro-m-xylene

R.T.: 3.883 min
Delta R.T.: 0.000 min
Response: 132947330
Conc: 48.27 ng/ml

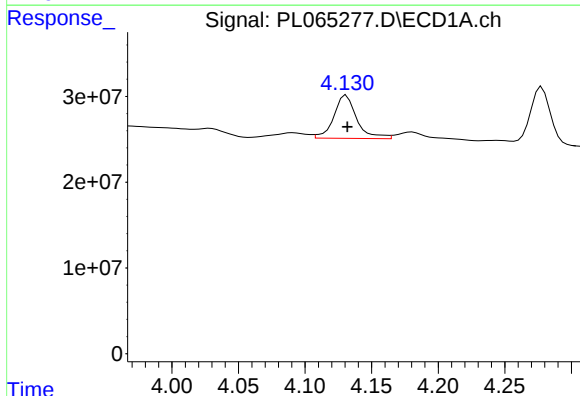


#23 Chlordane-1

R.T.: 4.131 min
Delta R.T.: 0.000 min
Response: 60273637
Conc: 581.56 ng/ml

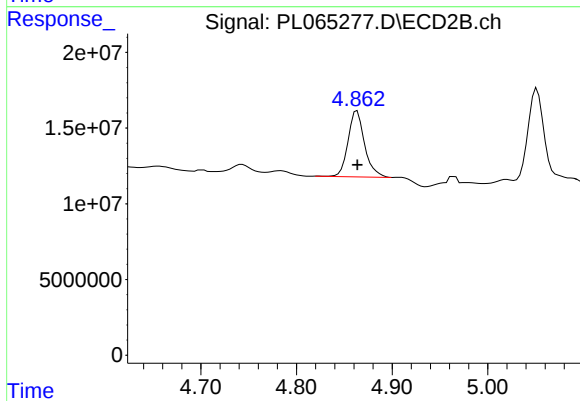

#23 Chlordane-1


R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 52435442
Conc: 536.58 ng/ml

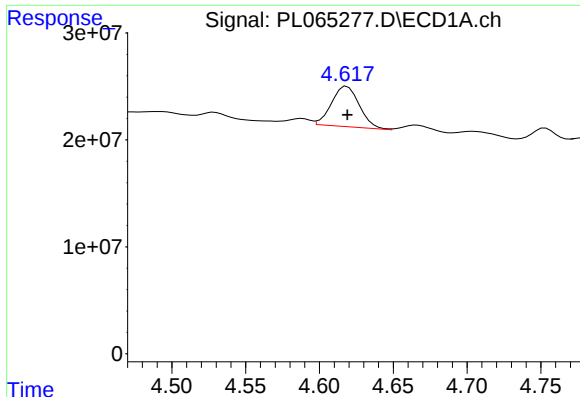

#24 Chlordane-2


R.T.: 4.619 min
Delta R.T.: 0.000 min
Response: 49791282
Conc: 501.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

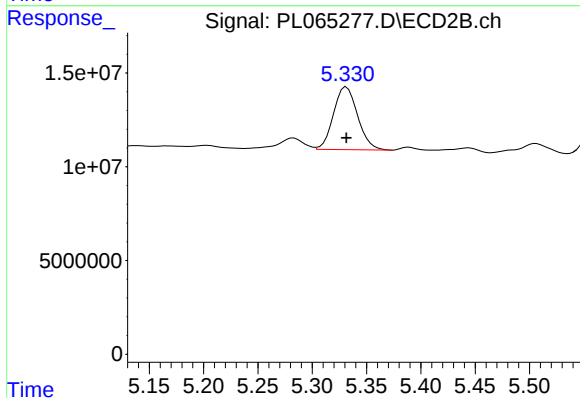


#24 Chlordane-2

R.T.: 5.331 min
Delta R.T.: 0.000 min
Response: 51745868
Conc: 502.77 ng/ml

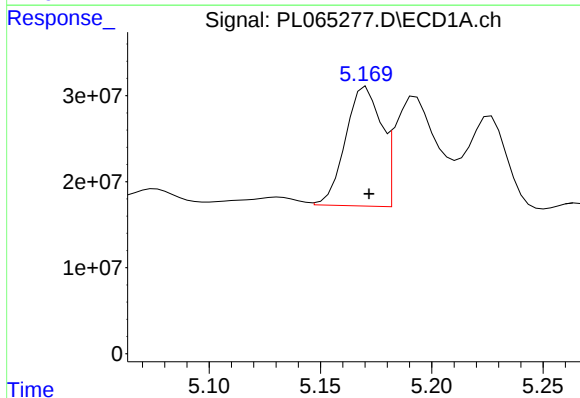


#25 Chlordane-3

R.T.: 5.171 min
Delta R.T.: -0.001 min
Response: 153399027
Conc: 510.05 ng/ml

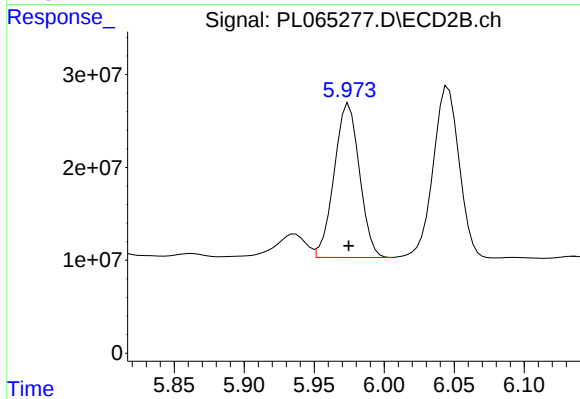

#25 Chlordane-3


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 208496809
Conc: 510.12 ng/ml

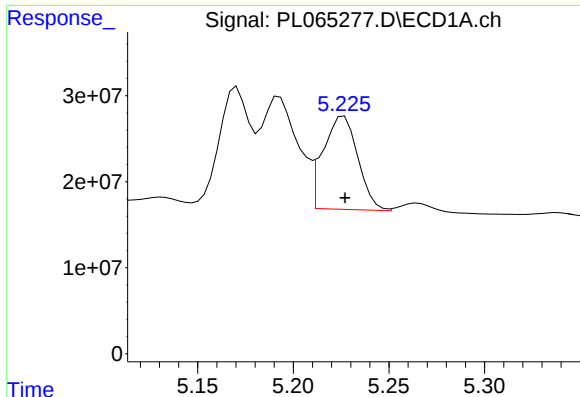

#26 Chlordane-4


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 137220150
Conc: 504.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

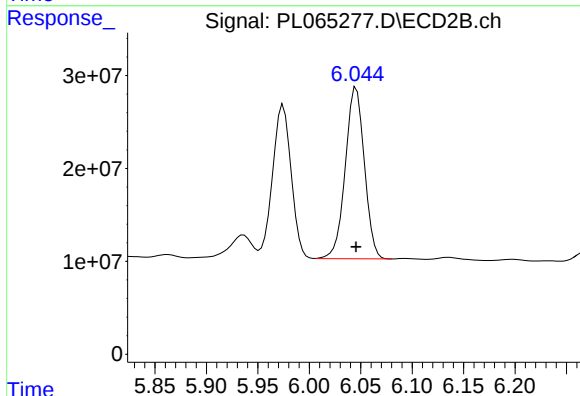


#26 Chlordane-4

R.T.: 6.046 min
Delta R.T.: 0.000 min
Response: 238721040
Conc: 503.52 ng/ml

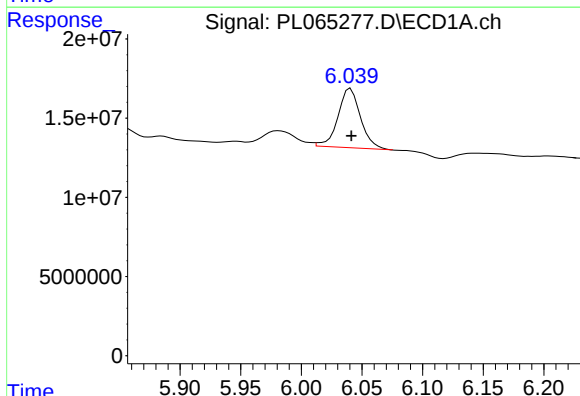


#27 Chlordane-5

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 48133452
Conc: 530.21 ng/ml

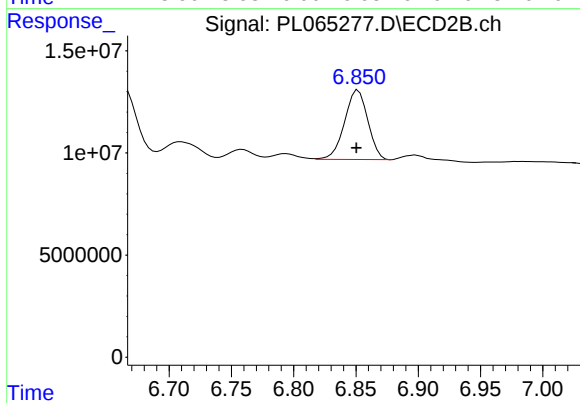

#27 Chlordane-5


R.T.: 6.852 min
Delta R.T.: 0.001 min
Response: 44189717
Conc: 557.10 ng/ml

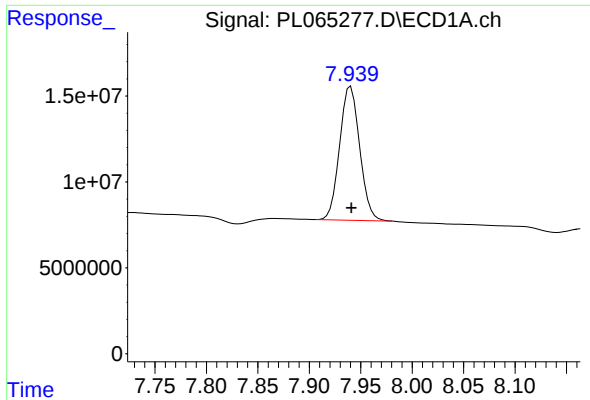

#28 Decachlorobiphenyl

R.T.: 7.940 min
Delta R.T.: 0.000 min
Response: 105543514
Conc: 48.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

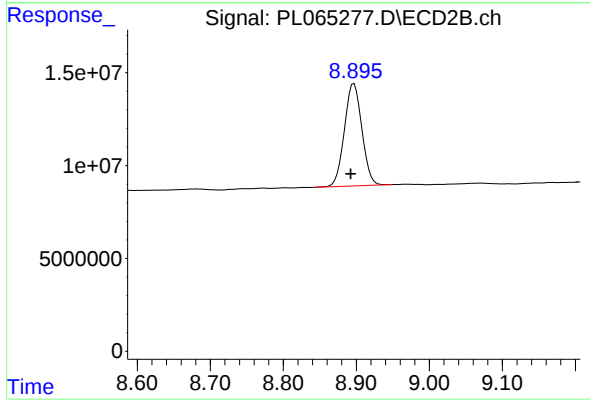

#28 Decachlorobiphenyl

R.T.: 8.897 min
Delta R.T.: 0.004 min
Response: 91916076
Conc: 50.03 ng/ml