

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
 Data File : PL065287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2021 02:03
 Operator : AR\AJ
 Sample : M1557-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PT-CHLR-WP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:50:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 01:11:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.293	3.885	67694339	64510572	28.733	23.420
28)	SA Decachlor...	7.939	8.896	48979212	43270795	22.729	23.553
Target Compounds							
23)	Chlordane-1	4.131	4.866	92415747	93535601	891.684	957.164
24)	Chlordane-2	4.618	5.333	79767436	91444553	803.632	888.483
25)	Chlordane-3	5.171	5.977	275.3E6	342.6E6	915.342	838.224
26)	Chlordane-4	5.226	6.048	241.3E6	384.0E6	886.881	810.043
27)	Chlordane-5	6.041	6.853	70808961	64878550	779.987	817.918



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
Data File : PL065287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2021 02:03
Operator : AR\AJ
Sample : M1557-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:50:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 01:11:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

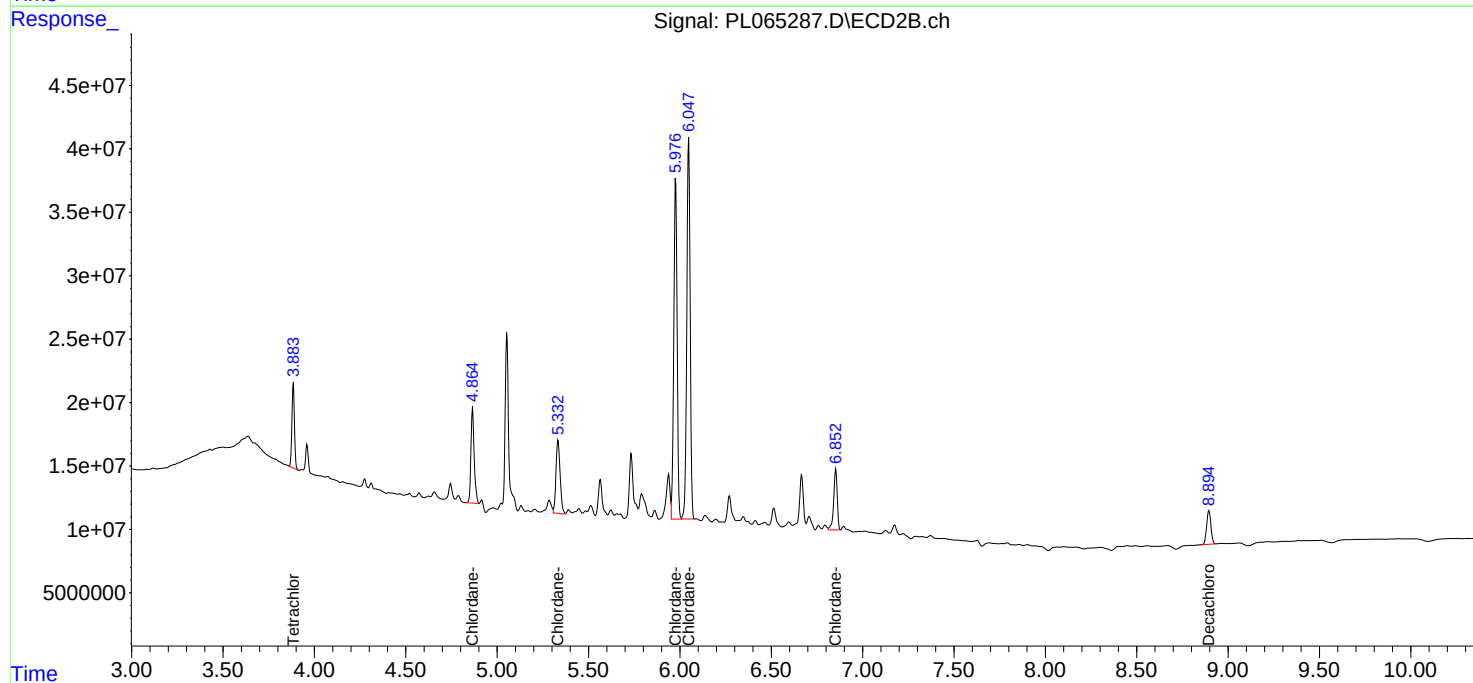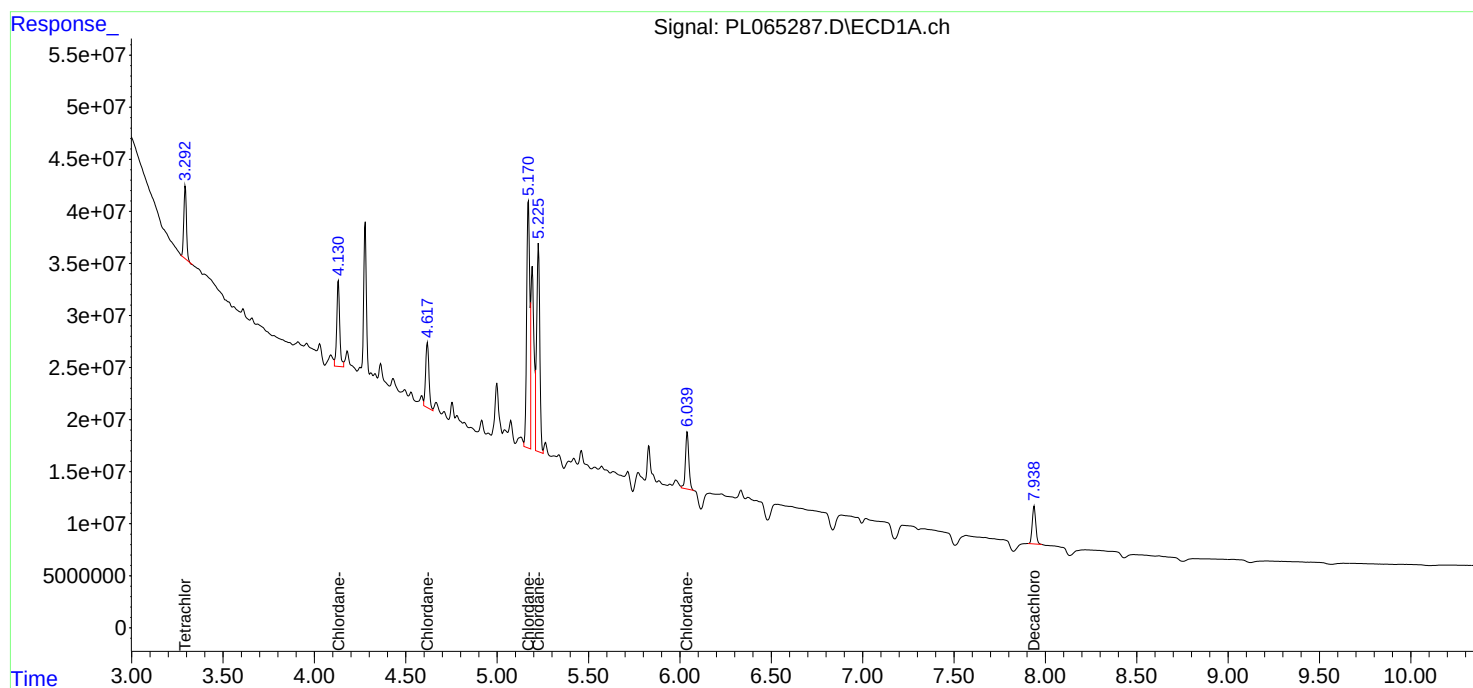


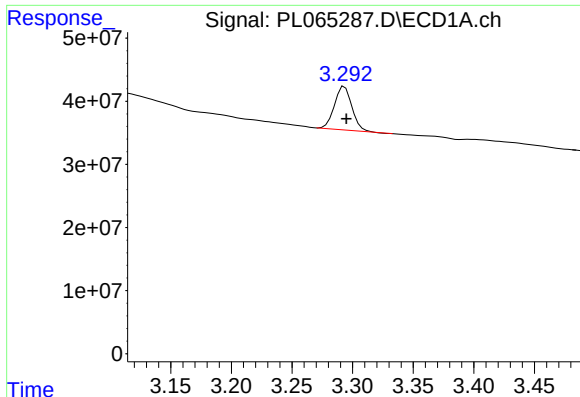

#1 Tetrachloro-m-xylene


R.T.: 3.293 min
Delta R.T.: -0.002 min
Response: 67694339
Conc: 28.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

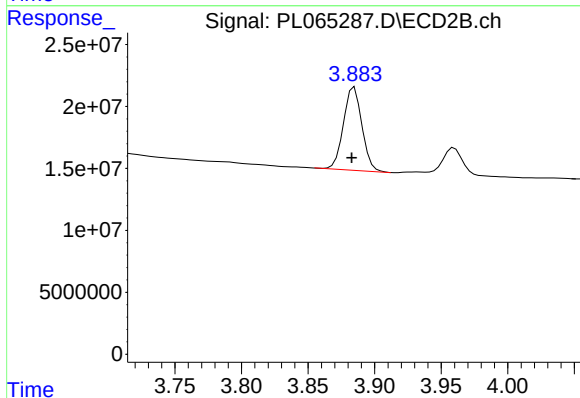


#1 Tetrachloro-m-xylene

R.T.: 3.885 min
Delta R.T.: 0.002 min
Response: 64510572
Conc: 23.42 ng/ml

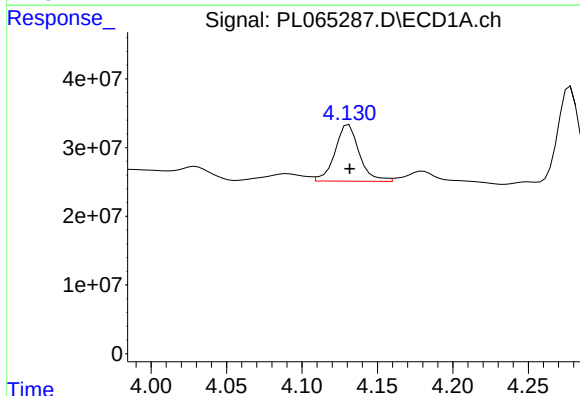


#23 Chlordane-1

R.T.: 4.131 min
Delta R.T.: 0.000 min
Response: 92415747
Conc: 891.68 ng/ml

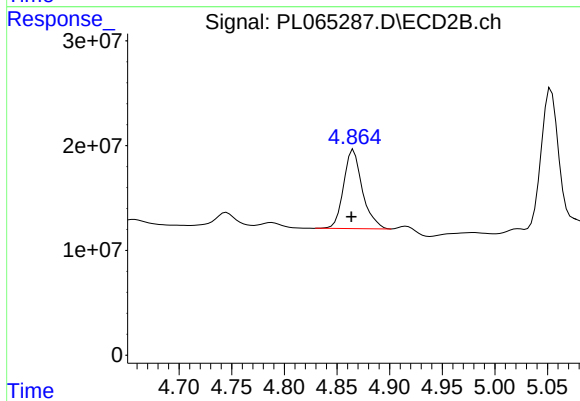

#23 Chlordane-1


R.T.: 4.866 min
Delta R.T.: 0.002 min
Response: 93535601
Conc: 957.16 ng/ml

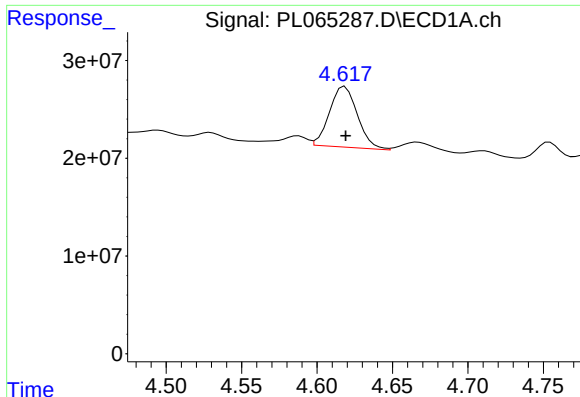

#24 Chlordane-2


R.T.: 4.618 min
Delta R.T.: 0.000 min
Response: 79767436
Conc: 803.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

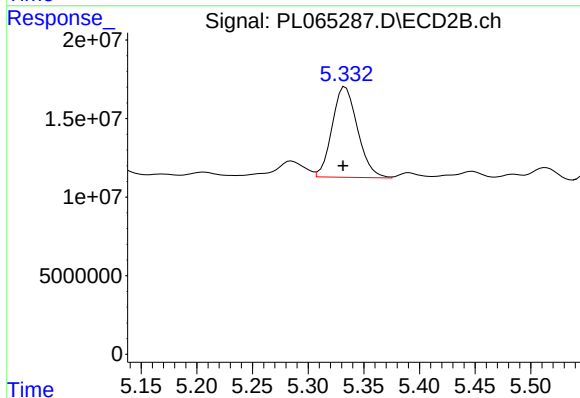


#24 Chlordane-2

R.T.: 5.333 min
Delta R.T.: 0.002 min
Response: 91444553
Conc: 888.48 ng/ml

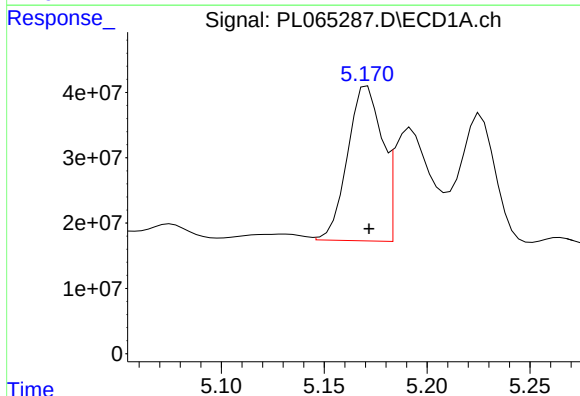


#25 Chlordane-3

R.T.: 5.171 min
Delta R.T.: 0.000 min
Response: 275289875
Conc: 915.34 ng/ml

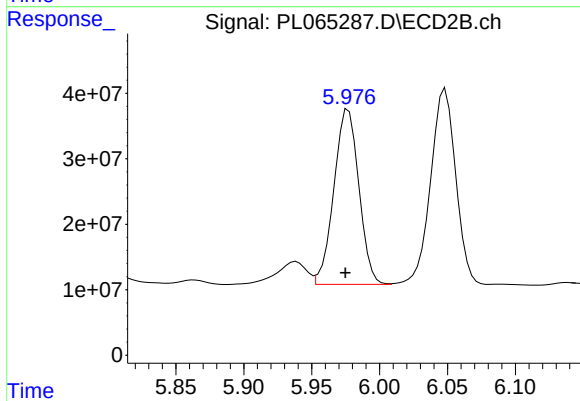

#25 Chlordane-3


R.T.: 5.977 min
Delta R.T.: 0.002 min
Response: 342600567
Conc: 838.22 ng/ml

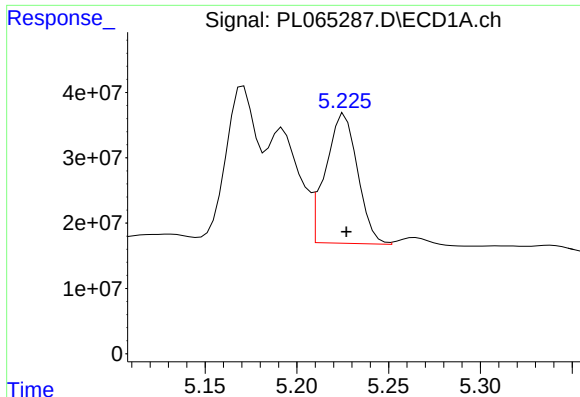

#26 Chlordane-4


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 241288811
Conc: 886.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

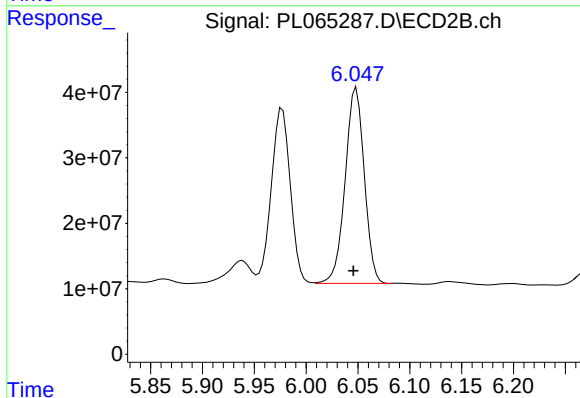


#26 Chlordane-4

R.T.: 6.048 min
Delta R.T.: 0.003 min
Response: 384047262
Conc: 810.04 ng/ml

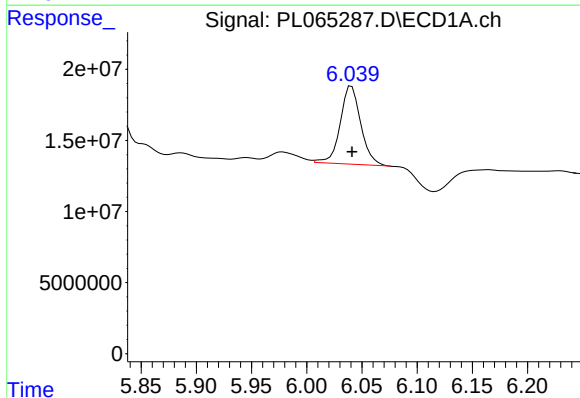


#27 Chlordane-5

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 70808961
Conc: 779.99 ng/ml

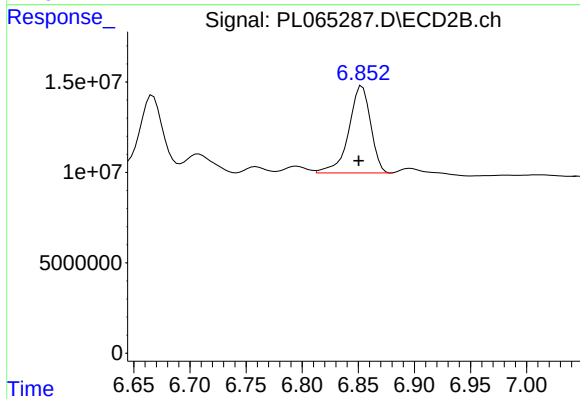

#27 Chlordane-5


R.T.: 6.853 min
Delta R.T.: 0.003 min
Response: 64878550
Conc: 817.92 ng/ml

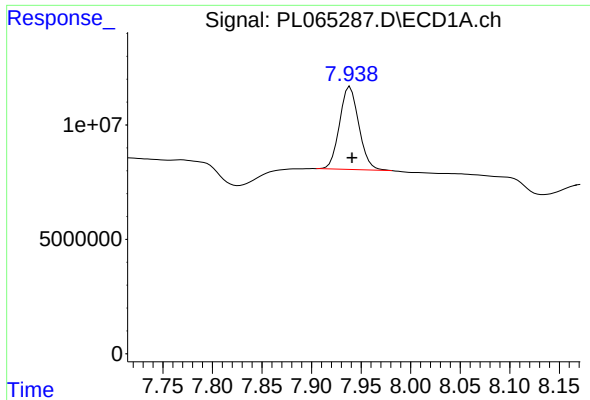

#28 Decachlorobiphenyl

R.T.: 7.939 min
Delta R.T.: -0.002 min
Response: 48979212
Conc: 22.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

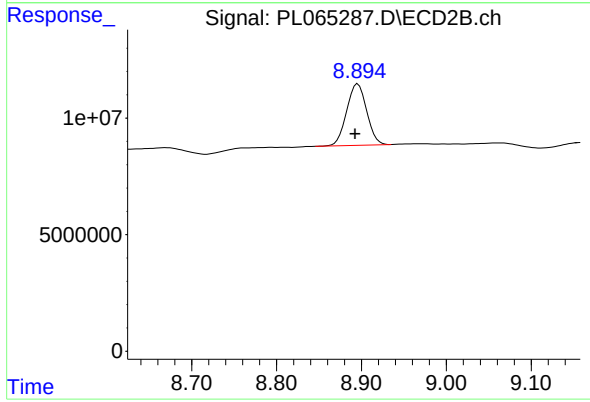

#28 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.003 min
Response: 43270795
Conc: 23.55 ng/ml