

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
 Data File : PL065294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2021 03:58
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:50:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 01:11:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.886	120.6E6	130.2E6	51.173	47.253
28)	SA Decachlor...	7.940	8.898	100.8E6	88543708	46.791	48.195
Target Compounds							
23)	Chlordane-1	4.131	4.867	44486543	50941026	429.234	521.287
24)	Chlordane-2	4.619	5.336	47462299	50064118	478.168	486.427
25)	Chlordane-3	5.171	5.979	145.9E6	203.0E6	485.066	496.790
26)	Chlordane-4	5.226	6.049	128.8E6	232.1E6	473.589	489.493
27)	Chlordane-5	6.041	6.855	44042336	39455987	485.143	497.418



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031321\
Data File : PL065294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2021 03:58
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:50:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 01:11:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

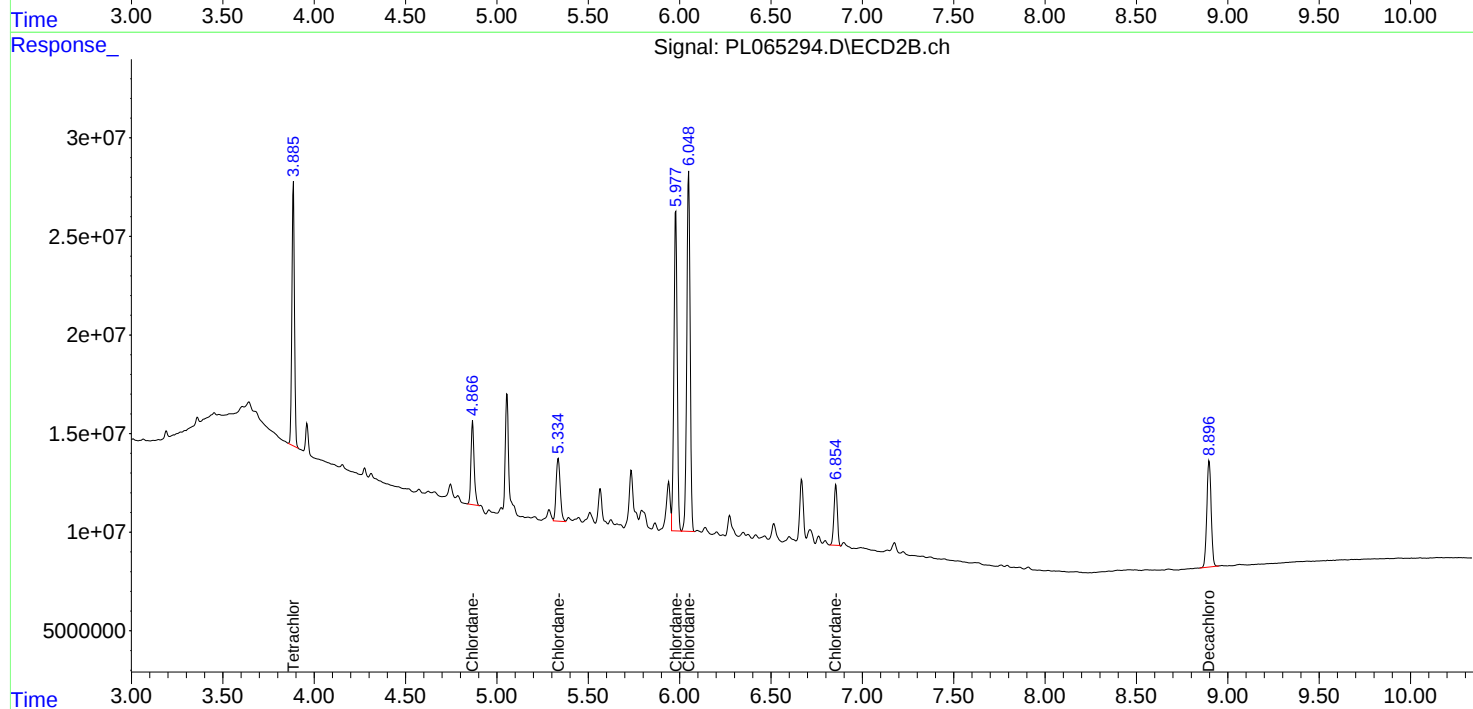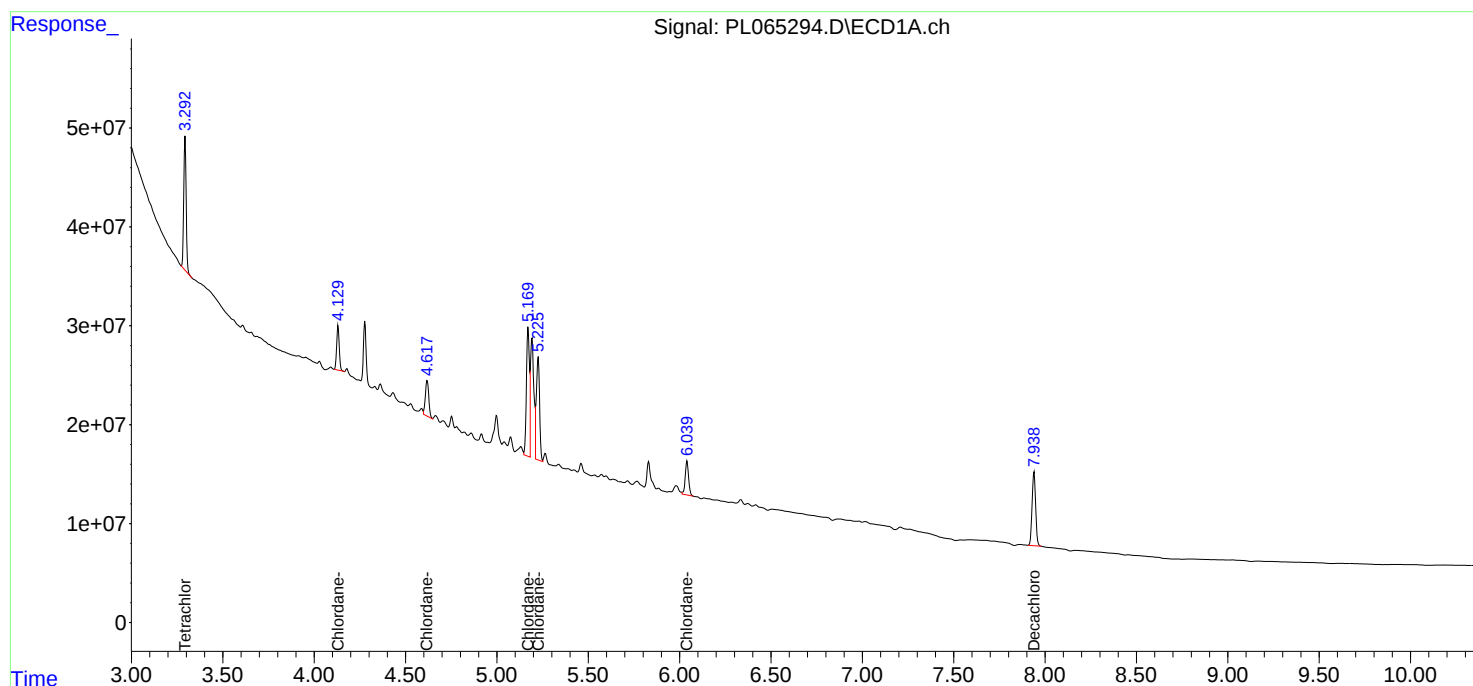


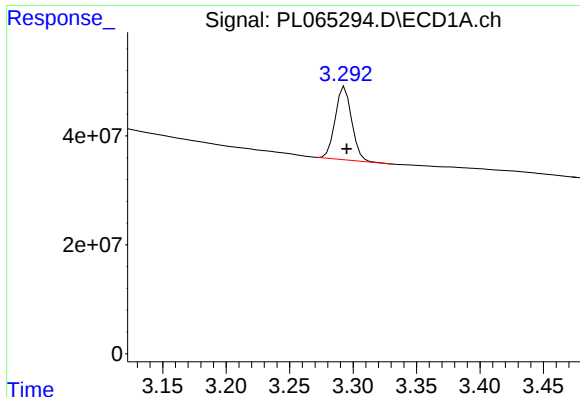

#1 Tetrachloro-m-xylene


R.T.: 3.294 min
Delta R.T.: -0.001 min
Response: 120563287
Conc: 51.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

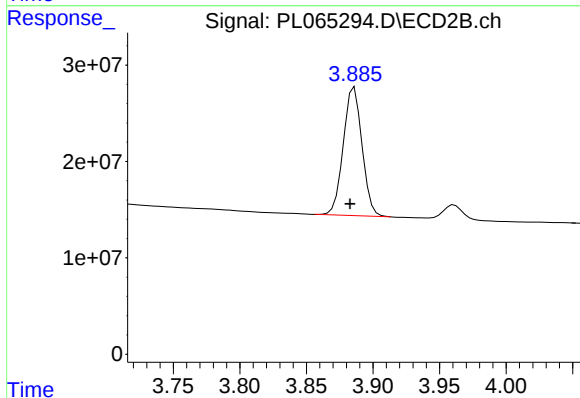


#1 Tetrachloro-m-xylene

R.T.: 3.886 min
Delta R.T.: 0.003 min
Response: 130157130
Conc: 47.25 ng/ml

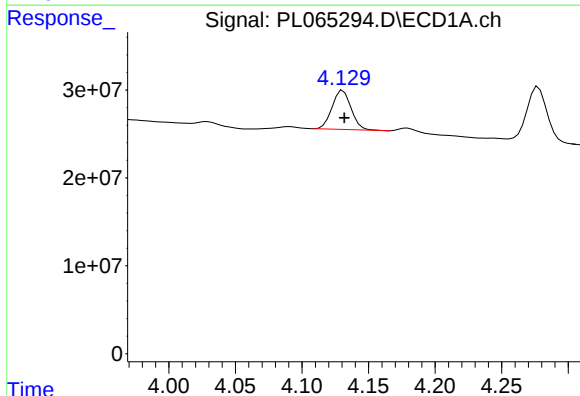


#23 Chlordane-1

R.T.: 4.131 min
Delta R.T.: 0.000 min
Response: 44486543
Conc: 429.23 ng/ml

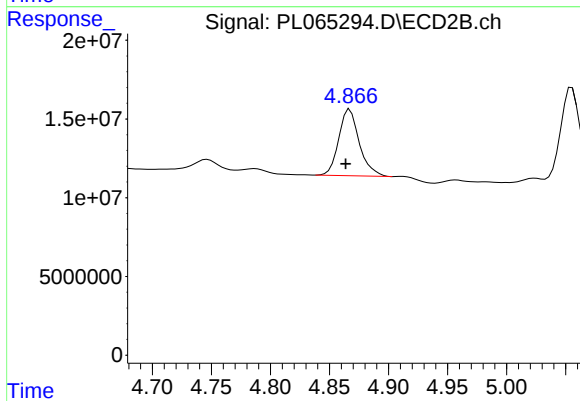

#23 Chlordane-1


R.T.: 4.867 min
Delta R.T.: 0.003 min
Response: 50941026
Conc: 521.29 ng/ml

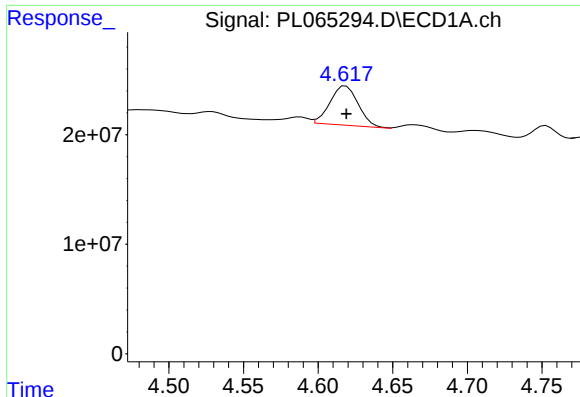

#24 Chlordane-2


R.T.: 4.619 min
Delta R.T.: 0.000 min
Response: 47462299
Conc: 478.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

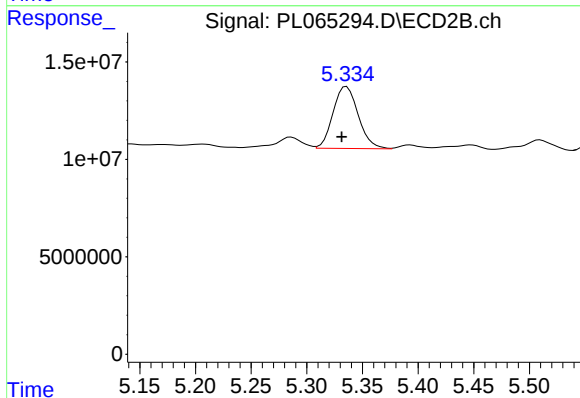


#24 Chlordane-2

R.T.: 5.336 min
Delta R.T.: 0.004 min
Response: 50064118
Conc: 486.43 ng/ml

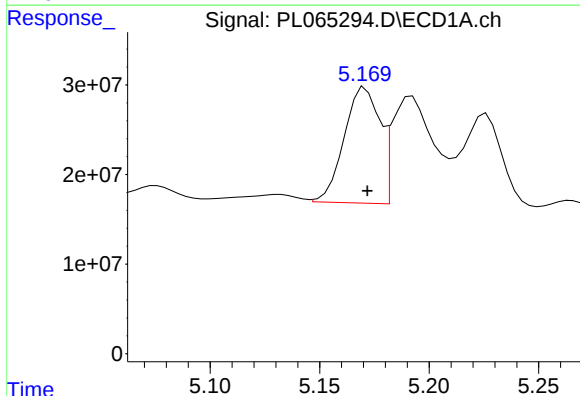


#25 Chlordane-3

R.T.: 5.171 min
Delta R.T.: 0.000 min
Response: 145884162
Conc: 485.07 ng/ml

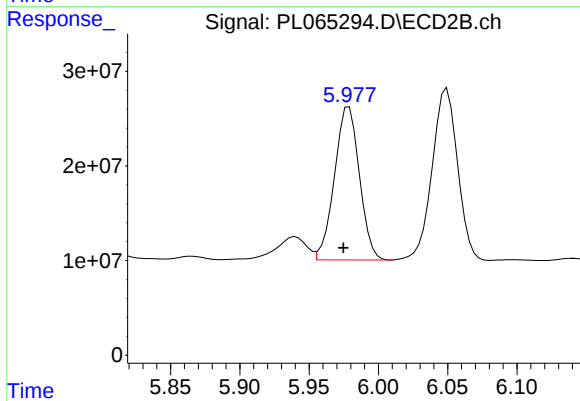

#25 Chlordane-3


R.T.: 5.979 min
Delta R.T.: 0.004 min
Response: 203048960
Conc: 496.79 ng/ml

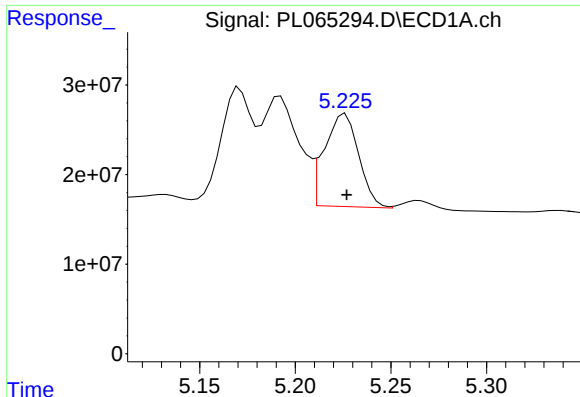

#26 Chlordane-4


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 128846602
Conc: 473.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

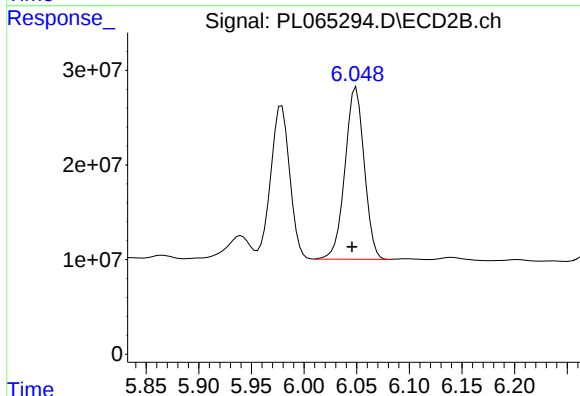


#26 Chlordane-4

R.T.: 6.049 min
Delta R.T.: 0.004 min
Response: 232072396
Conc: 489.49 ng/ml

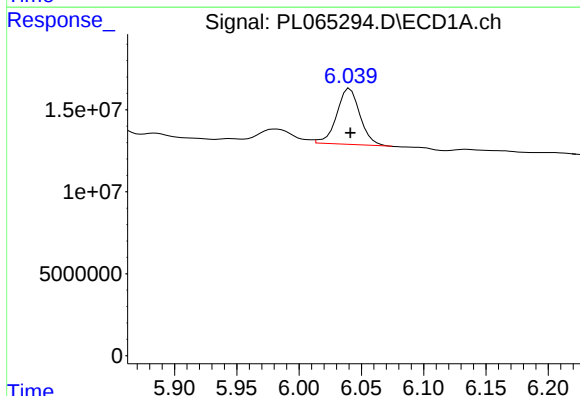


#27 Chlordane-5

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 44042336
Conc: 485.14 ng/ml

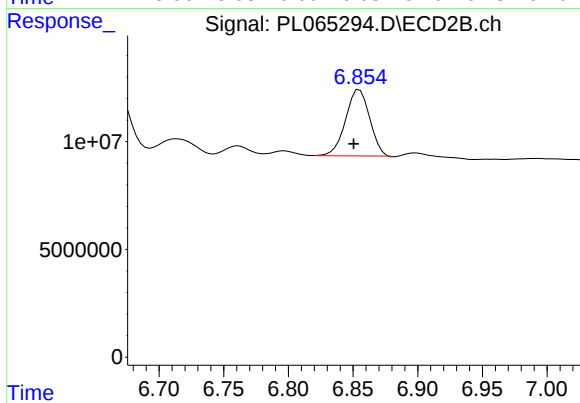

#27 Chlordane-5


R.T.: 6.855 min
Delta R.T.: 0.005 min
Response: 39455987
Conc: 497.42 ng/ml

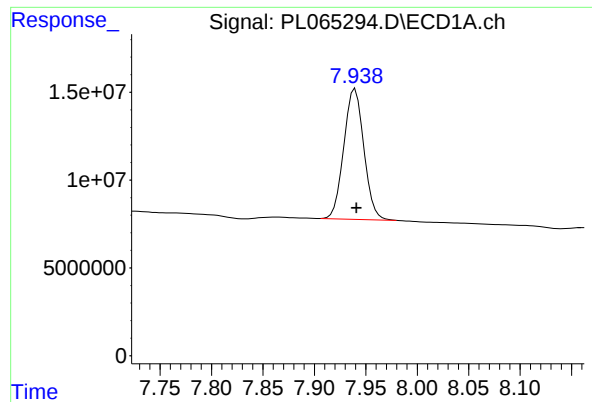

#28 Decachlorobiphenyl

R.T.: 7.940 min
Delta R.T.: -0.001 min
Response: 100830038
Conc: 46.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

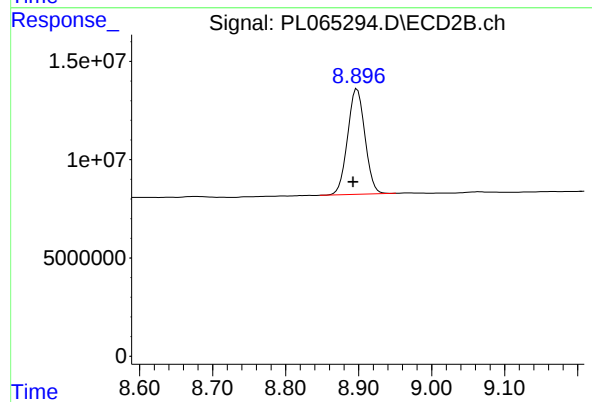

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.005 min
Response: 88543708
Conc: 48.20 ng/ml