

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031419\
 Data File : PL045926.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2019 18:45
 Operator : AJ\SJ
 Sample : K1807-44
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-22

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:12:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	94663083	31369783	13.761	14.648
28)	SA Decachlor...	8.042	9.038	102.9E6	29926762	12.296	13.097
Target Compounds							
12)	B 4,4'-DDE	5.481	6.317	707.2E6	193.9E6	80.568	83.026
13)	MA Dieldrin	5.606	6.466	106.8E6	32088306	11.177	12.487
14)	MA Endrin	5.863	6.711f	121.6E6	5088564	13.503	2.236 #
15)	B Endosulfa...	0.000	6.893	0	3671521	N.D.	1.561 #
16)	A 4,4'-DDD	5.992	6.807	25728394	8301478	3.514	4.317
17)	MA 4,4'-DDT	6.228	7.105	1218.0E6	327.9E6	162.393	166.167
18)	B Endrin al...	6.285f	0.000	15173568	0	2.076	N.D. #
19)	B Endosulfa...	6.513	7.240	12942901	4291868	1.592	1.908
21)	B Endrin ke...	6.987	0.000	6735441	0	0.731	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031419\
Data File : PL045926.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2019 18:45
Operator : AJ\SJ
Sample : K1807-44
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-22

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:12:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

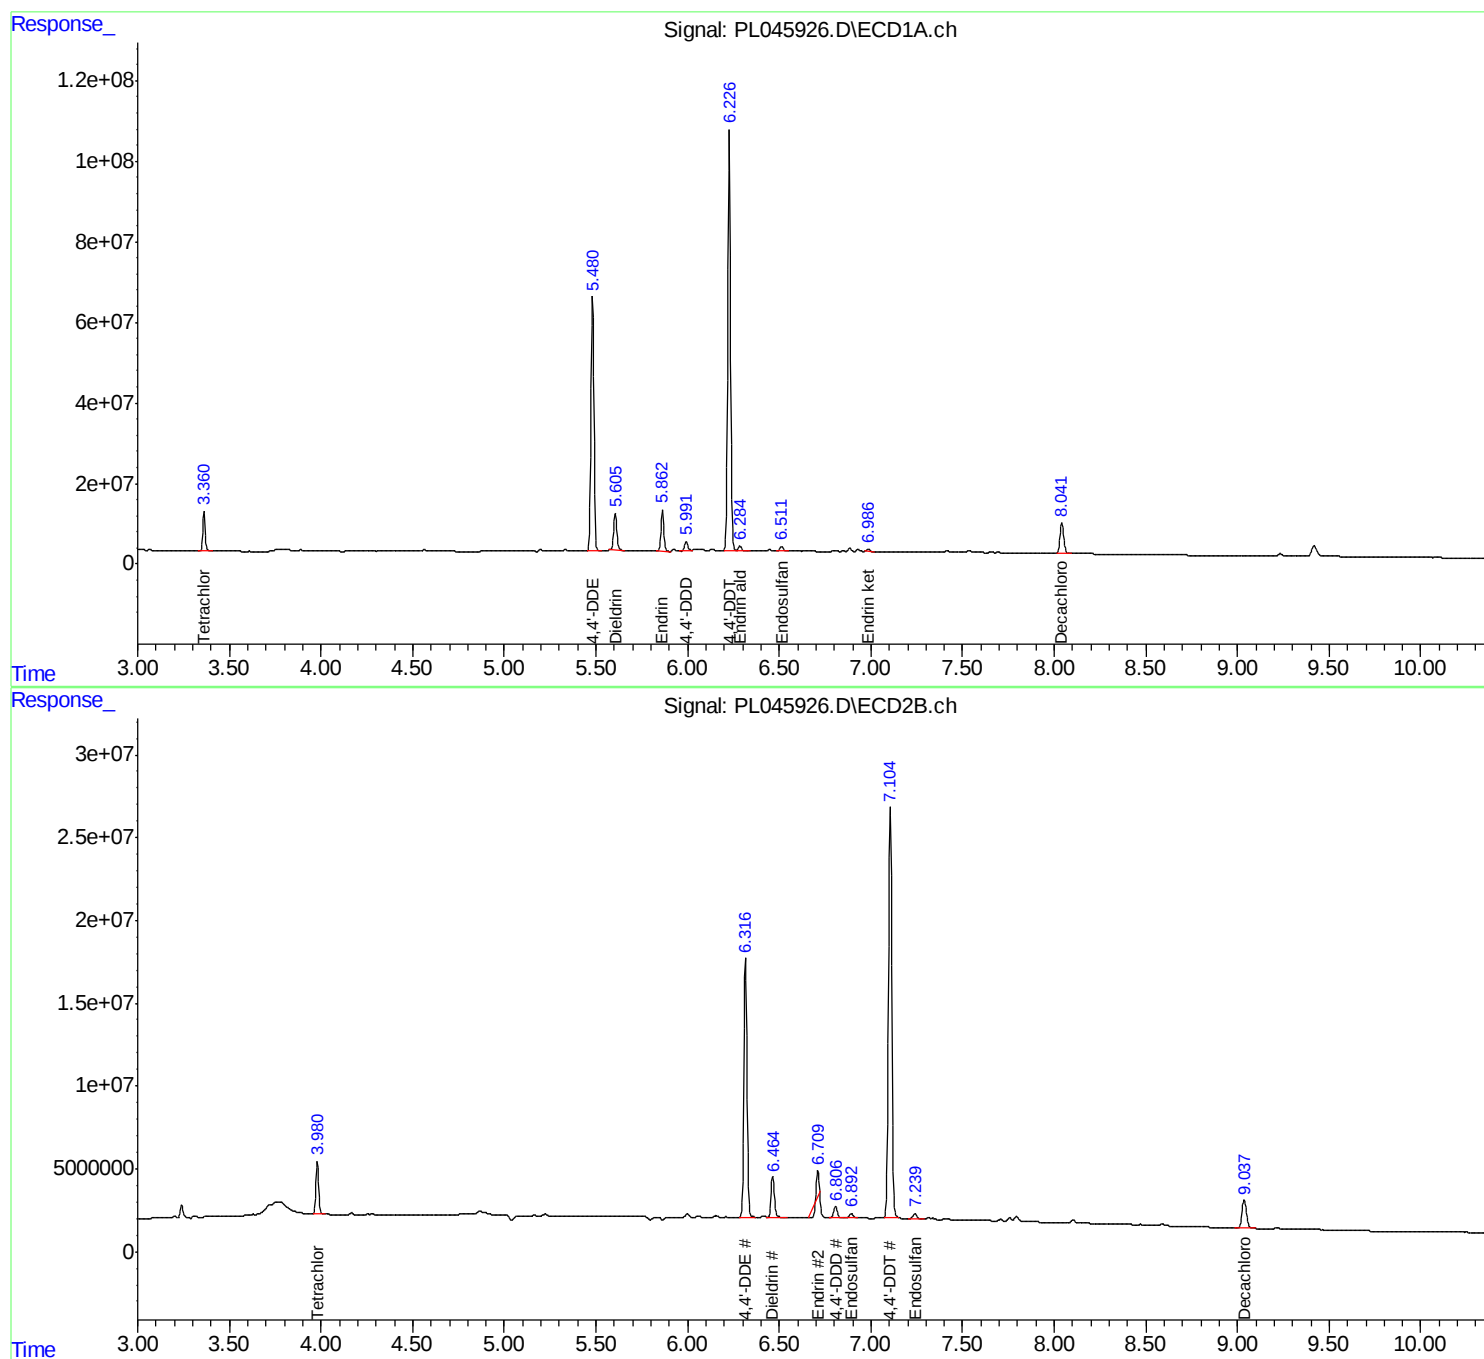


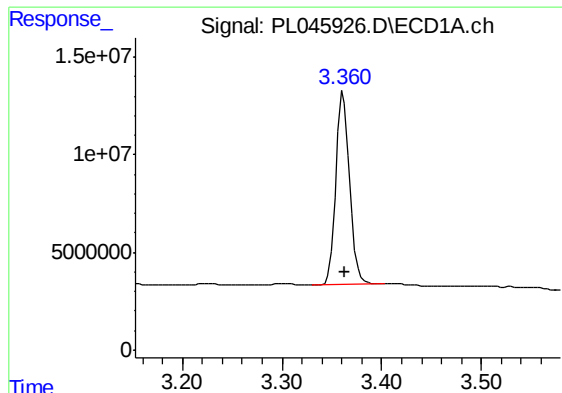

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: -0.001 min
Response: 94663083
Conc: 13.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-22

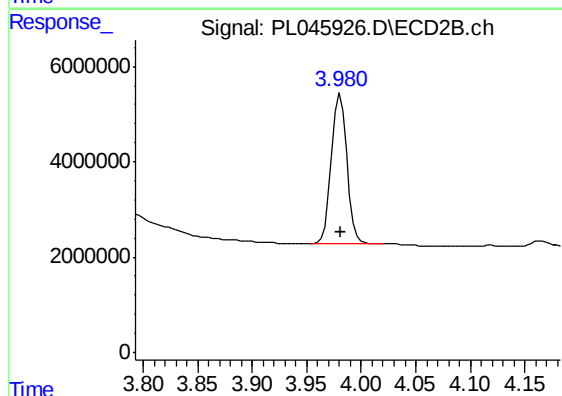


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 31369783
Conc: 14.65 ng/ml

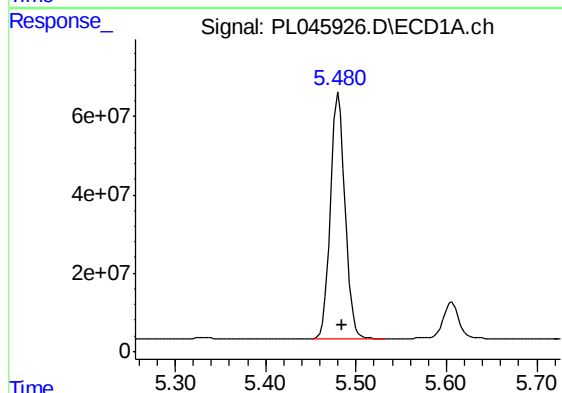


#12 4,4'-DDE

R.T.: 5.481 min
Delta R.T.: -0.003 min
Response: 707245023
Conc: 80.57 ng/ml

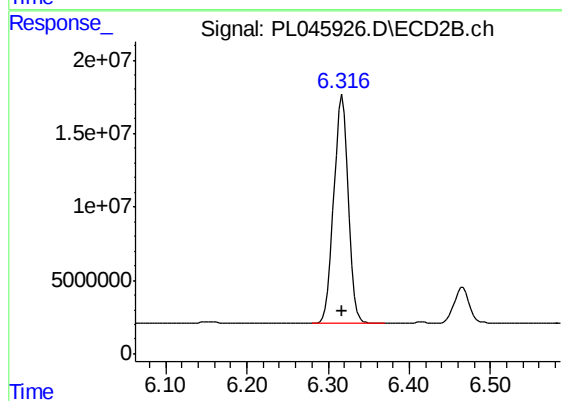

#12 4,4'-DDE


R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 193941051
Conc: 83.03 ng/ml

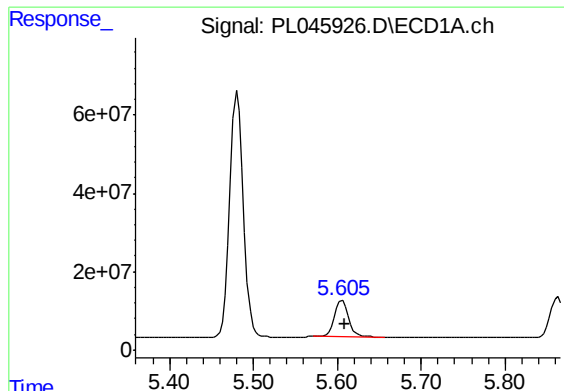

#13 Dielldrin


R.T.: 5.606 min
Delta R.T.: -0.003 min
Response: 106825585
Conc: 11.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-22

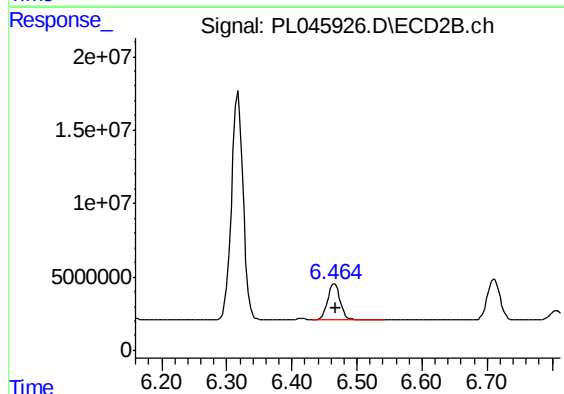


#13 Dielldrin

R.T.: 6.466 min
Delta R.T.: -0.001 min
Response: 32088306
Conc: 12.49 ng/ml

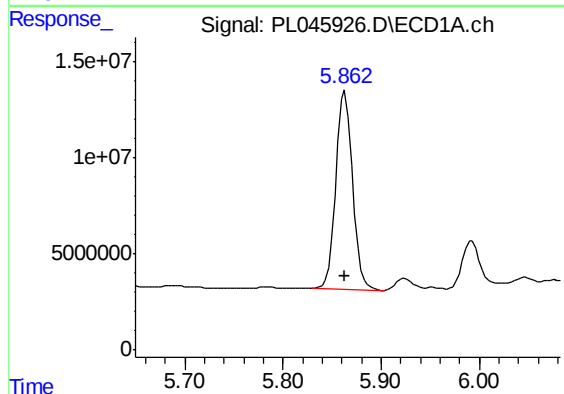


#14 Endrin

R.T.: 5.863 min
Delta R.T.: 0.000 min
Response: 121604222
Conc: 13.50 ng/ml

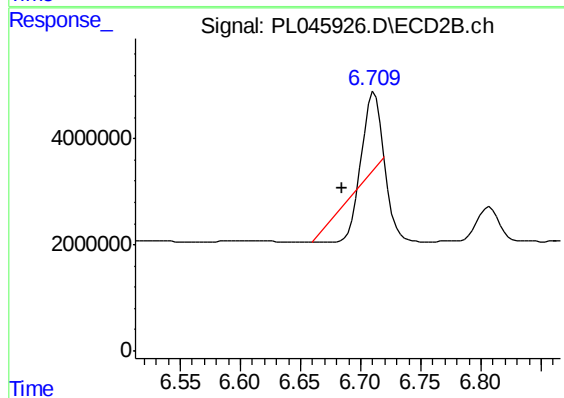

#14 Endrin


R.T.: 6.711 min
Delta R.T.: 0.027 min
Response: 5088564
Conc: 2.24 ng/ml

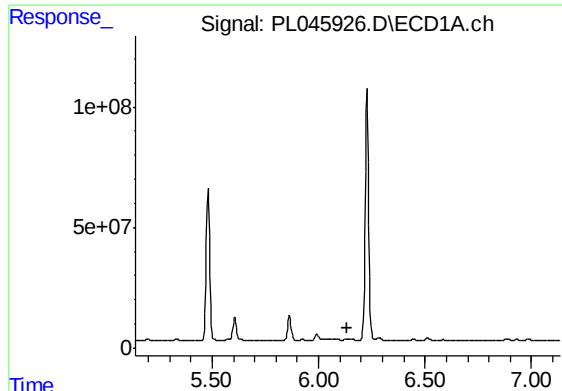

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.137 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-22

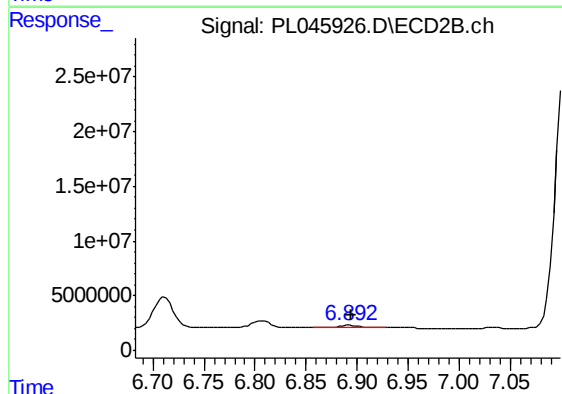


#15 Endosulfan II

R.T.: 6.893 min
Delta R.T.: 0.000 min
Response: 3671521
Conc: 1.56 ng/ml

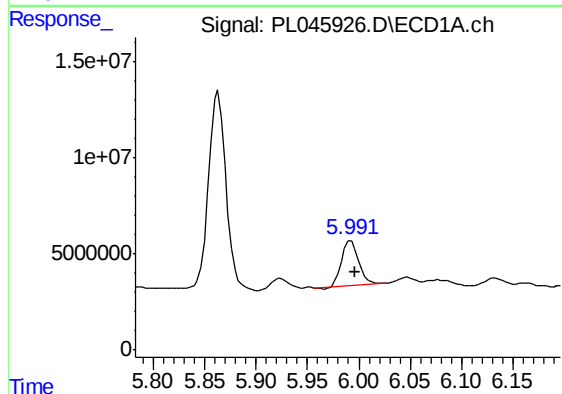


#16 4,4'-DDD

R.T.: 5.992 min
Delta R.T.: -0.003 min
Response: 25728394
Conc: 3.51 ng/ml

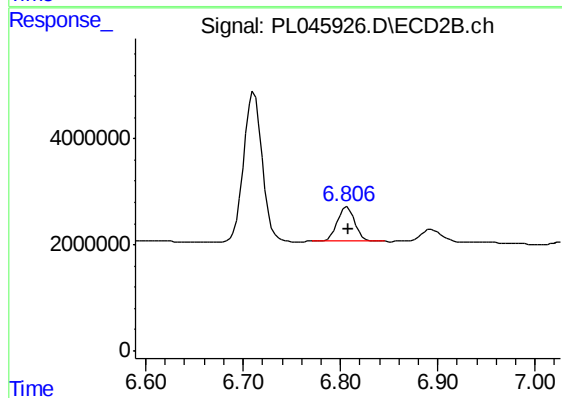

#16 4,4'-DDD


R.T.: 6.807 min
Delta R.T.: 0.000 min
Response: 8301478
Conc: 4.32 ng/ml

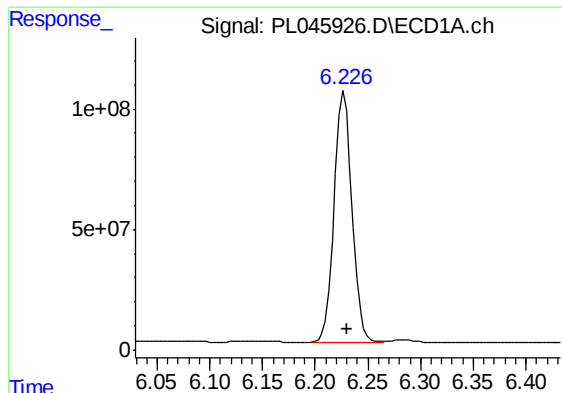

#17 4,4'-DDT


R.T.: 6.228 min
Delta R.T.: -0.003 min
Response: 1217967153
Conc: 162.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-22

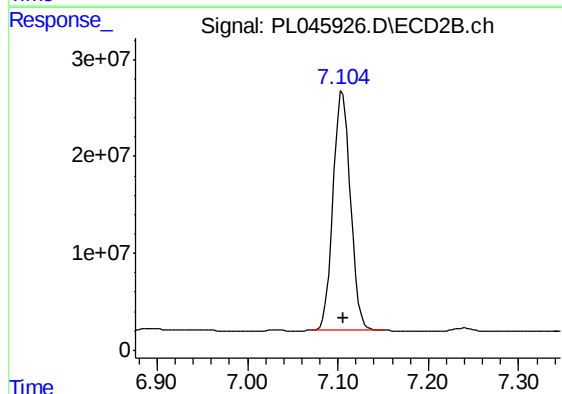


#17 4,4'-DDT

R.T.: 7.105 min
Delta R.T.: 0.000 min
Response: 327921920
Conc: 166.17 ng/ml

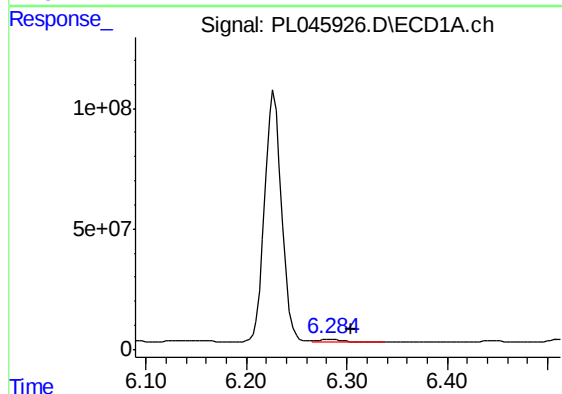


#18 Endrin aldehyde

R.T.: 6.285 min
Delta R.T.: -0.019 min
Response: 15173568
Conc: 2.08 ng/ml

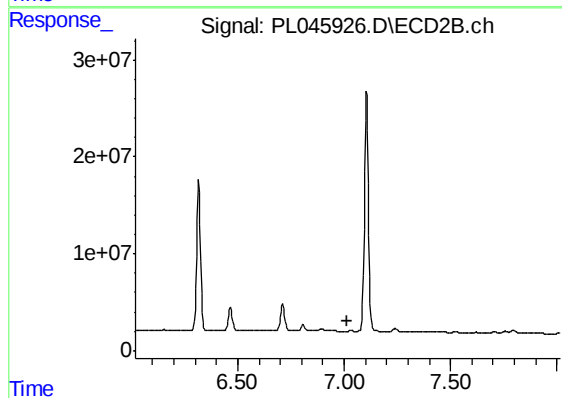

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.017 min
Response: 0
Conc: N.D.

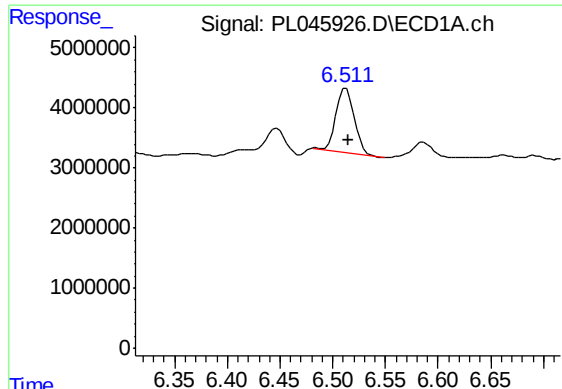

#19 Endosulfan Sulfate


R.T.: 6.513 min
Delta R.T.: -0.003 min
Response: 12942901
Conc: 1.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-22

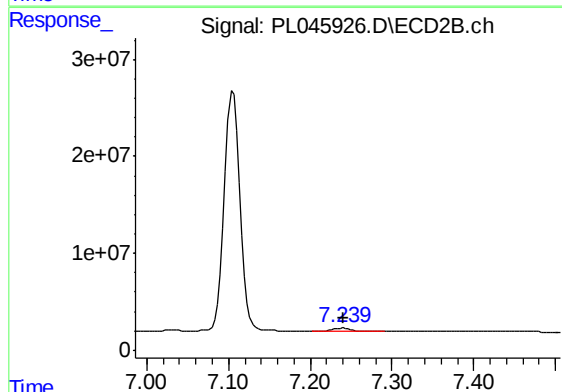


#19 Endosulfan Sulfate

R.T.: 7.240 min
Delta R.T.: 0.000 min
Response: 4291868
Conc: 1.91 ng/ml

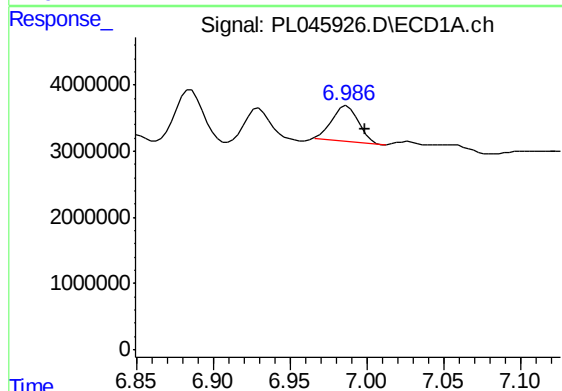


#21 Endrin ketone

R.T.: 6.987 min
Delta R.T.: -0.012 min
Response: 6735441
Conc: 0.73 ng/ml

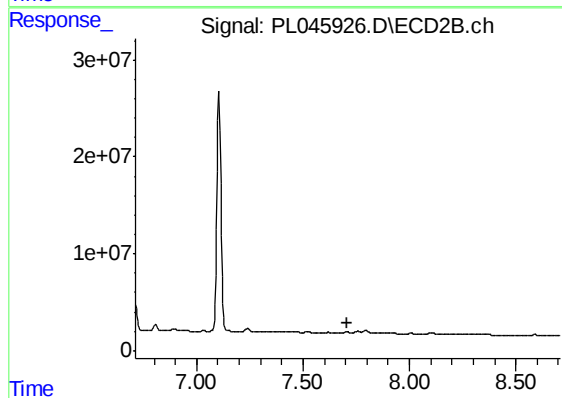

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

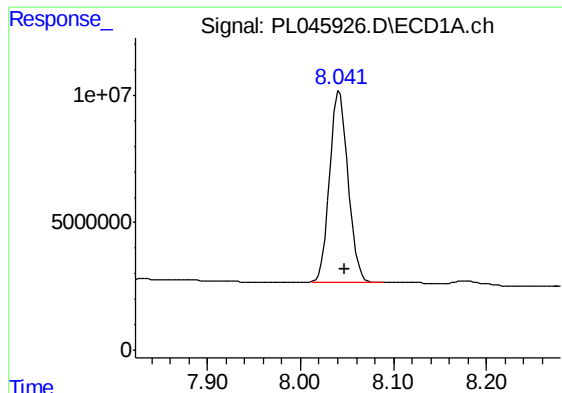

#28 Decachlorobiphenyl

R.T.: 8.042 min
Delta R.T.: -0.005 min
Response: 102883144
Conc: 12.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-22

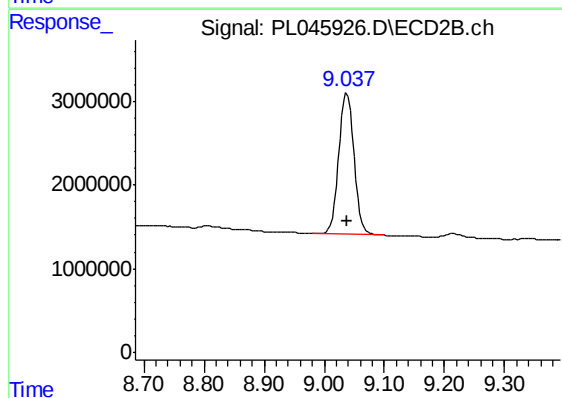

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 29926762
Conc: 13.10 ng/ml