

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031419\
 Data File : PL045935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2019 20:57
 Operator : AJ\SJ
 Sample : K1897-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:14:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	53565150	18163605	7.786	8.482
28)	SA Decachlor...	8.043	9.038	71276039	20765590	8.518	9.088
Target Compounds							
10)	B gamma-Chl...	0.000	6.059f	0	1389073	N.D.	0.518 #
12)	B 4,4'-DDE	5.481	6.318	902.4E6	248.4E6	102.802	106.320
14)	MA Endrin	5.864	0.000	40509430	0	4.498	N.D. #
15)	B Endosulfa...	0.000	6.883	0	224.8E6	N.D.	95.590 #
16)	A 4,4'-DDD	5.992	0.000	12913521	0	1.764	N.D. #
17)	MA 4,4'-DDT	6.228	7.105	170.8E6	44979304	22.772	22.792
19)	B Endosulfa...	6.506	0.000	9252723	0	1.138	N.D. #
20)	A Methoxychlor	6.751f	0.000	7338947	0	1.671	N.D. #
25)	Chlordane-3	0.000	6.059f	0	1389073	N.D.	3.565 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031419\
Data File : PL045935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2019 20:57
Operator : AJ\SJ
Sample : K1897-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:14:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

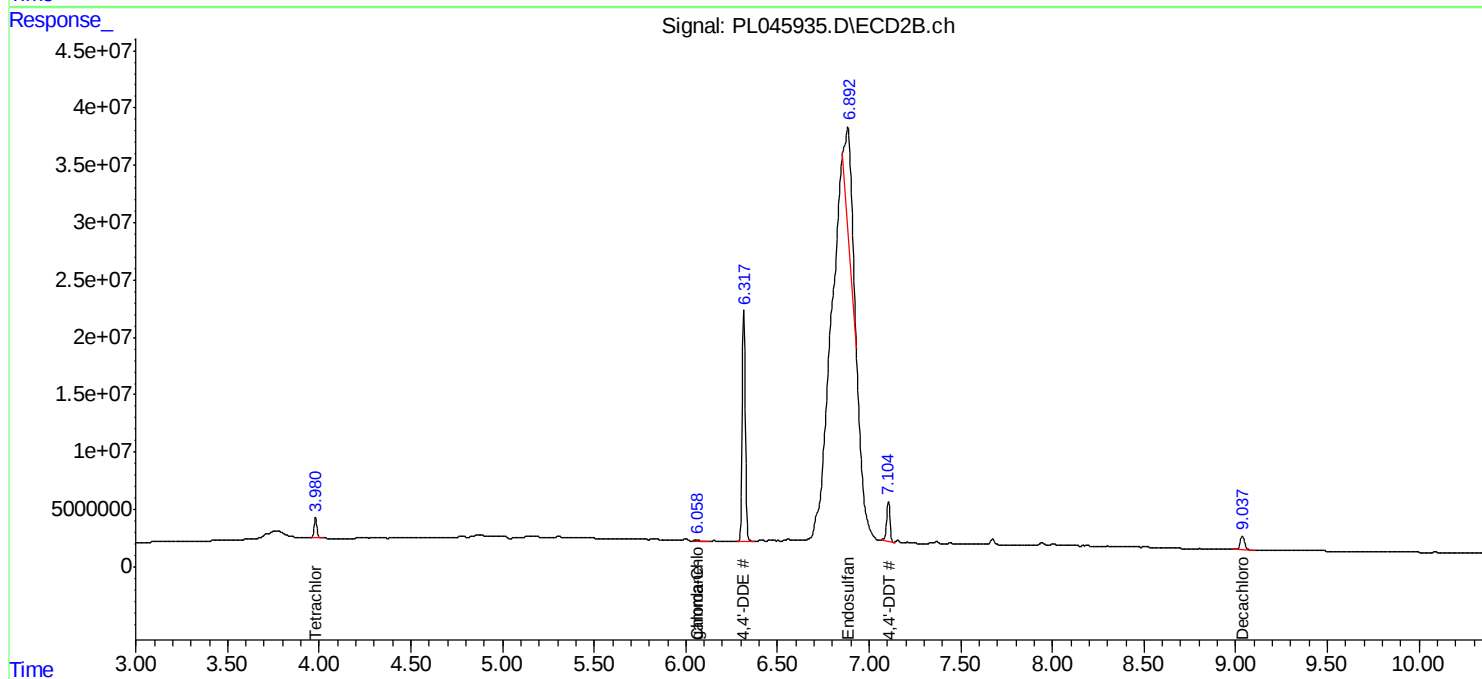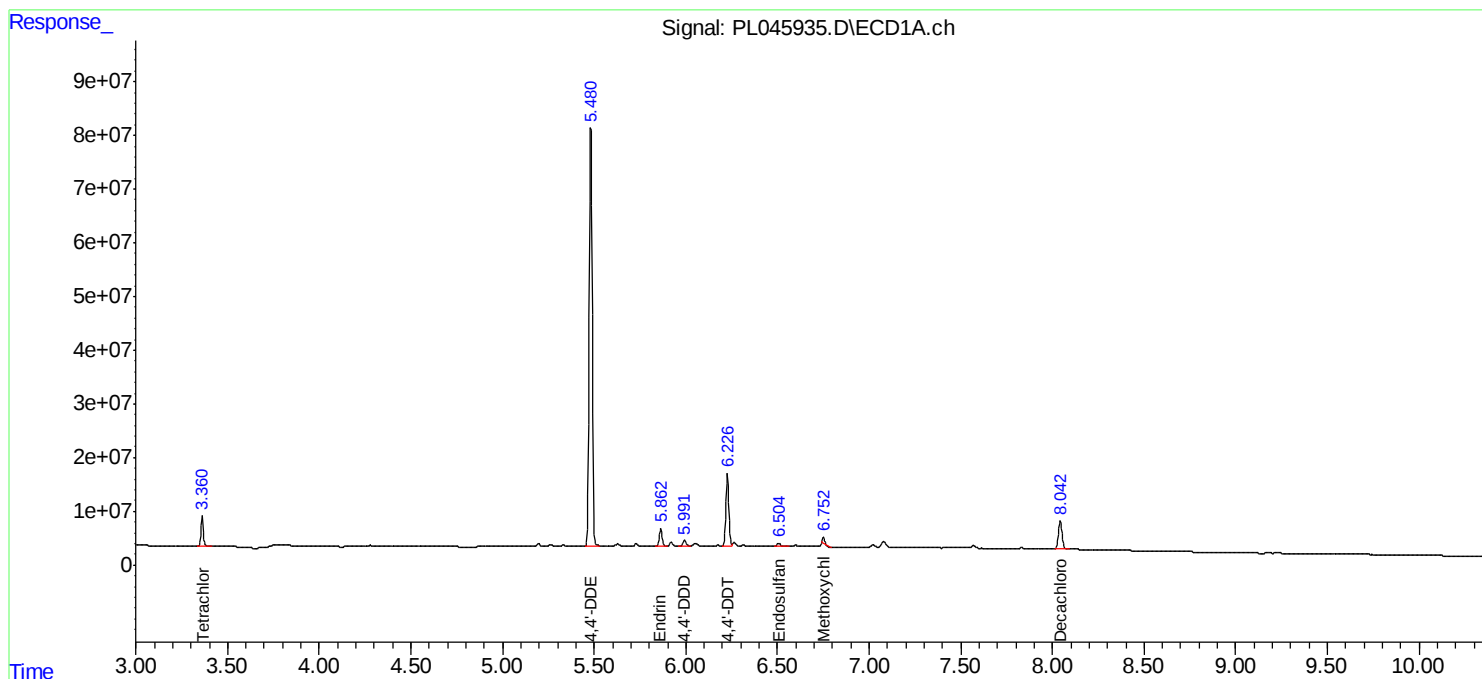


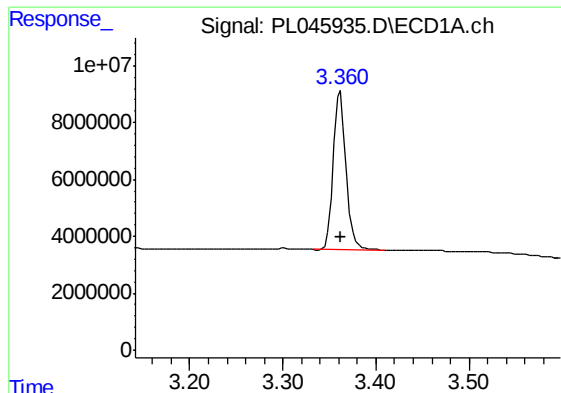

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: -0.001 min
Response: 53565150
Conc: 7.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

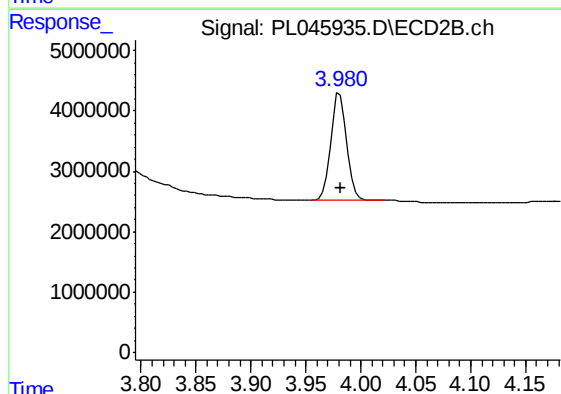


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 18163605
Conc: 8.48 ng/ml

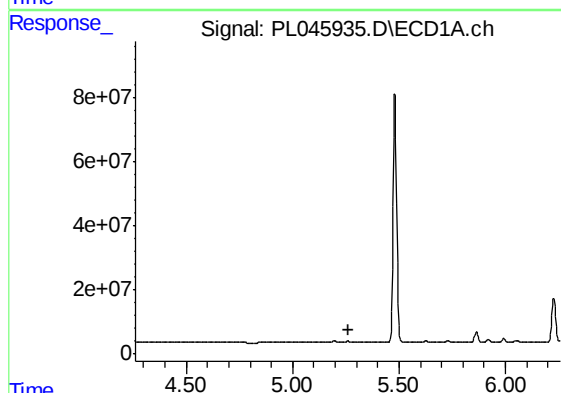


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

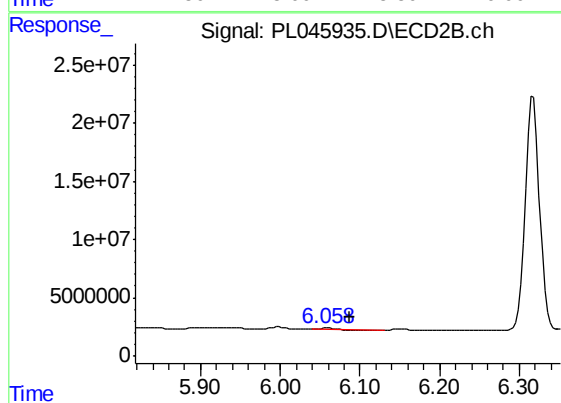

#10 gamma-Chlordane


R.T.: 6.059 min
Delta R.T.: -0.029 min
Response: 1389073
Conc: 0.52 ng/ml

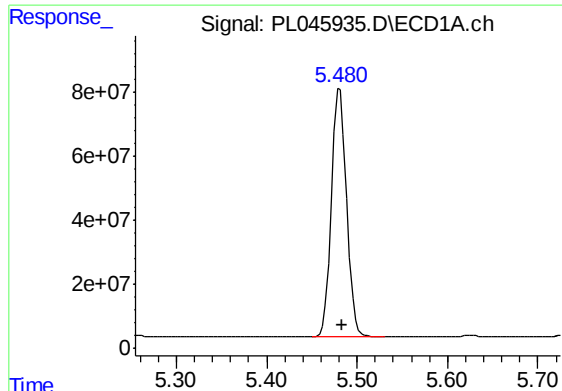

#12 4,4'-DDE


R.T.: 5.481 min
Delta R.T.: -0.003 min
Response: 902415100
Conc: 102.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

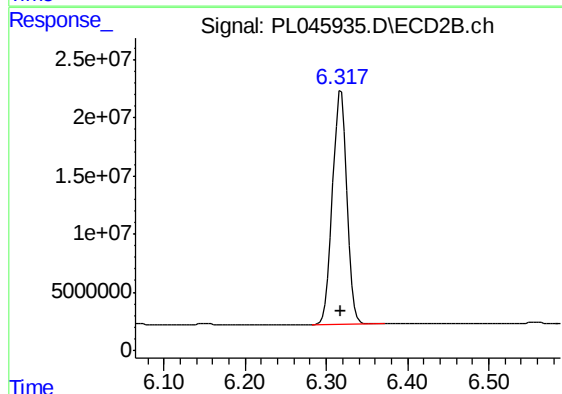


#12 4,4'-DDE

R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 248352757
Conc: 106.32 ng/ml

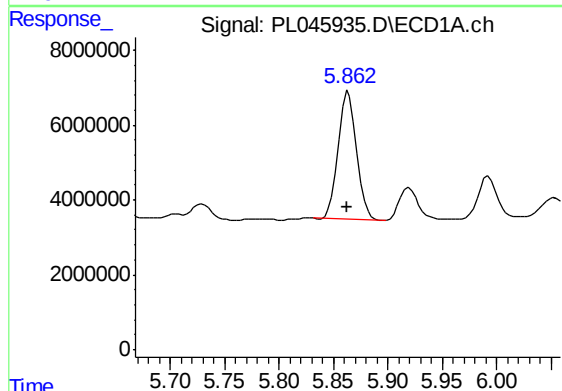


#14 Endrin

R.T.: 5.864 min
Delta R.T.: 0.001 min
Response: 40509430
Conc: 4.50 ng/ml

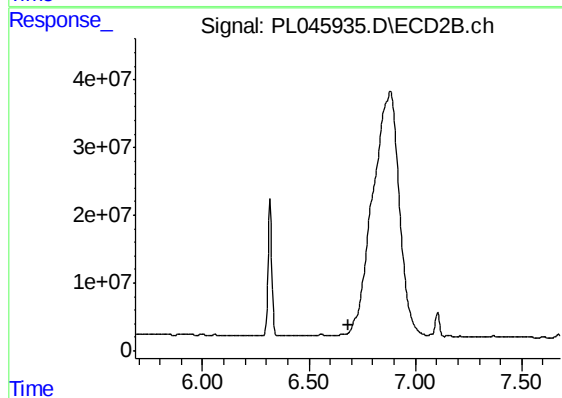

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.684 min
Response: 0
Conc: N.D.

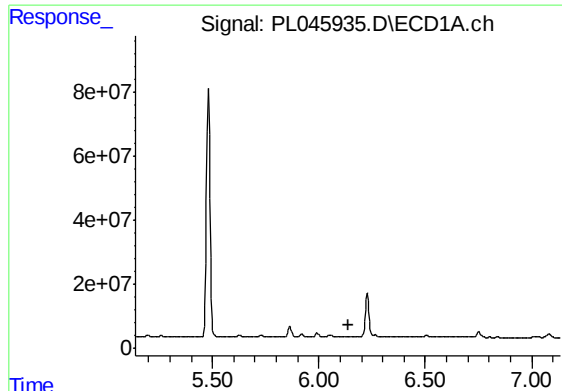

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.137 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

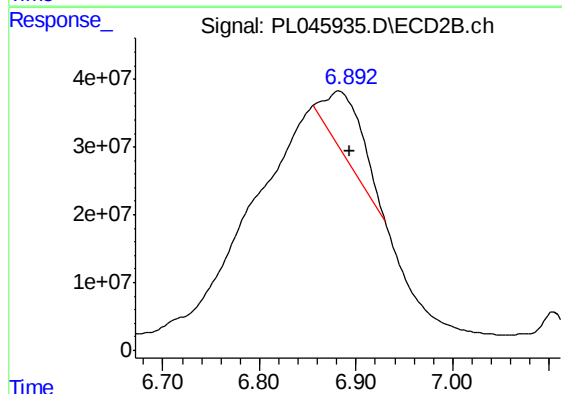


#15 Endosulfan II

R.T.: 6.883 min
Delta R.T.: -0.011 min
Response: 224792616
Conc: 95.59 ng/ml

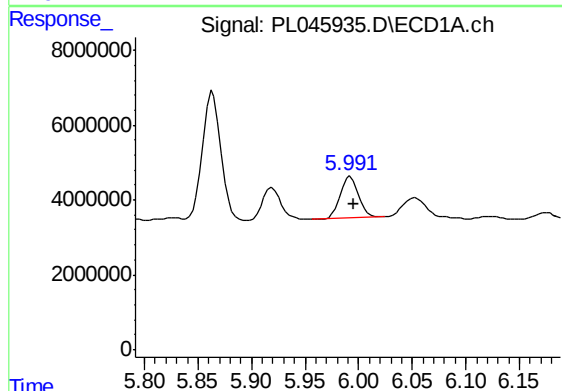


#16 4,4'-DDD

R.T.: 5.992 min
Delta R.T.: -0.003 min
Response: 12913521
Conc: 1.76 ng/ml

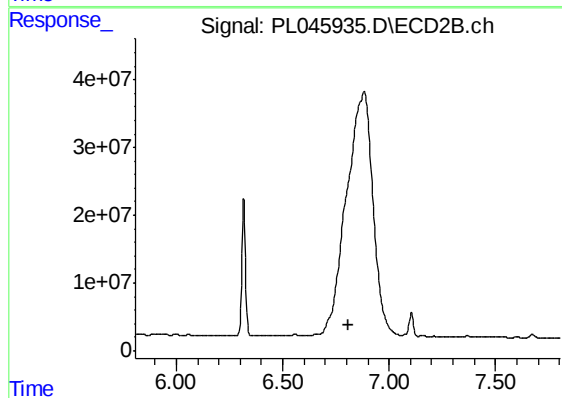

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.808 min
Response: 0
Conc: N.D.

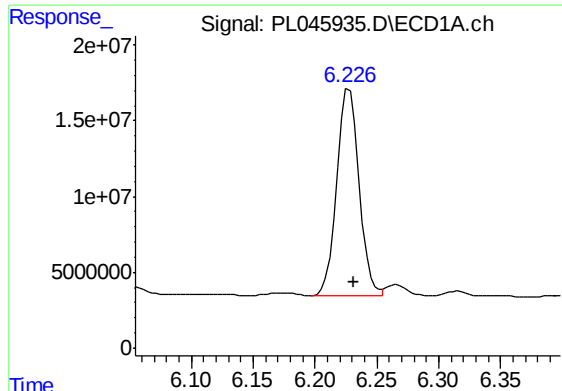

#17 4,4'-DDT


R.T.: 6.228 min
Delta R.T.: -0.003 min
Response: 170795477
Conc: 22.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

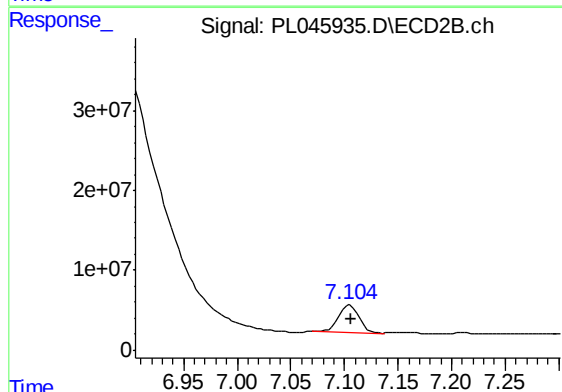


#17 4,4'-DDT

R.T.: 7.105 min
Delta R.T.: 0.000 min
Response: 44979304
Conc: 22.79 ng/ml

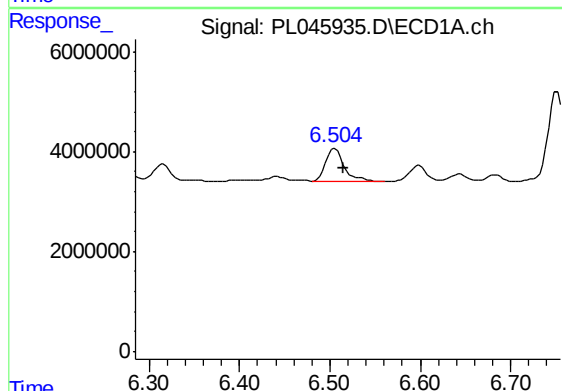


#19 Endosulfan Sulfate

R.T.: 6.506 min
Delta R.T.: -0.010 min
Response: 9252723
Conc: 1.14 ng/ml

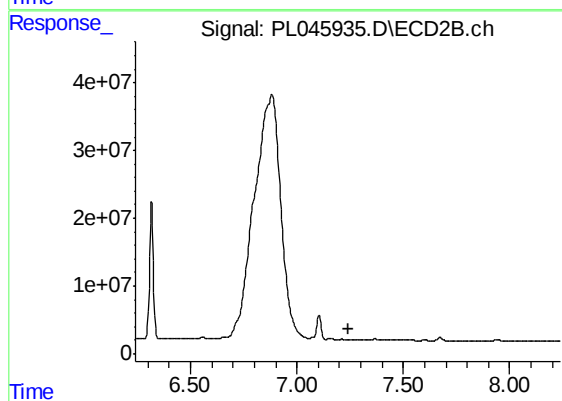

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.241 min
Response: 0
Conc: N.D.

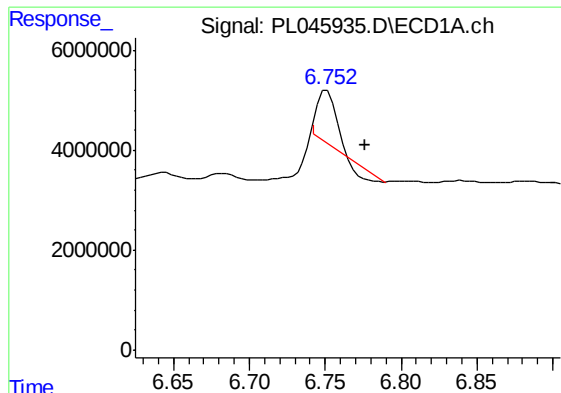

#20 Methoxychlor


R.T.: 6.751 min
Delta R.T.: -0.025 min
Response: 7338947
Conc: 1.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

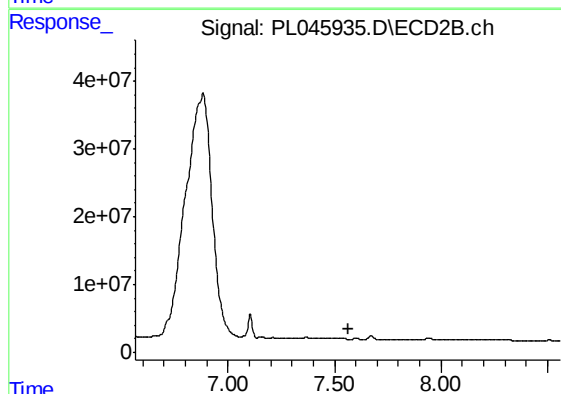


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.564 min
Response: 0
Conc: N.D.

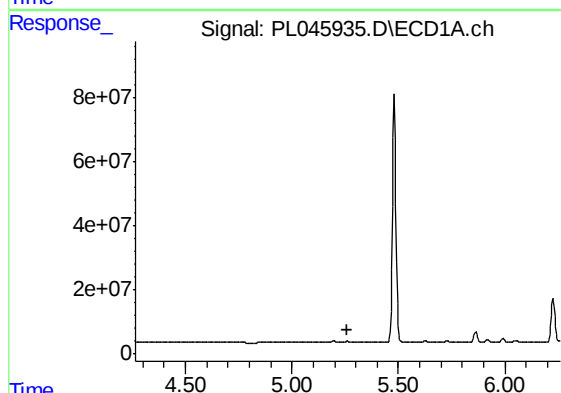


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.262 min
Response: 0
Conc: N.D.

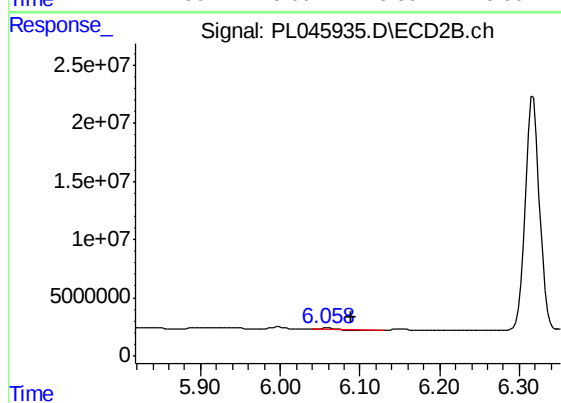

#25 Chlordane-3


R.T.: 6.059 min
Delta R.T.: -0.030 min
Response: 1389073
Conc: 3.57 ng/ml

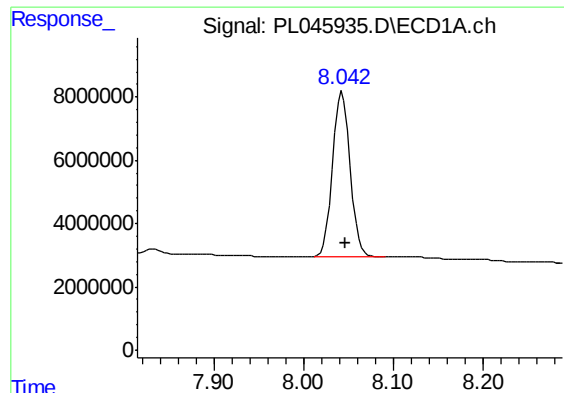

#28 Decachlorobiphenyl

R.T.: 8.043 min
Delta R.T.: -0.004 min
Response: 71276039
Conc: 8.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

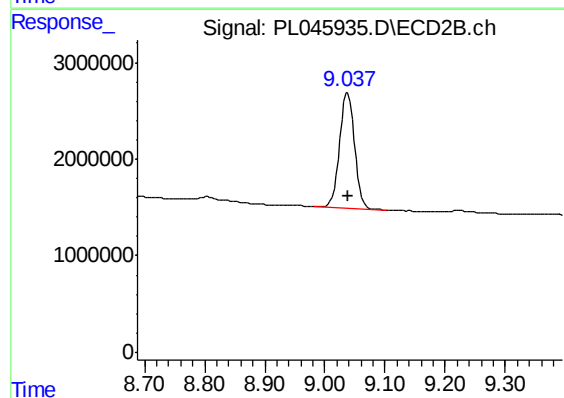

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 20765590
Conc: 9.09 ng/ml