

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031419\
 Data File : PL045936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2019 21:11
 Operator : AJ\SJ
 Sample : K1897-06
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:15:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	97071880	31690840	14.111	14.798
28)	SA Decachlor...	8.044	9.039	96283732	28467353	11.507	12.459
Target Compounds							
10)	B gamma-Chl...	5.260	6.060f	8436150	2126328	0.862	0.793
12)	B 4,4'-DDE	5.482	6.318	837.8E6	231.5E6	95.437	99.117
13)	MA Dieldrin	5.607	6.466	504.3E6	127.8E6	52.766	49.734
14)	MA Endrin	5.864	6.712f	77982537	14868814	8.659	6.535
15)	B Endosulfa...	0.000	6.894	0	3235987	N.D.	1.376 #
16)	A 4,4'-DDD	5.993	6.808	172.5E6	49848743	23.556	25.921
17)	MA 4,4'-DDT	6.229	7.106	545.4E6	148.4E6	72.714	75.184
18)	B Endrin al...	6.285f	0.000	8447214	0	1.156	N.D. #
19)	B Endosulfa...	0.000	7.241	0	3050843	N.D.	1.356 #
20)	A Methoxychlor	6.798f	0.000	6780580	0	1.544	N.D. #
21)	B Endrin ke...	0.000	7.707	0	1691262	N.D.	0.711 #
25)	Chlordane-3	5.260	6.060f	8436150	2126328	7.355	5.457 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031419\
Data File : PL045936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2019 21:11
Operator : AJ\SJ
Sample : K1897-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:15:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

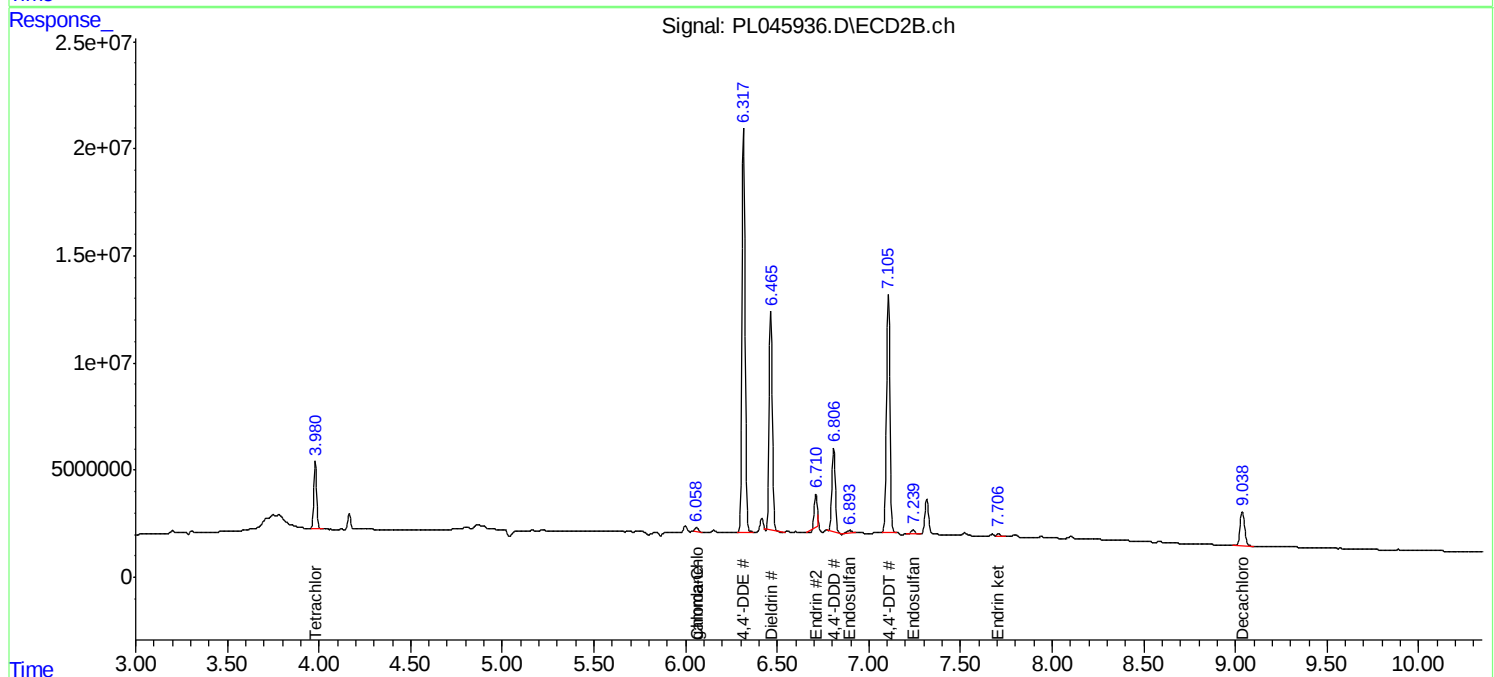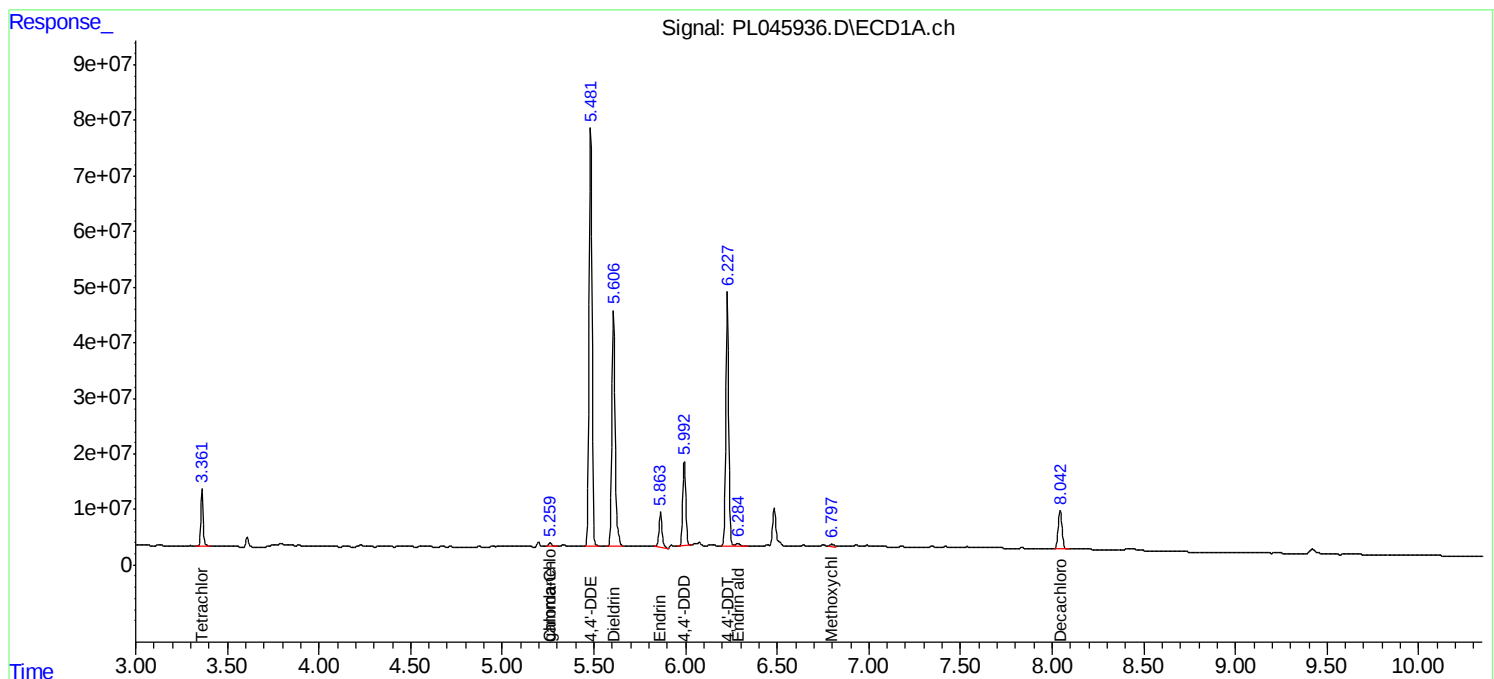


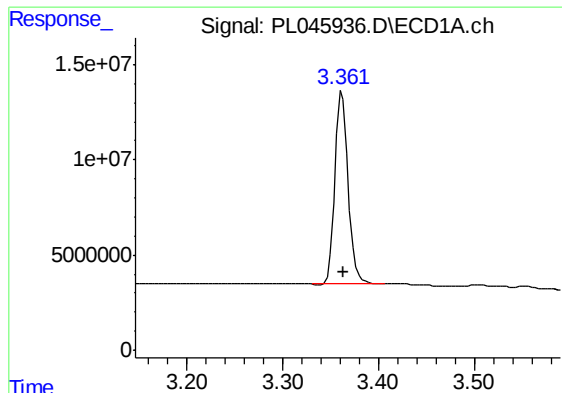

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 97071880
Conc: 14.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

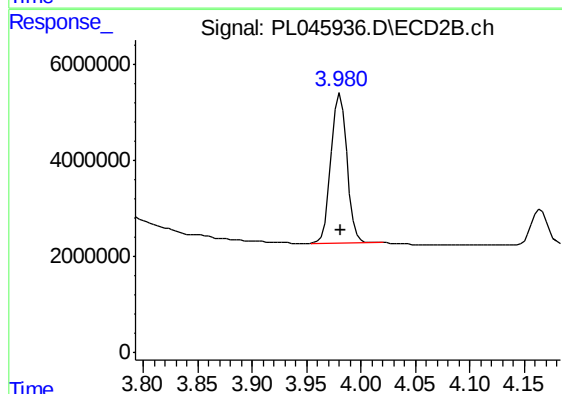


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 31690840
Conc: 14.80 ng/ml

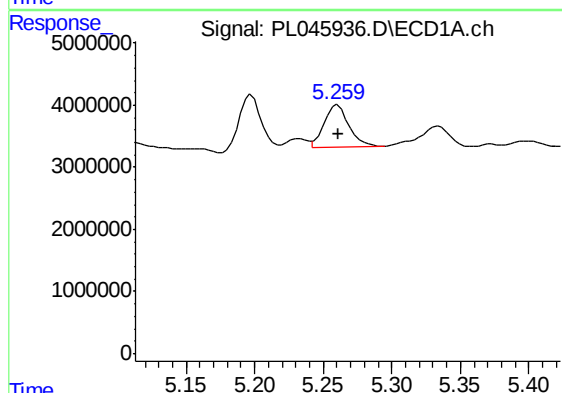


#10 gamma-Chlordane

R.T.: 5.260 min
Delta R.T.: 0.000 min
Response: 8436150
Conc: 0.86 ng/ml

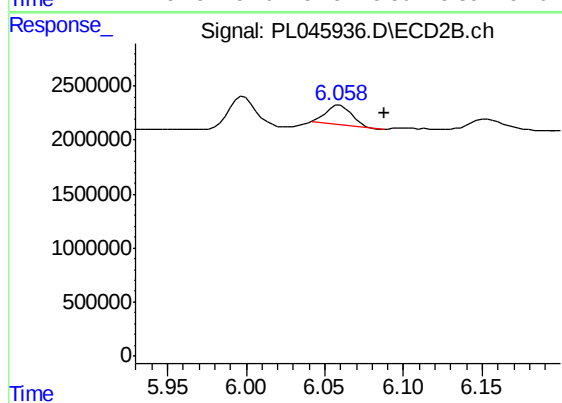

#10 gamma-Chlordane


R.T.: 6.060 min
Delta R.T.: -0.028 min
Response: 2126328
Conc: 0.79 ng/ml

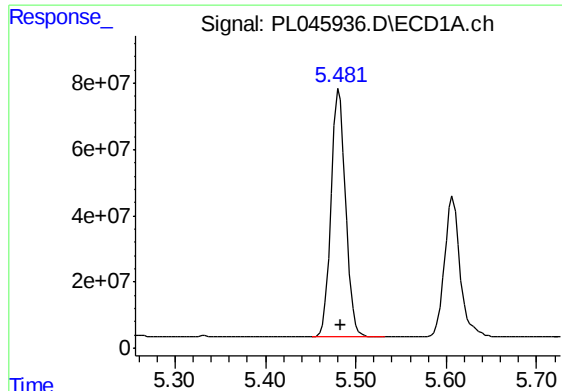

#12 4,4'-DDE


R.T.: 5.482 min
Delta R.T.: -0.002 min
Response: 837760774
Conc: 95.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

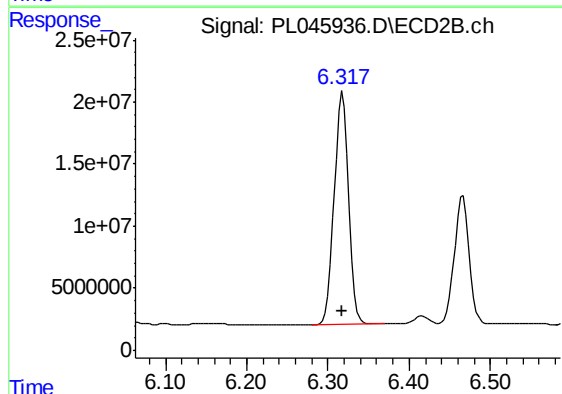


#12 4,4'-DDE

R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 231526594
Conc: 99.12 ng/ml

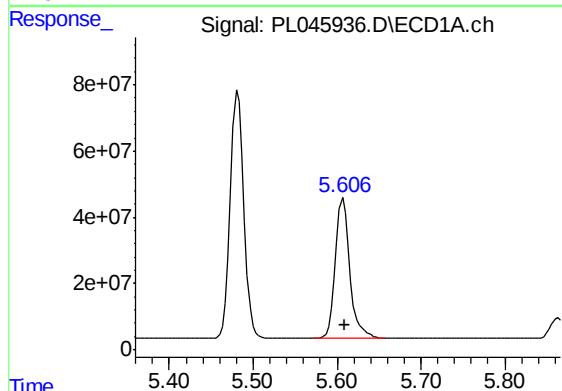


#13 Dieldrin

R.T.: 5.607 min
Delta R.T.: -0.002 min
Response: 504330945
Conc: 52.77 ng/ml

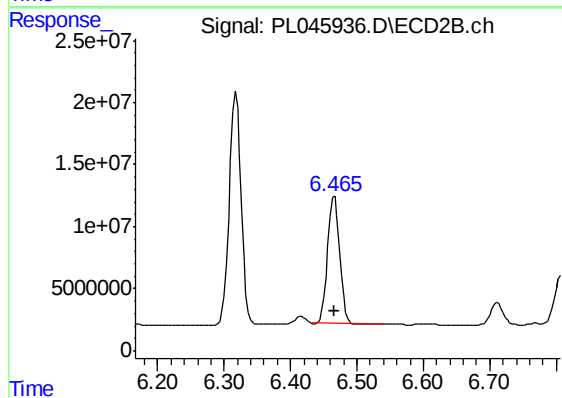

#13 Dieldrin


R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 127804141
Conc: 49.73 ng/ml

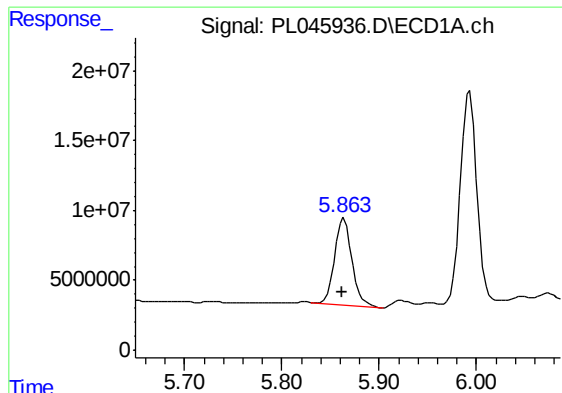

#14 Endrin


R.T.: 5.864 min
Delta R.T.: 0.002 min
Response: 77982537
Conc: 8.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

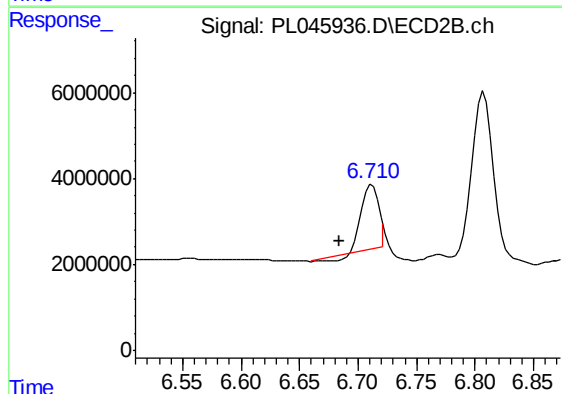


#14 Endrin

R.T.: 6.712 min
Delta R.T.: 0.028 min
Response: 14868814
Conc: 6.53 ng/ml

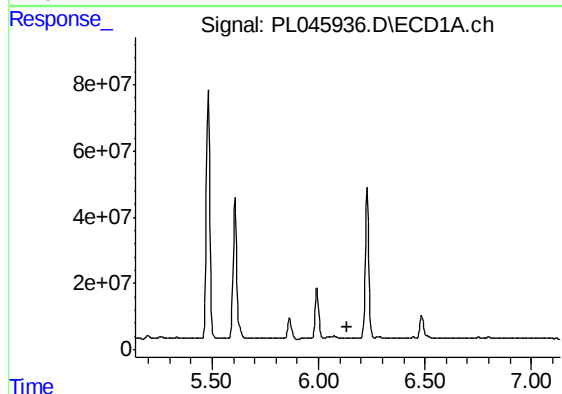


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.137 min
Response: 0
Conc: N.D.

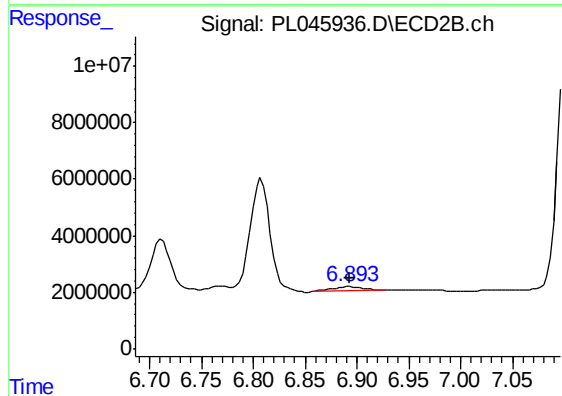

#15 Endosulfan II


R.T.: 6.894 min
Delta R.T.: 0.000 min
Response: 3235987
Conc: 1.38 ng/ml

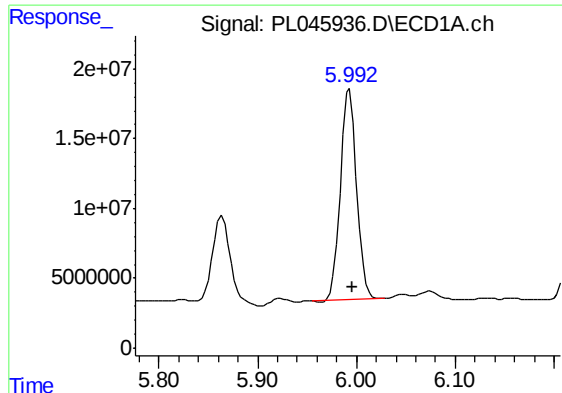

#16 4,4'-DDD


R.T.: 5.993 min
Delta R.T.: -0.003 min
Response: 172472737
Conc: 23.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

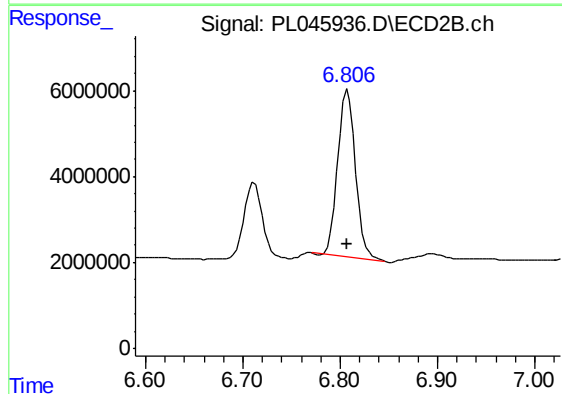


#16 4,4'-DDD

R.T.: 6.808 min
Delta R.T.: 0.000 min
Response: 49848743
Conc: 25.92 ng/ml

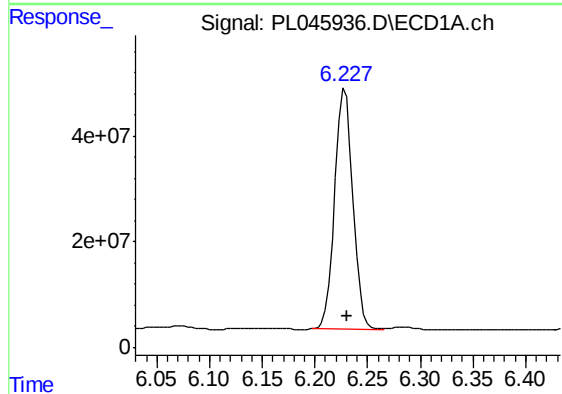


#17 4,4'-DDT

R.T.: 6.229 min
Delta R.T.: -0.002 min
Response: 545363567
Conc: 72.71 ng/ml

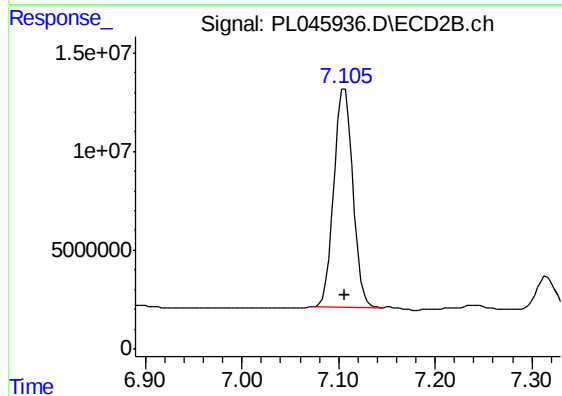

#17 4,4'-DDT


R.T.: 7.106 min
Delta R.T.: 0.000 min
Response: 148370646
Conc: 75.18 ng/ml

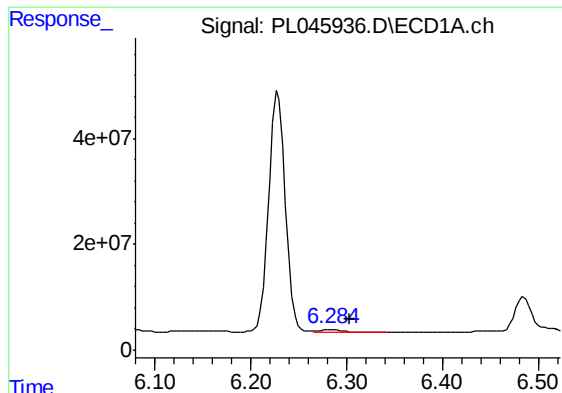

#18 Endrin aldehyde


R.T.: 6.285 min
Delta R.T.: -0.019 min
Response: 8447214
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

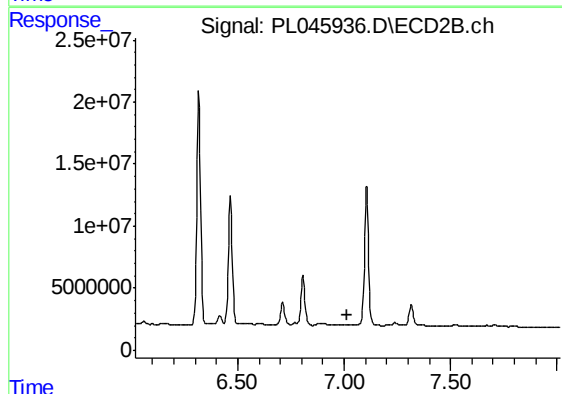


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.017 min
Response: 0
Conc: N.D.

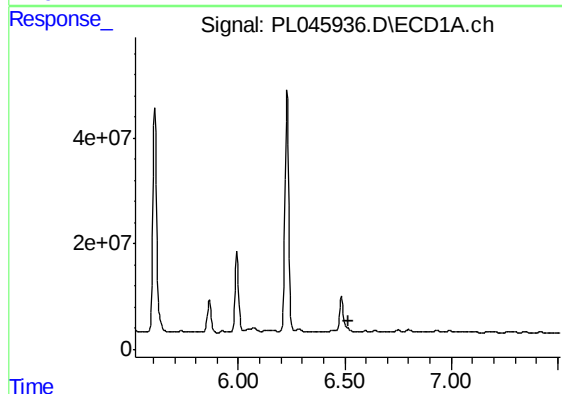


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.515 min
Response: 0
Conc: N.D.

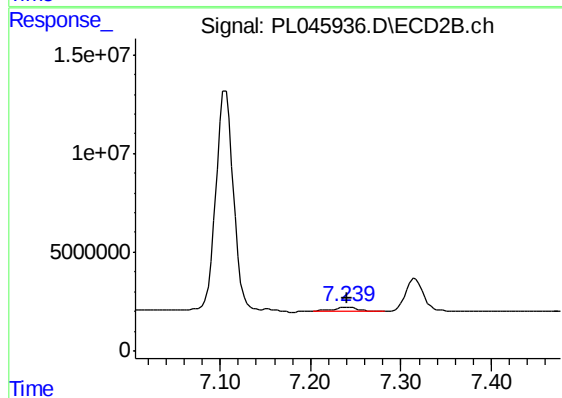

#19 Endosulfan Sulfate


R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 3050843
Conc: 1.36 ng/ml

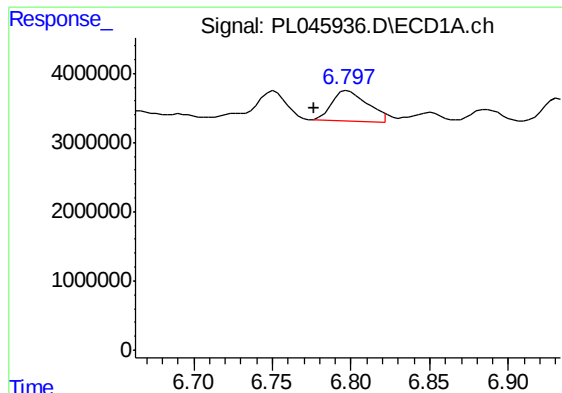

#20 Methoxychlor


R.T.: 6.798 min
Delta R.T.: 0.022 min
Response: 6780580
Conc: 1.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

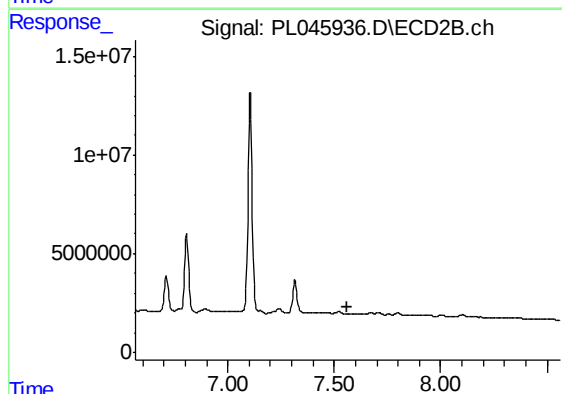


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.564 min
Response: 0
Conc: N.D.

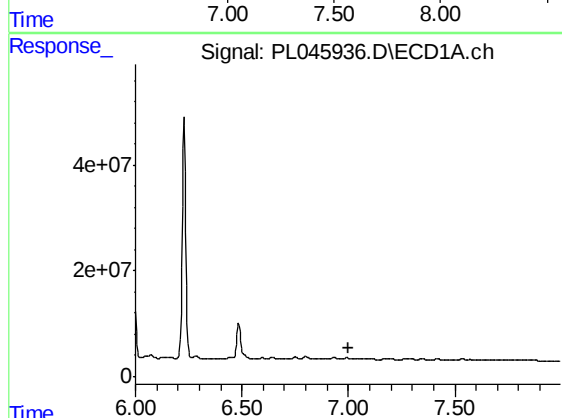


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

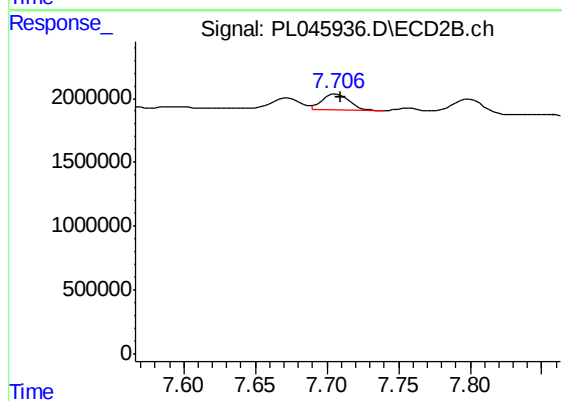

#21 Endrin ketone


R.T.: 7.707 min
Delta R.T.: -0.003 min
Response: 1691262
Conc: 0.71 ng/ml

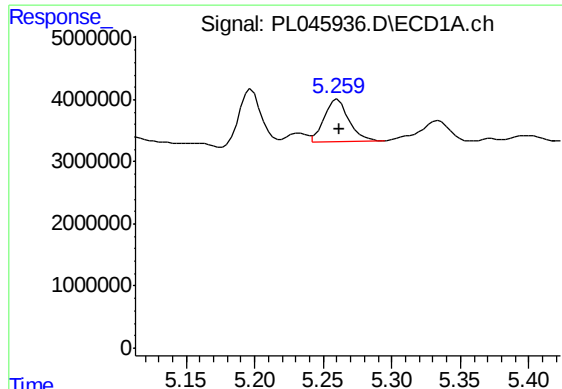

#25 Chlordane-3


R.T.: 5.260 min
Delta R.T.: -0.001 min
Response: 8436150
Conc: 7.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

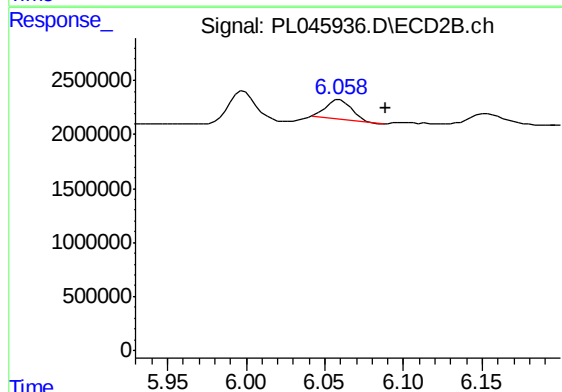


#25 Chlordane-3

R.T.: 6.060 min
Delta R.T.: -0.029 min
Response: 2126328
Conc: 5.46 ng/ml

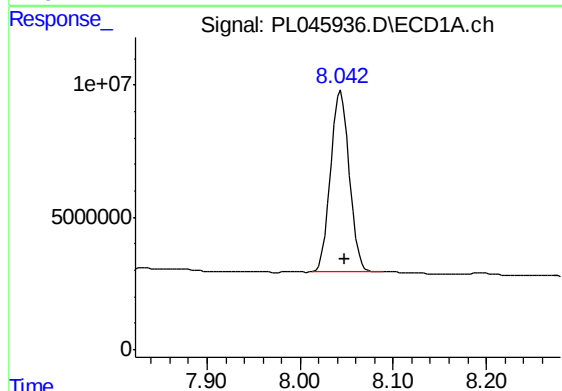

#28 Decachlorobiphenyl

R.T.: 8.044 min
Delta R.T.: -0.004 min
Response: 96283732
Conc: 11.51 ng/ml

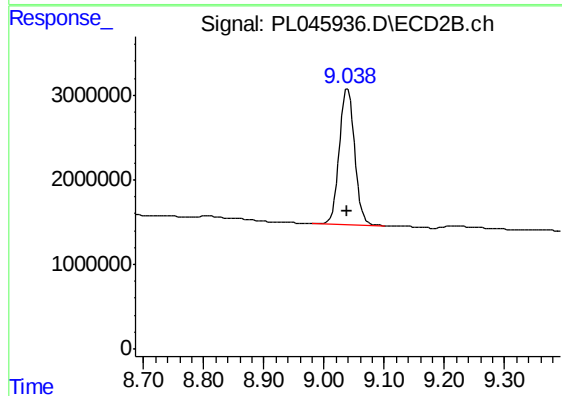

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 28467353
Conc: 12.46 ng/ml