

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031419\
 Data File : PL045947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2019 23:47
 Operator : AJ\SJ
 Sample : K1807-12
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6

Manual Integrations
 APPROVED

Sohil
 3/15/2019 11:37:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:17:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.362	3.981	119.2E6	38658499	17.321	18.052
28) SA Decachlor...	8.043	9.038	114.8E6	33351262	13.716	14.596
Target Compounds						
12) B 4,4'-DDE	5.481	6.316	4110517	1215916	0.468m	0.521m
13) MA Dieldrin	5.605	6.465	3327853	835251	0.348m	0.325m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031419\
Data File : PL045947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2019 23:47
Operator : AJ\SJ
Sample : K1807-12
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Sohil
3/15/2019 11:37:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:17:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

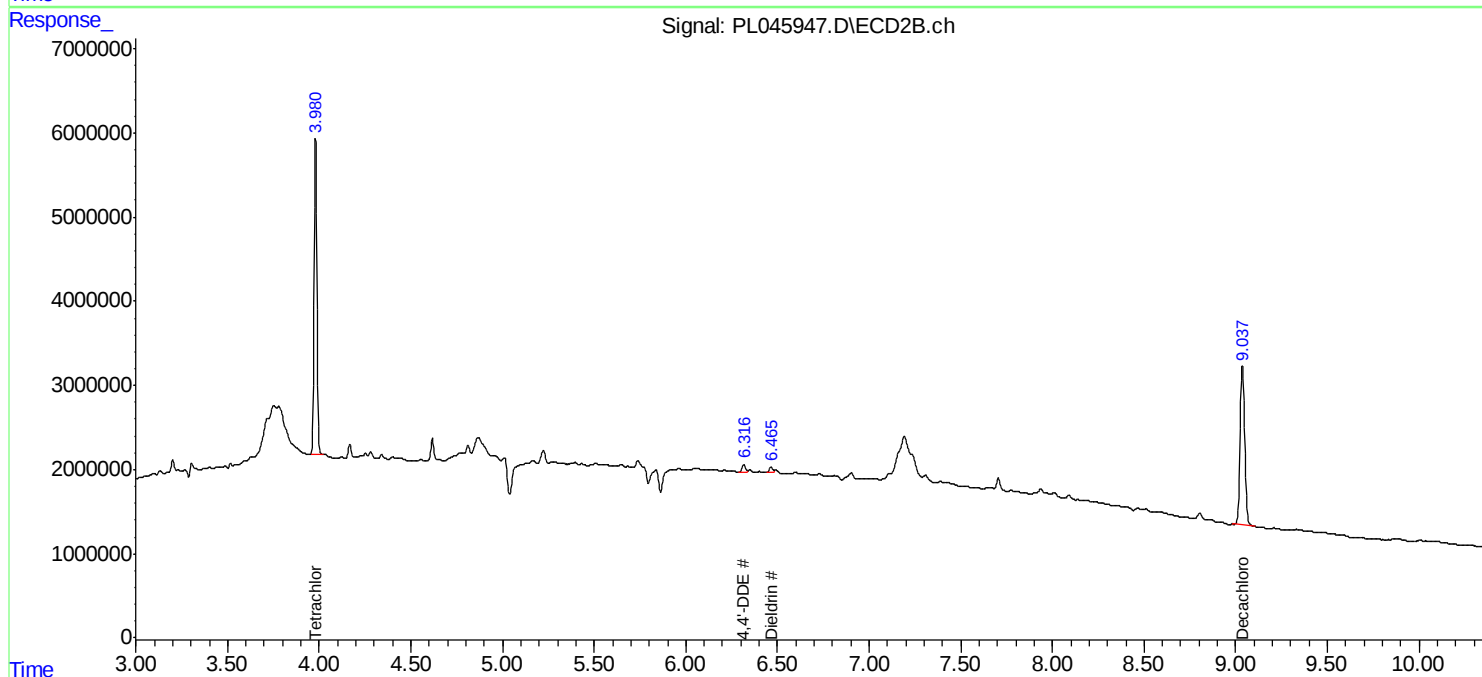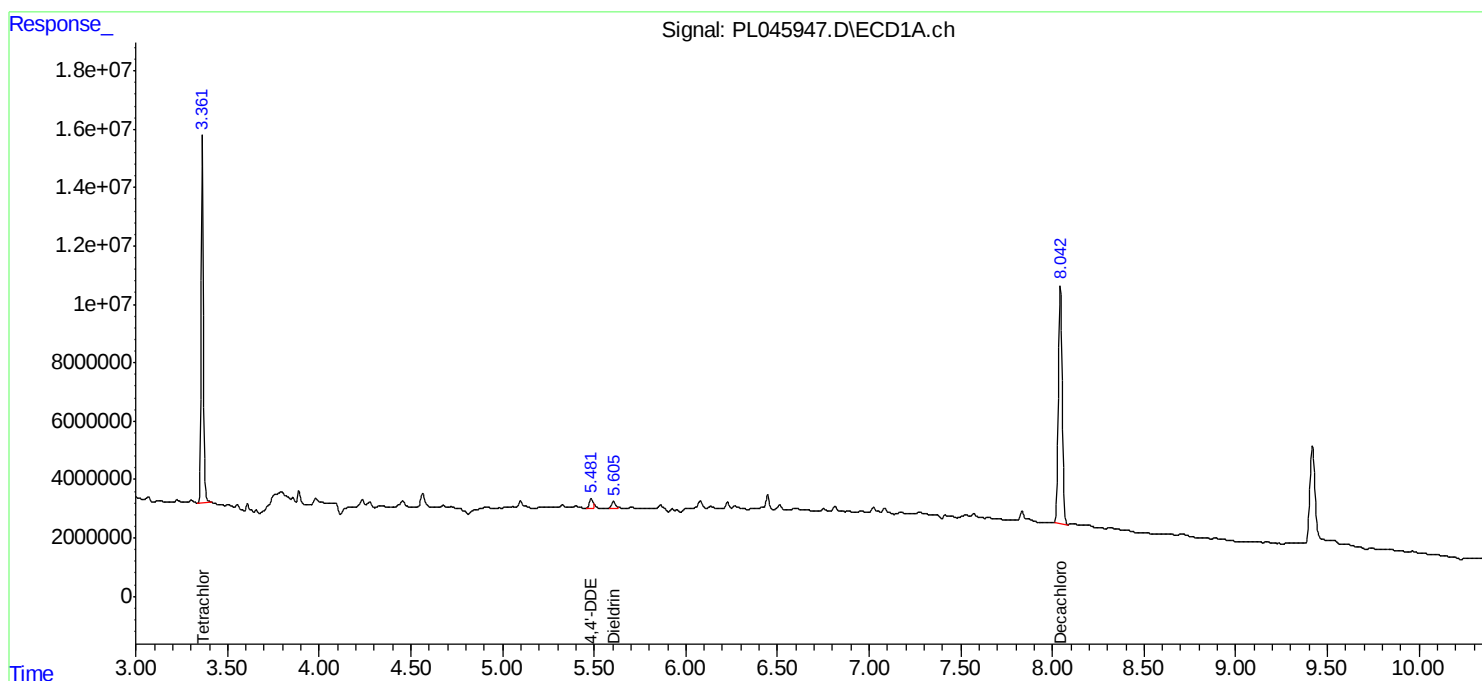

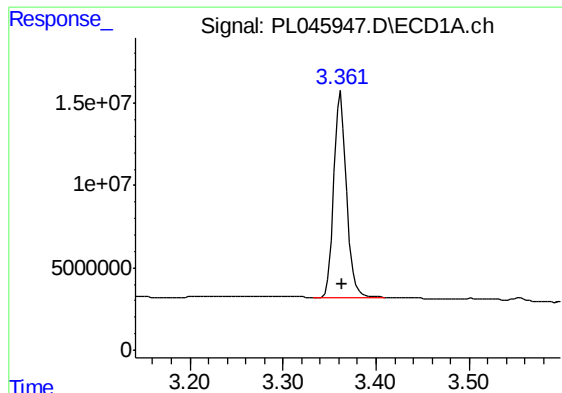


#1 Tetrachloro-m-xylene

R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 119157001
Conc: 17.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Sohil
3/15/2019 11:37:59 AM

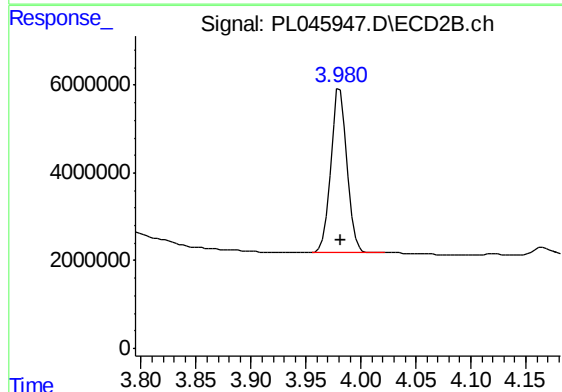


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 38658499
Conc: 18.05 ng/ml

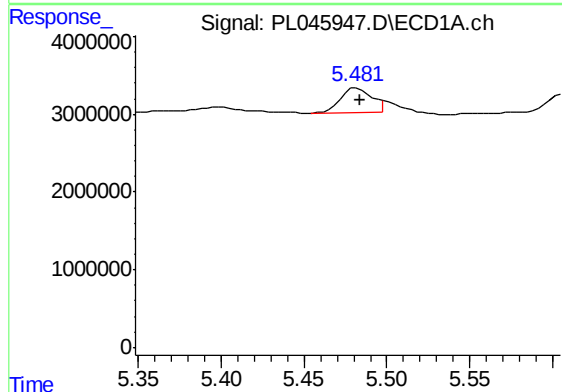


#12 4,4'-DDE

R.T.: 5.481 min
Delta R.T.: -0.003 min
Response: 4110517
Conc: 0.47 ng/ml m

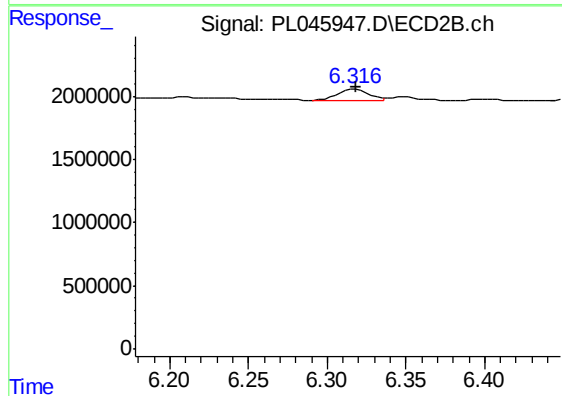

#12 4,4'-DDE

R.T.: 6.316 min
Delta R.T.: -0.002 min
Response: 1215916
Conc: 0.52 ng/ml m

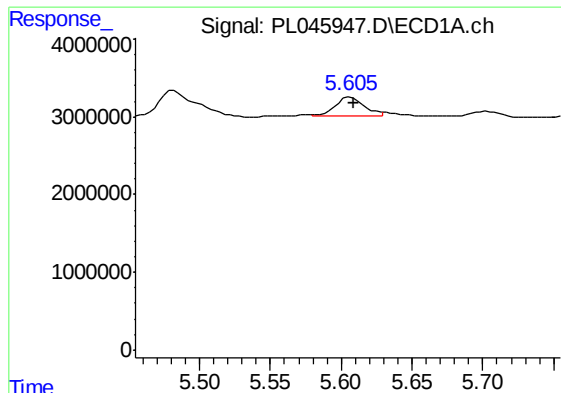


#13 Diieldrin

R.T.: 5.605 min
Delta R.T.: -0.004 min
Response: 3327853
Conc: 0.35 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Sohil
3/15/2019 11:37:59 AM

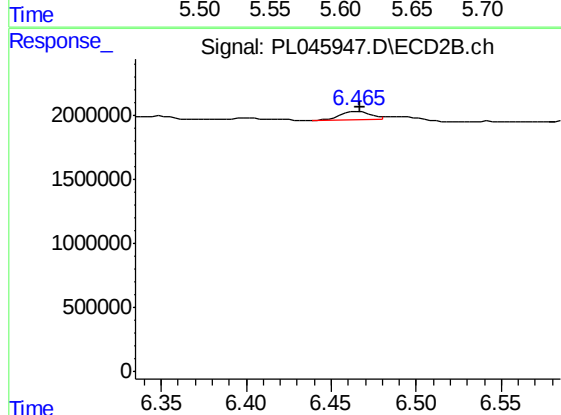


#13 Diieldrin

R.T.: 6.465 min
Delta R.T.: -0.002 min
Response: 835251
Conc: 0.33 ng/ml m

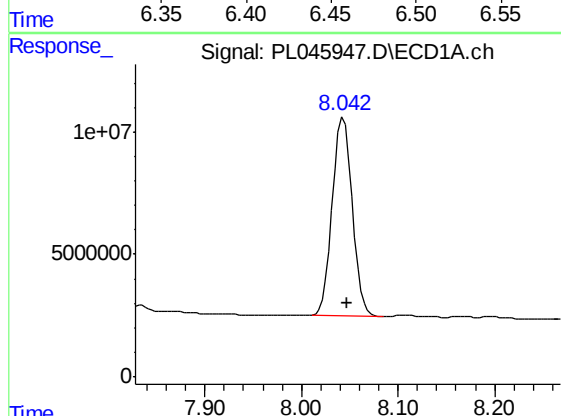

#28 Decachlorobiphenyl

R.T.: 8.043 min
Delta R.T.: -0.004 min
Response: 114768719
Conc: 13.72 ng/ml

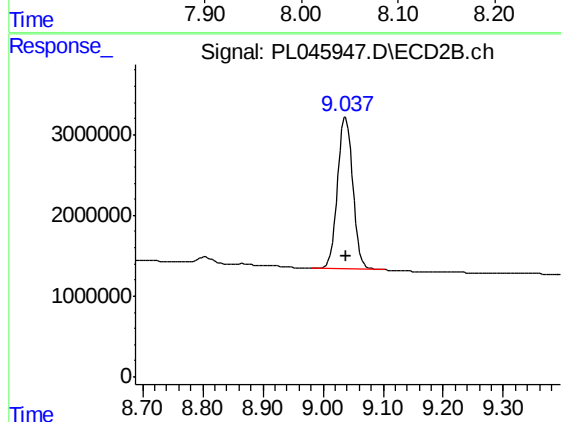

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: -0.001 min
Response: 33351262
Conc: 14.60 ng/ml