

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031419\
 Data File : PL045958.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2019 02:38
 Operator : AJ\SJ
 Sample : K1807-28
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-15

Manual Integrations
 APPROVED

Sohil
 3/15/2019 11:38:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:00:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.982	116.5E6	35730055	16.933	16.684
28)	SA Decachlor...	8.044	9.039	124.8E6	35487002	14.919	15.531
Target Compounds							
12)	B 4,4'-DDE	5.480	6.316	3802558	1030743	0.433m	0.441m
17)	MA 4,4'-DDT	6.227	7.106	2790879	737552	0.372m	0.374m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031419\
Data File : PL045958.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2019 02:38
Operator : AJ\SJ
Sample : K1807-28
Misc :
ALS Vial : 54 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-15


Manual Integrations
APPROVED

Sohil
3/15/2019 11:38:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:00:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

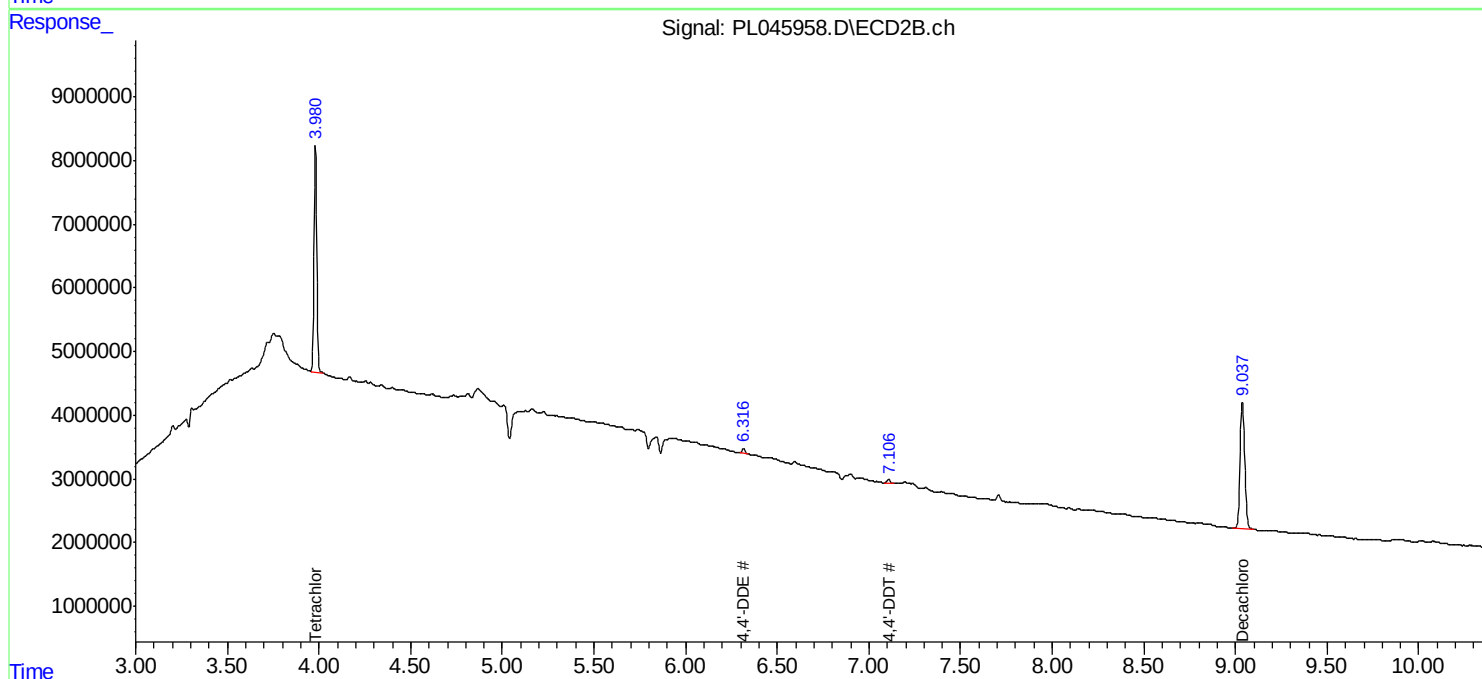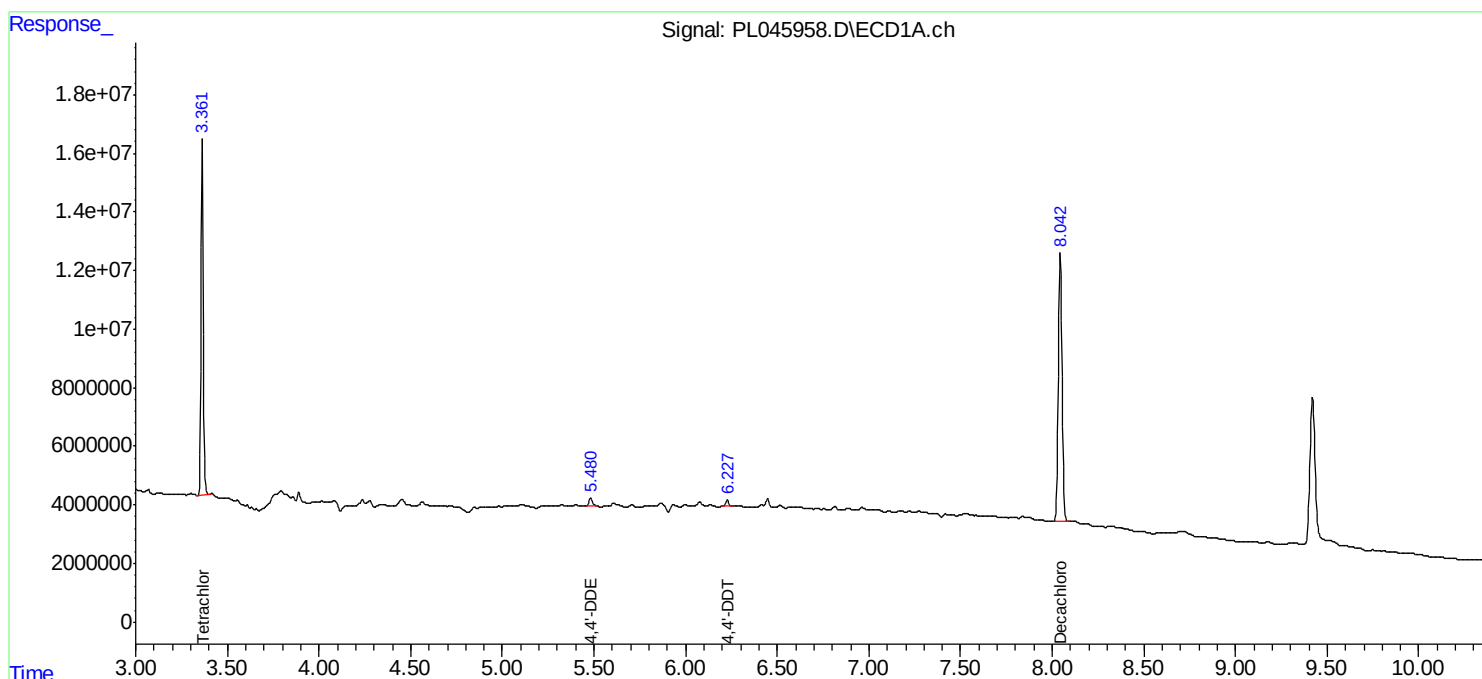

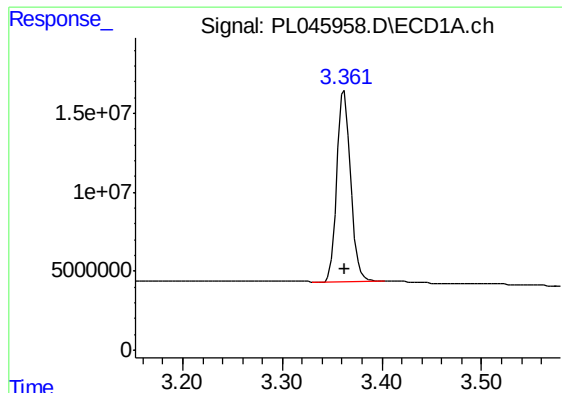


#1 Tetrachloro-m-xylene

R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 116487726
Conc: 16.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15


Manual Integrations
APPROVED

Sohil
3/15/2019 11:38:06 AM

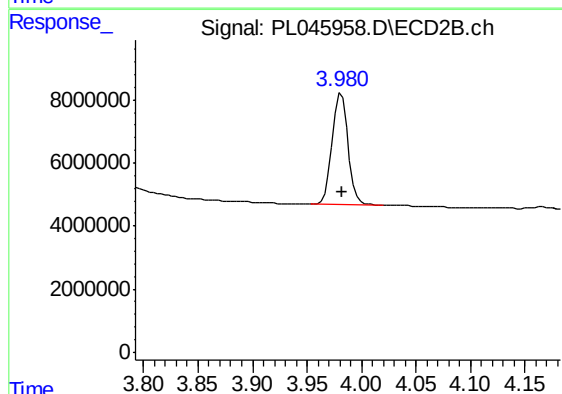


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 35730055
Conc: 16.68 ng/ml

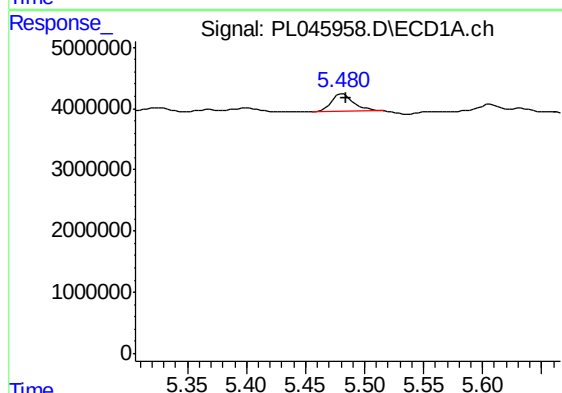


#12 4,4'-DDE

R.T.: 5.480 min
Delta R.T.: -0.004 min
Response: 3802558
Conc: 0.43 ng/ml m

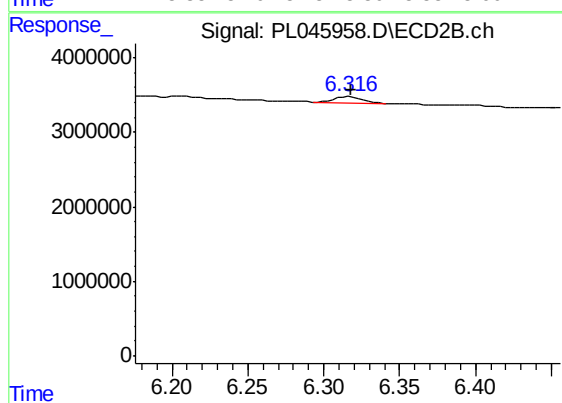

#12 4,4'-DDE

R.T.: 6.316 min
Delta R.T.: -0.002 min
Response: 1030743
Conc: 0.44 ng/ml m

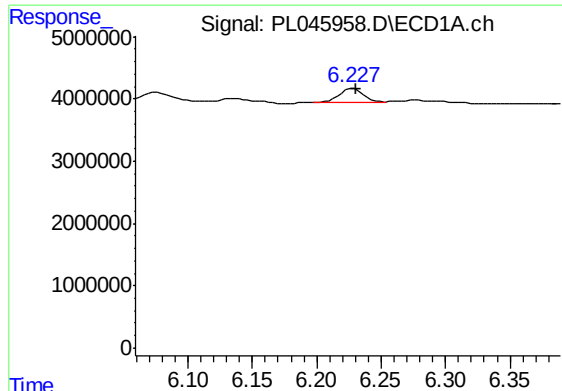


#17 4,4'-DDT

R.T.: 6.227 min
Delta R.T.: -0.004 min
Response: 2790879
Conc: 0.37 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-15


Manual Integrations
APPROVED

Sohil
3/15/2019 11:38:06 AM

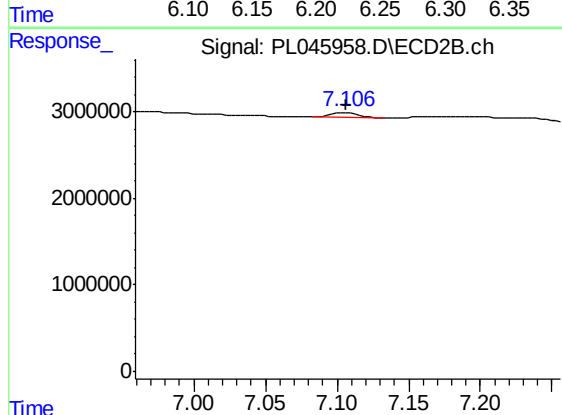


#17 4,4'-DDT

R.T.: 7.106 min
Delta R.T.: 0.000 min
Response: 737552
Conc: 0.37 ng/ml m

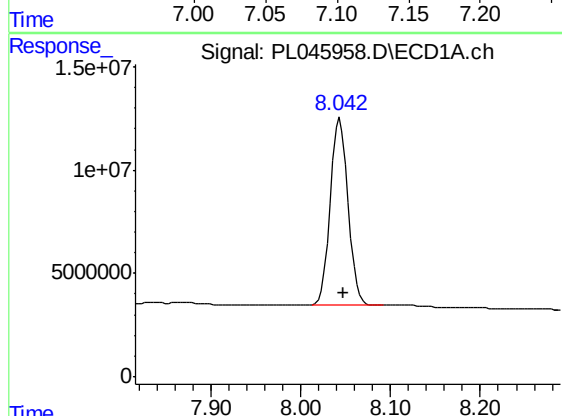

#28 Decachlorobiphenyl

R.T.: 8.044 min
Delta R.T.: -0.004 min
Response: 124832400
Conc: 14.92 ng/ml

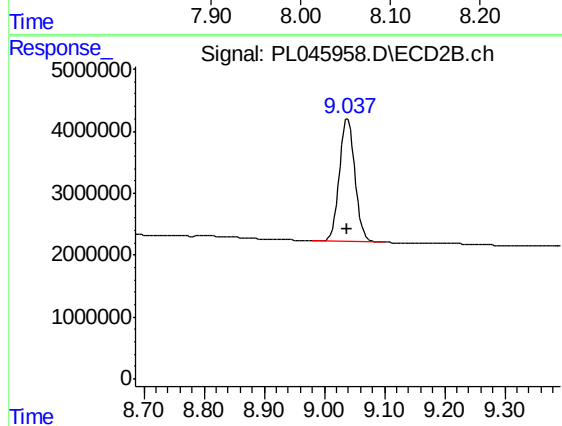

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 35487002
Conc: 15.53 ng/ml