

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031420\
 Data File : PL057376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2020 02:35
 Operator : AJ\MA
 Sample : PB127538TB
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB127538TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 03:34:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 14 00:45:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	177.1E6	40625617	19.102	18.725
28)	SA Decachlor...	8.206	8.978	167.5E6	39178350	15.833	17.669
Target Compounds							
2)	A alpha-BHC	3.889	0.000	2961433	0	0.186	N.D. #
4)	MA Heptachlor	0.000	5.134	0	8719483	N.D.	2.770 #
5)	MB Aldrin	4.735	0.000	243133	0	0.018	N.D. #
13)	MA Dieldrin	5.735f	0.000	118985	0	0.009	N.D. #
14)	MA Endrin	6.008	0.000	634231	0	0.055	N.D. #
18)	B Endrin al...	6.450	0.000	165342	0	0.018	N.D. #
22)	Mirex	7.334	0.000	91199	0	0.011	N.D. #
23)	Chlordane-1	4.356f	0.000	2068473	0	6.373	N.D. #
24)	Chlordane-2	4.855f	0.000	193830	0	0.533	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031420\
Data File : PL057376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2020 02:35
Operator : AJ\MA
Sample : PB127538TB
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB127538TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 03:34:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Sat Mar 14 00:45:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

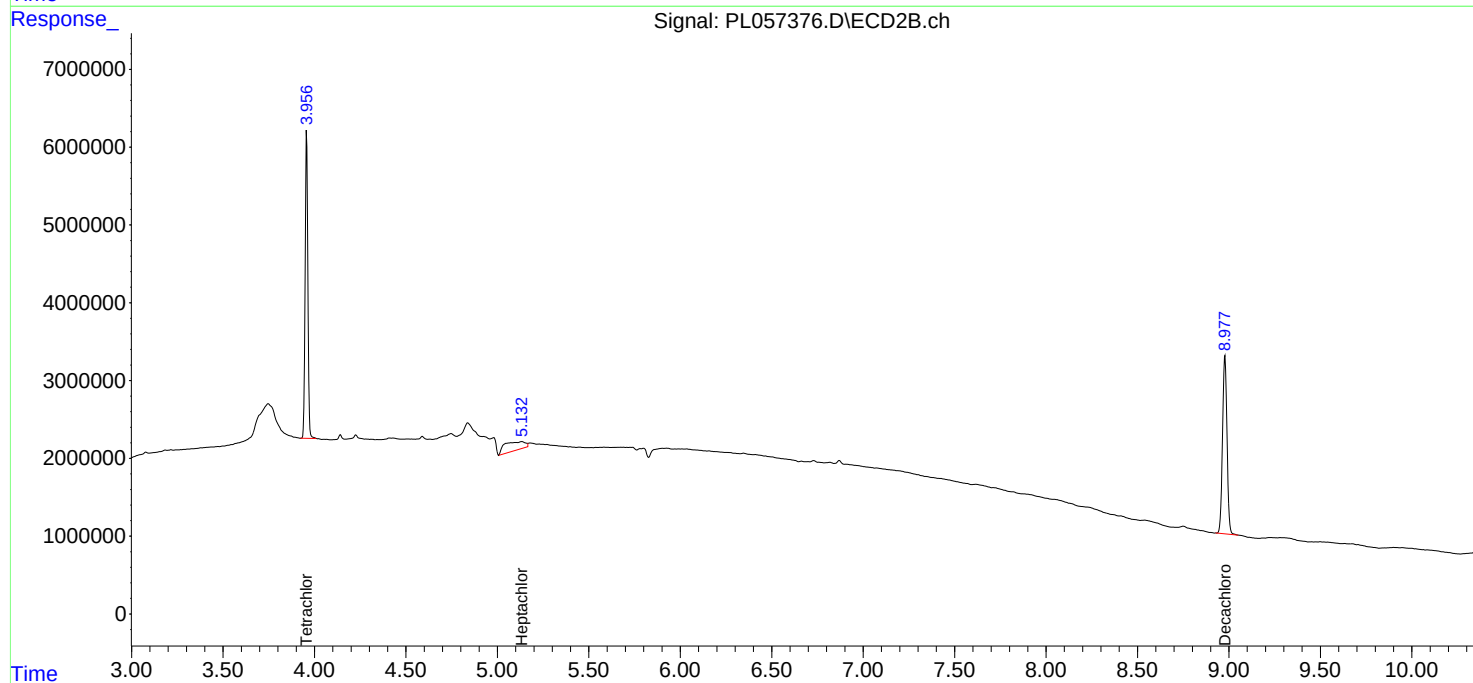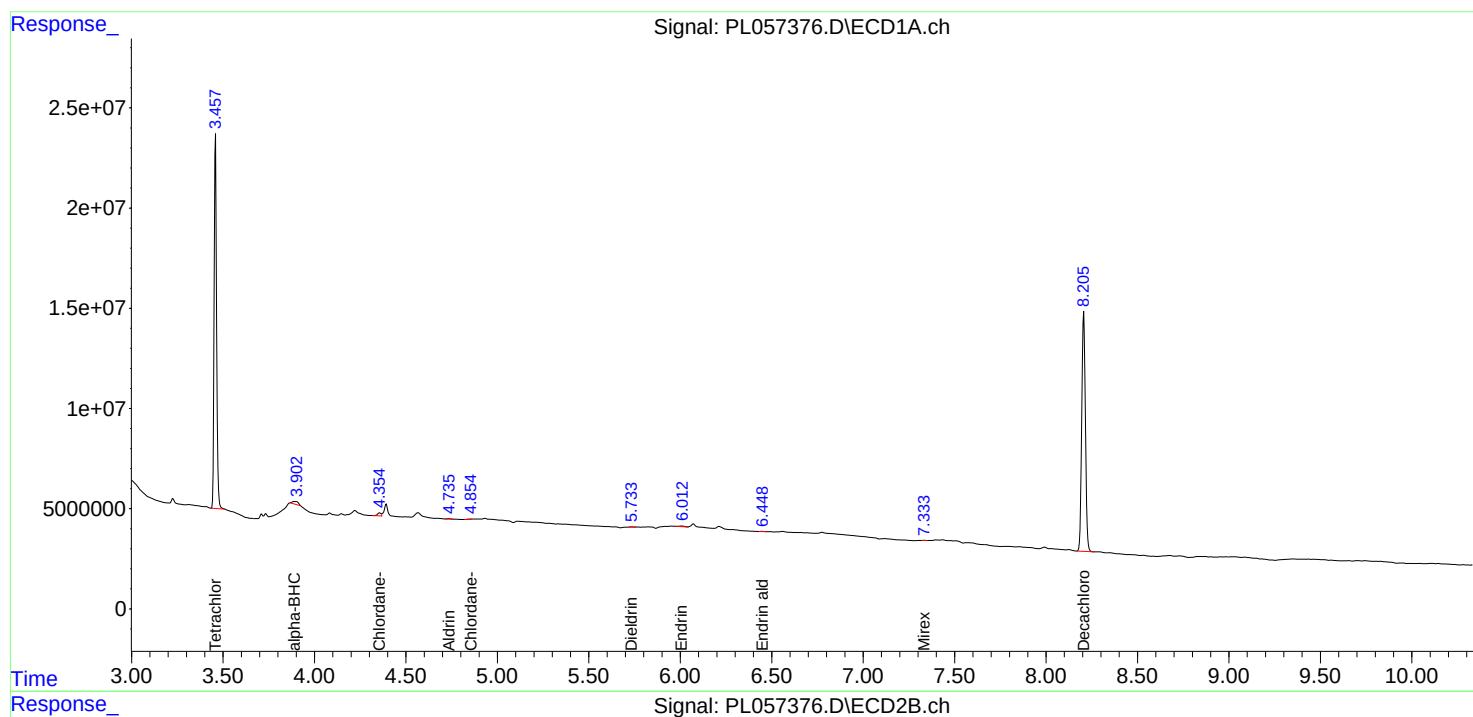


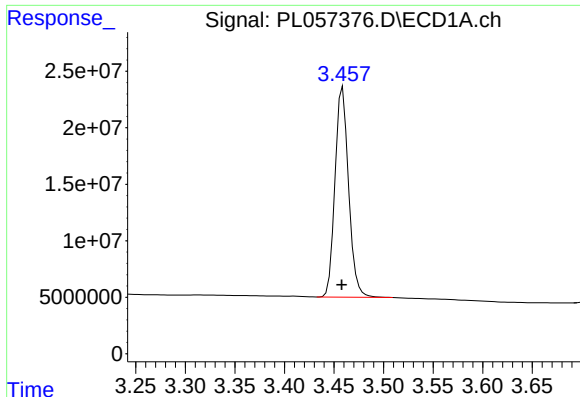

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 177060292
Conc: 19.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127538TB

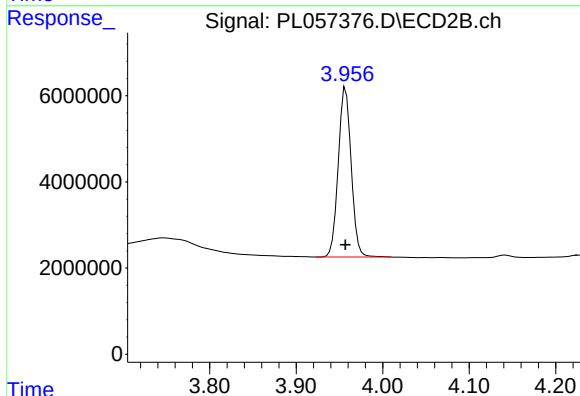


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 40625617
Conc: 18.73 ng/ml

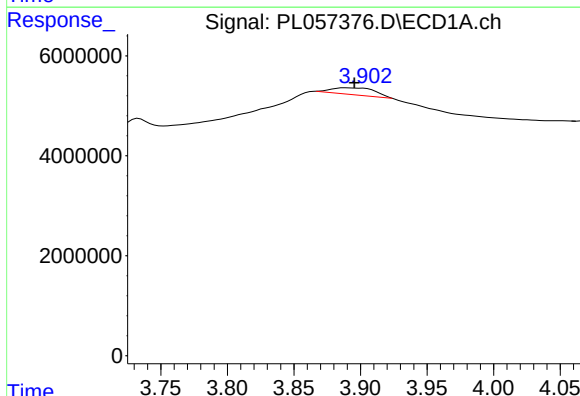


#2 alpha-BHC

R.T.: 3.889 min
Delta R.T.: -0.006 min
Response: 2961433
Conc: 0.19 ng/ml

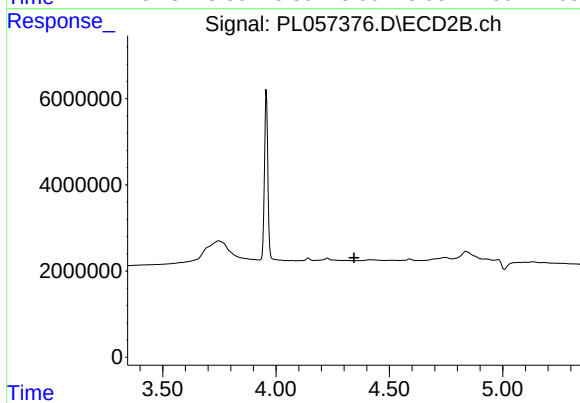

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

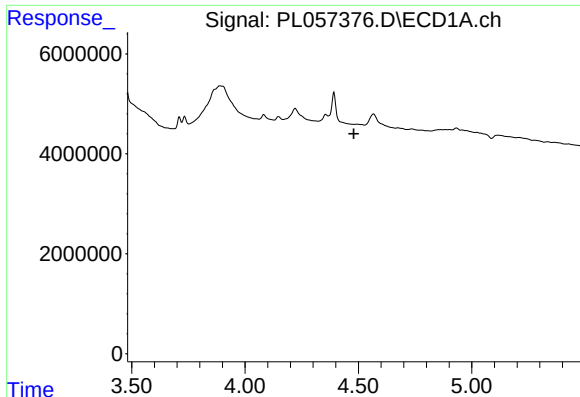

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB127538TB

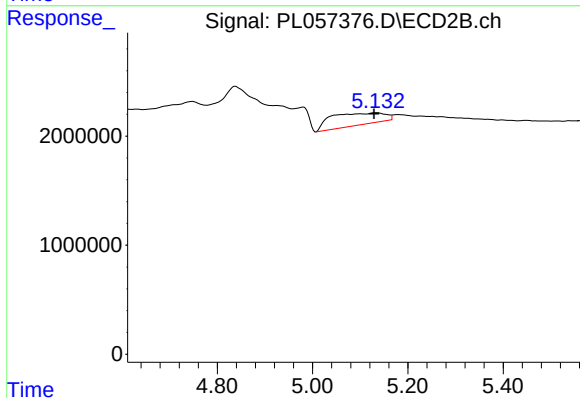


#4 Heptachlor

R.T.: 5.134 min
Delta R.T.: 0.005 min
Response: 8719483
Conc: 2.77 ng/ml

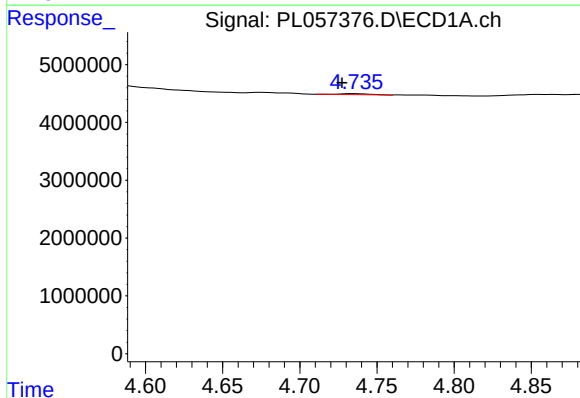


#5 Aldrin

R.T.: 4.735 min
Delta R.T.: 0.008 min
Response: 243133
Conc: 0.02 ng/ml

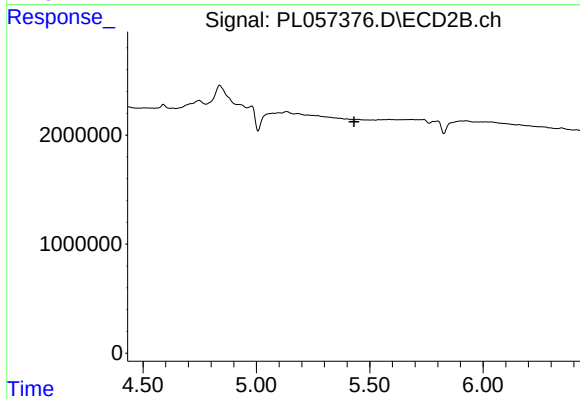

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.431 min
Response: 0
Conc: N.D.

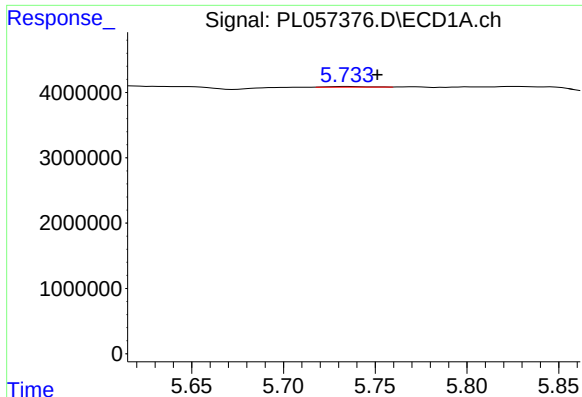

#13 Dieldrin


R.T.: 5.735 min
Delta R.T.: -0.016 min
Response: 118985
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127538TB

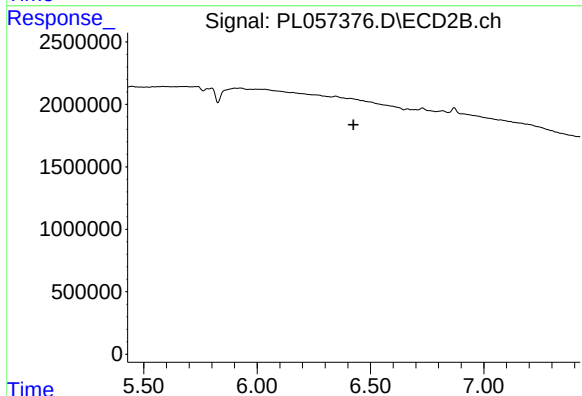


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

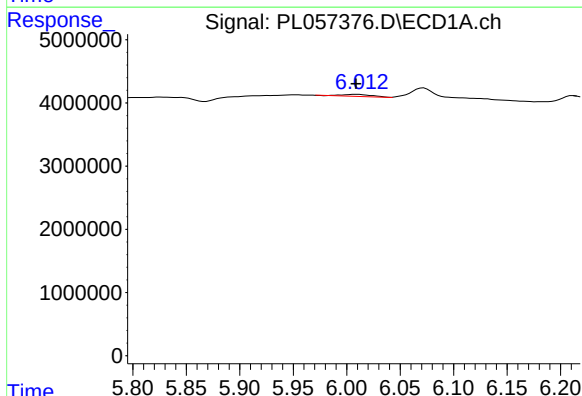


#14 Endrin

R.T.: 6.008 min
Delta R.T.: 0.000 min
Response: 634231
Conc: 0.06 ng/ml

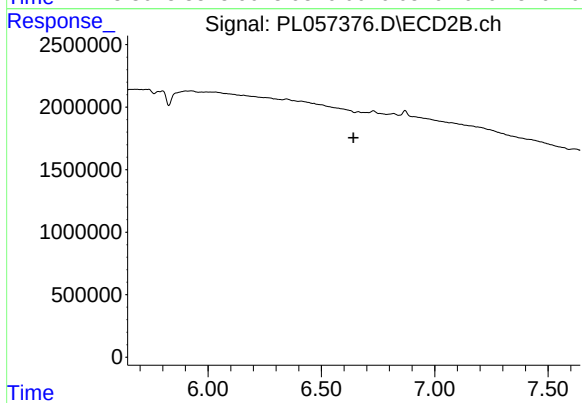

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

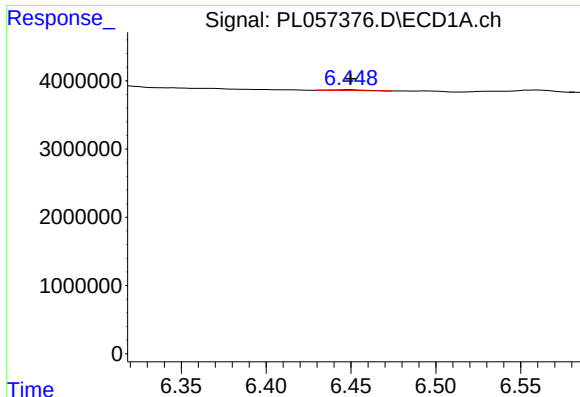

#18 Endrin aldehyde


R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 165342
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127538TB

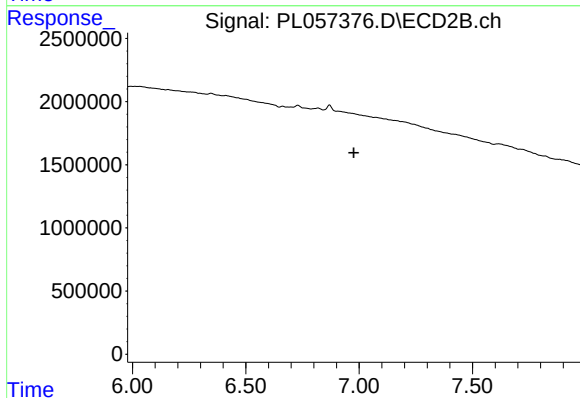


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

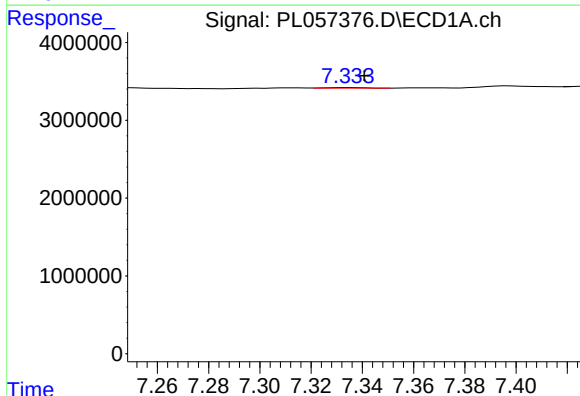


#22 Mirex

R.T.: 7.334 min
Delta R.T.: -0.007 min
Response: 91199
Conc: 0.01 ng/ml

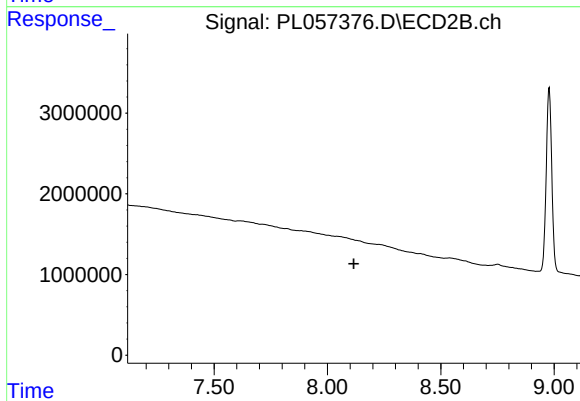

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

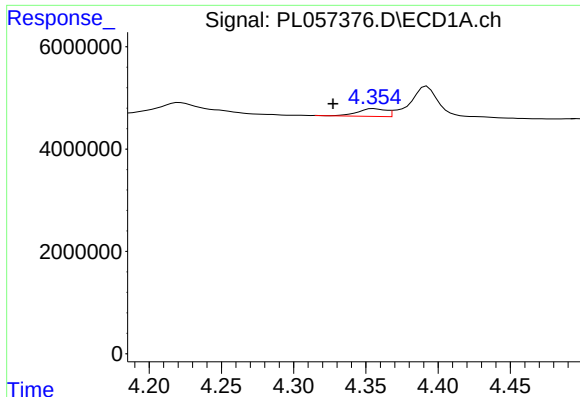

#23 Chlordane-1


R.T.: 4.356 min
Delta R.T.: 0.029 min
Response: 2068473
Conc: 6.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127538TB

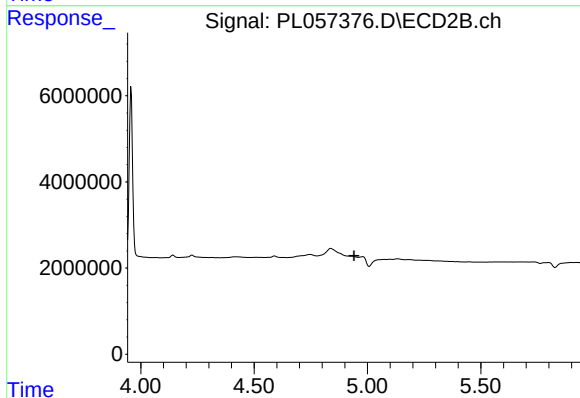


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

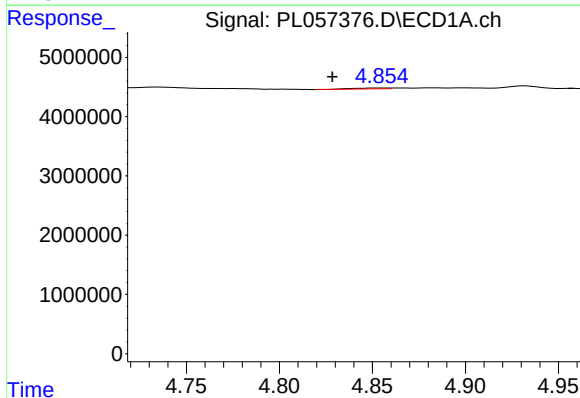


#24 Chlordane-2

R.T.: 4.855 min
Delta R.T.: 0.026 min
Response: 193830
Conc: 0.53 ng/ml

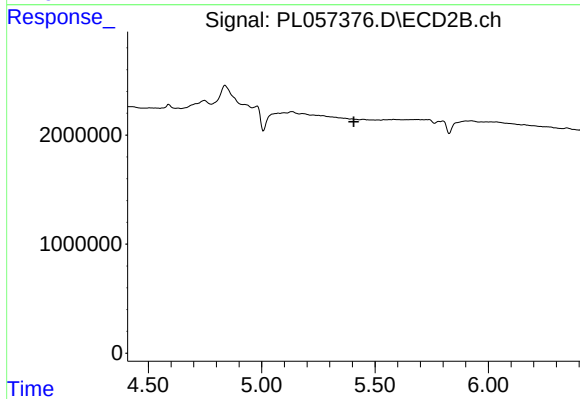

#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

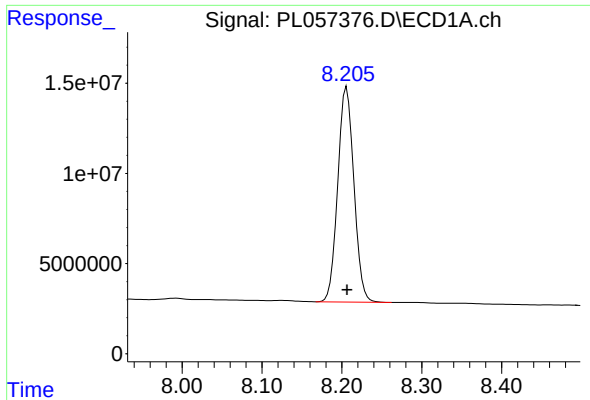

#28 Decachlorobiphenyl


R.T.: 8.206 min

Delta R.T.: 0.000 min

Response: 167535589

Conc: 15.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB127538TB

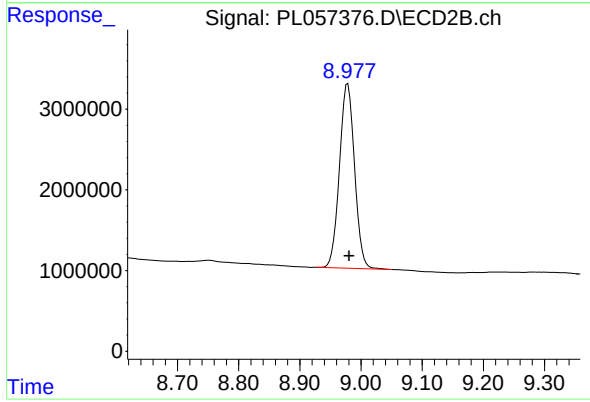

#28 Decachlorobiphenyl

R.T.: 8.978 min

Delta R.T.: -0.002 min

Response: 39178350

Conc: 17.67 ng/ml