

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031420\
 Data File : PL057333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 16:27
 Operator : AJ\MA
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 03:36:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 14 00:45:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.957	194.8E6	45209146	21.013	20.838
28)	SA Decachlor...	8.206	8.981	222.7E6	47083716	21.046	21.234
Target Compounds							
9)	A Endosulfan I	5.509	6.169	111.5E6	27408601	9.382	9.633
10)	B gamma-Chl...	5.397	6.048	119.0E6	29276097	9.124	9.499
12)	B 4,4'-DDE	5.619	6.280	242.2E6	53914925	19.444	18.968
13)	MA Dieldrin	5.751	6.426	245.4E6	57356749	19.456	19.391
19)	B Endosulfa...	6.663	7.198	199.7E6	47165105	19.882	19.337
20)	A Methoxychlor	6.920	7.524	534.8E6	122.9E6	99.668	94.499
21)	B Endrin ke...	7.154	7.665	219.5E6	51193454	19.417	19.776



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031420\
Data File : PL057333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 16:27
Operator : AJ\MA
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 03:36:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Sat Mar 14 00:45:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

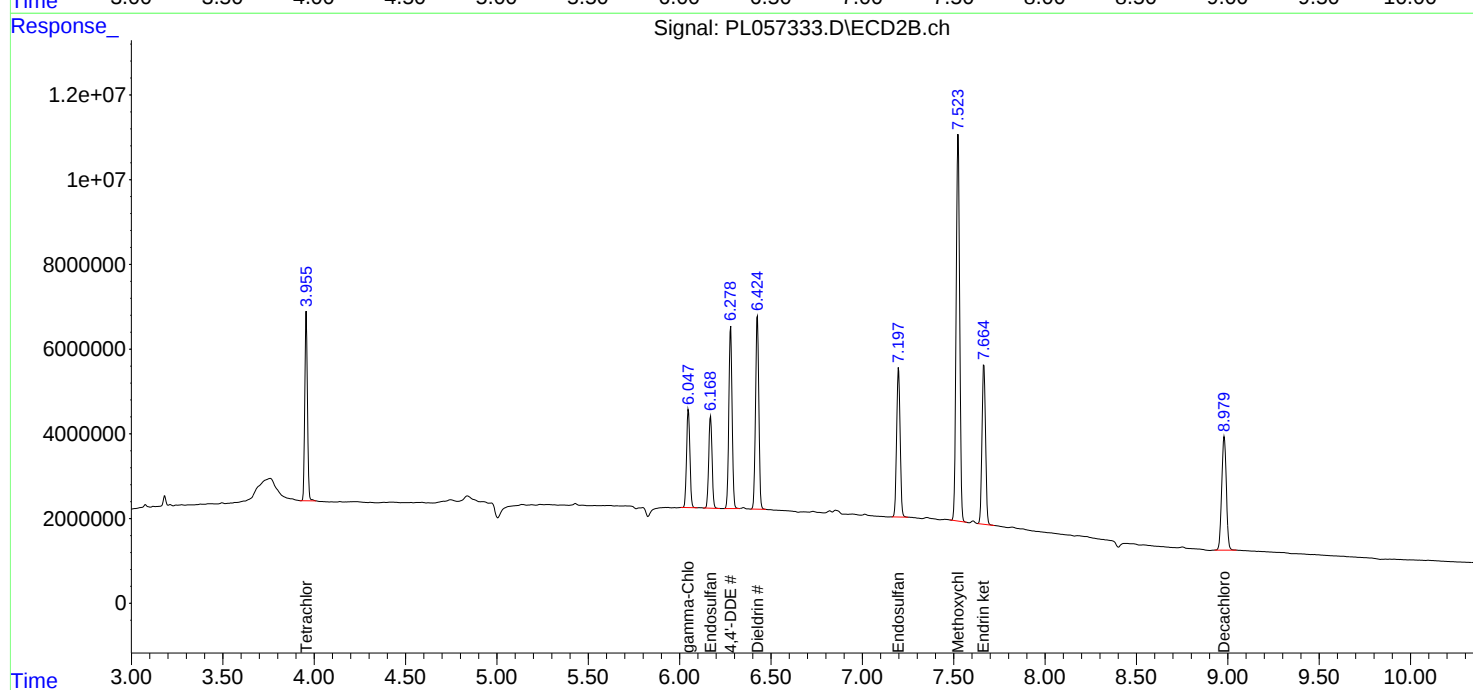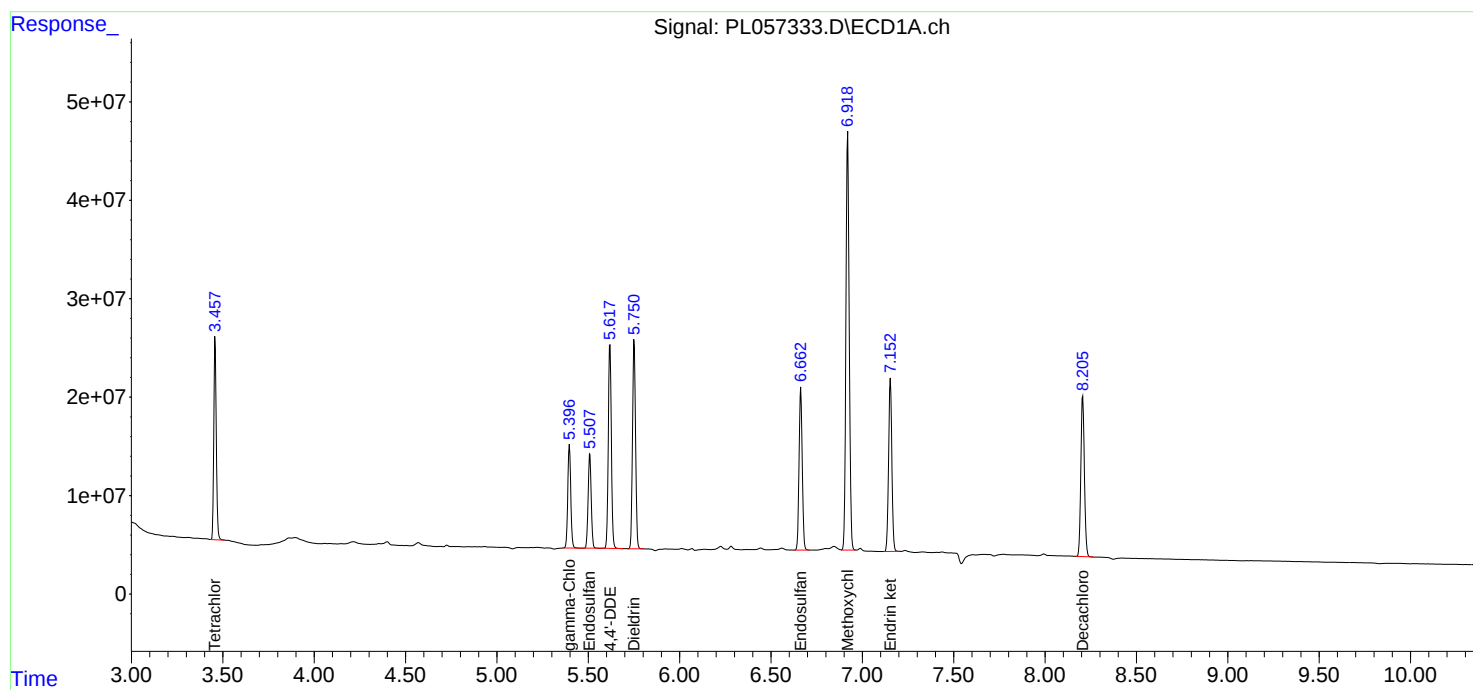


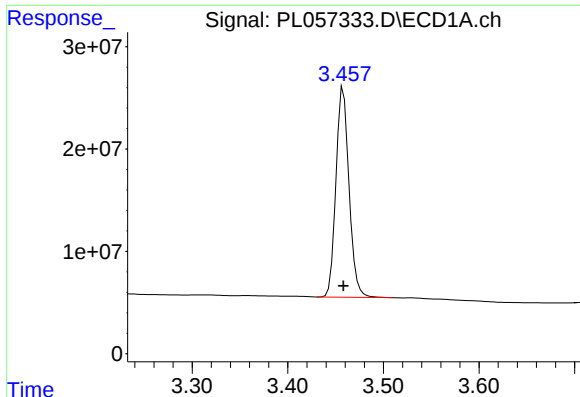

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 194779332
Conc: 21.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

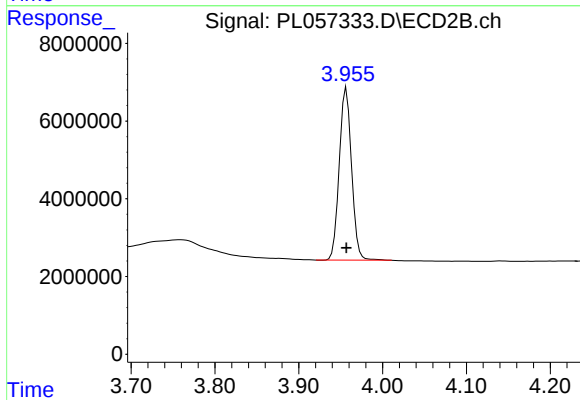


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 45209146
Conc: 20.84 ng/ml

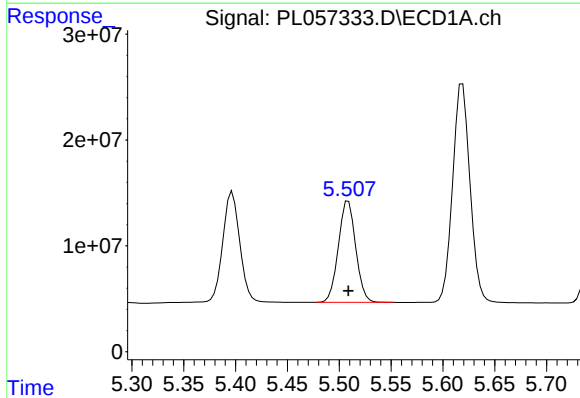


#9 Endosulfan I

R.T.: 5.509 min
Delta R.T.: 0.000 min
Response: 111545894
Conc: 9.38 ng/ml

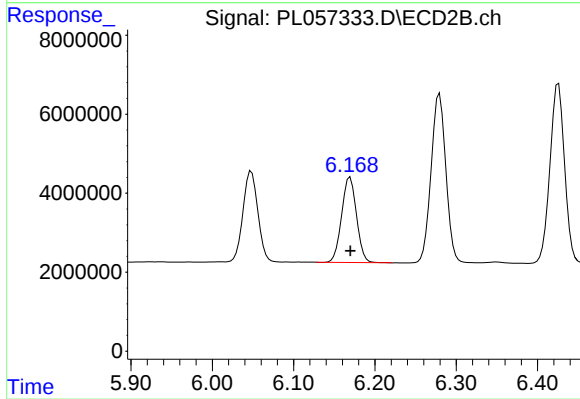

#9 Endosulfan I


R.T.: 6.169 min
Delta R.T.: 0.000 min
Response: 27408601
Conc: 9.63 ng/ml

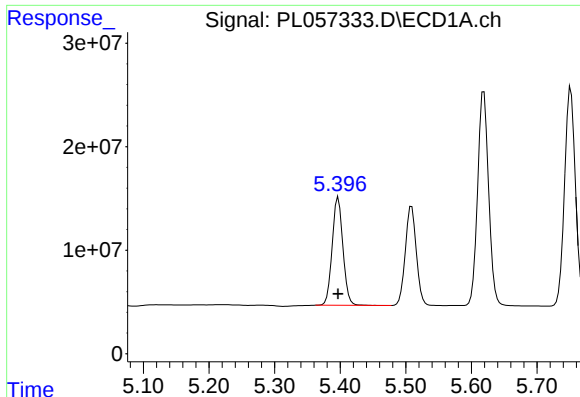

#10 gamma-Chlordane


R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 118974995
Conc: 9.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

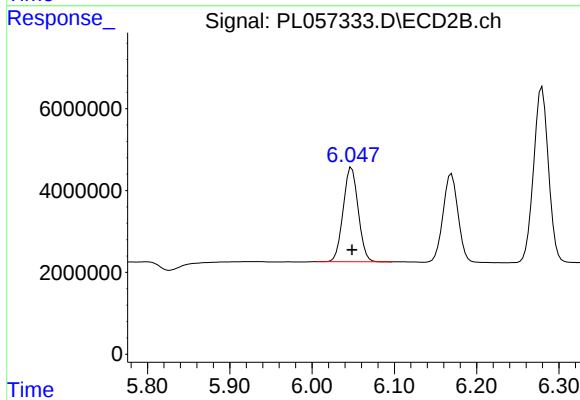


#10 gamma-Chlordane

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 29276097
Conc: 9.50 ng/ml

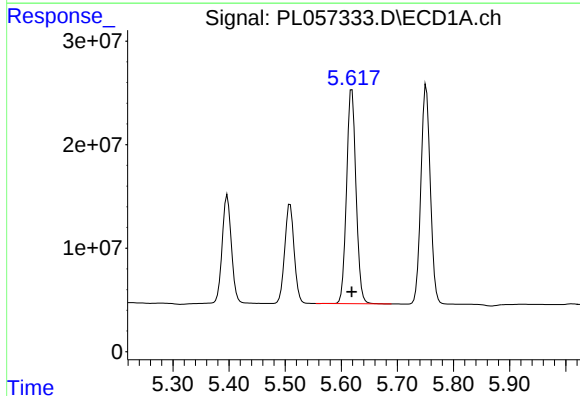


#12 4,4'-DDE

R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 242182492
Conc: 19.44 ng/ml

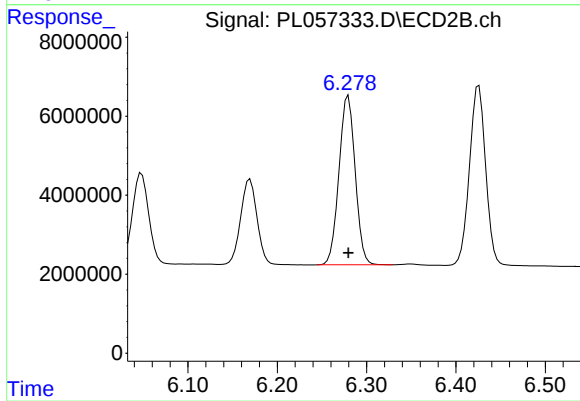

#12 4,4'-DDE


R.T.: 6.280 min
Delta R.T.: 0.000 min
Response: 53914925
Conc: 18.97 ng/ml

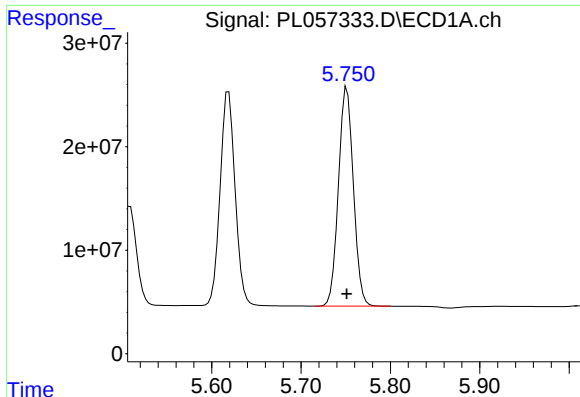

#13 Dieldrin


R.T.: 5.751 min
Delta R.T.: 0.000 min
Response: 245393385
Conc: 19.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

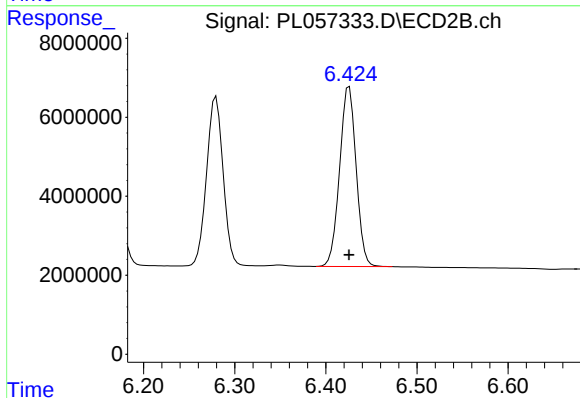


#13 Dieldrin

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 57356749
Conc: 19.39 ng/ml

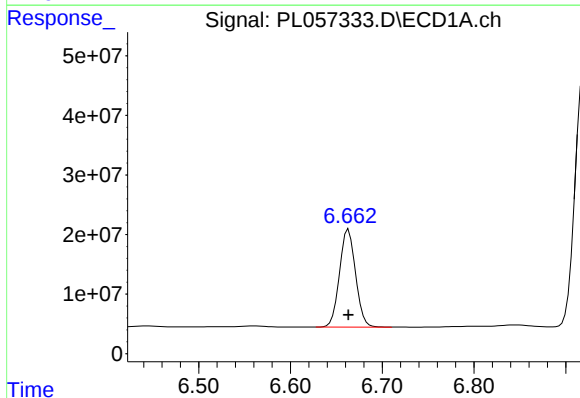


#19 Endosulfan Sulfate

R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 199662088
Conc: 19.88 ng/ml

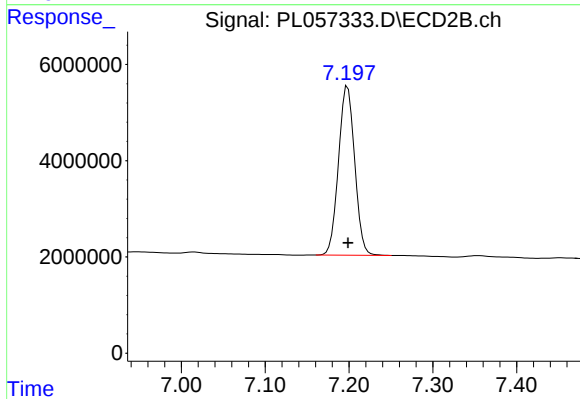

#19 Endosulfan Sulfate


R.T.: 7.198 min
Delta R.T.: 0.000 min
Response: 47165105
Conc: 19.34 ng/ml

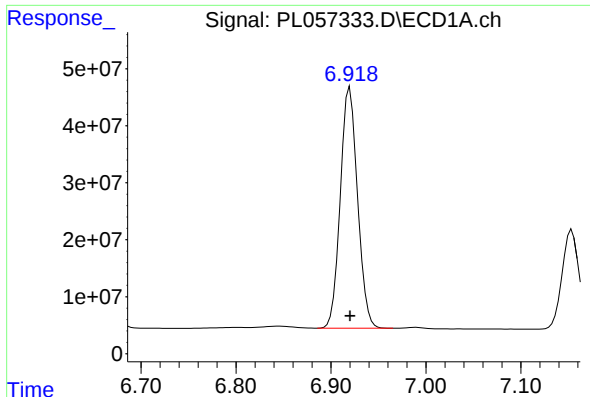

#20 Methoxychlor


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 534801227
Conc: 99.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

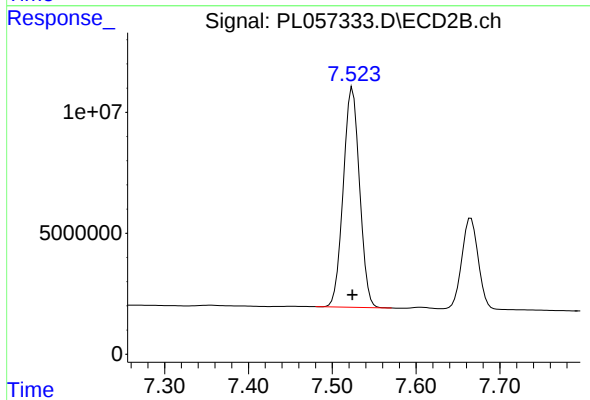


#20 Methoxychlor

R.T.: 7.524 min
Delta R.T.: 0.000 min
Response: 122903853
Conc: 94.50 ng/ml

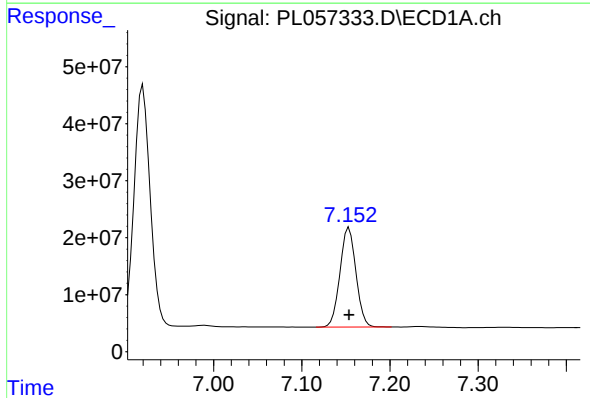


#21 Endrin ketone

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 219459451
Conc: 19.42 ng/ml

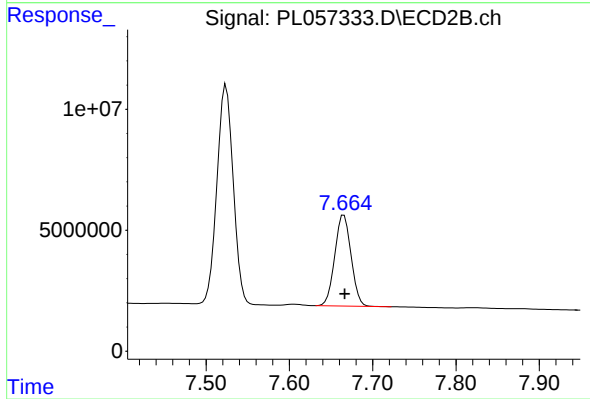

#21 Endrin ketone


R.T.: 7.665 min
Delta R.T.: 0.000 min
Response: 51193454
Conc: 19.78 ng/ml

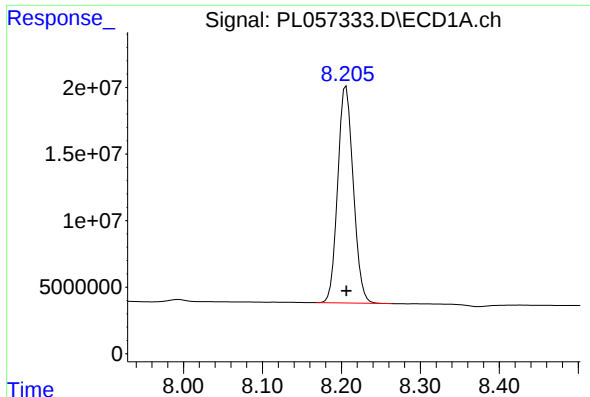

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 222695958
Conc: 21.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

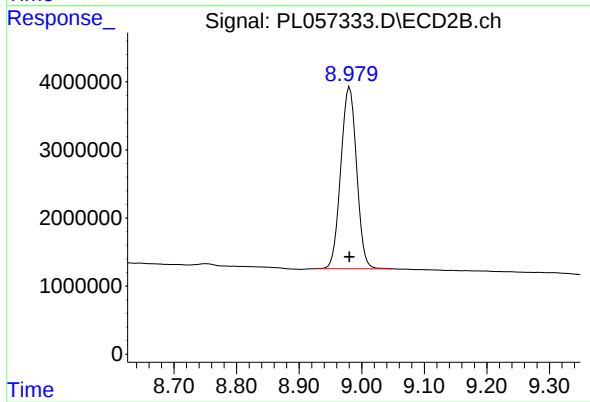

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 47083716
Conc: 21.23 ng/ml