

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031420\
 Data File : PL057339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2020 17:52
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 00:43:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 14 00:42:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.957	541.6E6	106.7E6	50.000	50.000
28)	SA Decachlor...	8.206	8.979	506.8E6	105.9E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.327	4.941	162.3E6	41549188	500.000	500.000
24)	Chlordane-2	4.829	5.406	181.7E6	47120572	500.000	500.000
25)	Chlordane-3	5.398	6.049	563.8E6	189.6E6	500.000	500.000
26)	Chlordane-4	5.454	6.122	479.3E6	228.8E6	500.000	500.000
27)	Chlordane-5	6.290	6.922	181.9E6	40067433	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031420\
Data File : PL057339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2020 17:52
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 00:43:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Sat Mar 14 00:42:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

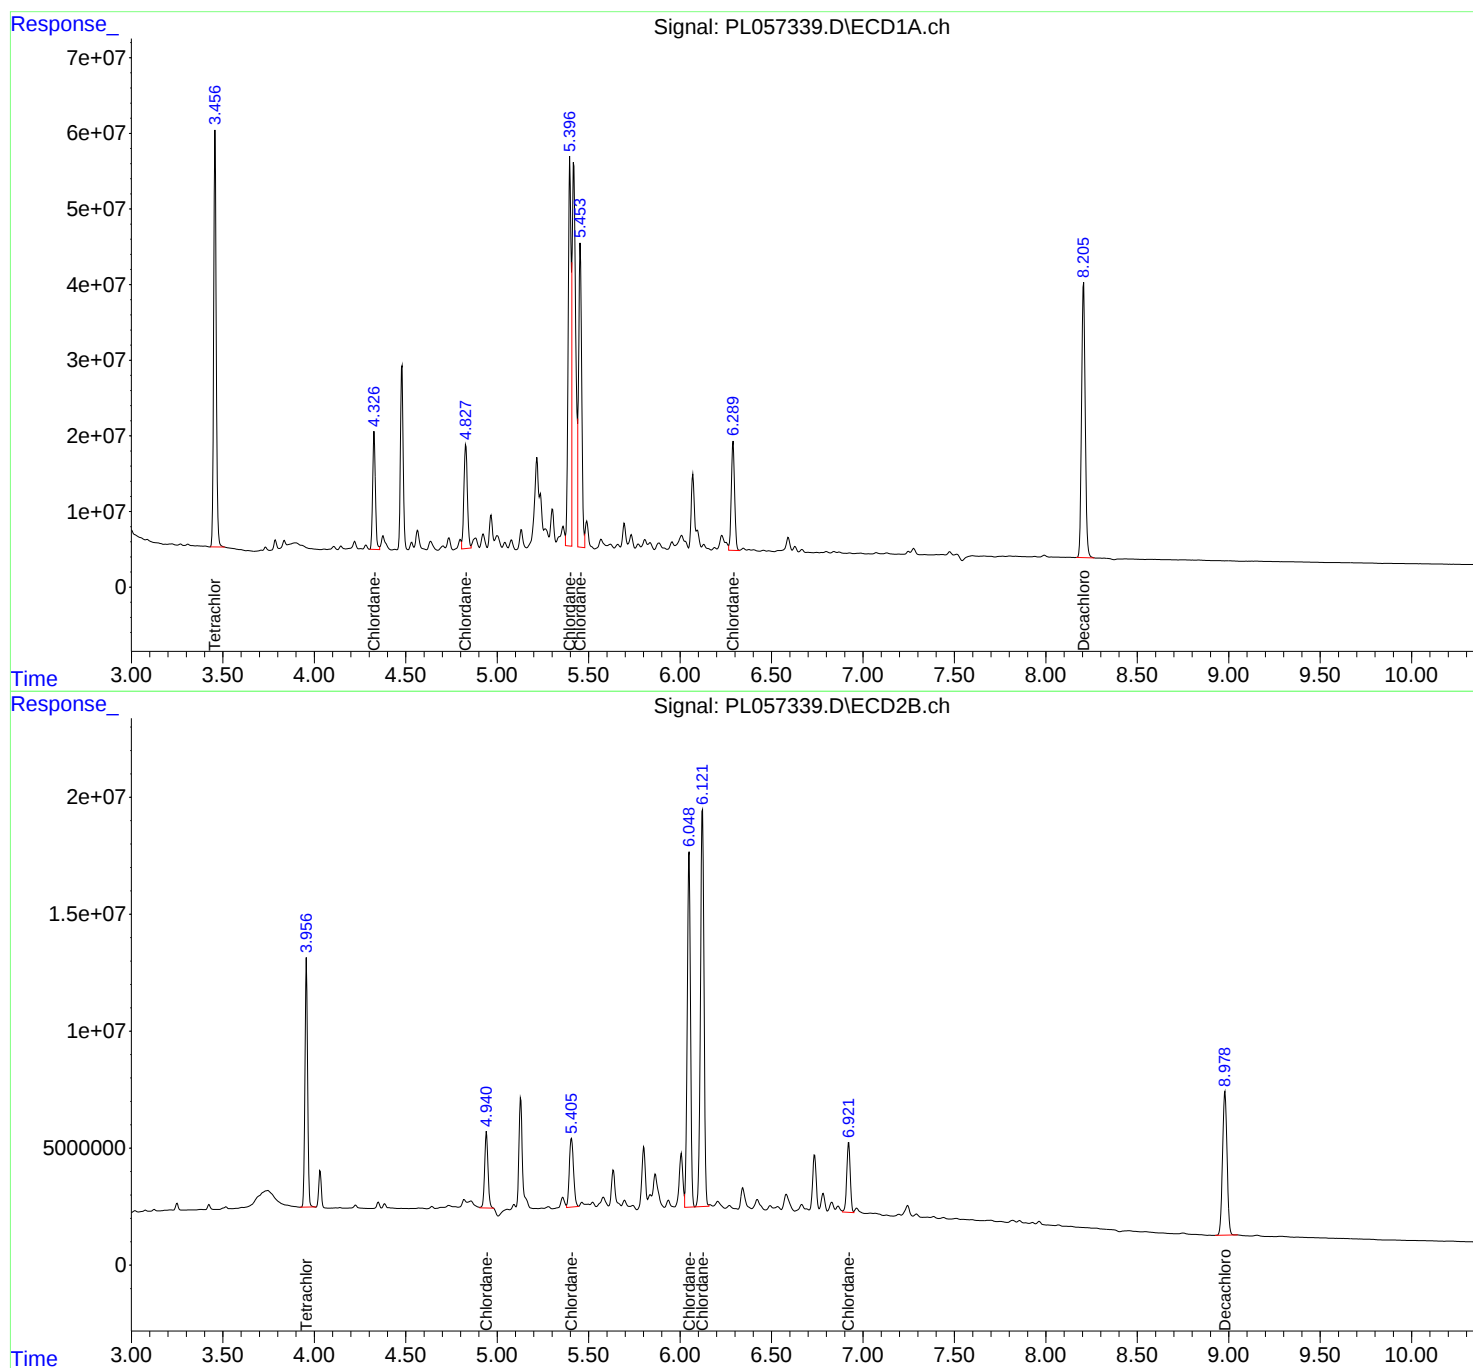


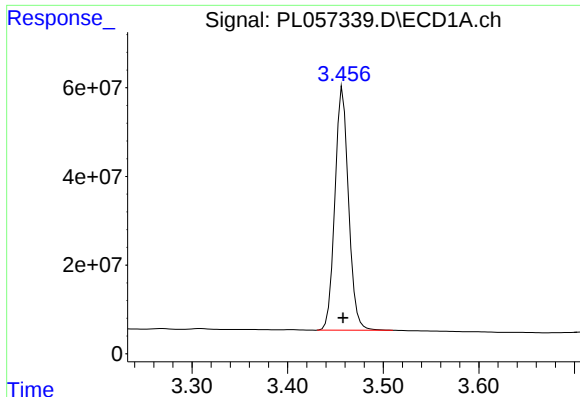

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 541561872
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

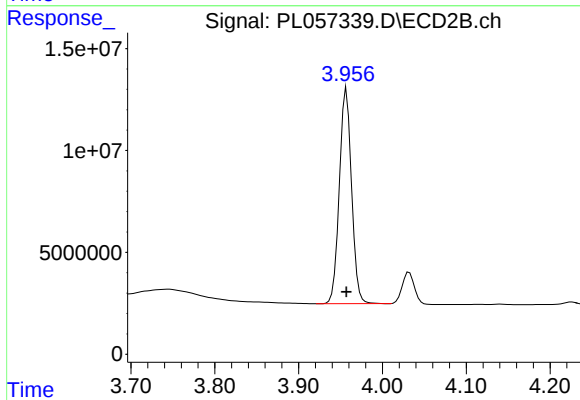


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 106742871
Conc: 50.00 ng/ml

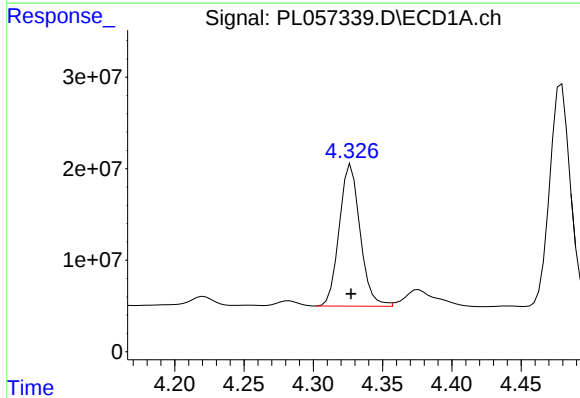


#23 Chlordane-1

R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 162283153
Conc: 500.00 ng/ml

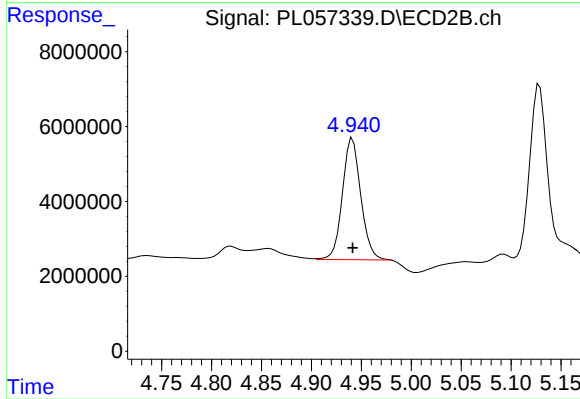

#23 Chlordane-1


R.T.: 4.941 min
Delta R.T.: 0.000 min
Response: 41549188
Conc: 500.00 ng/ml

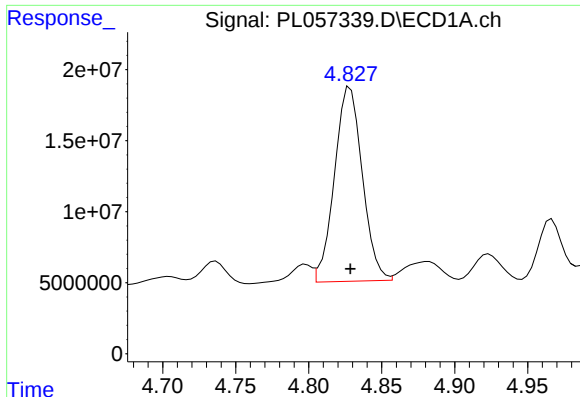

#24 Chlordane-2


R.T.: 4.829 min
Delta R.T.: 0.000 min
Response: 181684783
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

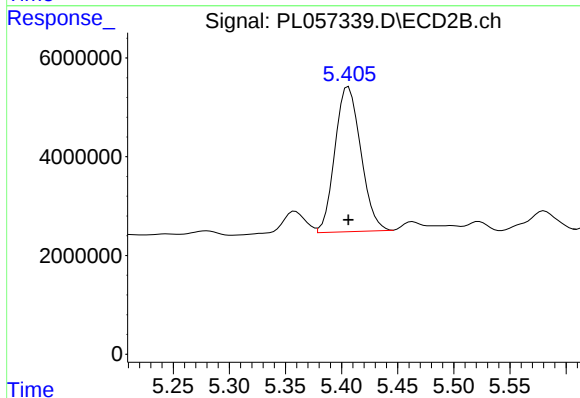


#24 Chlordane-2

R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 47120572
Conc: 500.00 ng/ml

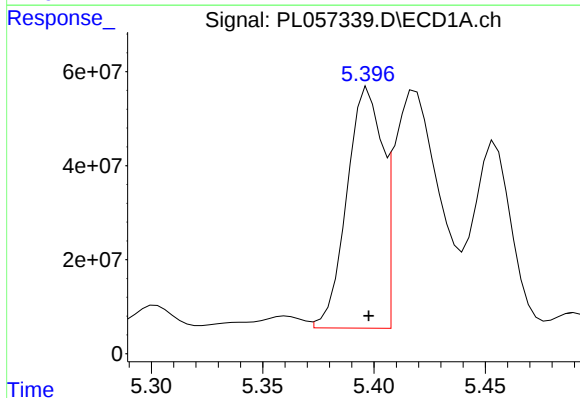


#25 Chlordane-3

R.T.: 5.398 min
Delta R.T.: 0.000 min
Response: 563840362
Conc: 500.00 ng/ml

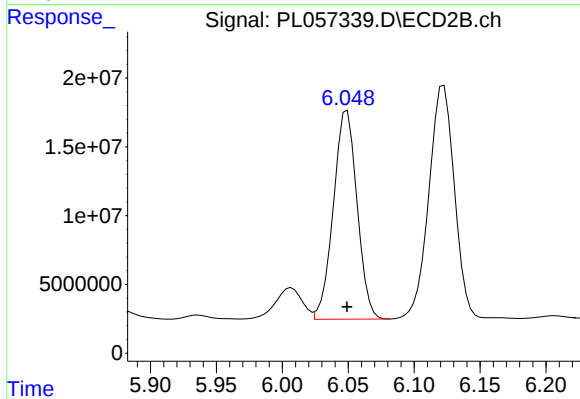

#25 Chlordane-3


R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 189599676
Conc: 500.00 ng/ml

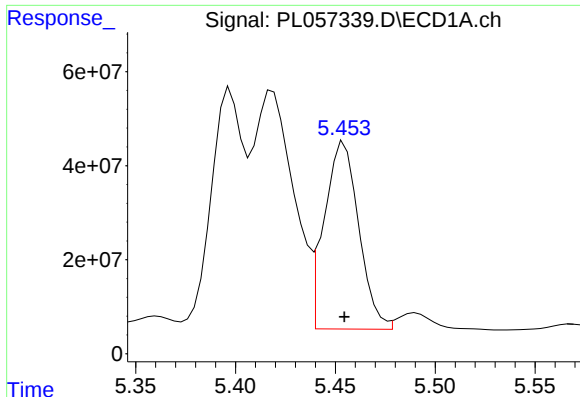

#26 Chlordane-4


R.T.: 5.454 min
Delta R.T.: 0.000 min
Response: 479335039
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

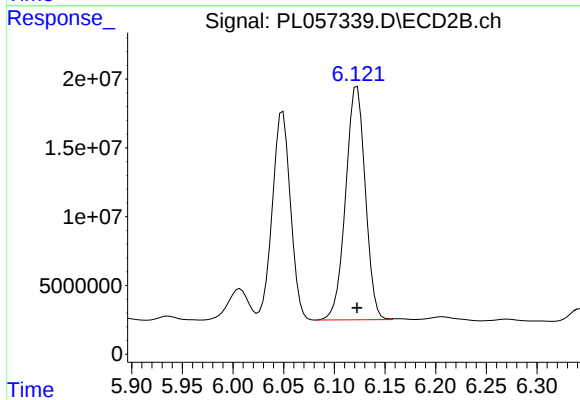


#26 Chlordane-4

R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 228847696
Conc: 500.00 ng/ml

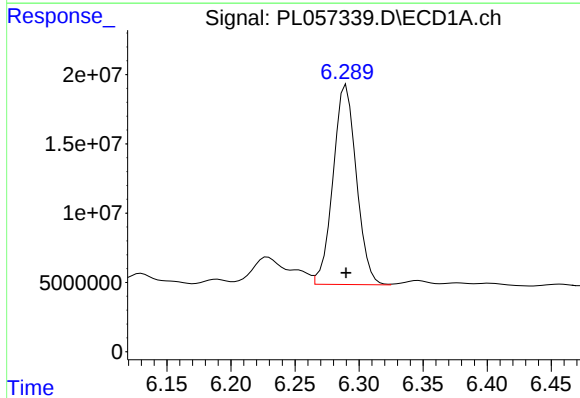


#27 Chlordane-5

R.T.: 6.290 min
Delta R.T.: 0.000 min
Response: 181928890
Conc: 500.00 ng/ml

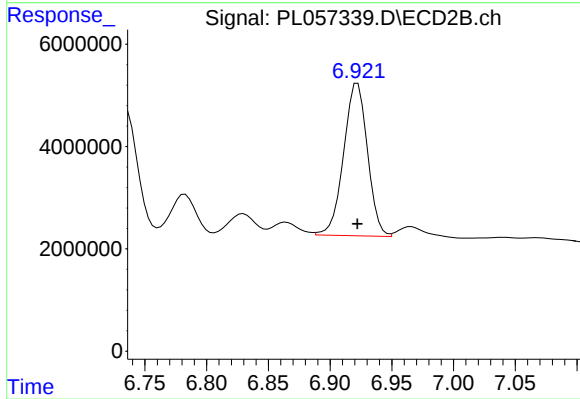

#27 Chlordane-5


R.T.: 6.922 min
Delta R.T.: 0.000 min
Response: 40067433
Conc: 500.00 ng/ml

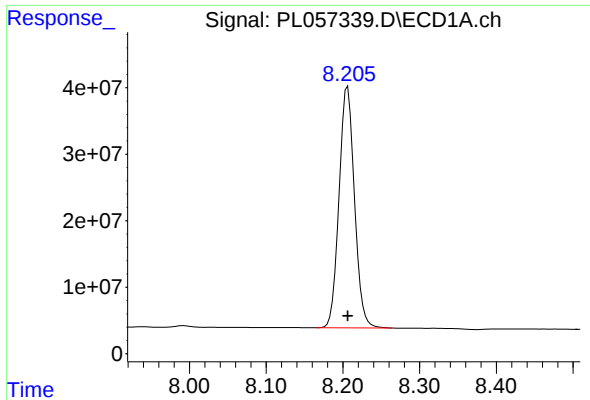

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 506811916
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

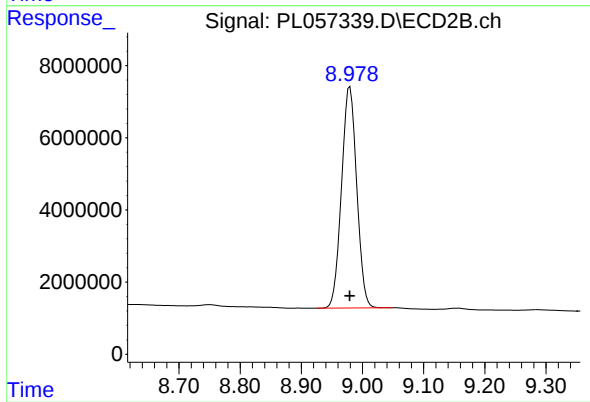

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: 0.000 min
Response: 105882796
Conc: 50.00 ng/ml