

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031420\
 Data File : PL057371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2020 01:24
 Operator : AJ\MA
 Sample : L1913-06
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MK-031220-0-2-COMP-B3

Manual Integrations
 APPROVED

mohammad
 3/17/2020 2:36:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 03:32:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 14 00:45:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.458	3.957	235.8E6	52413570	25.437	24.159
28) SA Decachlor...	8.206	8.979	173.8E6	45263501	16.421	20.413
Target Compounds						
13) MA Dieldrin	5.750	6.423	11153110	1558517	0.884m	0.527 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031420\
Data File : PL057371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2020 01:24
Operator : AJ\MA
Sample : L1913-06
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MK-031220-0-2-COMP-B3


Manual Integrations
APPROVED

mohammad
3/17/2020 2:36:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 03:32:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Sat Mar 14 00:45:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

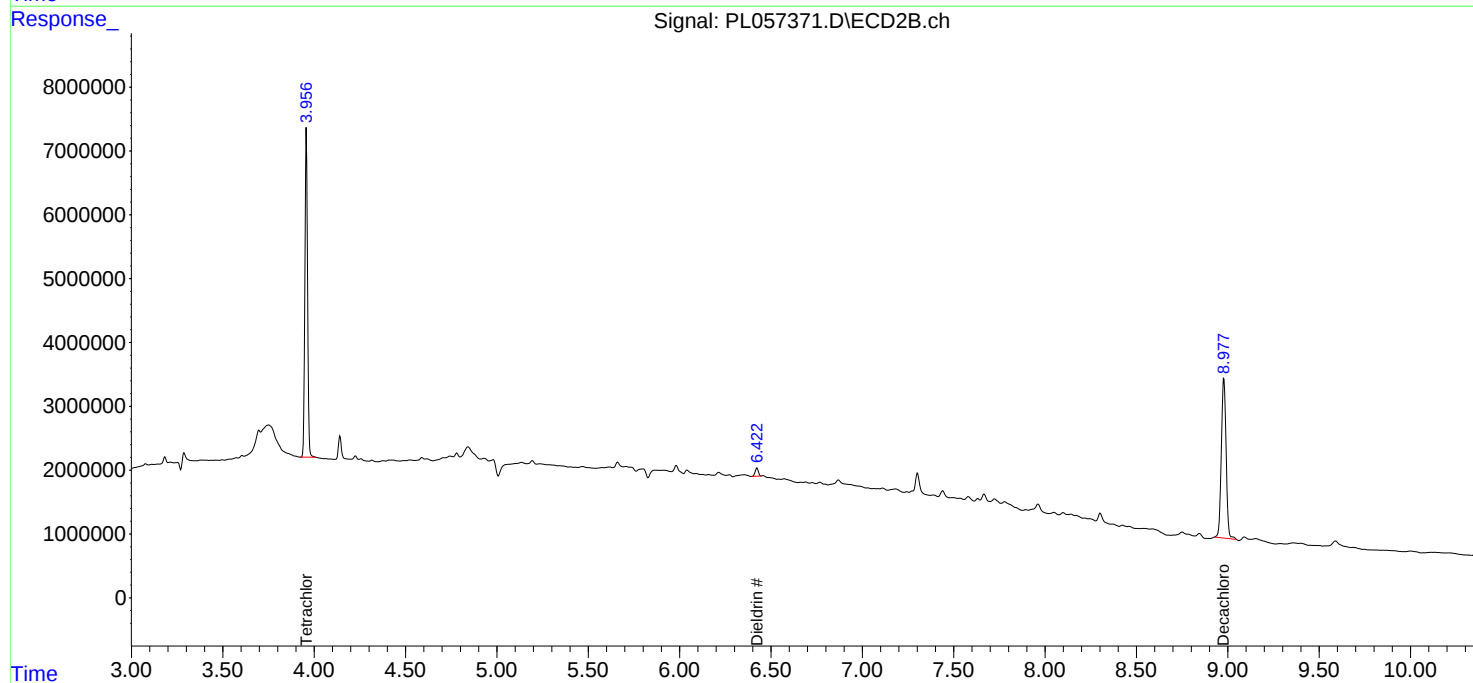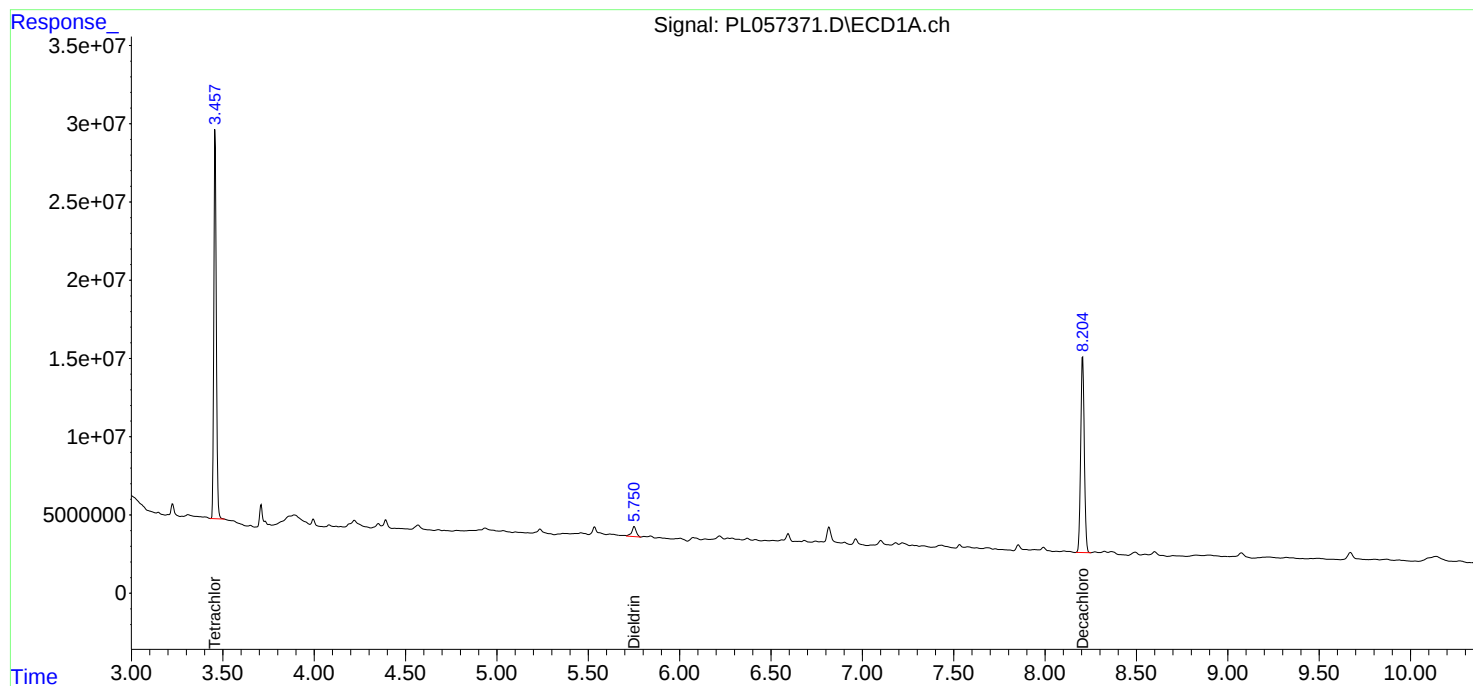

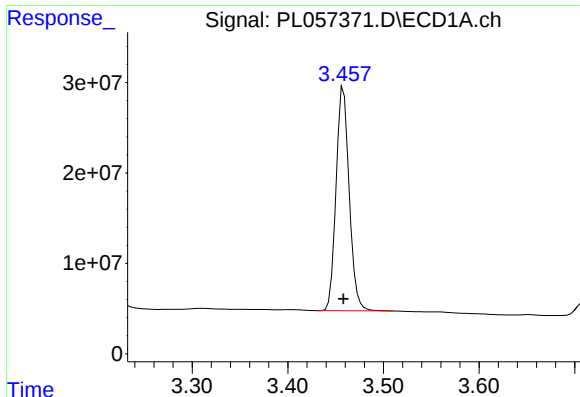


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 235782566
Conc: 25.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
MK-031220-0-2-COMP-B3


Manual Integrations
APPROVED

mohammad
3/17/2020 2:36:13 PM

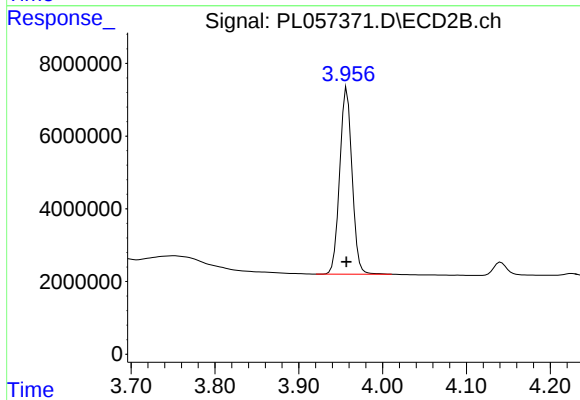


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 52413570
Conc: 24.16 ng/ml

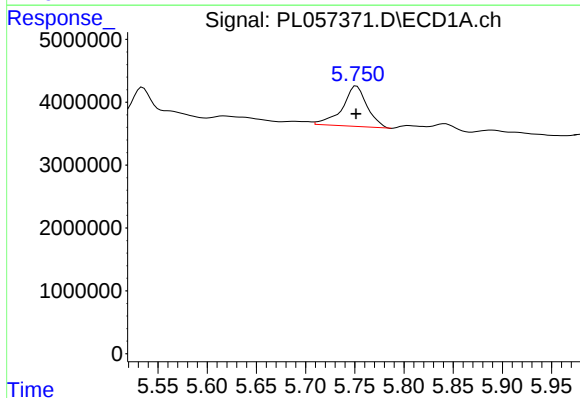


#13 Dieldrin

R.T.: 5.750 min
Delta R.T.: 0.000 min
Response: 11153110
Conc: 0.88 ng/ml m

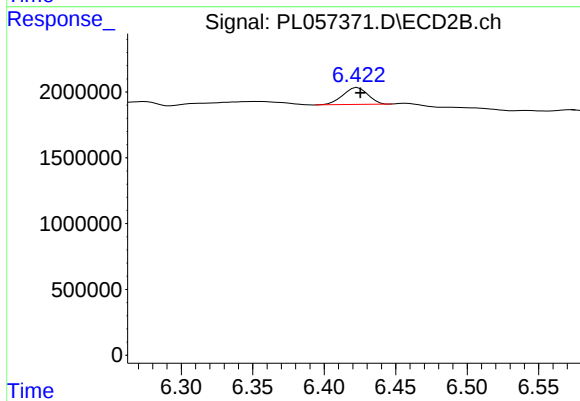

#13 Dieldrin

R.T.: 6.423 min
Delta R.T.: -0.002 min
Response: 1558517
Conc: 0.53 ng/ml

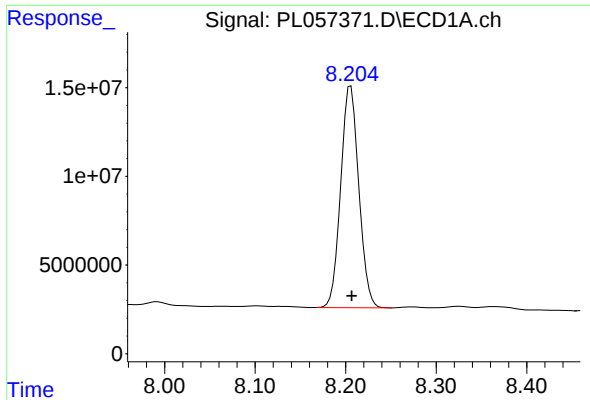


#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 173759052
Conc: 16.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
MK-031220-0-2-COMP-B3

Manual Integrations
APPROVED

mohammad
3/17/2020 2:36:13 PM

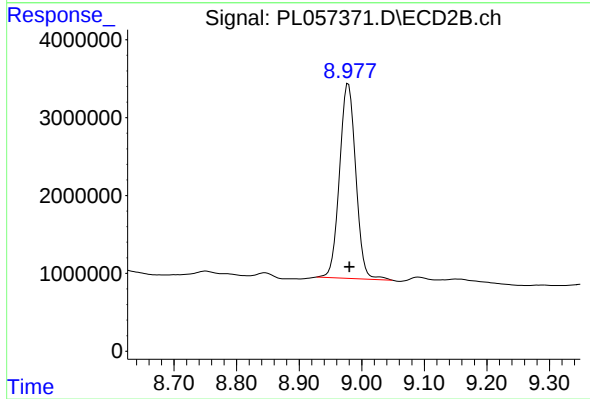

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.002 min
Response: 45263501
Conc: 20.41 ng/ml