

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031420\
 Data File : PL057380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2020 03:31
 Operator : AJ\MA
 Sample : L1907-04
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6-SA

Manual Integrations
 APPROVED

mohammad
 3/17/2020 2:36:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 04:10:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 14 00:45:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.957	187.9E6	42726205	20.274m	19.694
28)	SA Decachlor...	8.205	8.978	143.6E6	33006953	13.567	14.886

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031420\
Data File : PL057380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2020 03:31
Operator : AJ\MA
Sample : L1907-04
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-6-SA


Manual Integrations
APPROVED

mohammad
3/17/2020 2:36:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 04:10:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Sat Mar 14 00:45:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

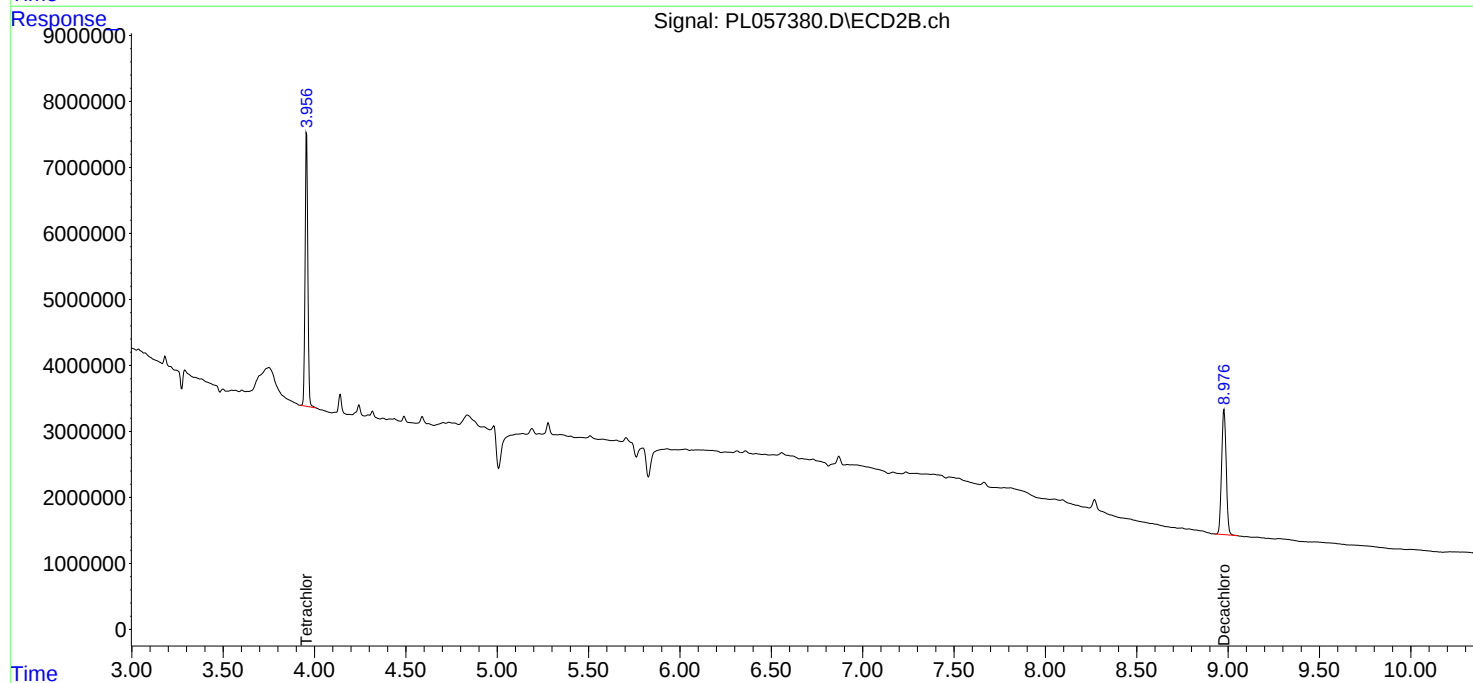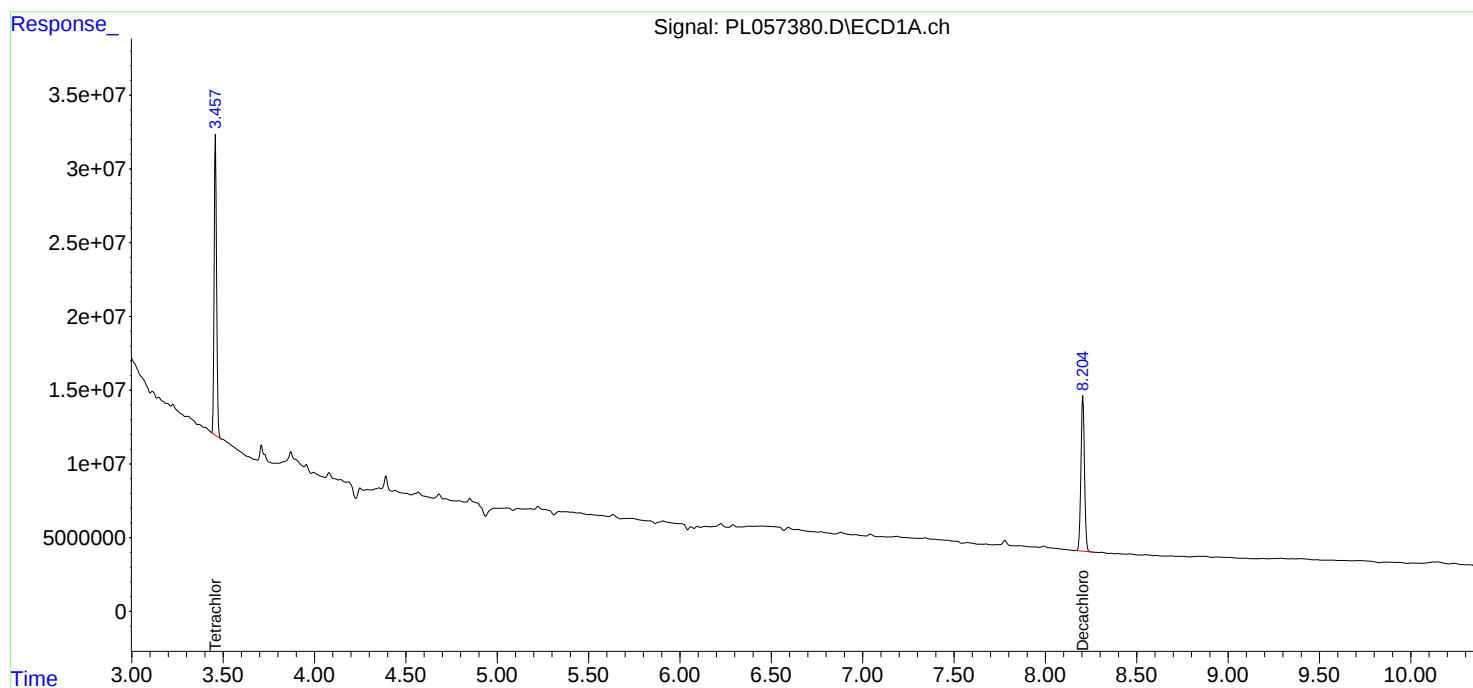

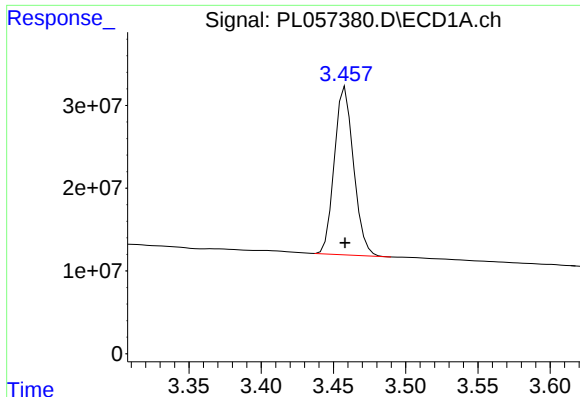


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 187930828
Conc: 20.27 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-6-SA


Manual Integrations
APPROVED

mohammad
3/17/2020 2:36:24 PM

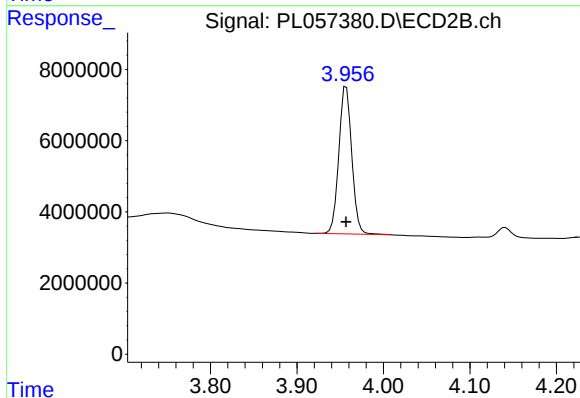


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 42726205
Conc: 19.69 ng/ml

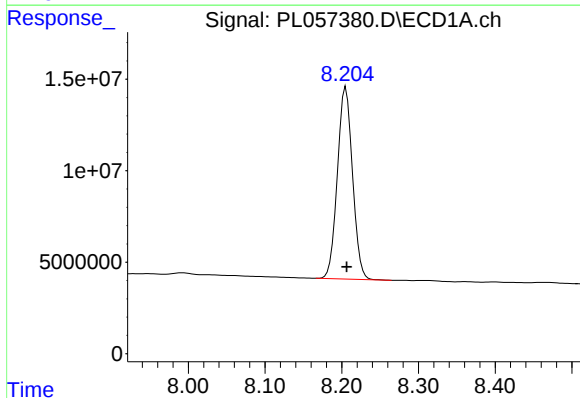

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.001 min
Response: 143559918
Conc: 13.57 ng/ml

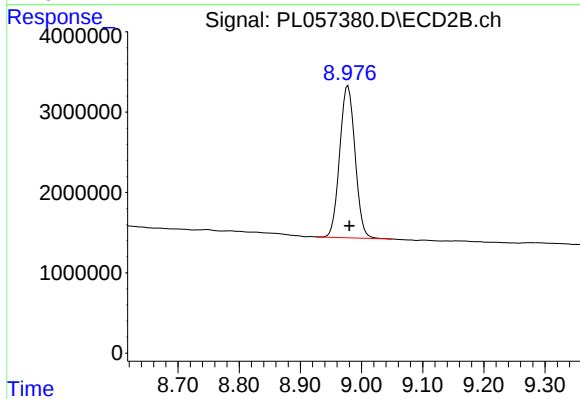

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.002 min
Response: 33006953
Conc: 14.89 ng/ml